
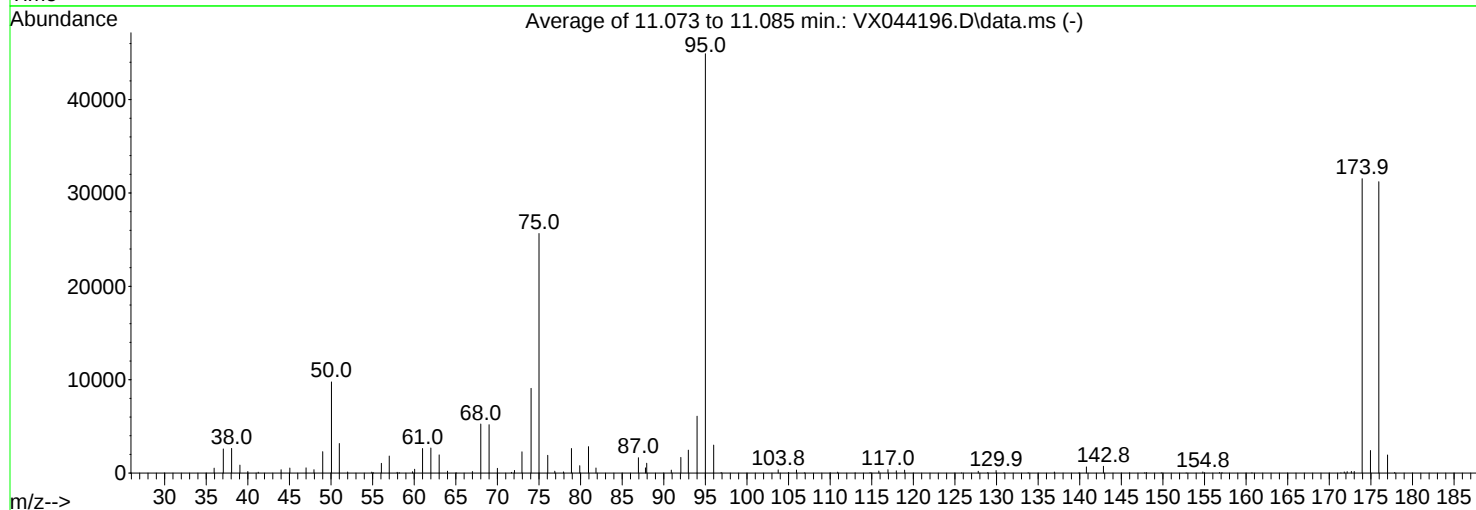


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121024\
Data File : VX044196.D
Acq On : 10 Dec 2024 09:01
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X112124W.M
Title : SW846 8260
Last Update : Fri Nov 22 03:45:52 2024

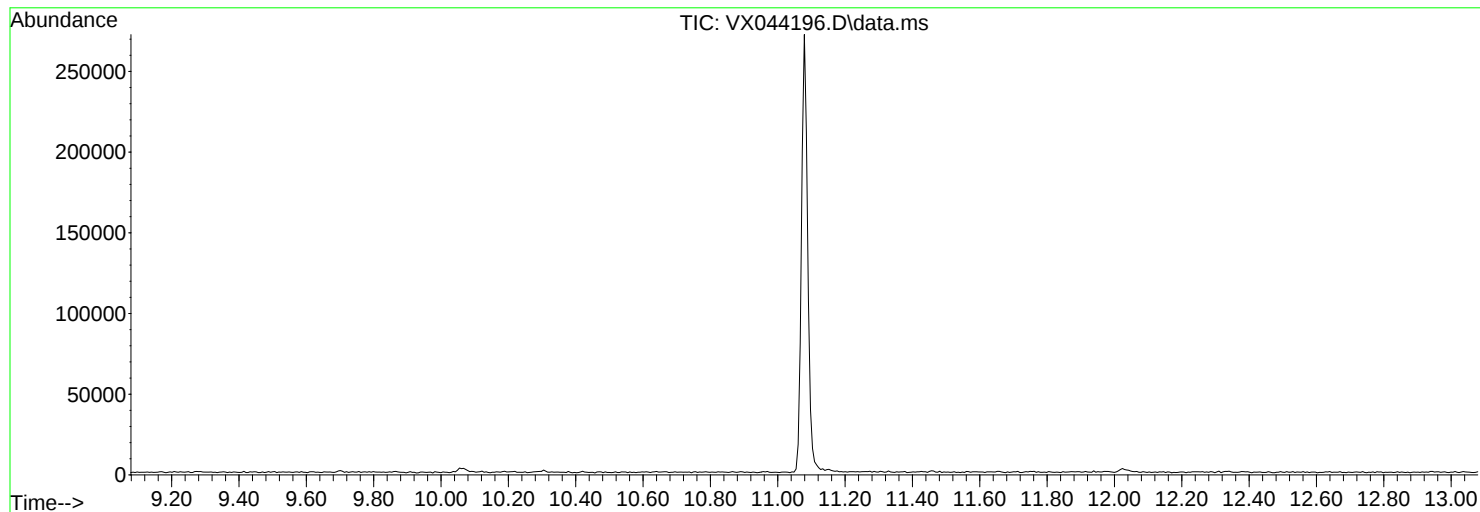

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	9765	PASS
75	95	30	60	57.1	25659	PASS
95	95	100	100	100.0	44912	PASS
96	95	5	9	6.7	2997	PASS
173	174	0.00	2	0.6	175	PASS
174	95	50	100	70.2	31531	PASS
175	174	5	9	7.7	2414	PASS
176	174	95	101	99.0	31205	PASS
177	176	5	9	6.2	1936	PASS