


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX121118\
 Data File : VX006410.D
 Acq On : 11 Dec 2018 10:12
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
 Title : SW846 8260
 Last Update : Fri Nov 30 03:55:33 2018

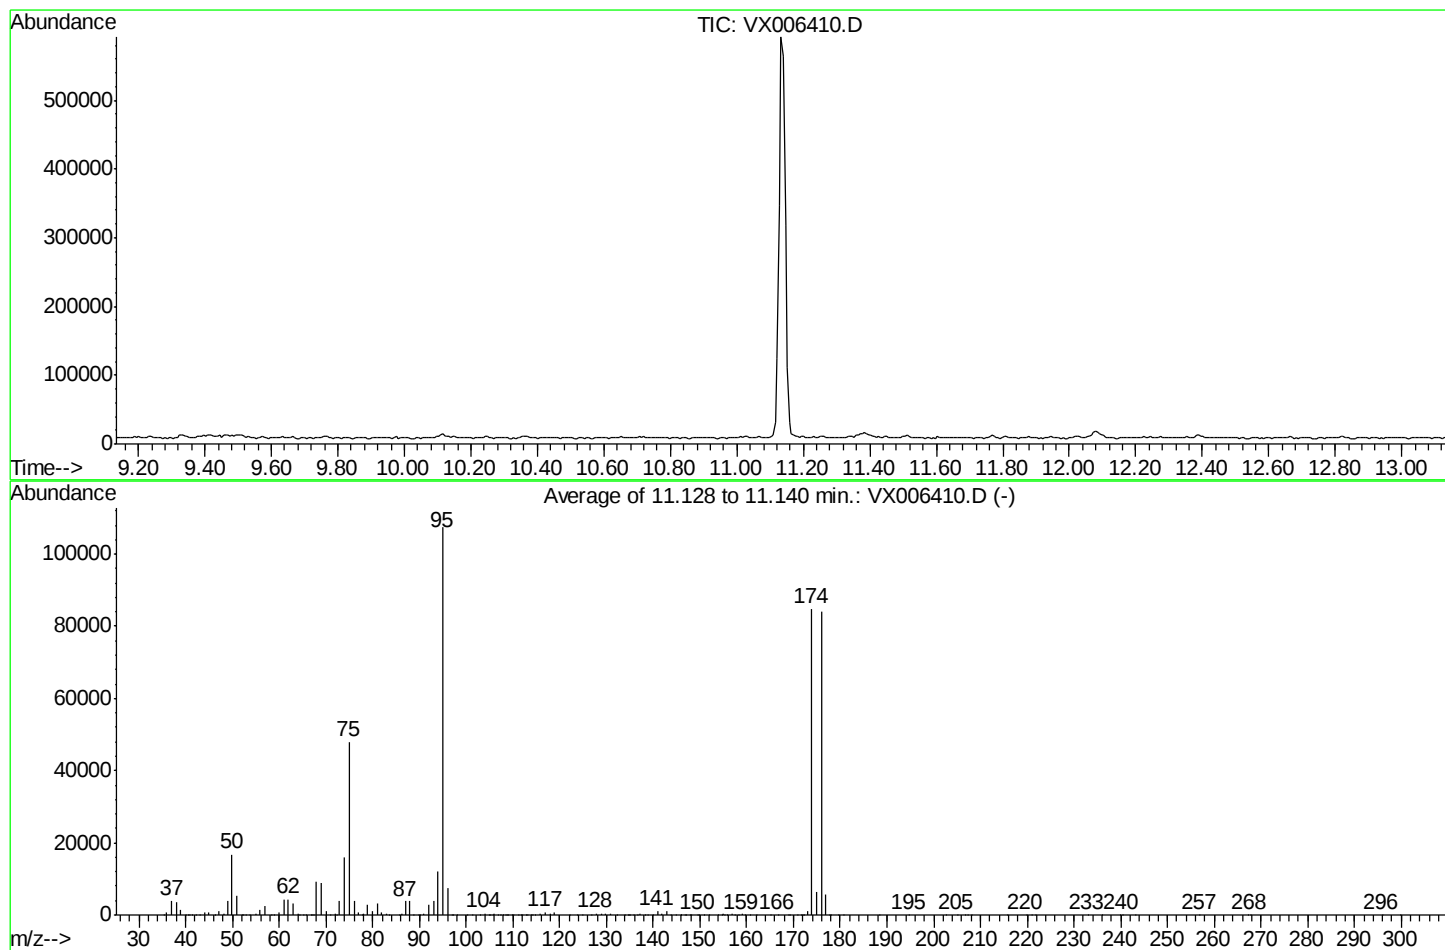

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	16820	PASS
75	95	30	60	44.6	47945	PASS
95	95	100	100	100.0	107413	PASS
96	95	5	9	7.0	7470	PASS
173	174	0.00	2	1.2	1034	PASS
174	95	50	100	79.0	84909	PASS
175	174	5	9	7.5	6397	PASS
176	174	95	101	99.0	84066	PASS
177	176	5	9	6.6	5580	PASS