


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX121119\
 Data File : VX013956.D
 Acq On : 11 Dec 2019 20:38
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112619W.M
 Title : SW846 8260
 Last Update : Tue Nov 26 15:53:00 2019

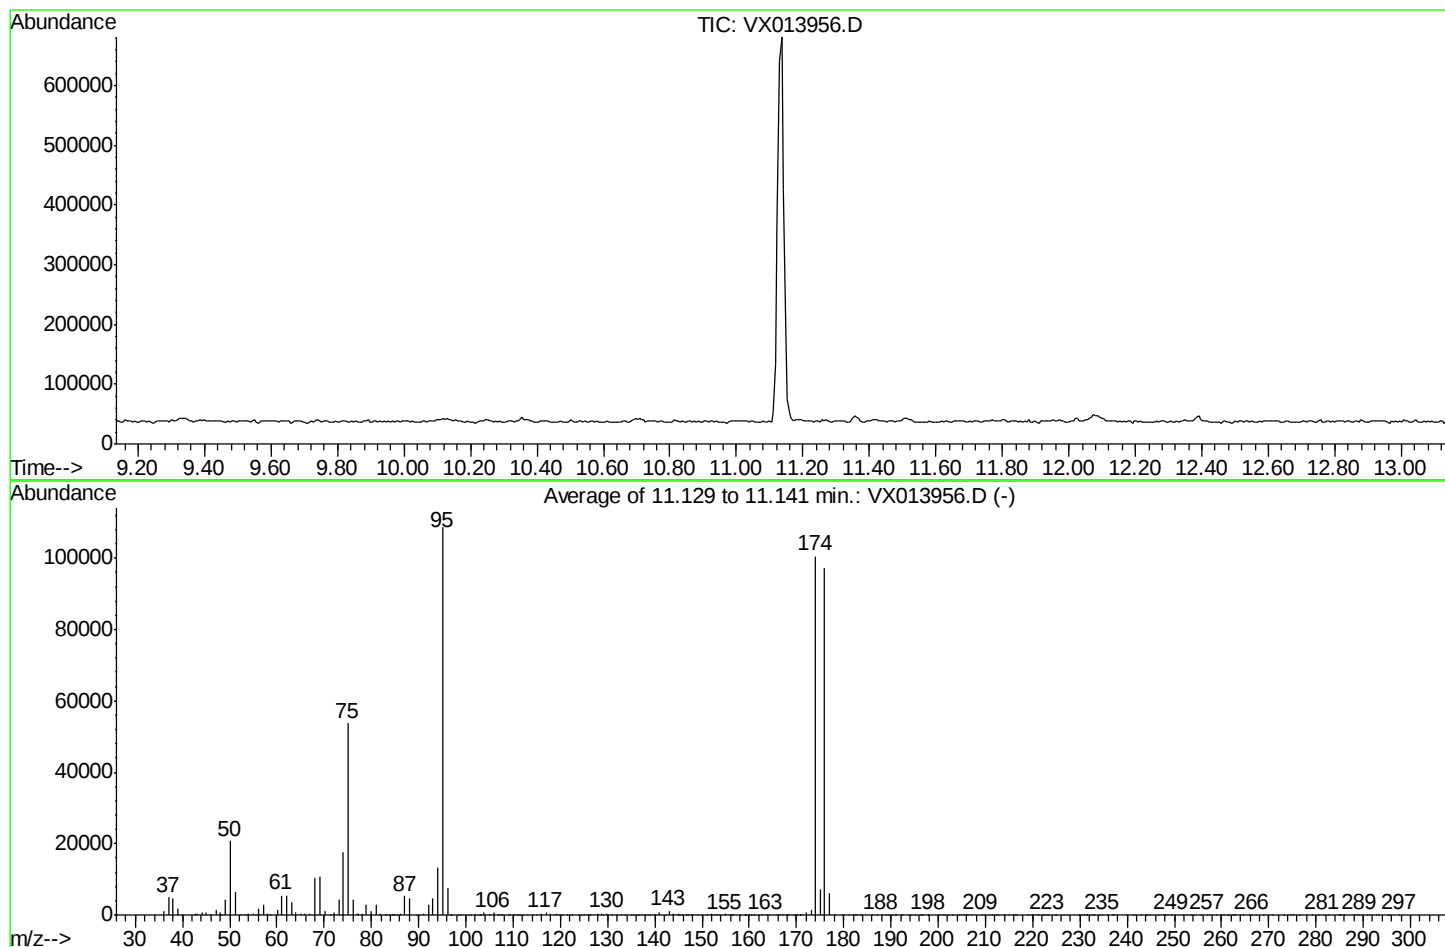

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	20646	PASS
75	95	30	60	49.4	53680	PASS
95	95	100	100	100.0	108626	PASS
96	95	5	9	6.8	7394	PASS
173	174	0.00	2	1.5	1485	PASS
174	95	50	100	92.5	100526	PASS
175	174	5	9	7.3	7361	PASS
176	174	95	101	96.8	97295	PASS
177	176	5	9	6.3	6115	PASS