

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025753.D
 Acq On : 11 Dec 2021 19:06
 Operator : JC/MD
 Sample : M5026-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COD10

Quant Time: Dec 12 06:36:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 11 00:48:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	83689	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	78543	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	32816	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	21186	37.094	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	74.180%		
7) Chloroethane-d5	1.666	69	19649	41.684	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	83.360%		
11) 1,1-Dichloroethene-d2	2.306	63	31978	35.115	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	70.240%		
21) 2-Butanone-d5	4.458	46	43576	102.494	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	102.490%		
24) Chloroform-d	5.068	84	48444	48.532	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.060%		
26) 1,2-Dichloroethane-d4	5.964	65	32626	52.438	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	104.880%		
32) Benzene-d6	5.976	84	93395	44.866	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.740%		
36) 1,2-Dichloropropane-d6	7.312	67	29419	45.646	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.300%		
41) Toluene-d8	8.653	98	84931	43.226	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.460%		
43) trans-1,3-Dichloroprop...	8.951	79	13358	41.225	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.440%		
47) 2-Hexanone-d5	9.384	63	29636	88.337	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	88.340%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	43074	47.290	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.580%		
66) 1,2-Dichlorobenzene-d4	12.323	152	30564	47.487	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.980%		
Target Compounds					Qvalue	
13) Acetone	2.386	43	963	2.755	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025753.D
Acq On : 11 Dec 2021 19:06
Operator : JC/MD
Sample : M5026-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0D10

Quant Time: Dec 12 06:36:39 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 11 00:48:07 2021
Response via : Initial Calibration

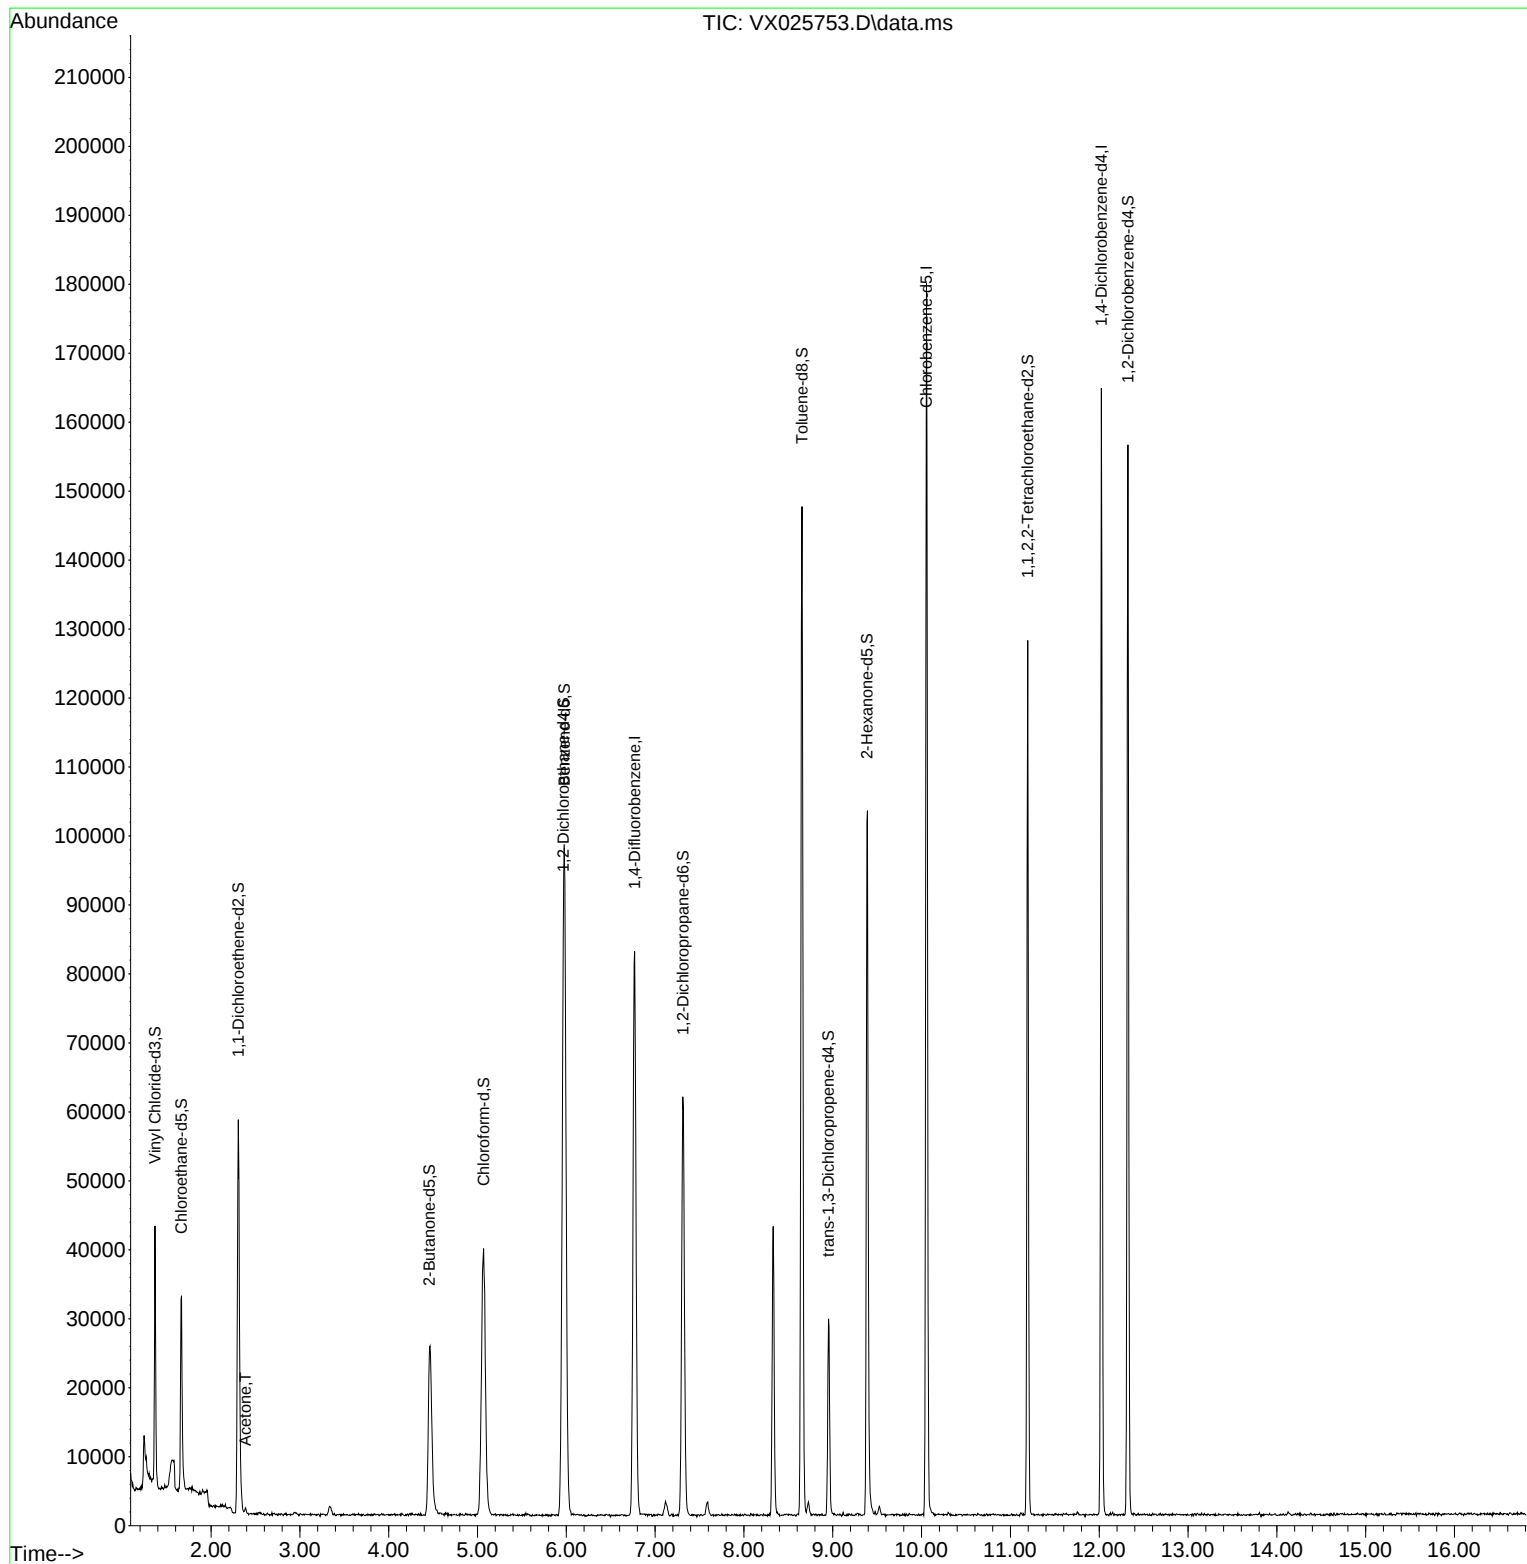

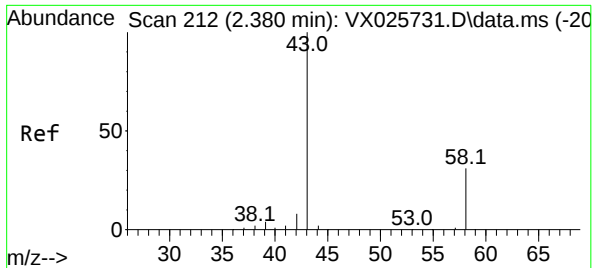

#13
 Acetone
 Concen: 2.755 ug/L
 RT: 2.386 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX025753.D
 Acq: 11 Dec 2021 19:06

Instrument :
 MSVOA_X
 ClientSampleId :
 C0D10

Tgt Ion: 43 Resp: 963
 Ion Ratio Lower Upper
 43 100
 58 29.1 0.0 65.6

