

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025732.D
 Acq On : 11 Dec 2021 10:42
 Operator : JC/MD
 Sample : VX1211MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK651

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025732.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	54	rVB	51331	50535	14.27%	1.816%
2	1.666	91	95	106	rVB	38300	49664	14.02%	1.785%
3	2.306	194	200	211	rVB	78636	129392	36.53%	4.650%
4	2.513	230	234	236	rBV	531	696	0.20%	0.025%
5	3.038	318	320	323	rVB	232	267	0.08%	0.010%
6	3.355	370	372	374	rBV2	256	252	0.07%	0.009%
7	3.501	393	396	397	rBV	285	223	0.06%	0.008%
8	3.733	432	434	441	rVB	268	241	0.07%	0.009%
9	3.800	444	445	447	rVB	415	196	0.06%	0.007%
10	3.824	447	449	452	rBV2	154	234	0.07%	0.008%
11	4.141	499	501	502	rBV	329	224	0.06%	0.008%
12	4.458	544	553	571	rBV	27712	78073	22.04%	2.806%
13	4.696	590	592	594	rBV	194	247	0.07%	0.009%
14	4.793	606	608	610	rBV	207	237	0.07%	0.009%
15	4.830	612	614	616	rVB2	298	230	0.06%	0.008%
16	4.909	624	627	630	rBV2	236	245	0.07%	0.009%
17	4.976	636	638	640	rBV	374	353	0.10%	0.013%
18	5.062	640	652	667	rVV	46925	148917	42.04%	5.352%
19	5.324	693	695	696	rBV	353	289	0.08%	0.010%
20	5.391	705	706	709	rVB2	270	194	0.05%	0.007%
21	5.495	721	723	724	rBV	290	224	0.06%	0.008%
22	5.549	730	732	734	rBV2	261	307	0.09%	0.011%
23	5.616	742	743	746	rBV	264	212	0.06%	0.008%
24	5.891	786	788	789	rBV	242	219	0.06%	0.008%
25	5.970	790	801	814	rVB2	119114	354203	100.00%	12.730%
26	6.299	853	855	857	rBV	270	237	0.07%	0.009%
27	6.513	887	890	894	rVB2	286	505	0.14%	0.018%
28	6.641	909	911	912	rBV	231	200	0.06%	0.007%
29	6.763	923	931	945	rBV2	95144	221129	62.43%	7.947%
30	7.110	984	988	994	rVV3	1567	3748	1.06%	0.135%
31	7.226	1005	1007	1008	rVV	393	263	0.07%	0.009%
32	7.311	1012	1021	1033	rVV	73706	160099	45.20%	5.754%
33	7.433	1038	1041	1042	rBV	253	227	0.06%	0.008%
34	7.458	1044	1045	1047	rBV2	256	220	0.06%	0.008%
35	7.750	1092	1093	1095	rBV	367	197	0.06%	0.007%
36	7.805	1099	1102	1104	rVV2	301	358	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025732.D
 Acq On : 11 Dec 2021 10:42
 Operator : JC/MD
 Sample : VX1211MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK651

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	7.860	1109	1111	1113	rVB2	278	260	0.07%	0.009%
38	7.964	1126	1128	1130	rBV2	258	229	0.06%	0.008%
39	8.025	1135	1138	1141	rBV2	331	488	0.14%	0.018%
40	8.098	1149	1150	1152	rBV2	289	245	0.07%	0.009%
41	8.220	1167	1170	1171	rBV2	337	249	0.07%	0.009%
42	8.281	1177	1180	1181	rBV	254	254	0.07%	0.009%
43	8.323	1181	1187	1197	rVV	52540	86566	24.44%	3.111%
44	8.445	1206	1207	1210	rBV2	214	266	0.08%	0.010%
45	8.531	1219	1221	1223	rBV	321	264	0.07%	0.009%
46	8.567	1226	1227	1229	rBV2	352	207	0.06%	0.007%
47	8.652	1234	1241	1248	rVV	185769	290438	82.00%	10.438%
48	8.720	1248	1252	1259	rVB2	2492	4480	1.26%	0.161%
49	8.829	1268	1270	1275	rVB	236	232	0.07%	0.008%
50	8.951	1285	1290	1297	rBV	38801	56023	15.82%	2.013%
51	9.274	1341	1343	1346	rVB2	409	422	0.12%	0.015%
52	9.317	1346	1350	1351	rVB2	187	196	0.06%	0.007%
53	9.384	1356	1361	1374	rBV	120108	173152	48.88%	6.223%
54	9.616	1396	1399	1401	rVB	251	281	0.08%	0.010%
55	9.847	1435	1437	1438	rBV	259	242	0.07%	0.009%
56	9.963	1451	1456	1457	rBV2	390	472	0.13%	0.017%
57	10.055	1465	1471	1481	rBV	208985	274303	77.44%	9.858%
58	10.183	1490	1492	1493	rVB	433	246	0.07%	0.009%
59	10.201	1493	1495	1500	rVB	670	680	0.19%	0.024%
60	10.305	1509	1512	1518	rVB3	521	753	0.21%	0.027%
61	10.402	1526	1528	1530	rVV	294	228	0.06%	0.008%
62	10.445	1534	1535	1536	rBV	381	205	0.06%	0.007%
63	10.518	1545	1547	1552	rVB2	257	291	0.08%	0.010%
64	10.585	1556	1558	1562	rVB	295	348	0.10%	0.013%
65	10.622	1562	1564	1565	rBV2	243	219	0.06%	0.008%
66	10.872	1601	1605	1608	rBV2	245	389	0.11%	0.014%
67	10.963	1618	1620	1623	rVB2	344	284	0.08%	0.010%
68	11.122	1641	1646	1649	rBV2	1157	1538	0.43%	0.055%
69	11.195	1652	1658	1668	rBV	140888	178215	50.31%	6.405%
70	11.384	1688	1689	1691	rBV	344	239	0.07%	0.009%
71	11.457	1696	1701	1704	rBV3	575	910	0.26%	0.033%
72	11.749	1745	1749	1755	rVB4	1411	2052	0.58%	0.074%
73	11.798	1755	1757	1759	rBV	381	384	0.11%	0.014%
74	11.969	1783	1785	1789	rBV2	333	348	0.10%	0.013%
75	12.024	1789	1794	1801	rVV	196799	247319	69.82%	8.888%
76	12.121	1807	1810	1811	rBV	555	557	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025732.D
 Acq On : 11 Dec 2021 10:42
 Operator : JC/MD
 Sample : VX1211MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK651

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

77	12.152	1813	1815	1820	rVB	1017	965	0.27%	0.035%
78	12.323	1837	1843	1851	rBV	195776	246193	69.51%	8.848%
79	12.950	1943	1946	1948	rBV2	251	345	0.10%	0.012%
80	13.115	1971	1973	1976	rBV	353	383	0.11%	0.014%
81	13.304	2002	2004	2006	rBV	350	269	0.08%	0.010%
82	13.341	2008	2010	2013	rVB2	361	337	0.10%	0.012%
83	13.377	2013	2016	2020	rBV2	238	355	0.10%	0.013%
84	13.585	2049	2050	2053	rBV2	280	316	0.09%	0.011%
85	13.627	2056	2057	2059	rBV	229	207	0.06%	0.007%
86	13.774	2079	2081	2087	rVB3	343	499	0.14%	0.018%
87	13.914	2102	2104	2107	rBV2	220	307	0.09%	0.011%
88	14.023	2119	2122	2123	rBV	470	358	0.10%	0.013%
89	14.054	2126	2127	2130	rBV2	389	422	0.12%	0.015%
90	14.133	2138	2140	2144	rVB2	626	625	0.18%	0.022%
91	14.310	2167	2169	2171	rBV2	380	308	0.09%	0.011%
92	14.688	2230	2231	2233	rBV	300	282	0.08%	0.010%
93	14.846	2255	2257	2259	rBV	469	391	0.11%	0.014%
94	14.981	2277	2279	2282	rBV	284	220	0.06%	0.008%
95	15.389	2344	2346	2350	rBV2	388	527	0.15%	0.019%
96	15.529	2367	2369	2373	rBV2	257	306	0.09%	0.011%
97	15.859	2421	2423	2425	rBV3	298	322	0.09%	0.012%
98	16.054	2452	2455	2457	rBV2	374	459	0.13%	0.016%
99	16.072	2457	2458	2460	rBV2	280	226	0.06%	0.008%
100	16.395	2509	2511	2514	rBV2	250	324	0.09%	0.012%




Sum of corrected areas: 2782477

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025732.D
Acq On : 11 Dec 2021 10:42
Operator : JC/MD
Sample : VX1211MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK651

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

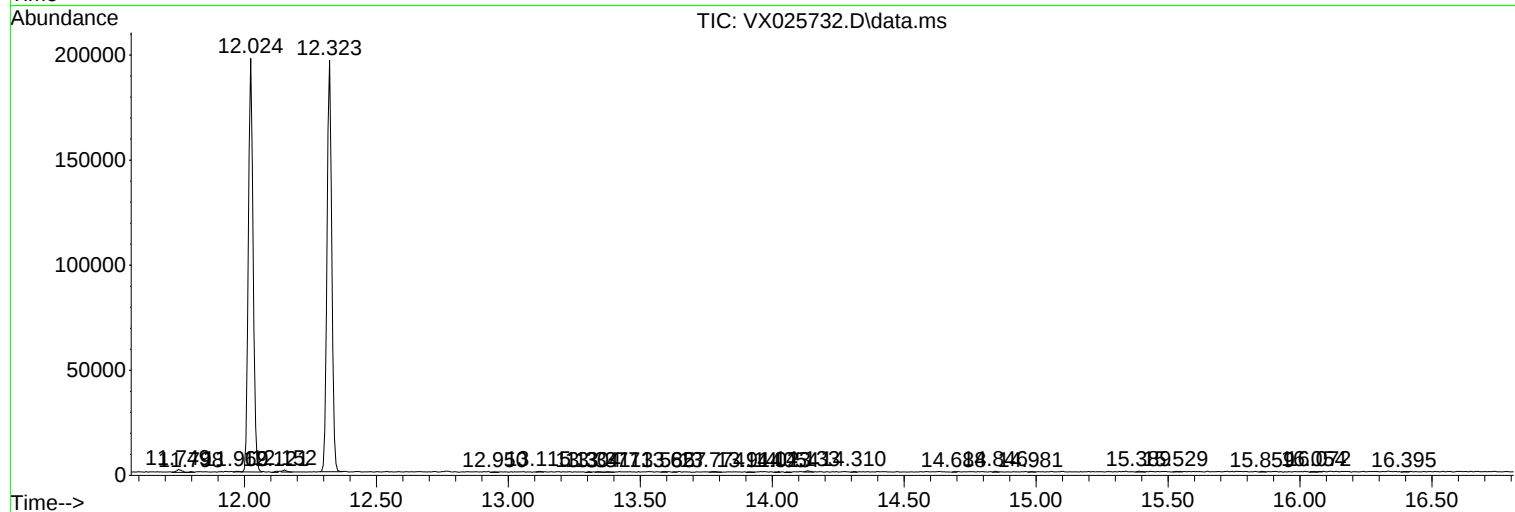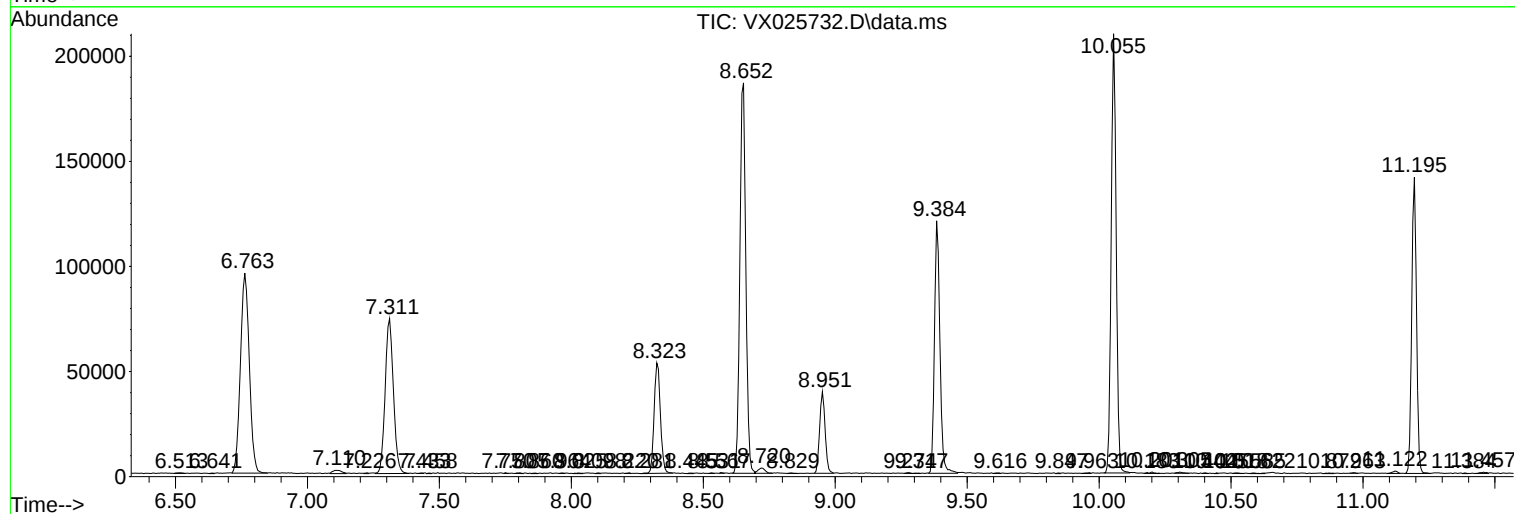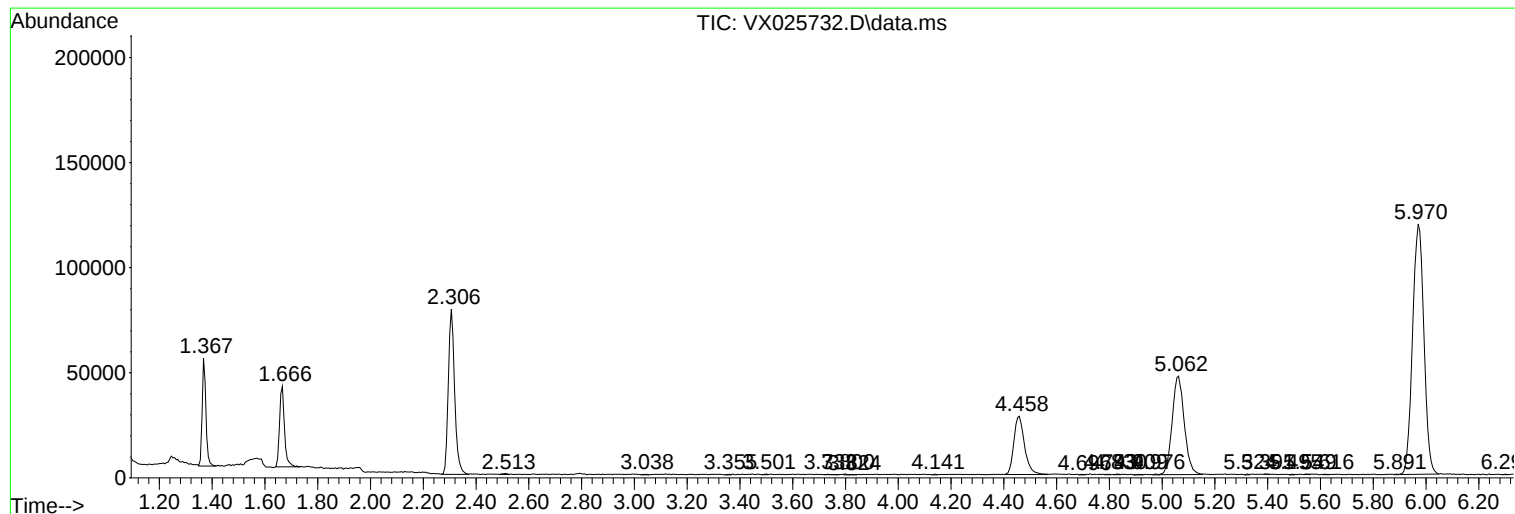

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025732.D
Acq On : 11 Dec 2021 10:42
Operator : JC/MD
Sample : VX1211MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK651

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025732.D
Acq On : 11 Dec 2021 10:42
Operator : JC/MD
Sample : VX1211MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK651

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc