

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025742.D
 Acq On : 11 Dec 2021 14:48
 Operator : JC/MD
 Sample : M4997-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW5R2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	33	rBV	10193	16024	5.07%	0.533%
2	1.368	43	46	53	rVB	44214	42956	13.59%	1.428%
3	1.666	91	95	103	rBV	35515	46588	14.74%	1.549%
4	2.306	194	200	209	rBV	70908	111535	35.30%	3.707%
5	2.739	269	271	273	rBV2	387	448	0.14%	0.015%
6	3.044	318	321	324	rBV2	294	444	0.14%	0.015%
7	3.093	324	329	339	rVB4	2470	5953	1.88%	0.198%
8	3.611	406	414	424	rBV	46424	109508	34.66%	3.640%
9	3.770	438	440	442	rBV2	322	403	0.13%	0.013%
10	4.026	480	482	485	rBV2	293	319	0.10%	0.011%
11	4.477	545	556	571	rBV3	33754	136635	43.24%	4.542%
12	4.946	631	633	635	rBV	217	217	0.07%	0.007%
13	5.062	640	652	666	rBV	43077	133526	42.26%	4.438%
14	5.288	687	689	692	rBV	314	276	0.09%	0.009%
15	5.391	695	706	722	rVB2	72197	223711	70.80%	7.436%
16	5.556	731	733	734	rBV	372	200	0.06%	0.007%
17	5.635	743	746	747	rBV	363	322	0.10%	0.011%
18	5.976	791	802	815	rBV2	109104	315975	100.00%	10.503%
19	6.562	894	898	900	rBV	280	379	0.12%	0.013%
20	6.769	923	932	943	rVB	88418	211799	67.03%	7.040%
21	7.129	983	991	999	rBV5	4548	10523	3.33%	0.350%
22	7.208	1002	1004	1006	rVB	312	238	0.08%	0.008%
23	7.312	1013	1021	1033	rVB	66646	144758	45.81%	4.812%
24	7.464	1044	1046	1048	rBV2	232	194	0.06%	0.006%
25	7.598	1066	1068	1069	rBV	255	232	0.07%	0.008%
26	7.824	1103	1105	1107	rBV	387	356	0.11%	0.012%
27	8.129	1153	1155	1159	rVB	270	284	0.09%	0.009%
28	8.159	1159	1160	1162	rBV	393	230	0.07%	0.008%
29	8.330	1182	1188	1195	rBV	48385	77315	24.47%	2.570%
30	8.567	1225	1227	1230	rBV	221	226	0.07%	0.008%
31	8.653	1234	1241	1249	rBV	166921	256338	81.13%	8.521%
32	8.775	1259	1261	1263	rBV	363	270	0.09%	0.009%
33	8.793	1263	1264	1267	rVB	329	217	0.07%	0.007%
34	8.952	1285	1290	1296	rBV	35392	49496	15.66%	1.645%
35	9.025	1300	1302	1304	rBV	330	357	0.11%	0.012%
36	9.238	1335	1337	1338	rBV	295	245	0.08%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025742.D
 Acq On : 11 Dec 2021 14:48
 Operator : JC/MD
 Sample : M4997-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW5R2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	9.275	1338	1343	1350	rVB2	16259	24139	7.64%	0.802%
38	9.384	1356	1361	1372	rBV	112634	164203	51.97%	5.458%
39	9.836	1434	1435	1442	rBV2	259	335	0.11%	0.011%
40	9.988	1458	1460	1462	rBV2	230	214	0.07%	0.007%
41	10.055	1466	1471	1481	rVV	195741	259129	82.01%	8.613%
42	10.201	1492	1495	1499	rVB2	842	881	0.28%	0.029%
43	10.305	1508	1512	1517	rVV2	1577	1896	0.60%	0.063%
44	10.482	1538	1541	1544	rBV	154	252	0.08%	0.008%
45	10.518	1544	1547	1549	rVV2	330	381	0.12%	0.013%
46	10.561	1552	1554	1556	rVB2	390	301	0.10%	0.010%
47	10.646	1565	1568	1574	rVB3	1315	1672	0.53%	0.056%
48	10.939	1614	1616	1618	rVB	360	263	0.08%	0.009%
49	10.957	1618	1619	1621	rBV2	424	274	0.09%	0.009%
50	11.037	1631	1632	1634	rVB	285	195	0.06%	0.006%
51	11.122	1642	1646	1649	rBV3	746	844	0.27%	0.028%
52	11.195	1653	1658	1664	rBV	132803	164699	52.12%	5.475%
53	11.311	1675	1677	1682	rVB3	887	1129	0.36%	0.038%
54	11.384	1685	1689	1697	rVB2	2150	3698	1.17%	0.123%
55	11.457	1697	1701	1704	rBV3	1119	1567	0.50%	0.052%
56	11.530	1711	1713	1714	rVB	455	307	0.10%	0.010%
57	11.555	1714	1717	1719	rBV2	417	531	0.17%	0.018%
58	11.616	1724	1727	1732	rVB2	1345	1829	0.58%	0.061%
59	11.658	1732	1734	1735	rBV2	247	239	0.08%	0.008%
60	11.677	1735	1737	1738	rVB2	378	227	0.07%	0.008%
61	11.756	1746	1750	1758	rVB2	5823	7693	2.43%	0.256%
62	11.988	1785	1788	1789	rBV2	239	200	0.06%	0.007%
63	12.024	1789	1794	1802	rVV	187415	235282	74.46%	7.821%
64	12.091	1802	1805	1808	rVB2	1954	2306	0.73%	0.077%
65	12.134	1808	1812	1813	rBV	415	435	0.14%	0.014%
66	12.152	1813	1815	1818	rVB2	615	521	0.16%	0.017%
67	12.244	1827	1830	1833	rBV3	548	621	0.20%	0.021%
68	12.323	1838	1843	1856	rVB	175713	223257	70.66%	7.421%
69	12.548	1877	1880	1886	rVV2	388	576	0.18%	0.019%
70	12.591	1886	1887	1889	rVB	311	180	0.06%	0.006%
71	12.762	1912	1915	1916	rVB2	473	318	0.10%	0.011%
72	12.811	1921	1923	1925	rBV	240	215	0.07%	0.007%
73	12.926	1940	1942	1944	rBV2	300	347	0.11%	0.012%
74	12.963	1947	1948	1951	rVV2	396	291	0.09%	0.010%
75	13.097	1969	1970	1973	rVV	225	184	0.06%	0.006%
76	13.134	1973	1976	1979	rVB	223	241	0.08%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025742.D
 Acq On : 11 Dec 2021 14:48
 Operator : JC/MD
 Sample : M4997-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW5R2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	13.268	1995	1998	1999	rBV	271	288	0.09%	0.010%
78	13.298	2002	2003	2006	rBV	310	319	0.10%	0.011%
79	13.426	2021	2024	2027	rBV	260	440	0.14%	0.015%
80	13.457	2027	2029	2030	rVB	298	182	0.06%	0.006%
81	13.634	2056	2058	2061	rBV	322	304	0.10%	0.010%
82	13.658	2061	2062	2066	rVV	243	246	0.08%	0.008%
83	13.707	2066	2070	2072	rVB	427	594	0.19%	0.020%
84	13.725	2072	2073	2075	rBV2	309	259	0.08%	0.009%
85	13.786	2079	2083	2087	rBV3	514	906	0.29%	0.030%
86	13.859	2091	2095	2096	rBV	334	263	0.08%	0.009%
87	13.902	2100	2102	2105	rVB	221	223	0.07%	0.007%
88	13.981	2112	2115	2117	rBV	296	334	0.11%	0.011%
89	14.280	2161	2164	2168	rBV	260	417	0.13%	0.014%
90	14.316	2168	2170	2173	rBV	311	394	0.12%	0.013%
91	14.457	2191	2193	2195	rBV	331	285	0.09%	0.009%
92	14.524	2202	2204	2207	rBV	260	249	0.08%	0.008%
93	14.597	2215	2216	2219	rBV	296	317	0.10%	0.011%
94	14.975	2276	2278	2279	rBV	381	229	0.07%	0.008%
95	15.011	2282	2284	2286	rBV	317	179	0.06%	0.006%
96	15.524	2366	2368	2370	rBV2	408	284	0.09%	0.009%
97	15.627	2383	2385	2387	rBV2	309	319	0.10%	0.011%
98	15.761	2405	2407	2409	rBV2	298	292	0.09%	0.010%
99	16.005	2443	2447	2448	rBV	310	418	0.13%	0.014%
100	16.048	2453	2454	2458	rVV2	352	358	0.11%	0.012%




Sum of corrected areas: 3008468

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025742.D
Acq On : 11 Dec 2021 14:48
Operator : JC/MD
Sample : M4997-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW5R2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

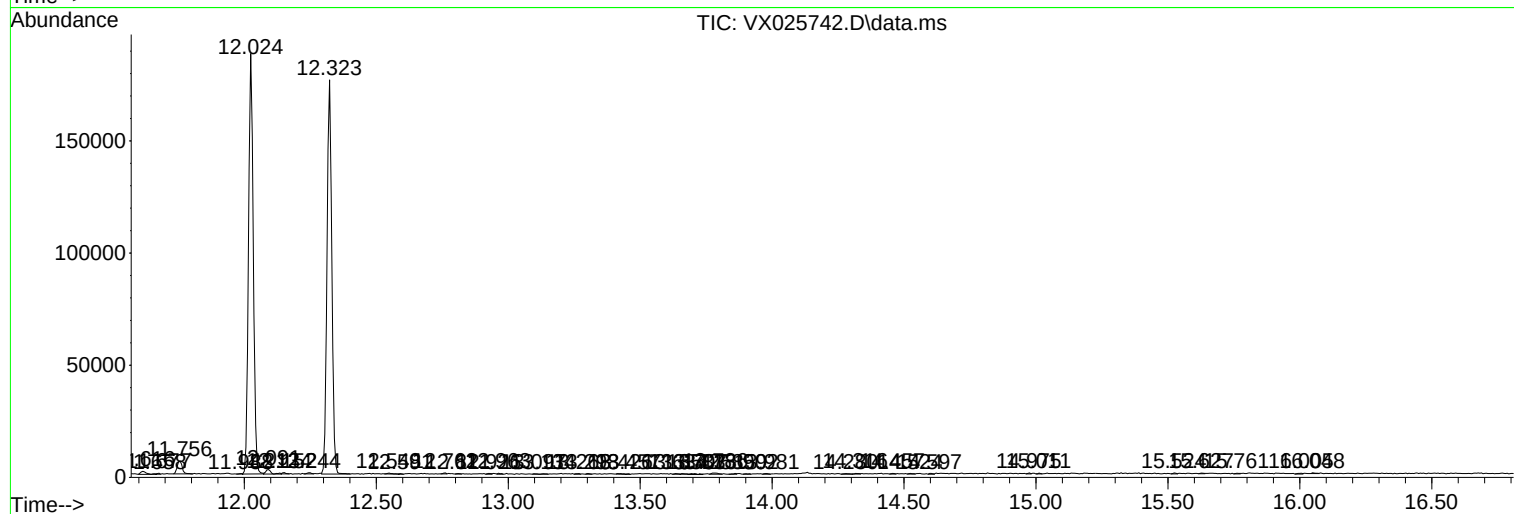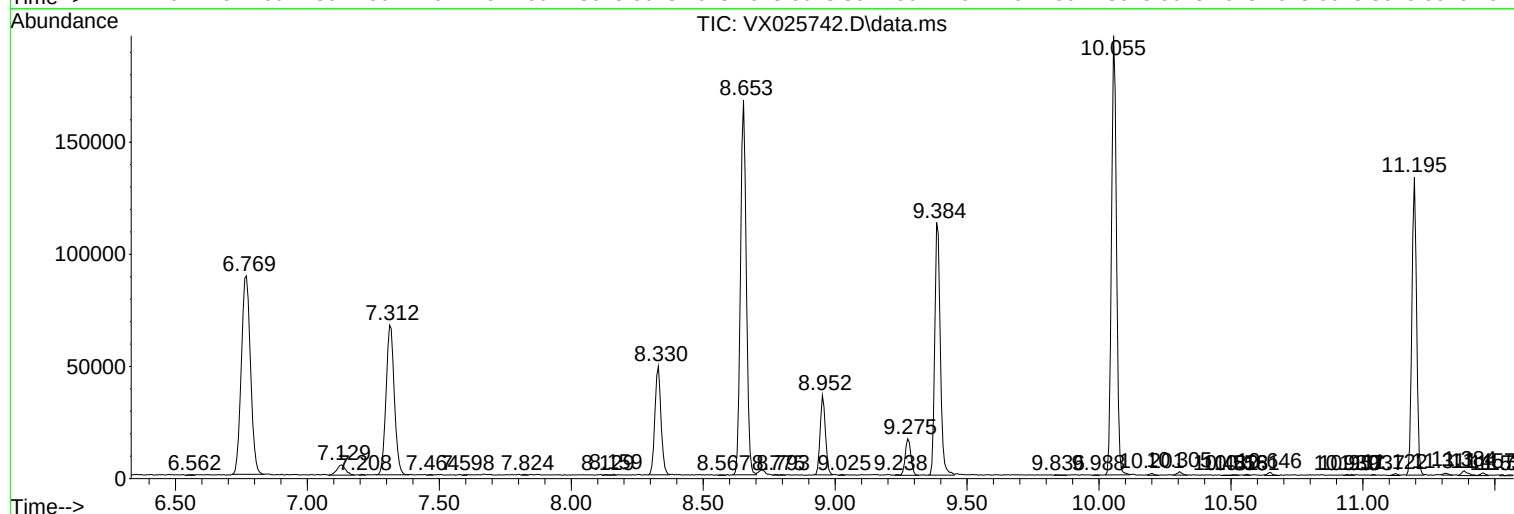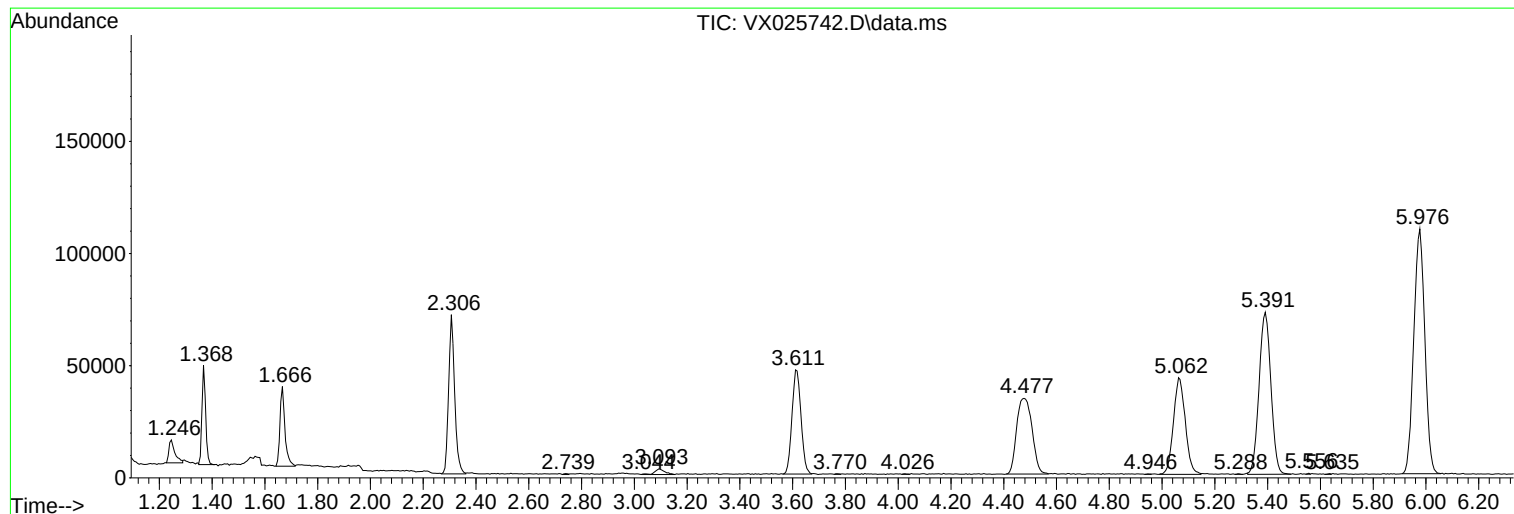

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025742.D
Acq On : 11 Dec 2021 14:48
Operator : JC/MD
Sample : M4997-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW5R2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025742.D
Acq On : 11 Dec 2021 14:48
Operator : JC/MD
Sample : M4997-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW5R2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc