

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025746.D
 Acq On : 11 Dec 2021 16:22
 Operator : JC/MD
 Sample : M5026-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025746.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	31	rBV	7169	11609	3.01%	0.396%
2	1.368	43	46	55	rVB	40975	39710	10.29%	1.355%
3	1.666	91	95	104	rVB	33226	43074	11.16%	1.469%
4	2.307	194	200	210	rVB2	68620	122327	31.69%	4.173%
5	2.520	231	235	236	rBV2	425	556	0.14%	0.019%
6	2.715	264	267	269	rVB3	372	508	0.13%	0.017%
7	2.928	299	302	303	rBV	406	396	0.10%	0.014%
8	3.154	337	339	342	rBV	154	147	0.04%	0.005%
9	3.178	342	343	346	rVV2	218	203	0.05%	0.007%
10	3.209	347	348	352	rVB	436	428	0.11%	0.015%
11	3.239	352	353	355	rBV	506	275	0.07%	0.009%
12	3.258	355	356	359	rBV	343	357	0.09%	0.012%
13	3.306	363	364	366	rBV2	191	193	0.05%	0.007%
14	3.434	383	385	389	rVB2	283	241	0.06%	0.008%
15	3.526	398	400	403	rBV2	222	185	0.05%	0.006%
16	3.611	409	414	425	rVB5	1005	2166	0.56%	0.074%
17	3.684	425	426	428	rBV	204	167	0.04%	0.006%
18	3.770	439	440	442	rVB2	342	231	0.06%	0.008%
19	3.788	442	443	444	rBV	399	180	0.05%	0.006%
20	3.855	453	454	457	rBV2	261	175	0.05%	0.006%
21	3.886	457	459	461	rBV	274	231	0.06%	0.008%
22	3.910	461	463	464	rVB2	259	178	0.05%	0.006%
23	4.032	480	483	484	rBV2	234	200	0.05%	0.007%
24	4.111	495	496	499	rVB	298	277	0.07%	0.009%
25	4.190	506	509	510	rBV2	198	265	0.07%	0.009%
26	4.270	521	522	525	rBV2	324	379	0.10%	0.013%
27	4.379	539	540	543	rBV2	200	232	0.06%	0.008%
28	4.465	545	554	572	rVV3	28528	101900	26.40%	3.476%
29	4.635	581	582	587	rVB3	367	400	0.10%	0.014%
30	4.684	587	590	591	rBV	322	284	0.07%	0.010%
31	4.879	621	622	625	rVV2	234	187	0.05%	0.006%
32	4.977	636	638	640	rVB	222	154	0.04%	0.005%
33	5.062	640	652	667	rBV	43097	130823	33.90%	4.463%
34	5.312	691	693	694	rBV	248	156	0.04%	0.005%
35	5.385	698	705	714	rVV3	2966	9158	2.37%	0.312%
36	5.623	743	744	748	rBV	237	253	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025746.D
 Acq On : 11 Dec 2021 16:22
 Operator : JC/MD
 Sample : M5026-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

37	5.751	763	765	766	rBV	286	159	0.04%	0.005%
38	5.977	788	802	816	rBV2	103387	309813	80.27%	10.569%
39	6.172	833	834	836	rBV	391	232	0.06%	0.008%
40	6.196	836	838	839	rBV	260	159	0.04%	0.005%
41	6.221	841	842	846	rVB	257	237	0.06%	0.008%
42	6.580	900	901	904	rBV2	308	329	0.09%	0.011%
43	6.769	922	932	944	rBV	86240	206027	53.38%	7.028%
44	6.995	968	969	970	rBV	373	200	0.05%	0.007%
45	7.129	982	991	1005	rVV	177321	385951	100.00%	13.166%
46	7.312	1012	1021	1031	rBV	65985	142869	37.02%	4.874%
47	7.611	1069	1070	1073	rBV	211	234	0.06%	0.008%
48	7.757	1091	1094	1095	rBV	304	293	0.08%	0.010%
49	8.141	1156	1157	1160	rVB	216	155	0.04%	0.005%
50	8.330	1182	1188	1196	rBV	46176	74412	19.28%	2.538%
51	8.458	1207	1209	1212	rBV2	265	254	0.07%	0.009%
52	8.653	1235	1241	1249	rBV	161754	249462	64.64%	8.510%
53	8.720	1250	1252	1259	rVB2	2176	3054	0.79%	0.104%
54	8.836	1268	1271	1274	rVB2	295	385	0.10%	0.013%
55	8.952	1285	1290	1299	rBV2	34379	47953	12.42%	1.636%
56	9.080	1309	1311	1314	rBV2	165	217	0.06%	0.007%
57	9.110	1314	1316	1317	rBV	224	152	0.04%	0.005%
58	9.183	1325	1328	1329	rBV2	235	239	0.06%	0.008%
59	9.281	1341	1344	1346	rVB3	615	680	0.18%	0.023%
60	9.391	1356	1362	1373	rBV	108428	163120	42.26%	5.565%
61	9.781	1423	1426	1428	rBV	302	280	0.07%	0.010%
62	10.055	1466	1471	1482	rBV	189833	254194	65.86%	8.671%
63	10.439	1532	1534	1536	rVB	278	150	0.04%	0.005%
64	10.567	1551	1555	1557	rBV2	254	374	0.10%	0.013%
65	10.640	1566	1567	1571	rVB	425	452	0.12%	0.015%
66	10.768	1584	1588	1590	rBV2	349	458	0.12%	0.016%
67	11.025	1628	1630	1633	rVB2	261	277	0.07%	0.009%
68	11.122	1643	1646	1649	rVV3	570	766	0.20%	0.026%
69	11.195	1653	1658	1666	rVB	131006	165421	42.86%	5.643%
70	11.494	1705	1707	1710	rBV	252	215	0.06%	0.007%
71	11.592	1722	1723	1724	rBV	322	148	0.04%	0.005%
72	11.640	1730	1731	1733	rBV	392	159	0.04%	0.005%
73	11.677	1733	1737	1738	rBV	247	307	0.08%	0.010%
74	11.866	1767	1768	1772	rVB	274	153	0.04%	0.005%
75	12.024	1789	1794	1801	rVV	184904	226852	58.78%	7.739%
76	12.146	1813	1814	1817	rBV2	376	391	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025746.D
 Acq On : 11 Dec 2021 16:22
 Operator : JC/MD
 Sample : M5026-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	12.213	1823	1825	1828	rBV	212	203	0.05%	0.007%
78	12.323	1837	1843	1849	rBV	178055	217997	56.48%	7.437%
79	12.786	1916	1919	1920	rBV	421	314	0.08%	0.011%
80	12.927	1940	1942	1943	rBV	352	231	0.06%	0.008%
81	13.555	2043	2045	2047	rVV2	214	186	0.05%	0.006%
82	13.933	2104	2107	2108	rBV2	195	197	0.05%	0.007%
83	14.097	2132	2134	2136	rVB	444	318	0.08%	0.011%
84	14.134	2136	2140	2144	rBV2	788	1437	0.37%	0.049%
85	14.378	2177	2180	2185	rBV	439	693	0.18%	0.024%
86	14.585	2210	2214	2216	rBV	235	324	0.08%	0.011%
87	14.603	2216	2217	2219	rVB	484	297	0.08%	0.010%
88	14.628	2219	2221	2224	rBV2	147	197	0.05%	0.007%
89	14.670	2227	2228	2231	rVB	382	233	0.06%	0.008%
90	14.841	2254	2256	2257	rBV	263	186	0.05%	0.006%
91	14.902	2264	2266	2270	rBV	268	384	0.10%	0.013%
92	15.103	2297	2299	2300	rBV	263	196	0.05%	0.007%
93	15.530	2367	2369	2371	rBV2	392	320	0.08%	0.011%
94	15.835	2415	2419	2421	rVB	379	510	0.13%	0.017%
95	16.115	2463	2465	2467	rBV	338	380	0.10%	0.013%
96	16.389	2508	2510	2512	rBV	324	205	0.05%	0.007%
97	16.524	2530	2532	2535	rBV2	313	275	0.07%	0.009%
98	16.560	2535	2538	2540	rBV2	351	443	0.11%	0.015%
99	16.706	2560	2562	2567	rVB2	425	281	0.07%	0.010%
100	16.743	2567	2568	2571	rBV3	269	205	0.05%	0.007%




Sum of corrected areas: 2931400

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025746.D
Acq On : 11 Dec 2021 16:22
Operator : JC/MD
Sample : M5026-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

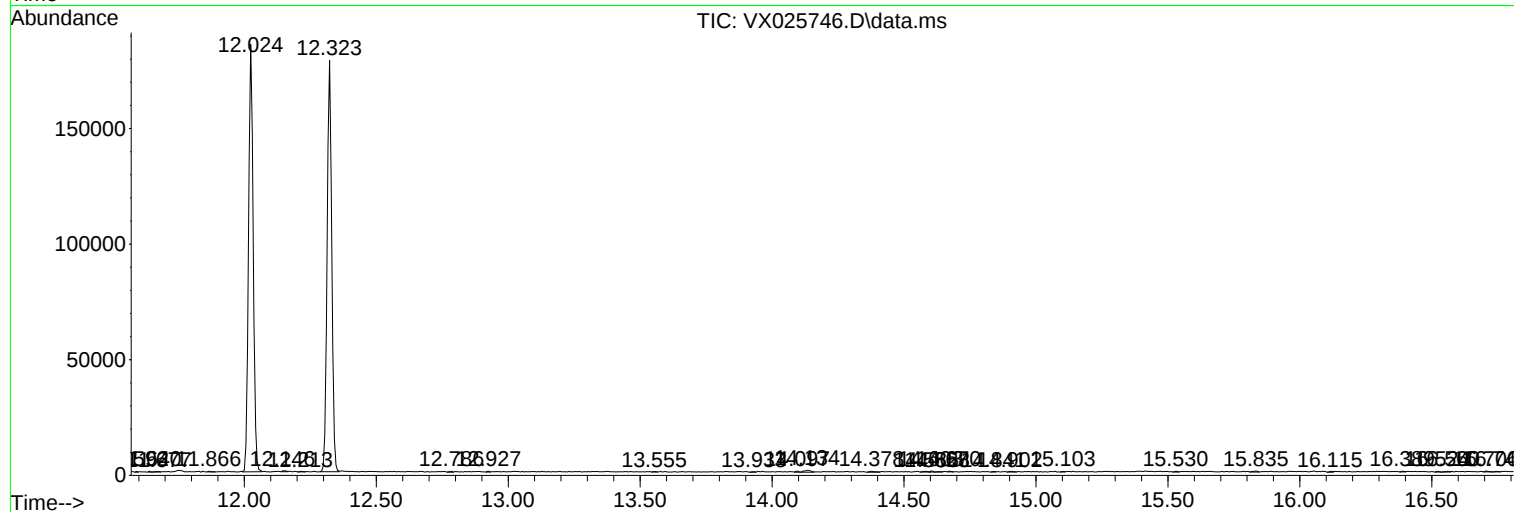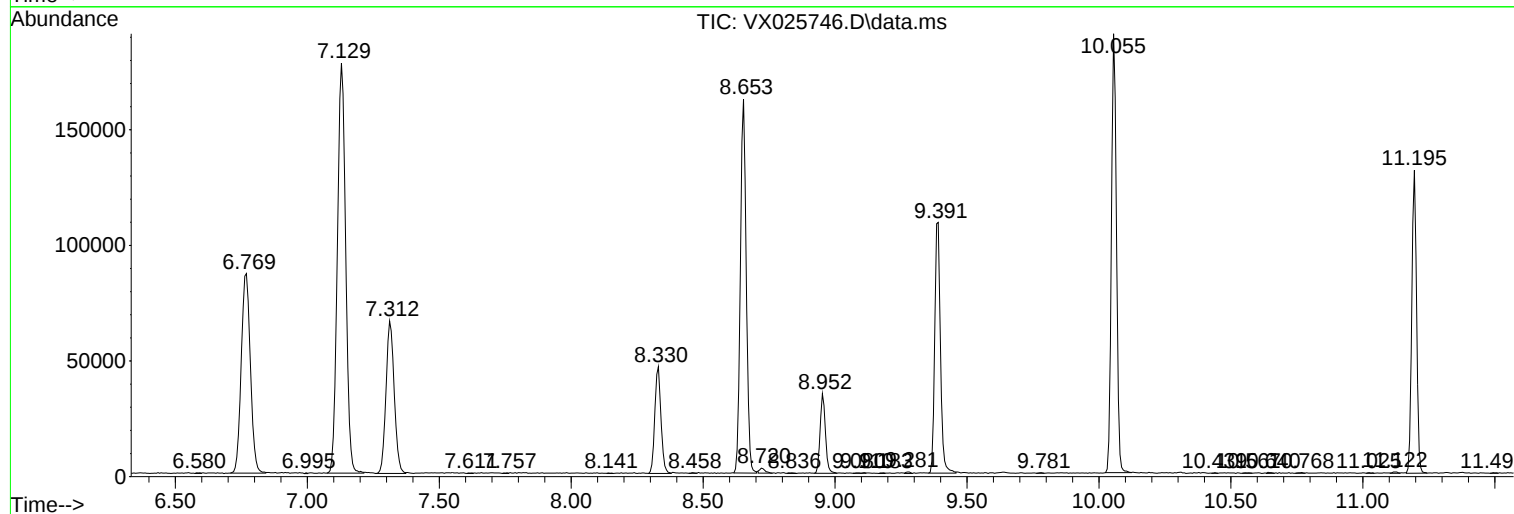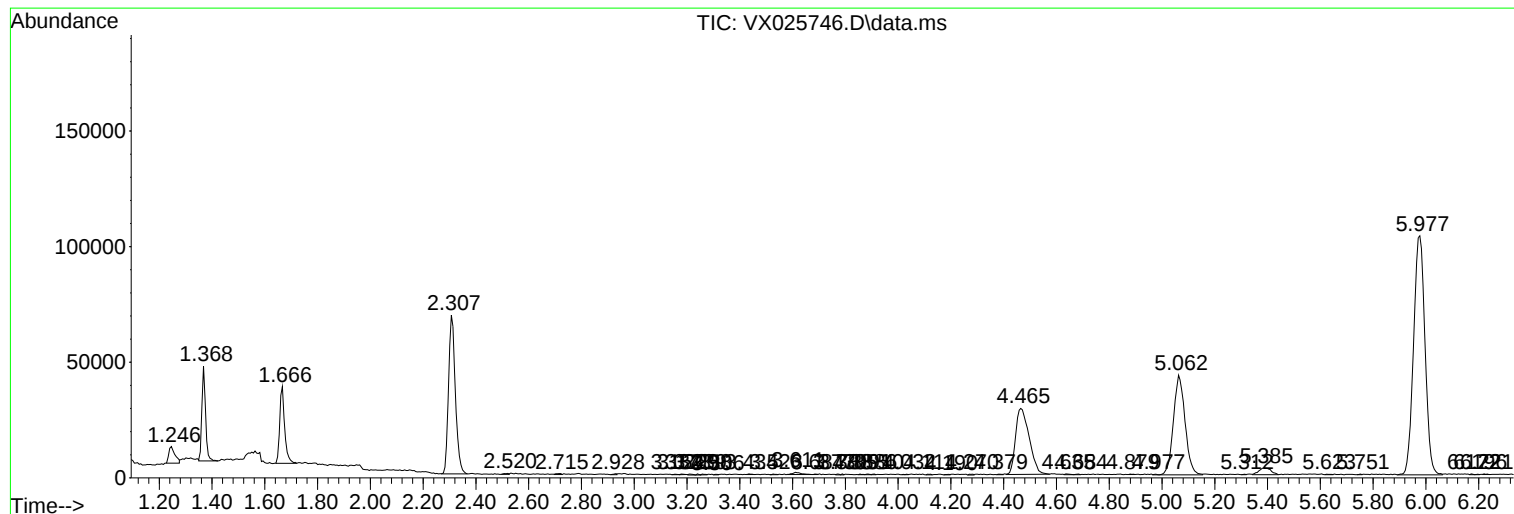

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025746.D
Acq On : 11 Dec 2021 16:22
Operator : JC/MD
Sample : M5026-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025746.D
Acq On : 11 Dec 2021 16:22
Operator : JC/MD
Sample : M5026-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc