

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025749.D
 Acq On : 11 Dec 2021 17:33
 Operator : JC/MD
 Sample : M5026-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025749.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.245	23	26	32	rBV	7597	10903	3.63%	0.462%
2	1.367	43	46	52	rVB	39175	37200	12.38%	1.576%
3	1.666	91	95	107	rVB	30135	39943	13.29%	1.693%
4	2.306	194	200	211	rVB	60647	100030	33.28%	4.239%
5	2.519	232	235	238	rBV2	271	383	0.13%	0.016%
6	2.751	271	273	275	rBV2	311	332	0.11%	0.014%
7	2.782	276	278	281	rBV2	291	318	0.11%	0.013%
8	3.111	330	332	334	rVB	359	275	0.09%	0.012%
9	3.154	337	339	343	rBV	407	450	0.15%	0.019%
10	3.269	356	358	361	rVB2	382	424	0.14%	0.018%
11	3.379	374	376	381	rBV	219	282	0.09%	0.012%
12	3.495	393	395	400	rBV	306	448	0.15%	0.019%
13	3.617	413	415	418	rVB2	307	313	0.10%	0.013%
14	3.647	418	420	422	rBV	252	259	0.09%	0.011%
15	3.696	426	428	431	rBV2	249	307	0.10%	0.013%
16	3.788	442	443	447	rVV2	189	252	0.08%	0.011%
17	3.836	449	451	452	rVV	361	244	0.08%	0.010%
18	4.031	481	483	485	rVB	390	248	0.08%	0.011%
19	4.062	486	488	490	rBV	359	275	0.09%	0.012%
20	4.464	540	554	569	rBV	26155	74361	24.74%	3.151%
21	4.793	607	608	611	rVV2	245	280	0.09%	0.012%
22	4.836	611	615	616	rVB	363	437	0.15%	0.019%
23	4.854	616	618	620	rBV	370	304	0.10%	0.013%
24	4.891	622	624	625	rBV	276	242	0.08%	0.010%
25	4.934	628	631	633	rBV	216	223	0.07%	0.009%
26	5.068	640	653	668	rBV	40551	127907	42.56%	5.420%
27	5.470	718	719	722	rBV2	365	325	0.11%	0.014%
28	5.525	724	728	729	rVV2	447	487	0.16%	0.021%
29	5.568	733	735	737	rBV	444	458	0.15%	0.019%
30	5.604	739	741	744	rVV	259	271	0.09%	0.011%
31	5.866	782	784	785	rBV	252	232	0.08%	0.010%
32	5.976	791	802	816	rBV2	102265	300552	100.00%	12.736%
33	6.159	830	832	835	rBV2	187	278	0.09%	0.012%
34	6.214	837	841	844	rBV2	398	617	0.21%	0.026%
35	6.659	910	914	915	rBV	249	286	0.10%	0.012%
36	6.769	923	932	943	rVB	79288	188717	62.79%	7.997%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025749.D
 Acq On : 11 Dec 2021 17:33
 Operator : JC/MD
 Sample : M5026-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

37	6.921	955	957	960	rVB2	317	218	0.07%	0.009%
38	7.116	983	989	996	rVB6	1800	4110	1.37%	0.174%
39	7.171	996	998	1001	rBV2	236	257	0.09%	0.011%
40	7.311	1013	1021	1031	rVB	62916	137502	45.75%	5.827%
41	7.762	1092	1095	1096	rBV	220	260	0.09%	0.011%
42	7.927	1121	1122	1125	rVV	260	274	0.09%	0.012%
43	7.970	1128	1129	1133	rVB	323	242	0.08%	0.010%
44	8.128	1152	1155	1156	rBV	292	260	0.09%	0.011%
45	8.195	1164	1166	1168	rBV	273	225	0.07%	0.010%
46	8.214	1168	1169	1173	rVB	361	251	0.08%	0.011%
47	8.256	1174	1176	1180	rVB2	221	230	0.08%	0.010%
48	8.329	1182	1188	1200	rVB	43412	71977	23.95%	3.050%
49	8.451	1205	1208	1209	rBV2	268	241	0.08%	0.010%
50	8.555	1223	1225	1227	rBV2	255	260	0.09%	0.011%
51	8.653	1235	1241	1249	rBV	153103	238387	79.32%	10.102%
52	8.726	1249	1253	1258	rVV4	1740	2972	0.99%	0.126%
53	8.951	1285	1290	1300	rBV	31223	45479	15.13%	1.927%
54	9.274	1338	1343	1345	rBV3	746	976	0.32%	0.041%
55	9.323	1348	1351	1353	rBV2	226	330	0.11%	0.014%
56	9.390	1356	1362	1376	rBV	107909	157709	52.47%	6.683%
57	9.927	1447	1450	1451	rBV	490	433	0.14%	0.018%
58	10.000	1461	1462	1465	rBV	227	251	0.08%	0.011%
59	10.055	1466	1471	1481	rVV	168066	229518	76.37%	9.726%
60	10.439	1529	1534	1535	rBV2	344	406	0.14%	0.017%
61	10.506	1543	1545	1550	rVB2	380	406	0.14%	0.017%
62	10.884	1604	1607	1609	rBV2	195	255	0.08%	0.011%
63	10.927	1612	1614	1615	rVB	383	225	0.07%	0.010%
64	10.939	1615	1616	1620	rBV2	259	339	0.11%	0.014%
65	11.073	1636	1638	1640	rVV2	284	283	0.09%	0.012%
66	11.115	1643	1645	1650	rVV2	507	733	0.24%	0.031%
67	11.195	1653	1658	1666	rVB	125507	156022	51.91%	6.612%
68	11.420	1693	1695	1697	rBV2	322	342	0.11%	0.014%
69	11.756	1746	1750	1751	rBV4	634	594	0.20%	0.025%
70	11.841	1761	1764	1768	rBV	327	552	0.18%	0.023%
71	11.908	1773	1775	1776	rBV	356	293	0.10%	0.012%
72	12.024	1789	1794	1803	rBV	162653	201519	67.05%	8.539%
73	12.121	1808	1810	1813	rVV3	316	362	0.12%	0.015%
74	12.152	1813	1815	1819	rVV2	632	613	0.20%	0.026%
75	12.323	1838	1843	1851	rVB	164998	206816	68.81%	8.764%
76	12.542	1875	1879	1880	rBV	250	243	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025749.D
 Acq On : 11 Dec 2021 17:33
 Operator : JC/MD
 Sample : M5026-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	12.621	1890	1892	1893	rVB2	406	235	0.08%	0.010%
78	12.957	1943	1947	1949	rBV2	295	479	0.16%	0.020%
79	13.127	1973	1975	1978	rVB2	309	294	0.10%	0.012%
80	13.164	1978	1981	1982	rBV	261	290	0.10%	0.012%
81	13.505	2035	2037	2039	rVV	297	251	0.08%	0.011%
82	13.920	2101	2105	2106	rVB2	226	278	0.09%	0.012%
83	13.932	2106	2107	2109	rBV2	241	222	0.07%	0.009%
84	14.133	2137	2140	2146	rVV2	702	1133	0.38%	0.048%
85	14.219	2153	2154	2156	rBV	358	260	0.09%	0.011%
86	14.487	2196	2198	2202	rVB	279	283	0.09%	0.012%
87	14.658	2224	2226	2228	rBV	443	391	0.13%	0.017%
88	14.719	2232	2236	2239	rVB2	329	524	0.17%	0.022%
89	14.767	2242	2244	2246	rBV2	259	223	0.07%	0.009%
90	14.804	2249	2250	2254	rBV	372	301	0.10%	0.013%
91	14.847	2254	2257	2258	rBV	304	301	0.10%	0.013%
92	14.920	2268	2269	2272	rVB	299	226	0.08%	0.010%
93	15.243	2319	2322	2324	rVB	377	384	0.13%	0.016%
94	15.273	2324	2327	2328	rBV2	358	434	0.14%	0.018%
95	15.474	2357	2360	2361	rBV	362	334	0.11%	0.014%
96	15.663	2388	2391	2395	rBV2	389	470	0.16%	0.020%
97	15.968	2438	2441	2442	rVB	393	331	0.11%	0.014%
98	16.182	2474	2476	2480	rBV3	224	328	0.11%	0.014%
99	16.596	2542	2544	2546	rBV	343	387	0.13%	0.016%
100	16.633	2549	2550	2552	rBV	439	263	0.09%	0.011%




Sum of corrected areas: 2359850

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025749.D
Acq On : 11 Dec 2021 17:33
Operator : JC/MD
Sample : M5026-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

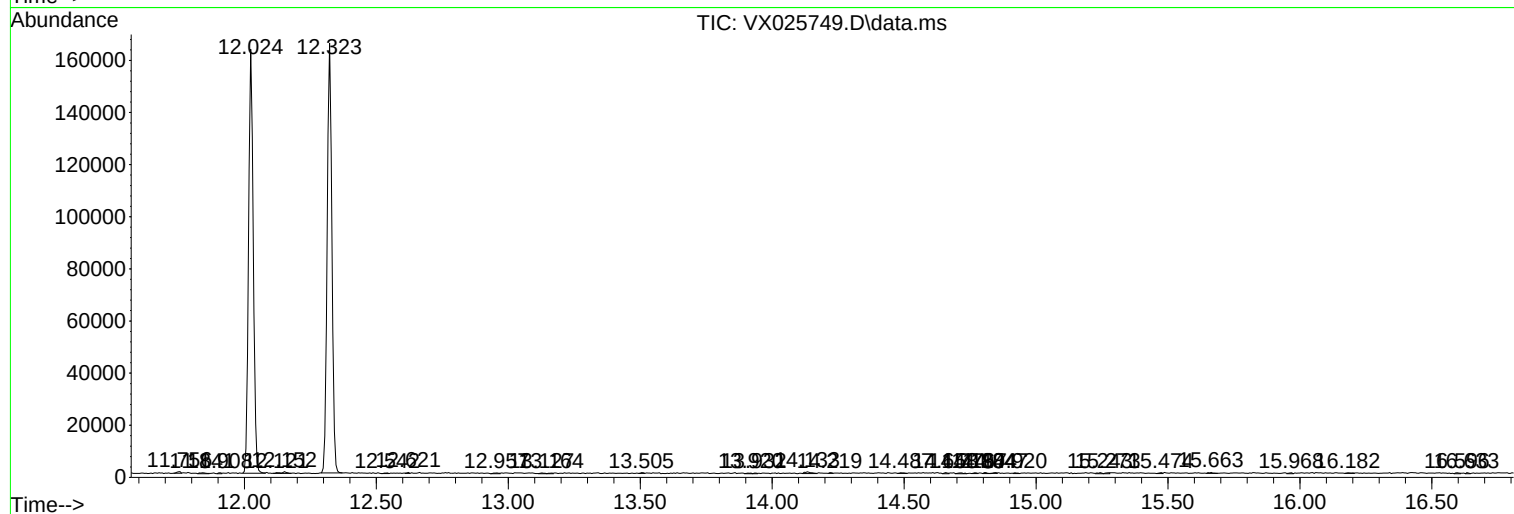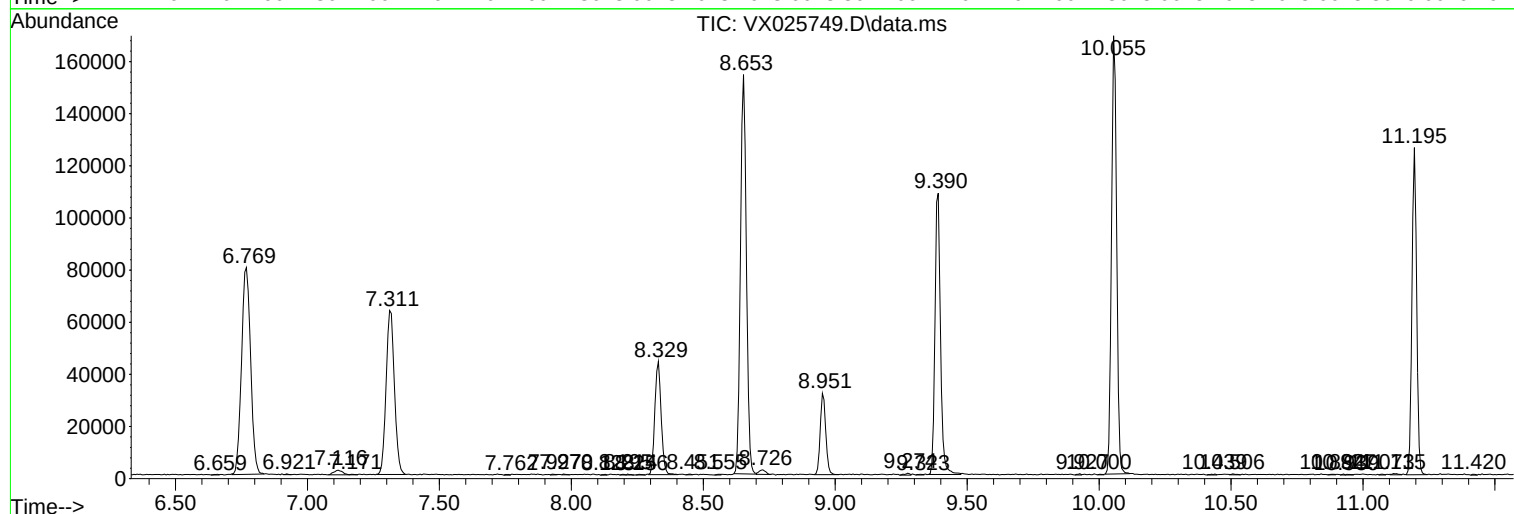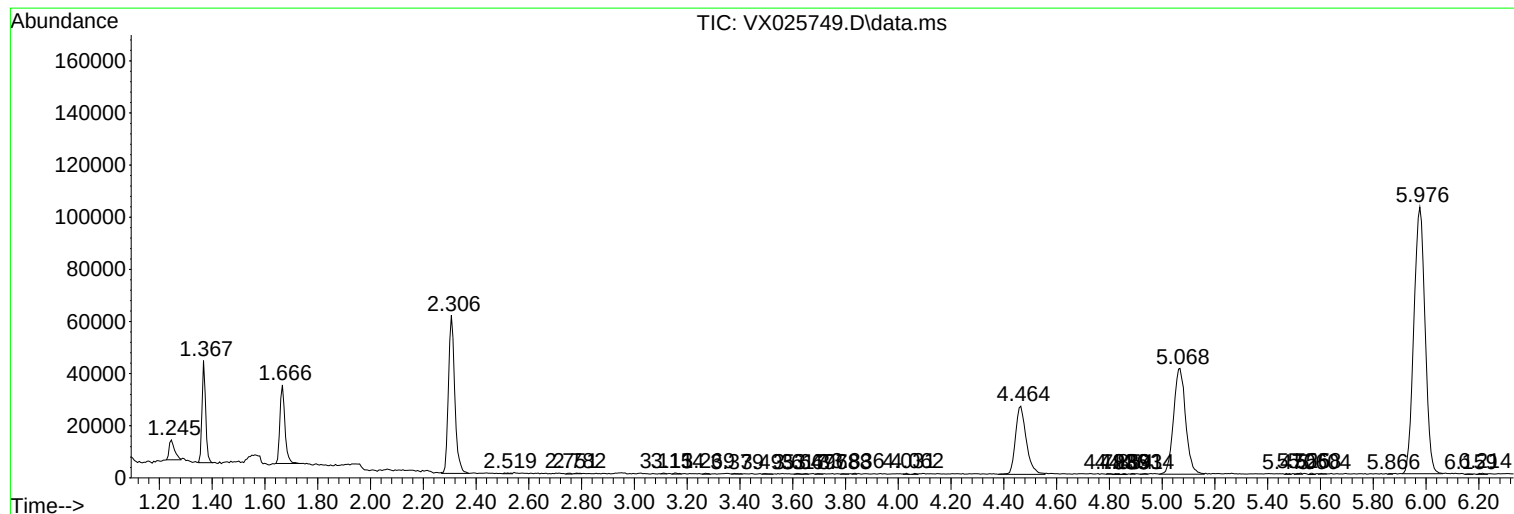

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025749.D
Acq On : 11 Dec 2021 17:33
Operator : JC/MD
Sample : M5026-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025749.D
Acq On : 11 Dec 2021 17:33
Operator : JC/MD
Sample : M5026-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc