

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025752.D
 Acq On : 11 Dec 2021 18:43
 Operator : JC/MD
 Sample : M5026-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0D02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	39	rVB2	6977	13938	4.91%	0.541%
2	1.367	43	46	52	rVB	39866	36404	12.82%	1.414%
3	1.666	91	95	104	rBV	31294	38817	13.67%	1.507%
4	2.306	194	200	210	rBV2	60865	105263	37.07%	4.088%
5	2.824	283	285	286	rBV	285	163	0.06%	0.006%
6	3.221	347	350	351	rBV	209	153	0.05%	0.006%
7	3.343	369	370	372	rBV	334	230	0.08%	0.009%
8	3.861	452	455	456	rBV2	255	271	0.10%	0.011%
9	3.904	461	462	465	rVB2	210	169	0.06%	0.007%
10	4.001	476	478	479	rBV	227	201	0.07%	0.008%
11	4.050	484	486	487	rBV2	401	212	0.07%	0.008%
12	4.086	489	492	496	rBV2	210	324	0.11%	0.013%
13	4.166	503	505	506	rBV	192	196	0.07%	0.008%
14	4.373	535	539	540	rBV2	243	295	0.10%	0.011%
15	4.391	540	542	543	rVV2	237	193	0.07%	0.007%
16	4.464	545	554	568	rVV2	25256	81643	28.75%	3.171%
17	4.611	577	578	580	rBV	387	277	0.10%	0.011%
18	4.653	584	585	587	rBV	336	304	0.11%	0.012%
19	5.068	642	653	667	rVB	38415	120048	42.28%	4.662%
20	5.391	699	706	713	rBV4	1467	4159	1.46%	0.162%
21	5.464	716	718	720	rVB2	270	250	0.09%	0.010%
22	5.483	720	721	723	rBV2	222	186	0.07%	0.007%
23	5.531	728	729	731	rBV	276	166	0.06%	0.006%
24	5.665	749	751	755	rVB2	264	311	0.11%	0.012%
25	5.757	765	766	768	rBV	342	303	0.11%	0.012%
26	5.976	790	802	817	rBV2	95966	283932	100.00%	11.027%
27	6.580	899	901	903	rVB	249	178	0.06%	0.007%
28	6.604	903	905	906	rBV	245	185	0.07%	0.007%
29	6.690	918	919	920	rBV	344	194	0.07%	0.008%
30	6.769	923	932	947	rVV	80328	186821	65.80%	7.255%
31	7.007	969	971	972	rBV	162	168	0.06%	0.007%
32	7.129	982	991	1003	rVV	127840	280698	98.86%	10.901%
33	7.311	1013	1021	1032	rVV	60824	132179	46.55%	5.133%
34	7.391	1032	1034	1036	rVB	306	192	0.07%	0.007%
35	7.415	1036	1038	1042	rBV2	403	476	0.17%	0.018%
36	7.452	1042	1044	1047	rBV2	313	243	0.09%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025752.D
 Acq On : 11 Dec 2021 18:43
 Operator : JC/MD
 Sample : M5026-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0D02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	7.525	1054	1056	1059	rBV	203	236	0.08%	0.009%
38	7.811	1100	1103	1105	rBV2	302	312	0.11%	0.012%
39	7.872	1111	1113	1114	rBV	208	153	0.05%	0.006%
40	8.049	1140	1142	1144	rVB2	309	168	0.06%	0.007%
41	8.238	1171	1173	1174	rBV	227	218	0.08%	0.008%
42	8.330	1182	1188	1196	rBV	42516	68044	23.96%	2.642%
43	8.494	1213	1215	1216	rBV	244	185	0.07%	0.007%
44	8.653	1234	1241	1248	rBV	150885	228186	80.37%	8.862%
45	8.726	1248	1253	1258	rVB2	2250	3911	1.38%	0.152%
46	8.878	1276	1278	1280	rBV	260	324	0.11%	0.013%
47	8.951	1285	1290	1302	rVB	30091	44160	15.55%	1.715%
48	9.244	1335	1338	1339	rBV	253	213	0.08%	0.008%
49	9.281	1341	1344	1346	rVB	563	615	0.22%	0.024%
50	9.384	1356	1361	1374	rBV	99675	149786	52.75%	5.817%
51	9.518	1381	1383	1384	rBV2	289	197	0.07%	0.008%
52	9.713	1414	1415	1418	rVB	339	203	0.07%	0.008%
53	10.055	1466	1471	1480	rBV	168944	230266	81.10%	8.942%
54	10.372	1520	1523	1525	rBV2	327	295	0.10%	0.011%
55	10.396	1525	1527	1528	rVV	293	174	0.06%	0.007%
56	10.445	1532	1535	1538	rVV	312	322	0.11%	0.013%
57	10.476	1538	1540	1541	rVV	254	170	0.06%	0.007%
58	10.500	1542	1544	1547	rVB	265	227	0.08%	0.009%
59	10.597	1558	1560	1565	rVB2	347	528	0.19%	0.021%
60	10.640	1565	1567	1568	rBV	388	294	0.10%	0.011%
61	10.665	1569	1571	1573	rVV	206	164	0.06%	0.006%
62	10.854	1600	1602	1603	rBV	170	152	0.05%	0.006%
63	10.933	1614	1615	1619	rVB2	361	397	0.14%	0.015%
64	10.963	1619	1620	1623	rBV	393	311	0.11%	0.012%
65	10.994	1623	1625	1626	rBV	256	228	0.08%	0.009%
66	11.116	1643	1645	1648	rVB2	453	496	0.17%	0.019%
67	11.195	1653	1658	1666	rVB	119513	148981	52.47%	5.786%
68	11.256	1666	1668	1672	rBV2	261	428	0.15%	0.017%
69	11.463	1700	1702	1703	rBV	228	168	0.06%	0.007%
70	11.646	1731	1732	1736	rVB	272	224	0.08%	0.009%
71	11.689	1736	1739	1740	rBV	256	247	0.09%	0.010%
72	11.750	1748	1749	1752	rVB	591	394	0.14%	0.015%
73	11.878	1769	1770	1772	rBV2	254	243	0.09%	0.009%
74	12.024	1789	1794	1803	rVB	160213	200548	70.63%	7.788%
75	12.152	1813	1815	1818	rVB2	363	260	0.09%	0.010%
76	12.219	1825	1826	1828	rVB	364	164	0.06%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025752.D
 Acq On : 11 Dec 2021 18:43
 Operator : JC/MD
 Sample : M5026-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0D02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

77	12.286	1835	1837	1838	rVV	350	172	0.06%	0.007%
78	12.323	1838	1843	1851	rVV	159379	196616	69.25%	7.636%
79	12.951	1944	1946	1949	rBV2	338	251	0.09%	0.010%
80	13.054	1961	1963	1966	rBV	232	281	0.10%	0.011%
81	13.188	1984	1985	1987	rBV	311	204	0.07%	0.008%
82	13.475	2030	2032	2034	rBV	205	203	0.07%	0.008%
83	13.627	2055	2057	2059	rBV2	241	247	0.09%	0.010%
84	13.719	2069	2072	2074	rBV2	224	218	0.08%	0.008%
85	13.944	2107	2109	2111	rBV2	193	205	0.07%	0.008%
86	14.316	2169	2170	2172	rBV	226	158	0.06%	0.006%
87	14.475	2194	2196	2198	rBV	229	262	0.09%	0.010%
88	14.518	2201	2203	2204	rBV	284	225	0.08%	0.009%
89	14.853	2256	2258	2261	rBV	270	350	0.12%	0.014%
90	14.975	2275	2278	2279	rBV2	376	387	0.14%	0.015%
91	14.993	2279	2281	2284	rVB2	221	244	0.09%	0.009%
92	15.145	2302	2306	2307	rBV2	275	394	0.14%	0.015%
93	15.353	2338	2340	2343	rVB	278	193	0.07%	0.007%
94	15.938	2433	2436	2438	rBV	347	428	0.15%	0.017%
95	16.066	2456	2457	2460	rVB	324	332	0.12%	0.013%
96	16.096	2460	2462	2463	rBV	325	153	0.05%	0.006%
97	16.157	2470	2472	2473	rBV	377	404	0.14%	0.016%
98	16.407	2511	2513	2514	rBV2	257	249	0.09%	0.010%
99	16.633	2549	2550	2552	rBV	198	171	0.06%	0.007%
100	16.706	2560	2562	2565	rBV2	328	313	0.11%	0.012%


Sum of corrected areas: 2574994

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025752.D
Acq On : 11 Dec 2021 18:43
Operator : JC/MD
Sample : M5026-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0D02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

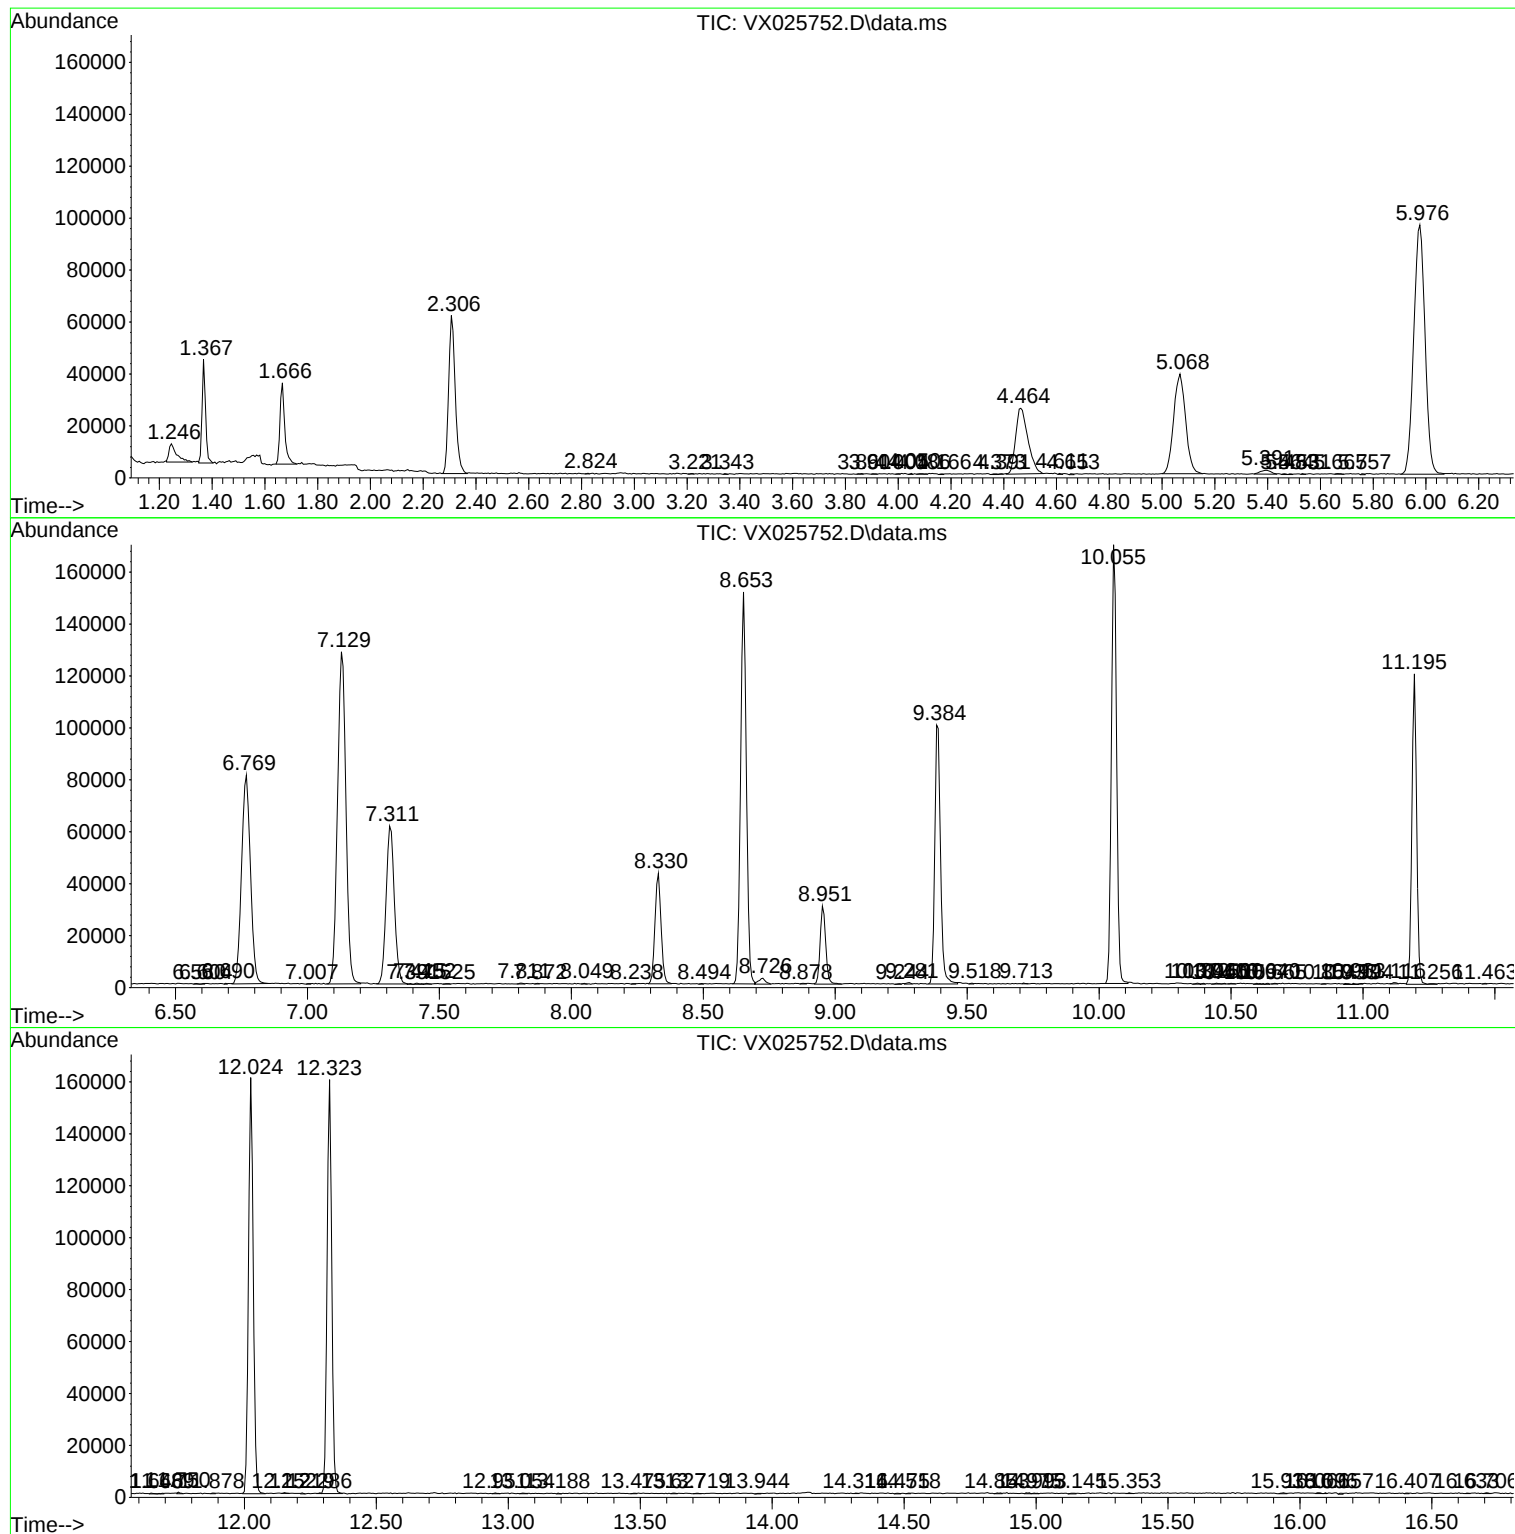

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025752.D
Acq On : 11 Dec 2021 18:43
Operator : JC/MD
Sample : M5026-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0D02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025752.D
Acq On : 11 Dec 2021 18:43
Operator : JC/MD
Sample : M5026-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0D02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc