

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025755.D
 Acq On : 11 Dec 2021 19:54
 Operator : JC/MD
 Sample : M5026-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0D12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025755.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	33	rBV2	6963	11340	3.96%	0.497%
2	1.368	43	46	52	rVB	37862	36185	12.62%	1.586%
3	1.666	91	95	106	rBV	29560	38941	13.59%	1.707%
4	2.306	194	200	210	rVB	58125	94526	32.98%	4.144%
5	2.459	224	225	226	rBV	332	187	0.07%	0.008%
6	2.526	234	236	237	rBV	390	273	0.10%	0.012%
7	2.788	278	279	283	rBV	337	255	0.09%	0.011%
8	2.843	285	288	289	rVB	283	244	0.09%	0.011%
9	2.861	289	291	293	rBV	209	187	0.07%	0.008%
10	2.886	293	295	296	rVB2	416	237	0.08%	0.010%
11	2.916	296	300	301	rBV2	321	413	0.14%	0.018%
12	2.947	301	305	307	rBV2	530	922	0.32%	0.040%
13	3.075	324	326	327	rBV	211	223	0.08%	0.010%
14	3.221	348	350	352	rBV	226	207	0.07%	0.009%
15	3.422	381	383	386	rBV2	198	238	0.08%	0.010%
16	3.581	407	409	410	rBV2	348	251	0.09%	0.011%
17	4.020	479	481	485	rVB2	240	256	0.09%	0.011%
18	4.465	545	554	569	rVV	25498	71660	25.00%	3.142%
19	5.068	641	653	667	rVB2	41398	123198	42.98%	5.401%
20	5.330	694	696	697	rBV	211	188	0.07%	0.008%
21	5.446	713	715	717	rBV2	248	199	0.07%	0.009%
22	5.507	721	725	727	rBV2	193	279	0.10%	0.012%
23	5.836	776	779	782	rBV2	173	256	0.09%	0.011%
24	5.976	790	802	816	rBV2	97567	286643	100.00%	12.566%
25	6.098	820	822	827	rVB2	270	351	0.12%	0.015%
26	6.141	827	829	831	rVB2	351	324	0.11%	0.014%
27	6.178	831	835	836	rBV	389	437	0.15%	0.019%
28	6.641	908	911	912	rBV2	199	207	0.07%	0.009%
29	6.684	915	918	920	rVV2	262	321	0.11%	0.014%
30	6.769	922	932	946	rVV	76973	185070	64.56%	8.113%
31	6.921	955	957	958	rVB	360	205	0.07%	0.009%
32	7.117	983	989	997	rBV6	1857	4503	1.57%	0.197%
33	7.257	1011	1012	1013	rBV	284	206	0.07%	0.009%
34	7.312	1013	1021	1032	rVB	61702	131506	45.88%	5.765%
35	7.488	1047	1050	1052	rVB3	242	289	0.10%	0.013%
36	7.562	1060	1062	1063	rVB	309	195	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025755.D
 Acq On : 11 Dec 2021 19:54
 Operator : JC/MD
 Sample : M5026-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0D12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	7.842	1106	1108	1112	rBV	151	213	0.07%	0.009%
38	7.921	1120	1121	1124	rBV	257	214	0.07%	0.009%
39	7.946	1124	1125	1128	rVB	349	264	0.09%	0.012%
40	7.970	1128	1129	1133	rBV	348	410	0.14%	0.018%
41	8.068	1142	1145	1147	rBV	359	512	0.18%	0.022%
42	8.165	1159	1161	1163	rBV2	179	201	0.07%	0.009%
43	8.250	1173	1175	1177	rBV	250	240	0.08%	0.011%
44	8.330	1182	1188	1200	rVV	40669	68086	23.75%	2.985%
45	8.464	1209	1210	1215	rVB	376	245	0.09%	0.011%
46	8.653	1234	1241	1249	rBV	149740	227095	79.23%	9.956%
47	8.720	1249	1252	1260	rVB	2137	3502	1.22%	0.154%
48	8.848	1271	1273	1276	rVV	277	253	0.09%	0.011%
49	8.952	1285	1290	1301	rVB	29717	43985	15.34%	1.928%
50	9.202	1329	1331	1332	rBV	264	219	0.08%	0.010%
51	9.281	1342	1344	1345	rBV2	318	189	0.07%	0.008%
52	9.330	1351	1352	1354	rBV2	234	197	0.07%	0.009%
53	9.391	1356	1362	1376	rBV	103562	156802	54.70%	6.874%
54	9.561	1388	1390	1393	rBV2	347	506	0.18%	0.022%
55	9.665	1406	1407	1409	rBV	231	240	0.08%	0.011%
56	9.714	1414	1415	1419	rBV2	265	364	0.13%	0.016%
57	9.768	1422	1424	1426	rVB2	250	202	0.07%	0.009%
58	10.055	1466	1471	1483	rBV	171758	228155	79.60%	10.002%
59	10.305	1510	1512	1515	rBV	353	450	0.16%	0.020%
60	10.463	1536	1538	1541	rVB	293	267	0.09%	0.012%
61	10.592	1557	1559	1560	rBV	312	271	0.09%	0.012%
62	10.988	1623	1624	1627	rVB2	343	286	0.10%	0.013%
63	11.043	1630	1633	1636	rVV	251	270	0.09%	0.012%
64	11.116	1644	1645	1647	rBV2	432	317	0.11%	0.014%
65	11.195	1652	1658	1669	rBV	122561	154287	53.83%	6.764%
66	11.512	1709	1710	1712	rBV	200	195	0.07%	0.009%
67	11.543	1714	1715	1718	rBV2	467	470	0.16%	0.021%
68	11.750	1746	1749	1752	rVB4	572	736	0.26%	0.032%
69	11.786	1752	1755	1758	rVB2	262	344	0.12%	0.015%
70	11.823	1758	1761	1762	rBV2	311	417	0.15%	0.018%
71	11.975	1784	1786	1787	rVB	348	220	0.08%	0.010%
72	12.024	1789	1794	1801	rVV	155364	195493	68.20%	8.570%
73	12.323	1837	1843	1852	rBV	154980	196644	68.60%	8.621%
74	12.512	1873	1874	1877	rVB2	317	253	0.09%	0.011%
75	12.664	1896	1899	1901	rBV2	282	339	0.12%	0.015%
76	12.725	1906	1909	1910	rVB	390	238	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025755.D
 Acq On : 11 Dec 2021 19:54
 Operator : JC/MD
 Sample : M5026-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0D12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

77	12.823	1922	1925	1926	rBV	292	221	0.08%	0.010%
78	13.054	1961	1963	1966	rVB	360	255	0.09%	0.011%
79	13.085	1966	1968	1970	rBV	262	194	0.07%	0.009%
80	13.140	1974	1977	1978	rBV	218	248	0.09%	0.011%
81	13.402	2017	2020	2021	rBV2	158	183	0.06%	0.008%
82	13.646	2055	2060	2061	rBV2	268	415	0.14%	0.018%
83	13.689	2066	2067	2070	rBV	236	253	0.09%	0.011%
84	14.073	2128	2130	2132	rVV	302	208	0.07%	0.009%
85	14.097	2132	2134	2136	rVB2	344	277	0.10%	0.012%
86	14.231	2154	2156	2159	rBV	176	195	0.07%	0.009%
87	14.603	2215	2217	2220	rVB	298	335	0.12%	0.015%
88	14.633	2220	2222	2225	rBV	365	422	0.15%	0.019%
89	14.890	2262	2264	2266	rBV	278	300	0.10%	0.013%
90	14.944	2272	2273	2277	rVB	284	204	0.07%	0.009%
91	15.207	2314	2316	2318	rBV2	290	228	0.08%	0.010%
92	15.322	2333	2335	2336	rBV	246	187	0.07%	0.008%
93	15.426	2350	2352	2355	rVB	432	468	0.16%	0.021%
94	15.463	2355	2358	2359	rBV2	426	513	0.18%	0.022%
95	15.767	2407	2408	2411	rBV2	282	229	0.08%	0.010%
96	15.871	2423	2425	2426	rBV2	287	204	0.07%	0.009%
97	16.109	2463	2464	2466	rBV2	335	300	0.10%	0.013%
98	16.182	2474	2476	2478	rBV2	269	298	0.10%	0.013%
99	16.590	2540	2543	2544	rVB	256	196	0.07%	0.009%
100	16.731	2563	2566	2567	rBV3	236	202	0.07%	0.009%




Sum of corrected areas: 2281048

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025755.D
Acq On : 11 Dec 2021 19:54
Operator : JC/MD
Sample : M5026-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0D12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

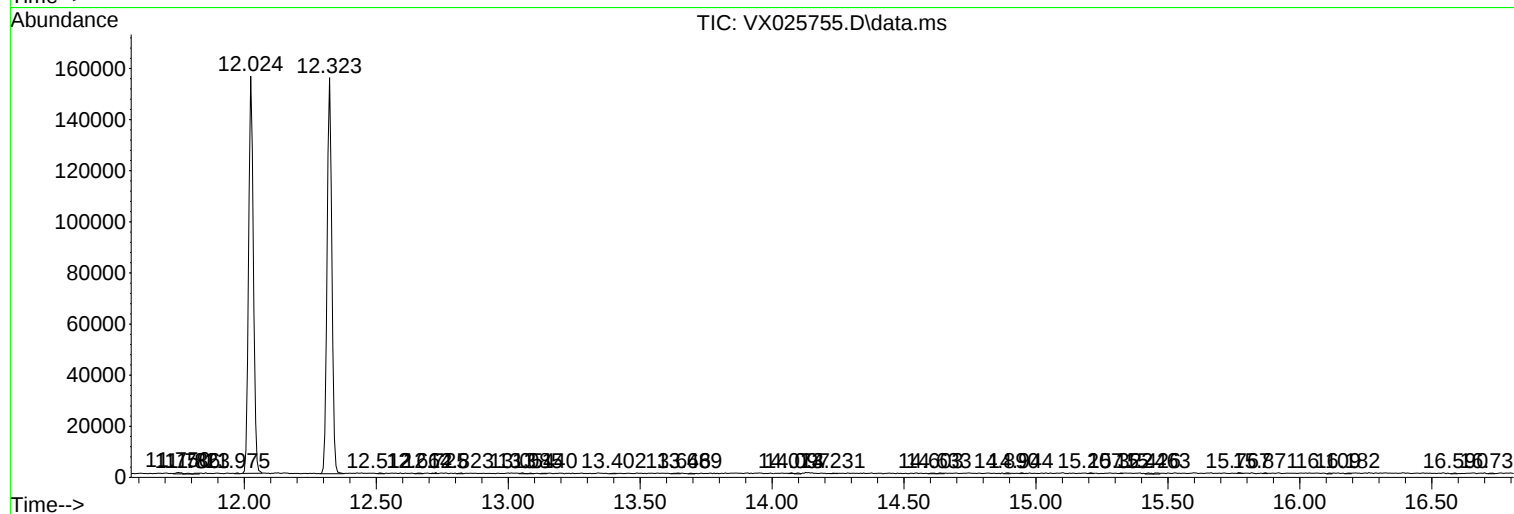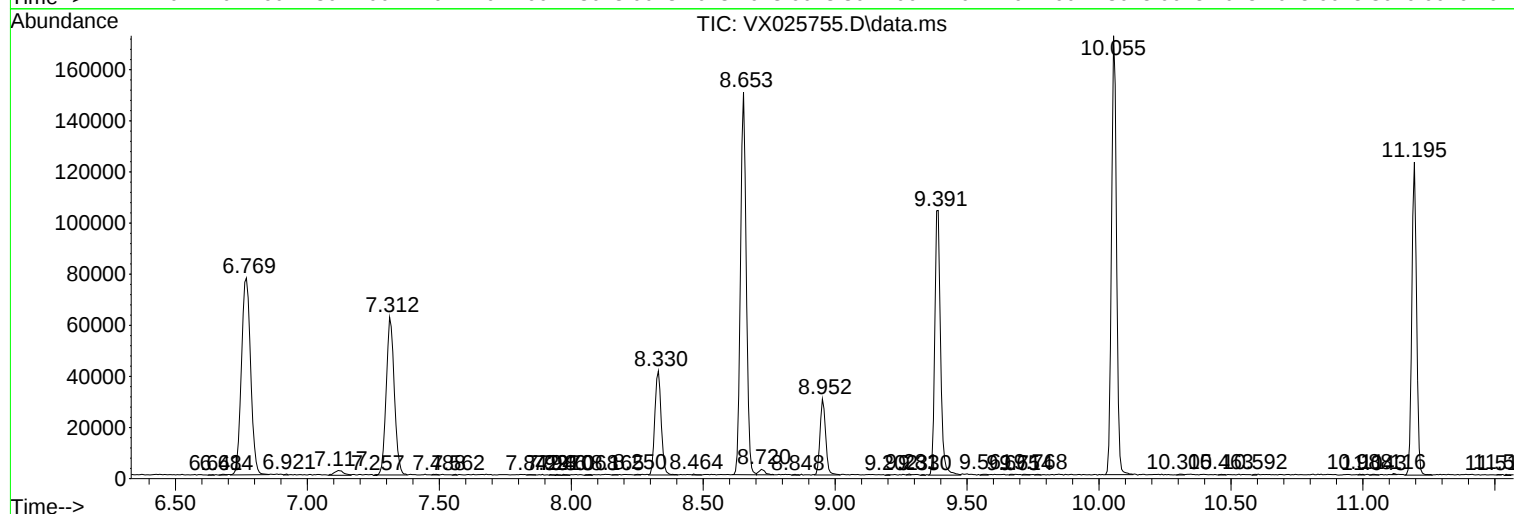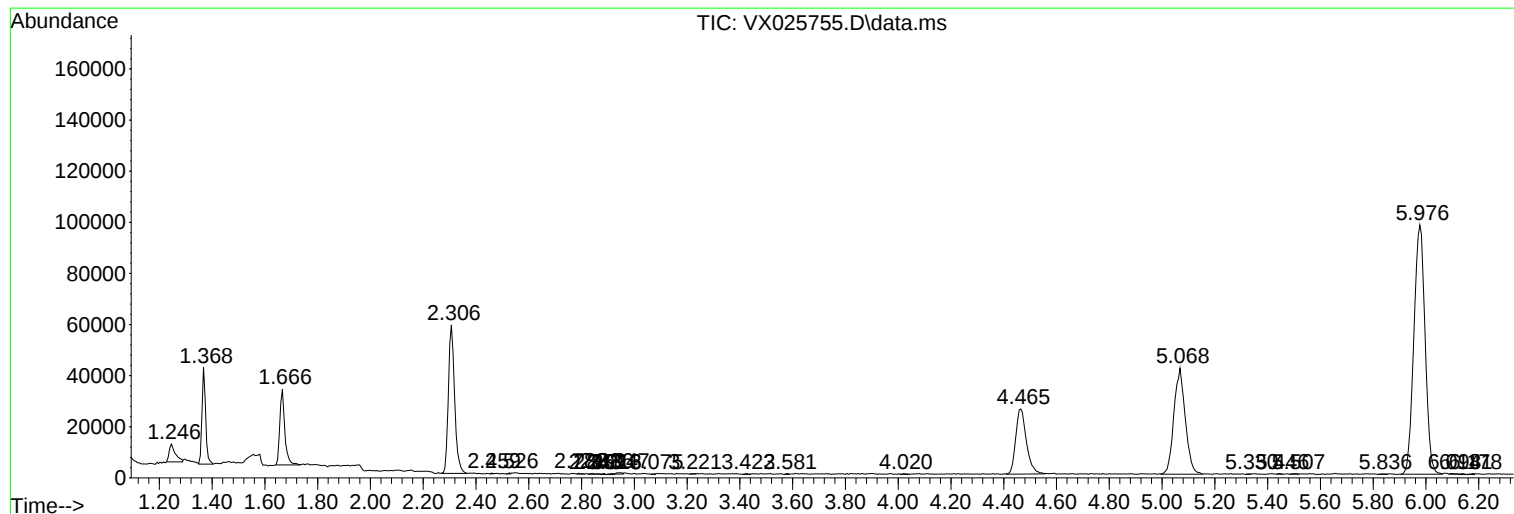

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025755.D
Acq On : 11 Dec 2021 19:54
Operator : JC/MD
Sample : M5026-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0D12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
Data File : VX025755.D
Acq On : 11 Dec 2021 19:54
Operator : JC/MD
Sample : M5026-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0D12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc