


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121121\
 Data File : VX025730.D
 Acq On : 11 Dec 2021 09:45
 Operator : JC/MD
 Sample : BFB623
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB623

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis
 Last Update : Thu Dec 16 00:37:00 2021

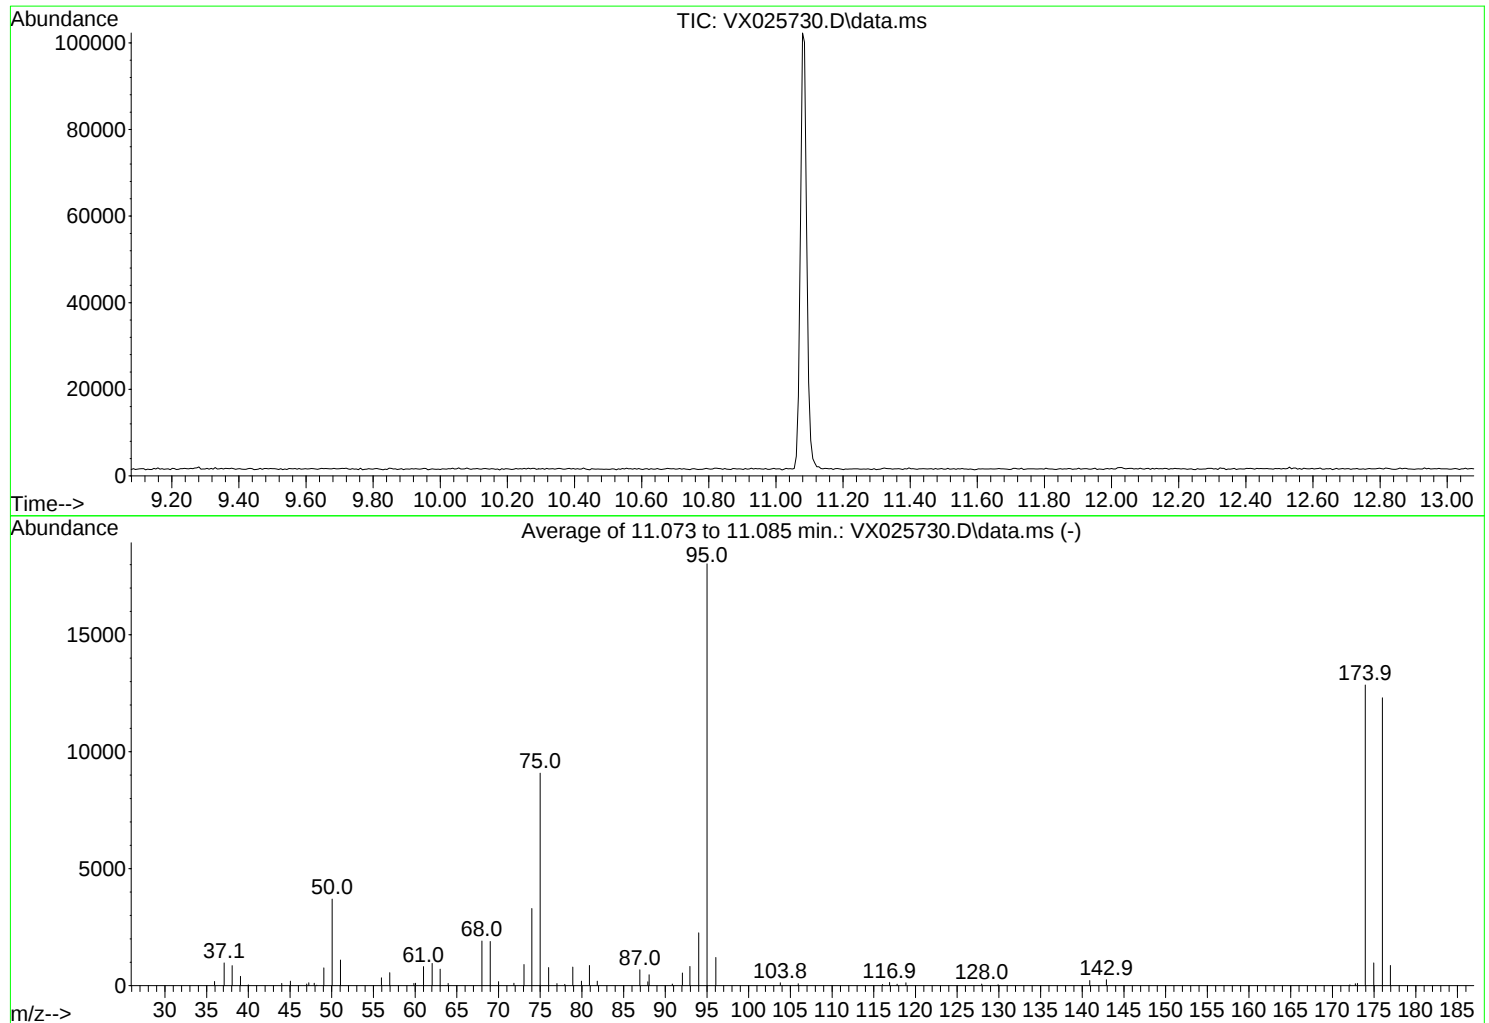

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1634

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	3702	PASS
75	95	30	80	50.4	9087	PASS
95	95	100	100	100.0	18033	PASS
96	95	5	9	6.7	1202	PASS
173	174	0.00	2	0.8	98	PASS
174	95	50	120	71.3	12856	PASS
175	174	5	9	7.6	971	PASS
176	174	95	101	95.7	12306	PASS
177	176	5	9	7.0	860	PASS

m/z	Abundance
40.00	1427.0
44.00	147.0

Instrument :
MSVOA_X
ClientSampleId :
BFB623

m/z	Abundance
36.00	124.0
37.10	654.0
38.10	668.0
39.10	262.0
40.00	1465.0
44.10	237.0
45.10	164.0
47.20	135.0
47.90	90.0
49.00	632.0
50.00	2700.0
51.10	819.0
56.00	200.0
57.00	464.0
59.90	122.0
61.00	555.0
62.00	748.0
63.00	510.0
64.00	86.0
68.00	1332.0
69.00	1408.0
70.00	141.0
71.90	63.0
73.00	636.0
74.00	2445.0
75.00	6442.0
76.00	552.0
76.90	77.0
78.90	609.0
79.90	179.0
80.90	577.0
81.80	130.0
86.90	515.0
87.90	500.0
92.00	373.0
93.00	582.0
94.00	1601.0
95.00	12082.0
96.00	938.0
103.70	69.0
105.90	55.0
116.90	105.0
118.80	95.0
128.00	56.0
129.90	65.0
140.80	125.0
142.90	164.0
172.80	95.0
173.00	87.0
173.90	7220.0
174.90	569.0
176.00	6832.0
176.90	487.0

Instrument :
MSVOA_X
ClientSampleId :
BFB623

m/z	Abundance
35.90	225.0
37.10	1258.0
38.00	1007.0
39.10	496.0
40.00	1452.0
44.00	287.0
45.00	223.0
47.30	241.0
48.00	140.0
49.00	880.0
50.10	4528.0
51.00	1344.0
55.90	396.0
57.00	532.0
59.80	170.0
60.10	167.0
61.00	941.0
62.00	1037.0
63.00	818.0
63.90	73.0
68.00	2395.0
69.00	2293.0
70.00	197.0
71.80	128.0
73.10	1042.0
74.00	3801.0
75.00	10980.0
76.00	877.0
77.00	95.0
78.00	67.0
78.90	860.0
80.00	175.0
80.90	1067.0
81.90	299.0
87.00	727.0
88.10	777.0
90.80	112.0
92.10	675.0
93.00	928.0
94.00	2801.0
95.00	21584.0
96.10	1363.0
103.80	140.0
106.00	99.0
116.10	83.0
117.00	141.0
117.80	74.0
118.90	139.0
128.00	71.0
140.90	265.0
142.90	272.0
172.70	145.0
174.00	15084.0
175.00	1156.0
176.00	14167.0
177.00	987.0

Instrument :
MSVOA_X
ClientSampleId :
BFB623

m/z	Abundance
36.00	186.0
37.10	1005.0
38.10	892.0
39.00	430.0
40.00	1459.0
43.90	215.0
45.00	199.0
47.00	206.0
47.80	82.0
48.20	69.0
49.10	766.0
50.00	3879.0
51.00	1120.0
56.00	409.0
56.90	664.0
60.00	136.0
61.00	937.0
62.10	1075.0
63.00	780.0
63.90	122.0
68.00	2010.0
69.00	1954.0
70.00	177.0
71.90	126.0
73.00	1025.0
74.00	3640.0
75.00	9840.0
76.00	880.0
77.10	92.0
77.90	103.0
78.90	916.0
79.90	218.0
80.90	947.0
81.80	157.0
86.90	788.0
88.00	626.0
90.90	97.0
92.00	577.0
92.90	962.0
94.00	2377.0
95.00	20432.0
96.00	1306.0
103.90	161.0
105.90	84.0
116.00	63.0
116.80	160.0
117.80	113.0
118.90	125.0
127.90	86.0
129.90	63.0
141.00	275.0
142.90	327.0
172.10	98.0
173.00	207.0
173.90	16265.0
175.00	1189.0
176.00	15920.0
176.90	1106.0

Instrument :
MSVOA_X
ClientSampleId :
BFB623