

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039143.D
 Acq On : 11 Dec 2023 14:59
 Operator : JC/MD
 Sample : 05646-16DL 400X
 Misc : 2.63g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AS3DL

Quant Time: Dec 12 03:54:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 12 03:50:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	285521	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	255957	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	121009	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	87594	39.114	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.220%
7) Chloroethane-d5	1.666	69	66305	40.056	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.120%
11) 1,1-Dichloroethene-d2	2.306	65	43704	44.458	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.920%
21) 2-Butanone-d5	4.446	46	185127	91.323	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.320%
24) Chloroform-d	5.056	84	178641	45.061	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.120%
26) 1,2-Dichloroethane-d4	5.952	65	125476	48.872	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.740%
32) Benzene-d6	5.970	84	374253	47.378	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.760%
36) 1,2-Dichloropropane-d6	7.306	67	122095	48.028	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.060%
41) Toluene-d8	8.647	98	329877	46.081	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.160%
43) trans-1,3-Dichloroprop...	8.946	79	59917	46.315	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.640%
47) 2-Hexanone-d5	9.384	63	136658	90.004	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.000%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	170697	47.333	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.660%
66) 1,2-Dichlorobenzene-d4	12.317	152	113227	49.503	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.000%
Target Compounds						
					Qvalue	
51) Chlorobenzene	10.079	112	15217	2.856	ug/L	90
64) 1,3-Dichlorobenzene	11.969	146	7565	1.999	ug/L	94
65) 1,4-Dichlorobenzene	12.043	146	260570	67.943	ug/L	99
67) 1,2-Dichlorobenzene	12.335	146	48313	13.345	ug/L	100
70) 1,2,4-trichlorobenzene	13.585	180	184006	77.984	ug/L	99
72) 1,2,3-Trichlorobenzene	13.963	180	44529	19.490	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039143.D
Acq On : 11 Dec 2023 14:59
Operator : JC/MD
Sample : 05646-16DL 400X
Misc : 2.63g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS3DL

Quant Time: Dec 12 03:54:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 12 03:50:51 2023
Response via : Initial Calibration




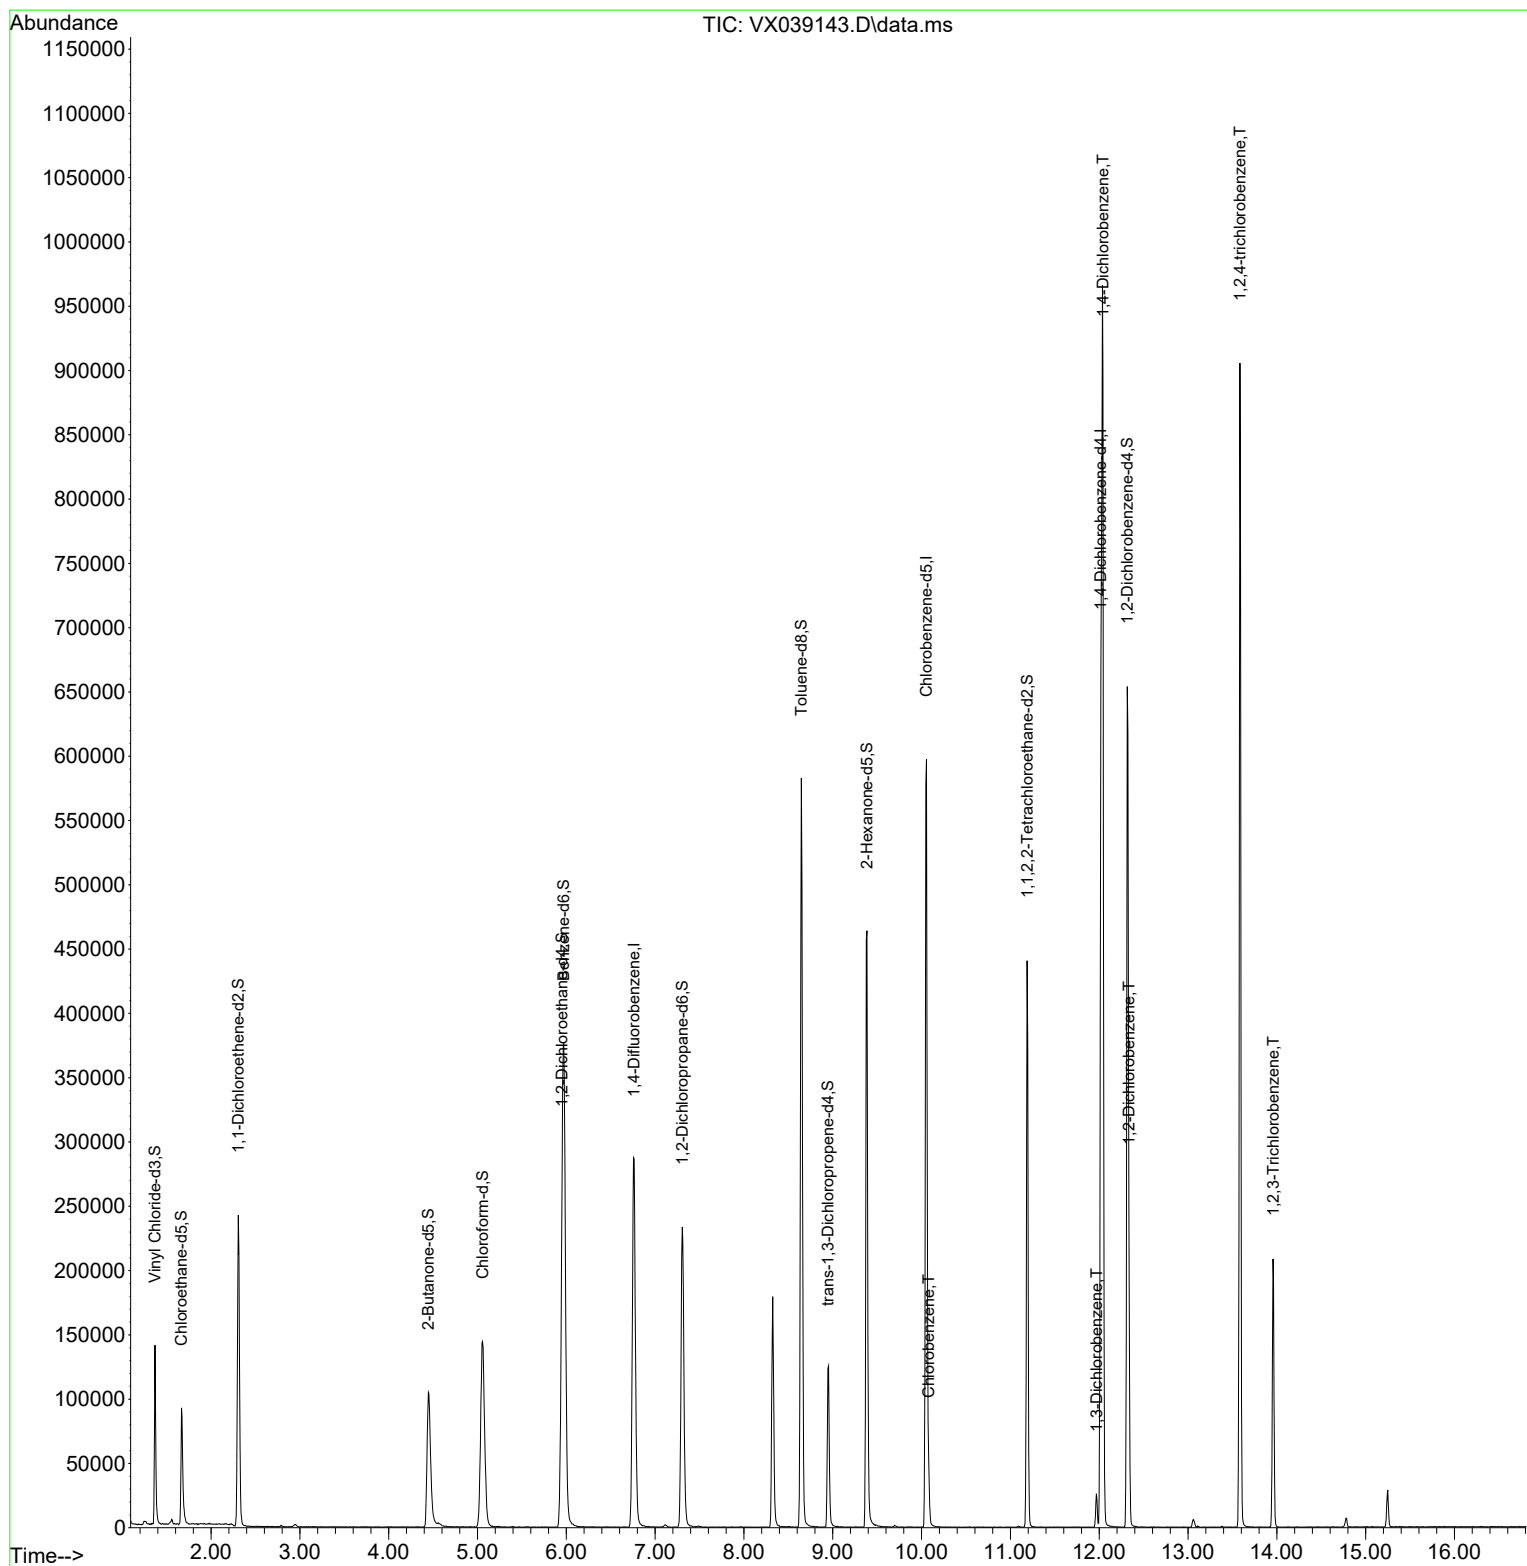


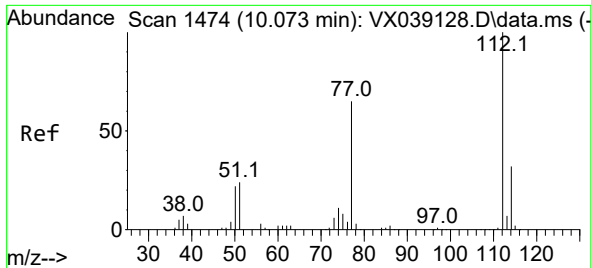

#51
Chlorobenzene
Concen: 2.856 ug/L
RT: 10.079 min Scan# 1474
Delta R.T. 0.006 min
Lab File: VX039143.D
Acq: 11 Dec 2023 14:59




Instrument :
MSVOA_X
ClientSampleId :
C0AS3DL


Tgt Ion:112 Resp: 15217
Ion Ratio Lower Upper
112 100
114 31.4 21.8 40.4
77 72.8 49.0 73.6

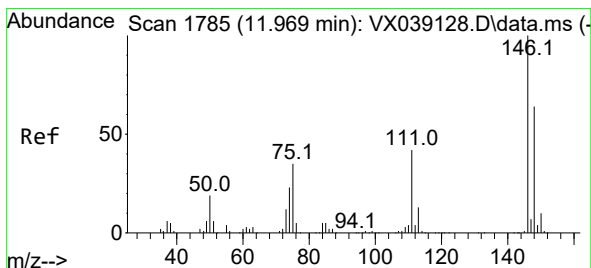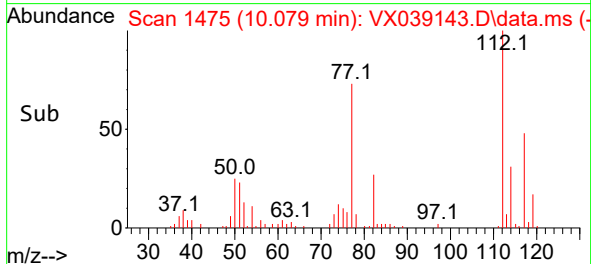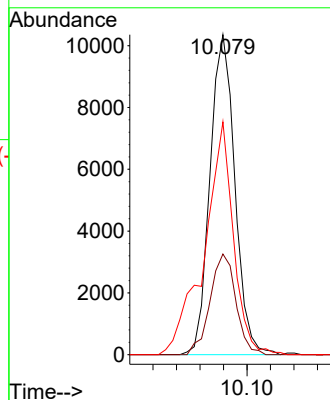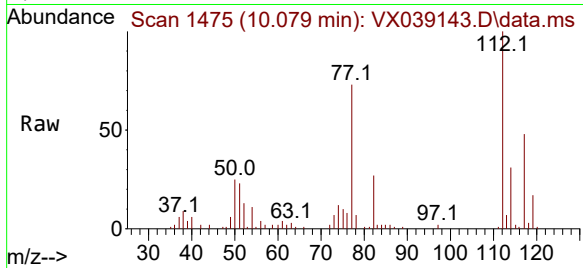

#64
1,3-Dichlorobenzene
Concen: 1.999 ug/L
RT: 11.969 min Scan# 1785
Delta R.T. -0.000 min
Lab File: VX039143.D
Acq: 11 Dec 2023 14:59

Tgt Ion:146 Resp: 7565
Ion Ratio Lower Upper
146 100
111 50.1 30.0 55.6
148 64.3 44.2 82.0


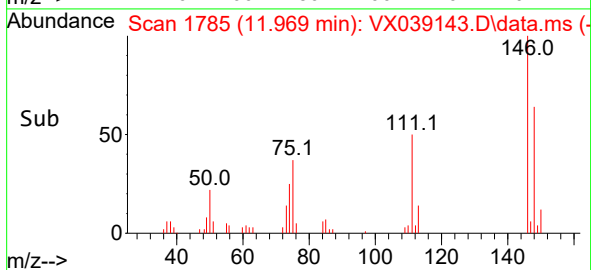
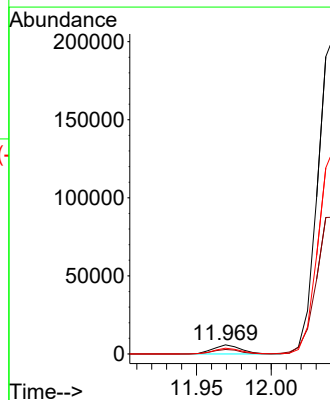
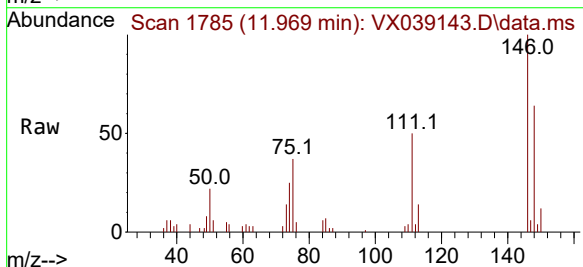


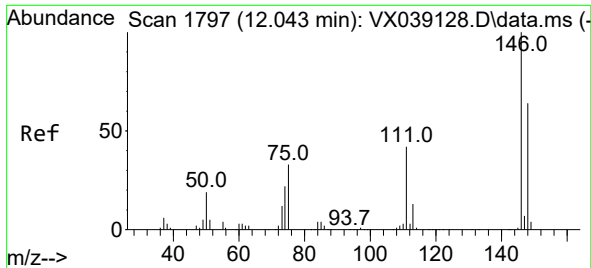

#65
1,4-Dichlorobenzene
Concen: 67.943 ug/L
RT: 12.043 min Scan# 1797
Delta R.T. -0.000 min
Lab File: VX039143.D
Acq: 11 Dec 2023 14:59




Instrument :
MSVOA_X
ClientSampleId :
C0AS3DL


Tgt Ion:146 Resp: 260570
Ion Ratio Lower Upper
146 100
111 42.7 29.7 55.1
148 64.8 45.8 85.2

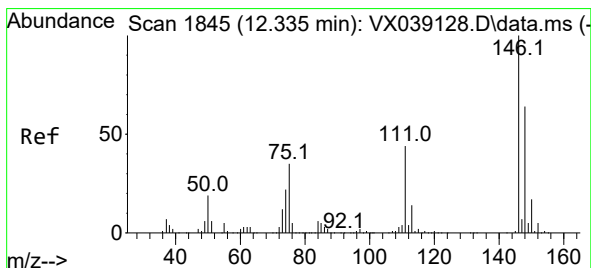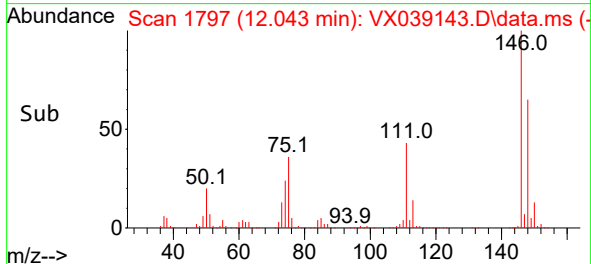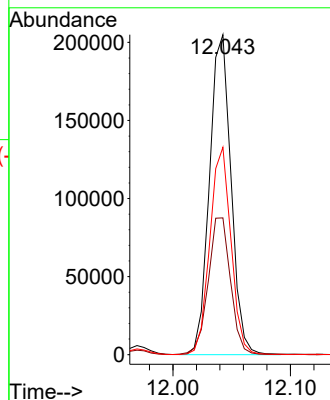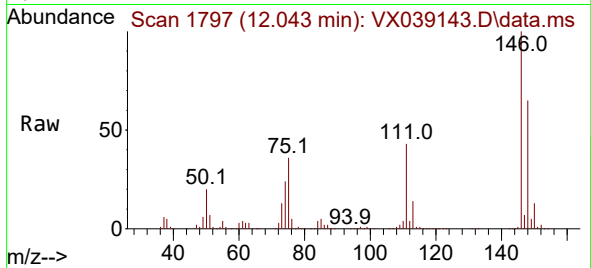

#67
1,2-Dichlorobenzene
Concen: 13.345 ug/L
RT: 12.335 min Scan# 1845
Delta R.T. -0.000 min
Lab File: VX039143.D
Acq: 11 Dec 2023 14:59

Tgt Ion:146 Resp: 48313
Ion Ratio Lower Upper
146 100
111 45.4 36.4 54.6
148 62.0 50.0 75.0

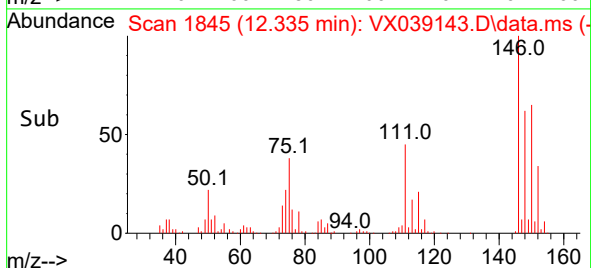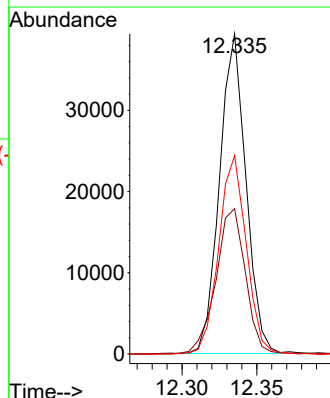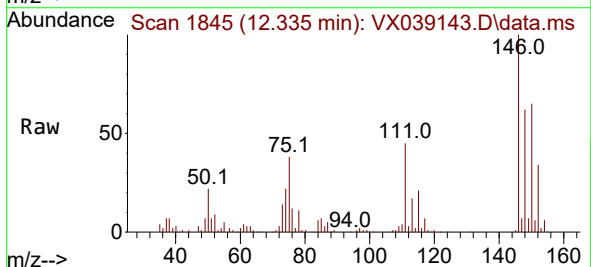

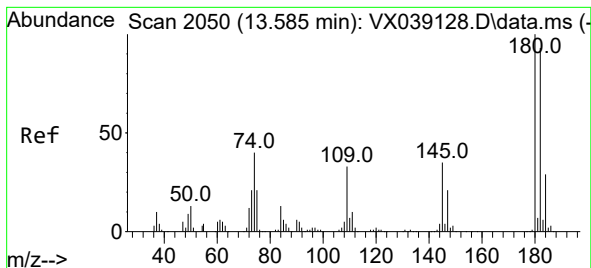

#70

1,2,4-trichlorobenzene

Concen: 77.984 ug/L

RT: 13.585 min Scan# 2050

Delta R.T. -0.000 min

Lab File: VX039143.D

Acq: 11 Dec 2023 14:59

Instrument :

MSVOA_X

ClientSampleId :

C0AS3DL





Tgt Ion:180 Resp: 184006

Ion Ratio Lower Upper

180 100

182 94.3 76.8 115.2

145 34.7 27.8 41.6

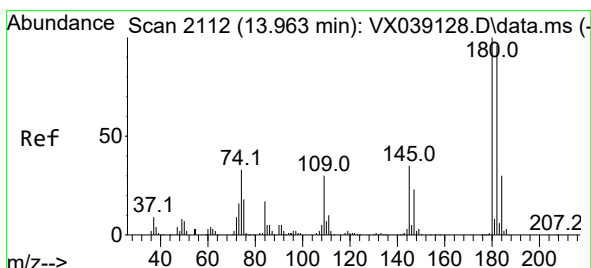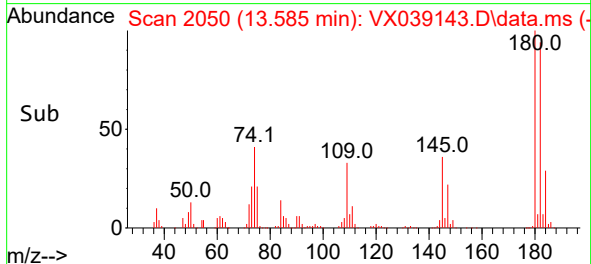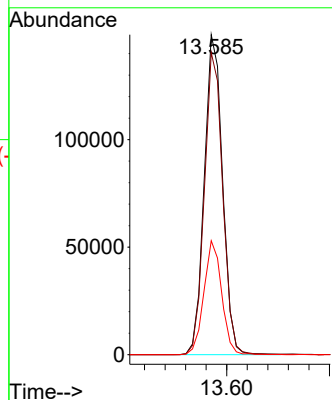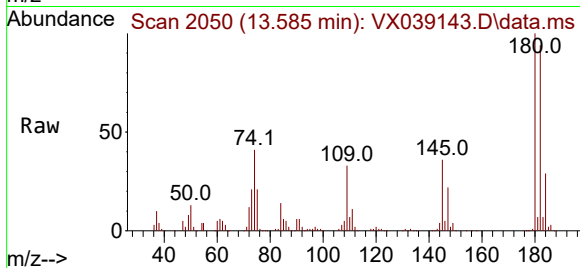

#72

1,2,3-Trichlorobenzene

Concen: 19.490 ug/L

RT: 13.963 min Scan# 2112

Delta R.T. -0.000 min

Lab File: VX039143.D

Acq: 11 Dec 2023 14:59

Tgt Ion:180 Resp: 44529

Ion Ratio Lower Upper

180 100

182 93.0 75.9 113.9

145 35.7 28.6 42.8

