

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039129.D
 Acq On : 11 Dec 2023 09:38
 Operator : JC/MD
 Sample : VX1211WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK643

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039129.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	23	25	26	rBV	2114	1707	0.16%	0.020%
2	1.367	43	46	56	rVB	133096	143381	13.17%	1.665%
3	1.672	91	96	107	rVB	86824	125247	11.50%	1.454%
4	2.306	194	200	209	rBV	231329	365523	33.56%	4.243%
5	2.611	248	250	251	rBV2	673	402	0.04%	0.005%
6	3.769	438	440	444	rVB	572	498	0.05%	0.006%
7	4.446	543	551	564	rBV	101553	288143	26.46%	3.345%
8	5.056	640	651	668	rVB	135065	428274	39.33%	4.972%
9	5.964	789	800	818	rBV2	366446	1089023	100.00%	12.643%
10	6.507	887	889	892	rBV2	627	775	0.07%	0.009%
11	6.757	921	930	944	rBV	276043	658186	60.44%	7.641%
12	7.110	983	988	995	rBV5	2065	4956	0.46%	0.058%
13	7.305	1011	1020	1031	rBV	224128	500065	45.92%	5.805%
14	7.799	1099	1101	1104	rBV	483	573	0.05%	0.007%
15	7.836	1104	1107	1110	rVV3	683	874	0.08%	0.010%
16	7.946	1120	1125	1127	rBV2	886	1468	0.13%	0.017%
17	8.061	1143	1144	1147	rVB	628	453	0.04%	0.005%
18	8.195	1165	1166	1168	rVB	664	280	0.03%	0.003%
19	8.275	1175	1179	1180	rBV	472	601	0.06%	0.007%
20	8.324	1180	1187	1207	rVV	164366	280988	25.80%	3.262%
21	8.549	1223	1224	1225	rBV	539	297	0.03%	0.003%
22	8.647	1233	1240	1250	rBV	538516	850847	78.13%	9.878%
23	8.945	1284	1289	1302	rBV	123710	186960	17.17%	2.170%
24	9.147	1320	1322	1324	rVB	465	308	0.03%	0.004%
25	9.177	1324	1327	1331	rVB2	658	814	0.07%	0.009%
26	9.244	1336	1338	1339	rBV2	485	293	0.03%	0.003%
27	9.378	1355	1360	1378	rBV	476811	699103	64.20%	8.116%
28	9.701	1409	1413	1417	rVV3	1429	2094	0.19%	0.024%
29	9.750	1419	1421	1423	rVB	476	388	0.04%	0.005%
30	9.774	1423	1425	1426	rVB	425	298	0.03%	0.003%
31	9.805	1426	1430	1432	rBV2	436	644	0.06%	0.007%
32	9.945	1451	1453	1454	rVB	621	382	0.04%	0.004%
33	9.970	1454	1457	1458	rBV2	371	409	0.04%	0.005%
34	10.055	1465	1471	1485	rBV	559888	807396	74.14%	9.373%
35	10.195	1492	1494	1497	rVB3	1342	1148	0.11%	0.013%
36	10.238	1499	1501	1503	rBV	406	331	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039129.D
 Acq On : 11 Dec 2023 09:38
 Operator : JC/MD
 Sample : VX1211WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK643

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	10.305	1510	1512	1517	rVB2	922	1083	0.10%	0.013%
38	10.421	1529	1531	1532	rBV2	379	361	0.03%	0.004%
39	10.433	1532	1533	1535	rVB	906	506	0.05%	0.006%
40	10.524	1546	1548	1549	rBV	390	295	0.03%	0.003%
41	10.646	1563	1568	1571	rBV3	1246	2034	0.19%	0.024%
42	10.744	1583	1584	1586	rBV	494	318	0.03%	0.004%
43	10.847	1597	1601	1602	rBV2	316	360	0.03%	0.004%
44	10.963	1618	1620	1623	rVB2	857	904	0.08%	0.010%
45	11.085	1637	1640	1644	rBV3	1273	1821	0.17%	0.021%
46	11.134	1644	1648	1651	rBV2	440	637	0.06%	0.007%
47	11.189	1652	1657	1669	rVB	438529	549258	50.44%	6.376%
48	11.451	1699	1700	1706	rVB2	1291	1517	0.14%	0.018%
49	11.567	1717	1719	1722	rVB	470	310	0.03%	0.004%
50	11.591	1722	1723	1728	rVB	662	432	0.04%	0.005%
51	11.634	1728	1730	1732	rBV2	409	364	0.03%	0.004%
52	11.713	1741	1743	1746	rBV2	647	501	0.05%	0.006%
53	11.756	1748	1750	1754	rVB2	1251	1400	0.13%	0.016%
54	11.817	1757	1760	1762	rBV2	349	521	0.05%	0.006%
55	11.969	1782	1785	1788	rBV3	1584	1905	0.17%	0.022%
56	12.018	1788	1793	1802	rVV	623426	816005	74.93%	9.473%
57	12.213	1824	1825	1827	rBV	593	572	0.05%	0.007%
58	12.317	1837	1842	1850	rBV	581449	744443	68.36%	8.642%
59	12.548	1877	1880	1882	rBV	381	391	0.04%	0.005%
60	12.689	1902	1903	1906	rBV2	331	362	0.03%	0.004%
61	13.048	1961	1962	1966	rBV	403	510	0.05%	0.006%
62	13.115	1970	1973	1977	rVB4	2554	3138	0.29%	0.036%
63	13.164	1980	1981	1985	rVV2	443	537	0.05%	0.006%
64	13.201	1985	1987	1991	rVB2	417	310	0.03%	0.004%
65	13.286	1999	2001	2004	rVB2	420	458	0.04%	0.005%
66	13.402	2017	2020	2021	rVB	622	524	0.05%	0.006%
67	13.432	2021	2025	2027	rBV2	499	724	0.07%	0.008%
68	13.536	2037	2042	2044	rBV2	295	413	0.04%	0.005%
69	13.591	2047	2051	2058	rVV4	5316	7056	0.65%	0.082%
70	13.664	2061	2063	2065	rVB2	501	341	0.03%	0.004%
71	13.688	2065	2067	2068	rBV	457	306	0.03%	0.004%
72	13.780	2077	2082	2089	rVV	6728	9132	0.84%	0.106%
73	13.963	2105	2112	2120	rVB3	5006	7616	0.70%	0.088%
74	14.024	2120	2122	2125	rBV2	286	376	0.03%	0.004%
75	14.109	2134	2136	2138	rBV2	556	417	0.04%	0.005%
76	14.219	2151	2154	2157	rBV2	477	586	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039129.D
 Acq On : 11 Dec 2023 09:38
 Operator : JC/MD
 Sample : VX1211WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK643

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	14.255	2157	2160	2161	rBV2	263	297	0.03%	0.003%
78	14.316	2168	2170	2173	rBV	625	590	0.05%	0.007%
79	14.377	2178	2180	2185	rVB3	321	500	0.05%	0.006%
80	14.560	2209	2210	2212	rBV	391	293	0.03%	0.003%
81	14.591	2212	2215	2219	rVV2	573	827	0.08%	0.010%
82	14.633	2221	2222	2226	rVB	396	286	0.03%	0.003%
83	14.688	2228	2231	2233	rBV2	459	532	0.05%	0.006%
84	14.767	2242	2244	2245	rBV	525	399	0.04%	0.005%
85	14.792	2245	2248	2249	rBV	468	372	0.03%	0.004%
86	14.847	2255	2257	2259	rBV	560	365	0.03%	0.004%
87	14.987	2278	2280	2282	rBV2	533	419	0.04%	0.005%
88	15.225	2315	2319	2320	rBV2	595	699	0.06%	0.008%
89	15.304	2330	2332	2334	rVB3	421	311	0.03%	0.004%
90	15.328	2334	2336	2337	rBV	661	366	0.03%	0.004%
91	15.462	2356	2358	2359	rBV	451	344	0.03%	0.004%
92	15.591	2377	2379	2380	rVB	742	397	0.04%	0.005%
93	15.609	2380	2382	2385	rBV2	548	526	0.05%	0.006%
94	15.804	2412	2414	2416	rBV	644	588	0.05%	0.007%
95	15.840	2418	2420	2421	rBV2	749	629	0.06%	0.007%
96	16.054	2454	2455	2457	rVB	445	289	0.03%	0.003%
97	16.090	2457	2461	2467	rBV3	766	1544	0.14%	0.018%
98	16.170	2472	2474	2476	rBV2	489	314	0.03%	0.004%
99	16.395	2507	2511	2514	rBV3	515	619	0.06%	0.007%
100	16.645	2550	2552	2553	rBV	595	416	0.04%	0.005%




Sum of corrected areas: 8613795

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039129.D
Acq On : 11 Dec 2023 09:38
Operator : JC/MD
Sample : VX1211WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK643

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

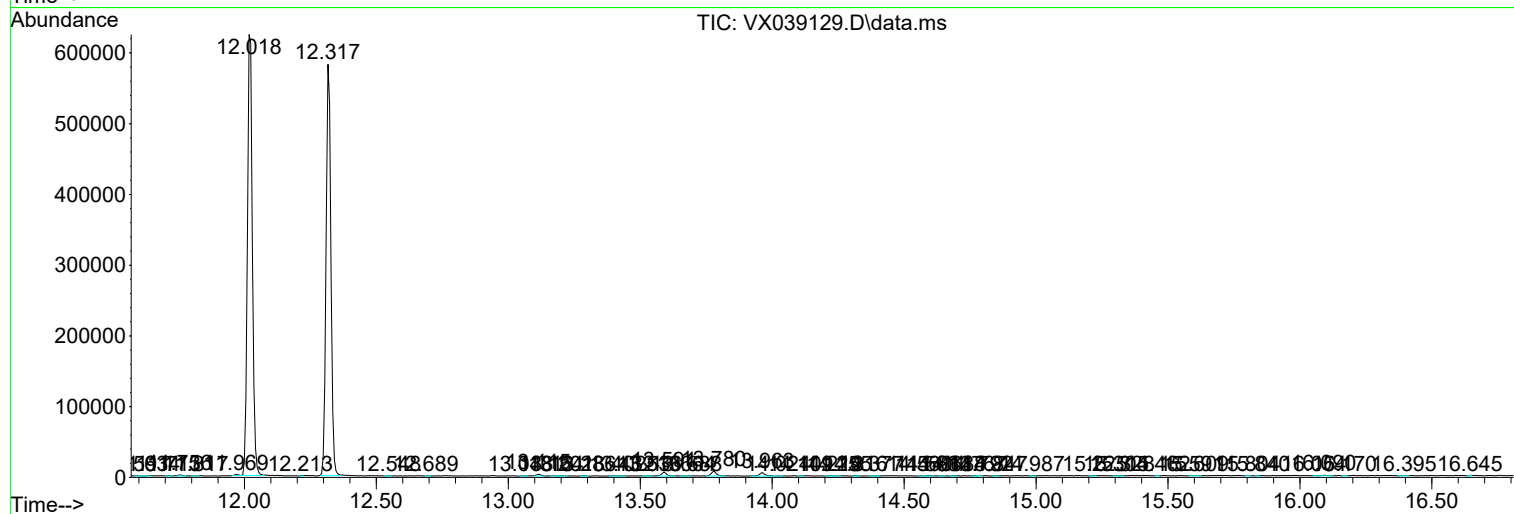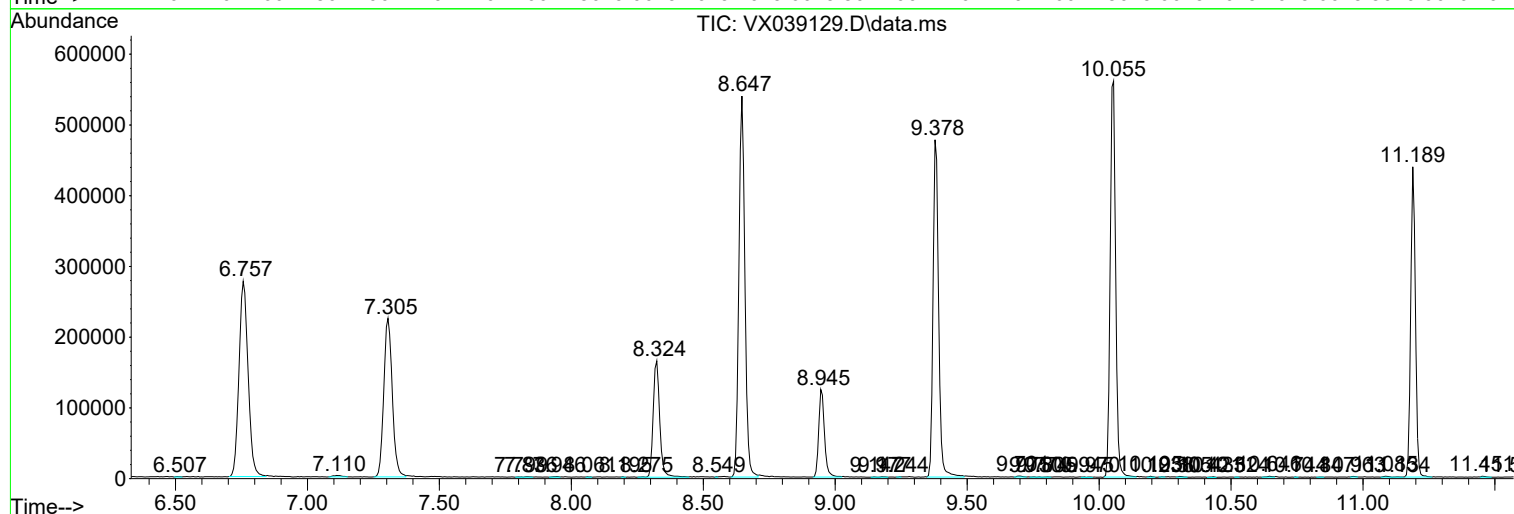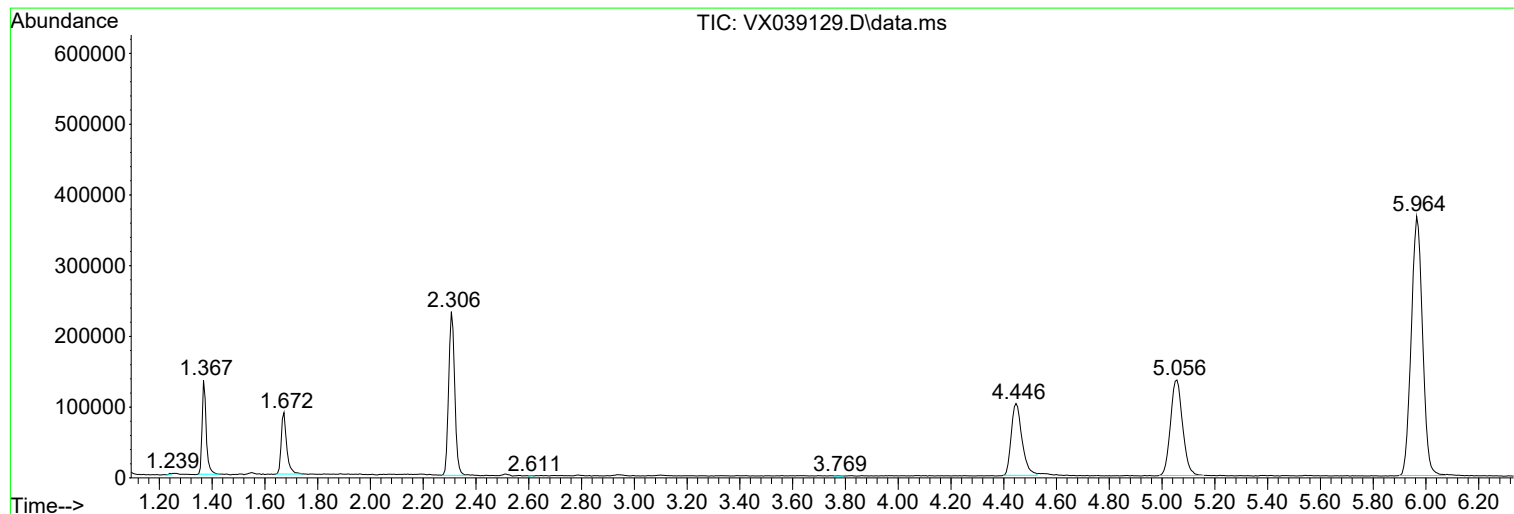

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039129.D
Acq On : 11 Dec 2023 09:38
Operator : JC/MD
Sample : VX1211WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK643

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039129.D
Acq On : 11 Dec 2023 09:38
Operator : JC/MD
Sample : VX1211WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK643

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------