

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039132.D
 Acq On : 11 Dec 2023 10:47
 Operator : JC/MD
 Sample : 05646-09 40X
 Misc : 2.02g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039132.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rVB	148468	154604	3.87%	1.234%
2	1.666	91	95	105	rVB	93151	129816	3.25%	1.036%
3	2.307	194	200	211	rVB	252828	396448	9.93%	3.165%
4	2.941	300	304	310	rVB	4375	7700	0.19%	0.061%
5	3.008	313	315	318	rVB	940	1096	0.03%	0.009%
6	3.032	318	319	321	rBV	637	590	0.01%	0.005%
7	3.136	334	336	337	rBV	640	665	0.02%	0.005%
8	3.258	353	356	358	rBV2	804	826	0.02%	0.007%
9	3.465	388	390	392	rBV2	602	678	0.02%	0.005%
10	3.593	410	411	413	rBV	774	702	0.02%	0.006%
11	3.715	430	431	438	rVB	780	1513	0.04%	0.012%
12	3.776	438	441	442	rBV2	748	720	0.02%	0.006%
13	3.825	447	449	450	rVV	770	667	0.02%	0.005%
14	3.855	452	454	456	rBV2	800	1020	0.03%	0.008%
15	3.879	456	458	462	rVV2	976	1123	0.03%	0.009%
16	3.934	464	467	468	rVV2	648	792	0.02%	0.006%
17	3.959	470	471	473	rBV	797	656	0.02%	0.005%
18	4.129	497	499	502	rVB	882	996	0.02%	0.008%
19	4.452	541	552	567	rBV	101063	297806	7.46%	2.377%
20	4.788	605	607	608	rBV	810	624	0.02%	0.005%
21	4.855	615	618	620	rBV2	956	1098	0.03%	0.009%
22	4.885	620	623	625	rVV2	725	760	0.02%	0.006%
23	4.904	625	626	630	rVB2	887	641	0.02%	0.005%
24	5.056	639	651	669	rBV	144623	459087	11.50%	3.665%
25	5.330	695	696	698	rVB	986	629	0.02%	0.005%
26	5.373	700	703	712	rVV4	1217	2966	0.07%	0.024%
27	5.538	726	730	733	rBV	874	1671	0.04%	0.013%
28	5.714	758	759	762	rBV2	763	843	0.02%	0.007%
29	5.855	779	782	784	rBV2	680	874	0.02%	0.007%
30	5.970	790	801	808	rBV2	387499	1203412	30.15%	9.607%
31	6.214	839	841	842	rBV	1094	803	0.02%	0.006%
32	6.757	921	930	945	rBV	296403	721853	18.09%	5.762%
33	6.952	960	962	963	rVV2	885	732	0.02%	0.006%
34	7.111	983	988	990	rBV4	2051	3657	0.09%	0.029%
35	7.159	994	996	997	rBV2	817	615	0.02%	0.005%
36	7.306	1011	1020	1033	rBV	240361	535646	13.42%	4.276%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039132.D
 Acq On : 11 Dec 2023 10:47
 Operator : JC/MD
 Sample : 05646-09 40X
 Misc : 2.02g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.873	1111	1113	1115	rBV	710	763	0.02%	0.006%
38	8.037	1139	1140	1142	rBV	1064	679	0.02%	0.005%
39	8.281	1176	1180	1181	rVV	956	908	0.02%	0.007%
40	8.324	1181	1187	1203	rVV	182824	302047	7.57%	2.411%
41	8.458	1207	1209	1211	rVB2	1123	938	0.02%	0.007%
42	8.647	1233	1240	1256	rBV	602787	957636	23.99%	7.645%
43	8.891	1279	1280	1284	rVB2	828	749	0.02%	0.006%
44	8.946	1284	1289	1301	rBV	130617	203378	5.10%	1.624%
45	9.049	1305	1306	1310	rVB	902	1014	0.03%	0.008%
46	9.092	1310	1313	1315	rBV	760	767	0.02%	0.006%
47	9.171	1325	1326	1329	rBV	739	688	0.02%	0.005%
48	9.202	1329	1331	1334	rVB	781	731	0.02%	0.006%
49	9.324	1348	1351	1355	rBV2	596	580	0.01%	0.005%
50	9.378	1355	1360	1374	rBV	462535	684208	17.14%	5.462%
51	9.702	1408	1413	1415	rBV3	1486	1900	0.05%	0.015%
52	9.799	1426	1429	1431	rBV2	1015	987	0.02%	0.008%
53	9.848	1435	1437	1439	rVV2	1093	1042	0.03%	0.008%
54	9.891	1443	1444	1446	rBV	698	597	0.01%	0.005%
55	10.080	1465	1475	1491	rBV2	2226636	3991071	100.00%	31.860%
56	10.482	1539	1541	1542	rBV	687	574	0.01%	0.005%
57	10.586	1554	1558	1560	rVB	871	1127	0.03%	0.009%
58	10.604	1560	1561	1565	rBV	967	1191	0.03%	0.010%
59	10.860	1600	1603	1605	rBV2	551	611	0.02%	0.005%
60	11.006	1623	1627	1628	rBV	779	950	0.02%	0.008%
61	11.092	1637	1641	1644	rBV3	1609	2242	0.06%	0.018%
62	11.189	1651	1657	1667	rBV	448432	570345	14.29%	4.553%
63	11.305	1674	1676	1679	rVB3	862	864	0.02%	0.007%
64	11.366	1681	1686	1692	rVB	21644	27970	0.70%	0.223%
65	11.457	1697	1701	1707	rVB3	5352	7933	0.20%	0.063%
66	11.530	1712	1713	1715	rBV	1191	677	0.02%	0.005%
67	11.640	1730	1731	1734	rVV2	683	696	0.02%	0.006%
68	11.677	1734	1737	1740	rVV	859	965	0.02%	0.008%
69	11.707	1740	1742	1744	rVV2	874	830	0.02%	0.007%
70	11.908	1773	1775	1777	rBV2	611	748	0.02%	0.006%
71	11.933	1777	1779	1780	rVB	1009	620	0.02%	0.005%
72	11.969	1780	1785	1788	rBV3	6522	9527	0.24%	0.076%
73	12.018	1788	1793	1804	rVB	663556	942761	23.62%	7.526%
74	12.171	1816	1818	1821	rBV2	671	747	0.02%	0.006%
75	12.219	1824	1826	1828	rBV	682	616	0.02%	0.005%
76	12.280	1834	1836	1837	rBV	663	630	0.02%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039132.D
 Acq On : 11 Dec 2023 10:47
 Operator : JC/MD
 Sample : 05646-09 40X
 Misc : 2.02g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1852	rVV	646236	816442	20.46%	6.517%
78	12.536	1876	1878	1880	rVB2	970	986	0.02%	0.008%
79	12.603	1885	1889	1890	rBV	829	695	0.02%	0.006%
80	13.061	1958	1964	1970	rBV2	19003	32899	0.82%	0.263%
81	13.207	1986	1988	1991	rVB	759	567	0.01%	0.005%
82	13.231	1991	1992	1995	rBV2	548	569	0.01%	0.005%
83	13.530	2039	2041	2043	rBV	761	617	0.02%	0.005%
84	13.591	2048	2051	2055	rVB3	2609	2984	0.07%	0.024%
85	13.817	2086	2088	2090	rVB	999	639	0.02%	0.005%
86	13.963	2110	2112	2115	rBV3	822	832	0.02%	0.007%
87	14.024	2118	2122	2124	rBV2	672	931	0.02%	0.007%
88	14.189	2147	2149	2152	rVB	690	650	0.02%	0.005%
89	14.390	2181	2182	2184	rBV	704	579	0.01%	0.005%
90	14.560	2207	2210	2211	rVB	933	740	0.02%	0.006%
91	14.786	2244	2247	2250	rBV	762	1284	0.03%	0.010%
92	14.835	2254	2255	2256	rBV	1057	612	0.02%	0.005%
93	15.060	2290	2292	2297	rBV2	903	1470	0.04%	0.012%
94	15.140	2303	2305	2307	rBV2	556	593	0.01%	0.005%
95	15.963	2438	2440	2442	rVB	1053	636	0.02%	0.005%
96	16.176	2473	2475	2479	rBV2	834	894	0.02%	0.007%
97	16.261	2486	2489	2490	rBV2	918	845	0.02%	0.007%
98	16.408	2509	2513	2514	rVV	933	944	0.02%	0.008%
99	16.426	2514	2516	2519	rBV2	925	996	0.02%	0.008%
100	16.633	2547	2550	2552	rBV	965	981	0.02%	0.008%




Sum of corrected areas: 12527021

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039132.D
Acq On : 11 Dec 2023 10:47
Operator : JC/MD
Sample : 05646-09 40X
Misc : 2.02g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

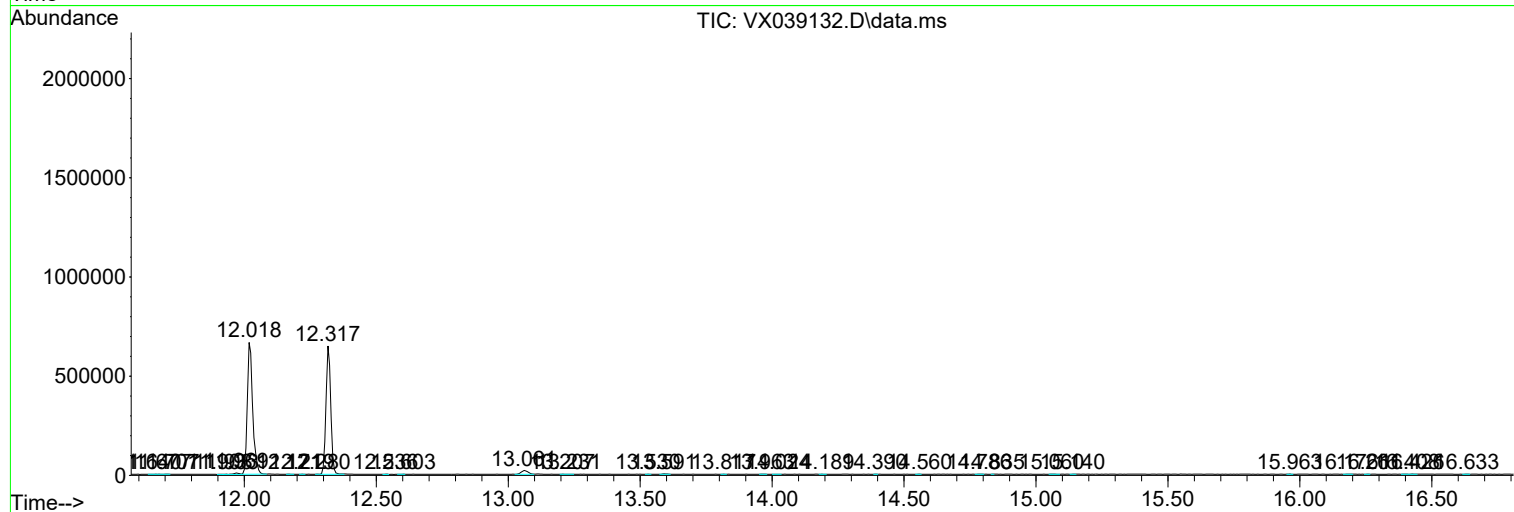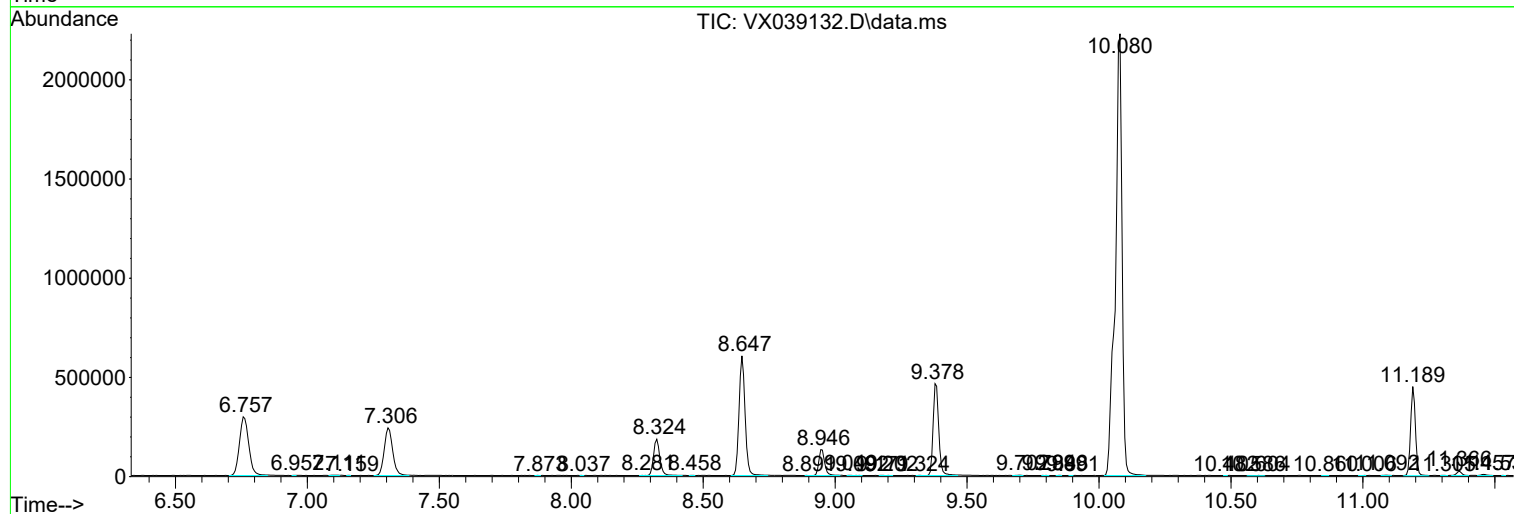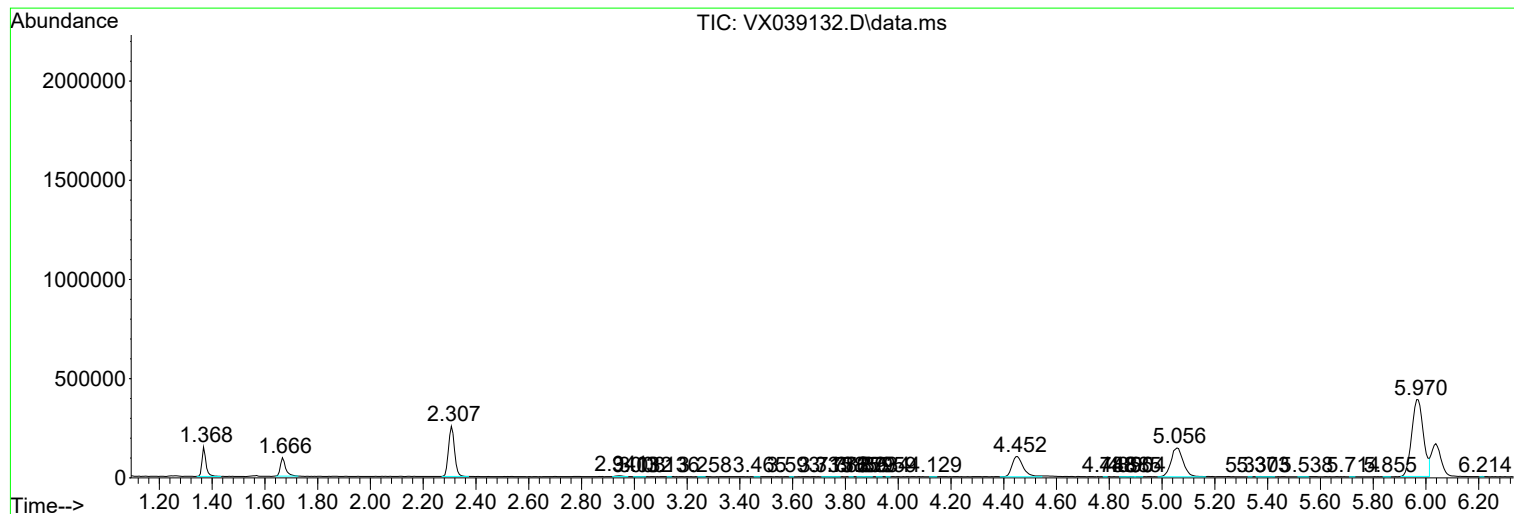

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039132.D
Acq On : 11 Dec 2023 10:47
Operator : JC/MD
Sample : 05646-09 40X
Misc : 2.02g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039132.D
Acq On : 11 Dec 2023 10:47
Operator : JC/MD
Sample : 05646-09 40X
Misc : 2.02g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc