

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039133.D
 Acq On : 11 Dec 2023 11:10
 Operator : JC/MD
 Sample : VIBLK624
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK624

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	56	rVB	140913	150168	13.13%	1.686%
2	1.672	91	96	107	rBV	93053	134131	11.73%	1.506%
3	2.306	194	200	213	rVB	248053	383915	33.57%	4.309%
4	4.446	544	551	565	rBV	104523	295295	25.82%	3.315%
5	5.056	641	651	666	rVB2	140319	432559	37.82%	4.855%
6	5.970	790	801	827	rVB2	372983	1143777	100.00%	12.838%
7	6.757	922	930	946	rBV	290334	702481	61.42%	7.885%
8	7.305	1012	1020	1035	rBV	238411	521171	45.57%	5.850%
9	7.567	1060	1063	1067	rBV	901	1645	0.14%	0.018%
10	7.647	1073	1076	1079	rBV2	780	1040	0.09%	0.012%
11	7.677	1079	1081	1082	rVV	586	272	0.02%	0.003%
12	7.708	1082	1086	1087	rVB	720	886	0.08%	0.010%
13	7.836	1106	1107	1108	rBV	676	309	0.03%	0.003%
14	8.019	1136	1137	1140	rBV2	632	718	0.06%	0.008%
15	8.262	1175	1177	1178	rBV	665	489	0.04%	0.005%
16	8.323	1181	1187	1201	rVV	172532	285517	24.96%	3.205%
17	8.646	1234	1240	1258	rBV	589922	917267	80.20%	10.296%
18	8.909	1281	1283	1284	rBV	571	295	0.03%	0.003%
19	8.951	1284	1290	1299	rVV	122773	192064	16.79%	2.156%
20	9.232	1334	1336	1338	rBV	618	656	0.06%	0.007%
21	9.384	1355	1361	1371	rBV	470598	685726	59.95%	7.697%
22	9.738	1418	1419	1420	rBV	668	246	0.02%	0.003%
23	10.055	1465	1471	1483	rBV	610983	853218	74.60%	9.577%
24	10.366	1520	1522	1523	rBV	664	360	0.03%	0.004%
25	10.421	1530	1531	1533	rBV	811	463	0.04%	0.005%
26	10.439	1533	1534	1536	rVB	922	506	0.04%	0.006%
27	10.500	1543	1544	1546	rBV2	639	562	0.05%	0.006%
28	10.585	1557	1558	1563	rBV	526	660	0.06%	0.007%
29	10.689	1573	1575	1576	rVB	643	359	0.03%	0.004%
30	10.707	1576	1578	1579	rBV	554	521	0.05%	0.006%
31	10.823	1595	1597	1598	rVB	692	434	0.04%	0.005%
32	10.841	1598	1600	1603	rBV	637	766	0.07%	0.009%
33	10.890	1606	1608	1611	rBV	499	552	0.05%	0.006%
34	11.091	1637	1641	1642	rBV	1584	1619	0.14%	0.018%
35	11.152	1650	1651	1652	rBV	650	285	0.02%	0.003%
36	11.189	1652	1657	1666	rVV	437300	555940	48.61%	6.240%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039133.D
 Acq On : 11 Dec 2023 11:10
 Operator : JC/MD
 Sample : VIBLK624
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK624

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	11.305	1674	1676	1679	rVB	871	604	0.05%	0.007%
38	11.542	1712	1715	1716	rBV	853	932	0.08%	0.010%
39	11.646	1730	1732	1733	rBV	410	383	0.03%	0.004%
40	11.969	1782	1785	1786	rBV2	703	917	0.08%	0.010%
41	12.024	1788	1794	1803	rVV	615647	821175	71.80%	9.217%
42	12.219	1825	1826	1827	rBV	777	306	0.03%	0.003%
43	12.317	1837	1842	1854	rBV	594988	778533	68.07%	8.739%
44	12.432	1860	1861	1862	rVB	1021	373	0.03%	0.004%
45	12.487	1868	1870	1872	rVB	582	475	0.04%	0.005%
46	12.530	1874	1877	1879	rBV	972	949	0.08%	0.011%
47	12.682	1898	1902	1905	rVB2	1022	1377	0.12%	0.015%
48	12.725	1907	1909	1911	rBV2	581	452	0.04%	0.005%
49	12.780	1917	1918	1920	rBV	545	444	0.04%	0.005%
50	12.841	1925	1928	1931	rBV2	597	810	0.07%	0.009%
51	12.902	1937	1938	1939	rVB	894	327	0.03%	0.004%
52	12.914	1939	1940	1942	rBV	901	782	0.07%	0.009%
53	12.944	1943	1945	1946	rVB	625	412	0.04%	0.005%
54	13.030	1957	1959	1961	rBV	364	376	0.03%	0.004%
55	13.048	1961	1962	1964	rVB	695	397	0.03%	0.004%
56	13.115	1972	1973	1974	rBV	684	359	0.03%	0.004%
57	13.194	1984	1986	1988	rBV	800	849	0.07%	0.010%
58	13.274	1997	1999	2003	rVB	763	735	0.06%	0.008%
59	13.310	2003	2005	2006	rBV	447	253	0.02%	0.003%
60	13.377	2014	2016	2017	rBV	582	504	0.04%	0.006%
61	13.450	2026	2028	2031	rVB	611	650	0.06%	0.007%
62	13.530	2039	2041	2042	rBV	429	290	0.03%	0.003%
63	13.591	2048	2051	2055	rVB3	1786	2447	0.21%	0.027%
64	13.639	2056	2059	2061	rVB	683	581	0.05%	0.007%
65	13.713	2070	2071	2073	rBV	462	299	0.03%	0.003%
66	13.780	2080	2082	2084	rBV2	557	469	0.04%	0.005%
67	13.822	2086	2089	2090	rBV	481	463	0.04%	0.005%
68	13.847	2090	2093	2096	rVB	1014	1365	0.12%	0.015%
69	13.877	2096	2098	2102	rBV	937	1229	0.11%	0.014%
70	13.914	2102	2104	2105	rBV	561	559	0.05%	0.006%
71	14.011	2118	2120	2121	rVB	622	340	0.03%	0.004%
72	14.042	2123	2125	2126	rVB	590	423	0.04%	0.005%
73	14.066	2126	2129	2133	rVB	775	1193	0.10%	0.013%
74	14.103	2133	2135	2136	rBV	908	613	0.05%	0.007%
75	14.334	2171	2173	2176	rBV	1132	1434	0.13%	0.016%
76	14.444	2190	2191	2196	rVB	732	1047	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039133.D
 Acq On : 11 Dec 2023 11:10
 Operator : JC/MD
 Sample : VIBLK624
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK624

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	14.487	2196	2198	2199	rBV	710	694	0.06%	0.008%
78	14.560	2208	2210	2212	rBV2	851	865	0.08%	0.010%
79	14.603	2216	2217	2219	rVV	744	447	0.04%	0.005%
80	14.682	2228	2230	2231	rBV2	637	284	0.02%	0.003%
81	14.810	2249	2251	2255	rVB	1064	1475	0.13%	0.017%
82	14.847	2255	2257	2259	rBV2	949	1126	0.10%	0.013%
83	15.011	2282	2284	2286	rBV2	456	502	0.04%	0.006%
84	15.237	2319	2321	2323	rBV2	737	686	0.06%	0.008%
85	15.286	2327	2329	2330	rVB	713	398	0.03%	0.004%
86	15.493	2361	2363	2365	rVB2	586	524	0.05%	0.006%
87	15.548	2371	2372	2374	rBV2	851	547	0.05%	0.006%
88	15.584	2376	2378	2381	rVB	830	796	0.07%	0.009%
89	15.615	2381	2383	2384	rBV	773	550	0.05%	0.006%
90	15.645	2384	2388	2392	rBV	994	1301	0.11%	0.015%
91	15.724	2399	2401	2402	rBV	488	366	0.03%	0.004%
92	15.798	2411	2413	2414	rBV	592	292	0.03%	0.003%
93	16.041	2451	2453	2456	rVB	976	814	0.07%	0.009%
94	16.078	2456	2459	2460	rBV	782	828	0.07%	0.009%
95	16.334	2499	2501	2502	rVB	686	377	0.03%	0.004%
96	16.432	2516	2517	2518	rBV	777	373	0.03%	0.004%
97	16.487	2524	2526	2531	rBV3	550	991	0.09%	0.011%
98	16.602	2544	2545	2546	rBV	688	283	0.02%	0.003%
99	16.694	2558	2560	2563	rVB2	835	828	0.07%	0.009%
100	16.724	2563	2565	2566	rBV	696	631	0.06%	0.007%




Sum of corrected areas: 8908976

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039133.D
Acq On : 11 Dec 2023 11:10
Operator : JC/MD
Sample : VIBLK624
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK624

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

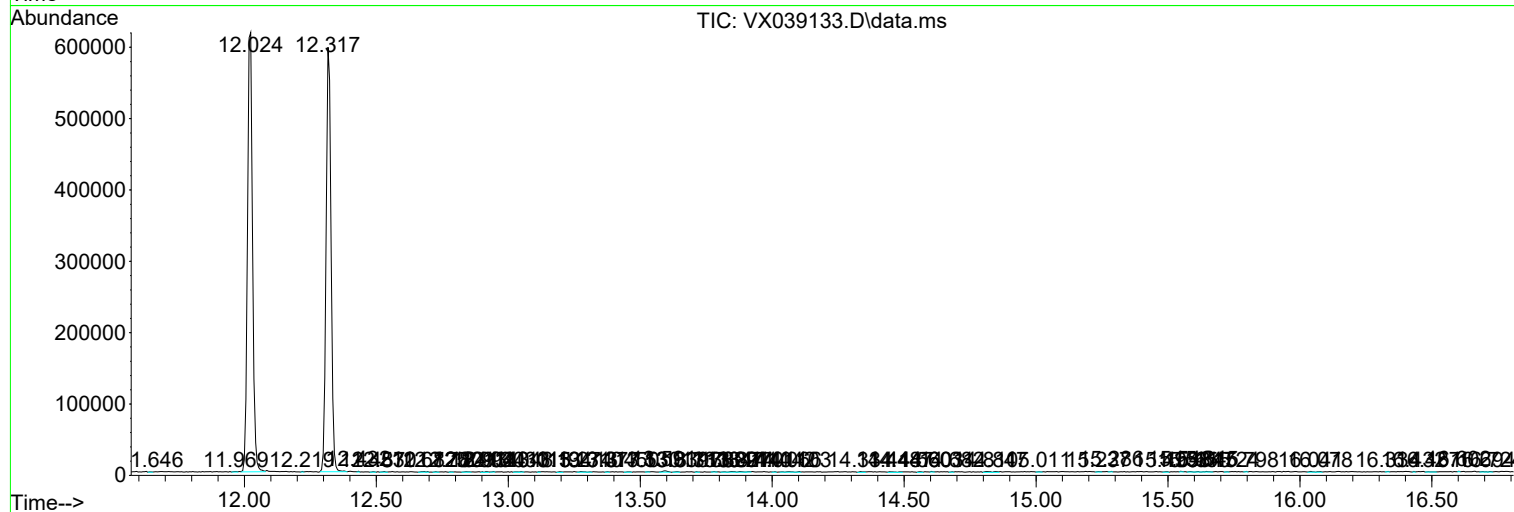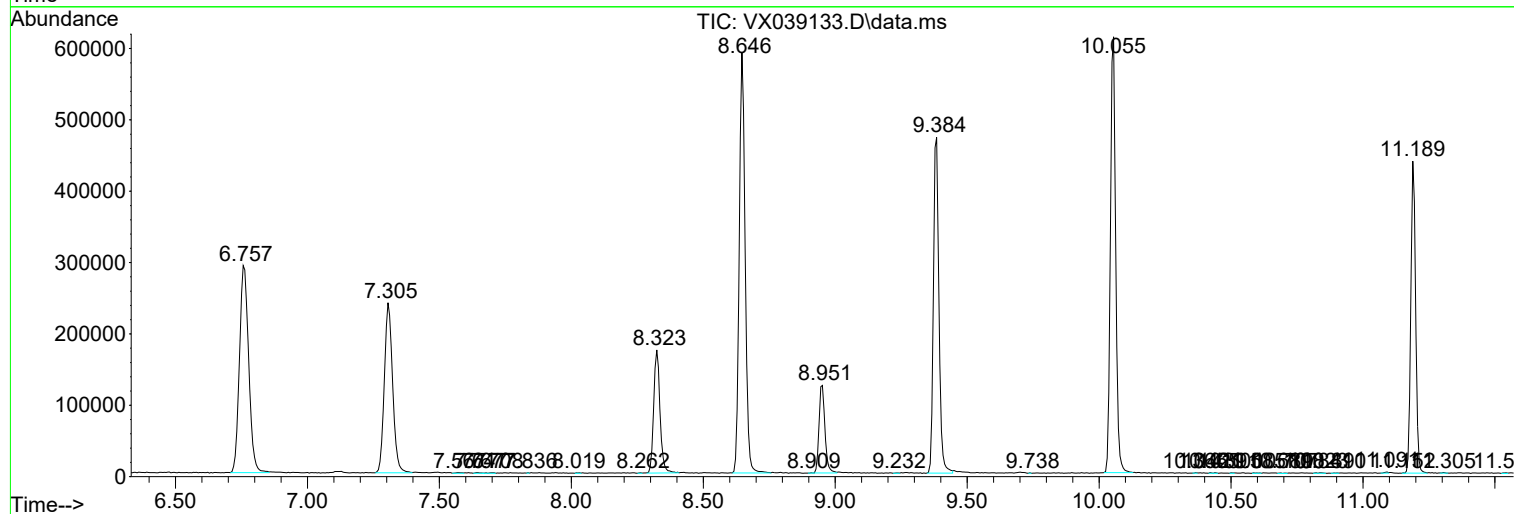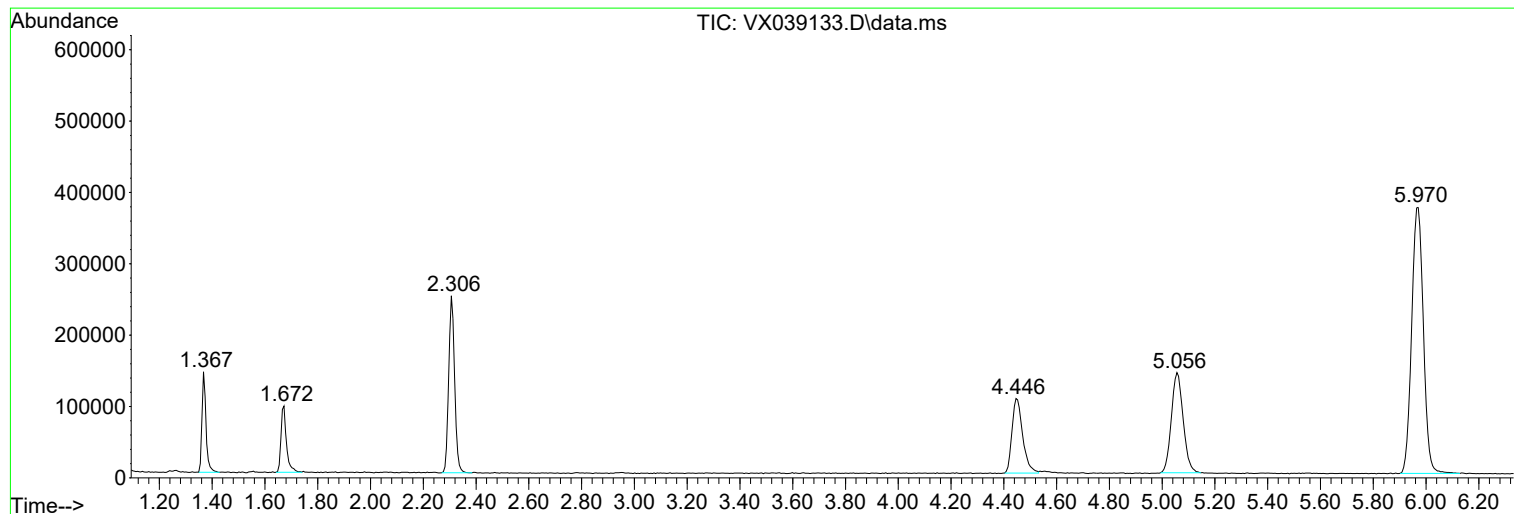

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039133.D
Acq On : 11 Dec 2023 11:10
Operator : JC/MD
Sample : VIBLK624
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK624

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039133.D
Acq On : 11 Dec 2023 11:10
Operator : JC/MD
Sample : VIBLK624
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK624

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc