

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039134.D
 Acq On : 11 Dec 2023 11:33
 Operator : JC/MD
 Sample : 05646-11 40X
 Misc : 3.70g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039134.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rBV	144702	148988	12.49%	1.609%
2	1.666	91	95	106	rVB	89293	125675	10.54%	1.357%
3	2.307	194	200	210	rVB	256158	385438	32.32%	4.162%
4	4.001	476	478	479	rBV	909	468	0.04%	0.005%
5	4.453	544	552	567	rBV	101787	291871	24.47%	3.151%
6	5.056	640	651	668	rBV	141425	439859	36.88%	4.749%
7	5.300	690	691	693	rVB	688	438	0.04%	0.005%
8	5.324	693	695	698	rVB2	932	744	0.06%	0.008%
9	5.434	712	713	715	rBV2	680	521	0.04%	0.006%
10	5.550	731	732	737	rVB	1007	1043	0.09%	0.011%
11	5.617	741	743	744	rBV	653	612	0.05%	0.007%
12	5.757	765	766	767	rVB	886	324	0.03%	0.003%
13	5.776	767	769	771	rBV2	499	521	0.04%	0.006%
14	5.830	776	778	779	rVB	660	326	0.03%	0.004%
15	5.867	782	784	786	rBV	781	787	0.07%	0.008%
16	5.971	789	801	823	rBV2	380398	1192722	100.00%	12.878%
17	6.391	868	870	872	rBV2	588	450	0.04%	0.005%
18	6.550	894	896	897	rBV	587	472	0.04%	0.005%
19	6.623	906	908	910	rBV2	519	388	0.03%	0.004%
20	6.641	910	911	914	rVB2	459	410	0.03%	0.004%
21	6.684	916	918	920	rBV	912	817	0.07%	0.009%
22	6.757	921	930	945	rBV	297397	716937	60.11%	7.741%
23	7.105	984	987	988	rBV3	1427	1443	0.12%	0.016%
24	7.184	998	1000	1002	rBV	547	618	0.05%	0.007%
25	7.239	1007	1009	1010	rBV	523	383	0.03%	0.004%
26	7.306	1012	1020	1032	rBV	231508	516132	43.27%	5.573%
27	7.562	1059	1062	1063	rBV	931	781	0.07%	0.008%
28	7.836	1106	1107	1109	rBV	678	434	0.04%	0.005%
29	7.860	1109	1111	1112	rVV	712	399	0.03%	0.004%
30	7.885	1112	1115	1118	rVB	566	667	0.06%	0.007%
31	8.019	1135	1137	1138	rBV	950	664	0.06%	0.007%
32	8.251	1173	1175	1177	rVB	576	467	0.04%	0.005%
33	8.269	1177	1178	1180	rBV	469	340	0.03%	0.004%
34	8.324	1180	1187	1199	rBV	176985	290046	24.32%	3.132%
35	8.647	1234	1240	1256	rBV	581277	918332	76.99%	9.915%
36	8.873	1276	1277	1279	rBV	429	338	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039134.D
 Acq On : 11 Dec 2023 11:33
 Operator : JC/MD
 Sample : 05646-11 40X
 Misc : 3.70g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	8.952	1284	1290	1298	rBV	127885	195011	16.35%	2.106%
38	9.129	1318	1319	1321	rBV	612	528	0.04%	0.006%
39	9.165	1324	1325	1327	rBV2	608	513	0.04%	0.006%
40	9.220	1332	1334	1336	rVV	705	583	0.05%	0.006%
41	9.385	1355	1361	1374	rBV	455715	679916	57.01%	7.341%
42	9.622	1398	1400	1403	rVB2	581	391	0.03%	0.004%
43	9.726	1415	1417	1418	rVB2	515	346	0.03%	0.004%
44	9.738	1418	1419	1421	rBV	649	435	0.04%	0.005%
45	9.769	1423	1424	1426	rVV	802	499	0.04%	0.005%
46	9.793	1426	1428	1431	rVV2	652	587	0.05%	0.006%
47	9.945	1451	1453	1455	rVB	590	450	0.04%	0.005%
48	9.976	1455	1458	1460	rBV	550	574	0.05%	0.006%
49	10.013	1460	1464	1465	rBV	815	858	0.07%	0.009%
50	10.055	1465	1471	1472	rBV	659694	884227	74.14%	9.547%
51	10.281	1505	1508	1510	rBV2	538	814	0.07%	0.009%
52	10.458	1536	1537	1541	rBV2	382	447	0.04%	0.005%
53	10.561	1553	1554	1556	rVB	812	549	0.05%	0.006%
54	10.610	1560	1562	1563	rVV	553	350	0.03%	0.004%
55	10.634	1563	1566	1567	rVV	421	373	0.03%	0.004%
56	10.714	1577	1579	1583	rBV	861	1108	0.09%	0.012%
57	10.793	1590	1592	1595	rBV	421	406	0.03%	0.004%
58	10.909	1610	1611	1614	rBV	682	668	0.06%	0.007%
59	10.933	1614	1615	1617	rVV	529	315	0.03%	0.003%
60	11.086	1637	1640	1645	rBV4	1073	1898	0.16%	0.020%
61	11.189	1649	1657	1667	rBV	438099	561930	47.11%	6.067%
62	11.256	1667	1668	1669	rVB	966	354	0.03%	0.004%
63	11.275	1669	1671	1672	rBV	811	646	0.05%	0.007%
64	11.366	1684	1686	1687	rVV	790	572	0.05%	0.006%
65	11.396	1690	1691	1693	rBV2	847	536	0.04%	0.006%
66	11.506	1706	1709	1711	rVB2	948	1014	0.09%	0.011%
67	11.531	1711	1713	1714	rBV2	641	478	0.04%	0.005%
68	11.543	1714	1715	1719	rVV2	639	763	0.06%	0.008%
69	11.573	1719	1720	1722	rBV	653	418	0.04%	0.005%
70	11.744	1745	1748	1751	rBV	620	874	0.07%	0.009%
71	11.848	1763	1765	1769	rVB2	601	710	0.06%	0.008%
72	11.896	1769	1773	1774	rBV	788	953	0.08%	0.010%
73	11.970	1779	1785	1789	rBV	49310	64293	5.39%	0.694%
74	12.024	1789	1794	1803	rVB2	647370	1003108	84.10%	10.831%
75	12.207	1822	1824	1826	rBV2	522	441	0.04%	0.005%
76	12.317	1837	1842	1850	rBV	615485	794674	66.63%	8.580%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039134.D
 Acq On : 11 Dec 2023 11:33
 Operator : JC/MD
 Sample : 05646-11 40X
 Misc : 3.70g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.634	1893	1894	1896	rBV	740	524	0.04%	0.006%
78	12.811	1921	1923	1924	rBV	608	417	0.03%	0.005%
79	12.823	1924	1925	1927	rBV	653	521	0.04%	0.006%
80	12.994	1952	1953	1957	rVB	711	407	0.03%	0.004%
81	13.225	1989	1991	1993	rBV	382	328	0.03%	0.004%
82	13.360	2011	2013	2014	rBV	822	386	0.03%	0.004%
83	13.597	2048	2052	2054	rVV3	1888	2309	0.19%	0.025%
84	13.713	2069	2071	2072	rBV	603	418	0.04%	0.005%
85	13.744	2074	2076	2078	rBV	719	776	0.07%	0.008%
86	13.969	2109	2113	2116	rBV3	1084	1838	0.15%	0.020%
87	14.000	2116	2118	2119	rVB2	810	506	0.04%	0.005%
88	14.048	2125	2126	2127	rBV	671	479	0.04%	0.005%
89	14.225	2154	2155	2157	rBV	474	399	0.03%	0.004%
90	14.365	2176	2178	2180	rBV	636	460	0.04%	0.005%
91	14.658	2224	2226	2229	rBV2	790	1078	0.09%	0.012%
92	14.847	2255	2257	2262	rBV3	928	990	0.08%	0.011%
93	15.006	2281	2283	2286	rVB	1024	951	0.08%	0.010%
94	15.048	2286	2290	2291	rBV2	813	1089	0.09%	0.012%
95	15.164	2307	2309	2312	rBV2	661	636	0.05%	0.007%
96	15.280	2326	2328	2329	rBV	660	397	0.03%	0.004%
97	16.042	2451	2453	2455	rVB	867	457	0.04%	0.005%
98	16.542	2533	2535	2537	rVB	841	567	0.05%	0.006%
99	16.713	2562	2563	2566	rVB	1052	775	0.06%	0.008%
100	16.761	2570	2571	2574	rBV	736	639	0.05%	0.007%




Sum of corrected areas: 9261812

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039134.D
Acq On : 11 Dec 2023 11:33
Operator : JC/MD
Sample : 05646-11 40X
Misc : 3.70g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

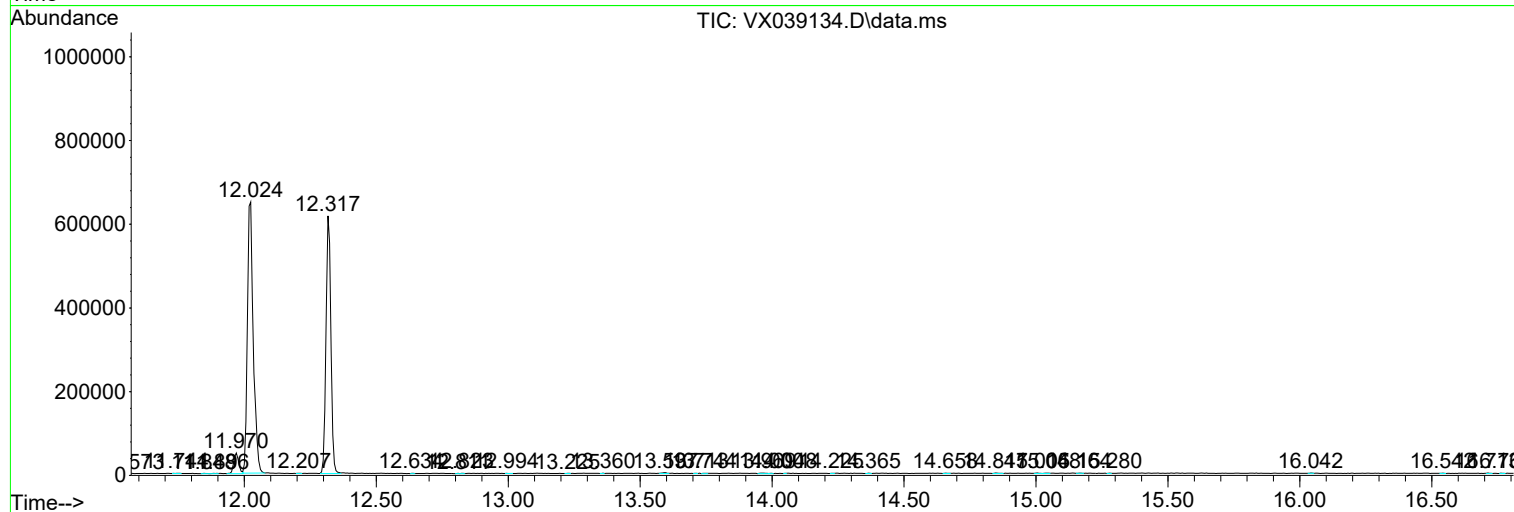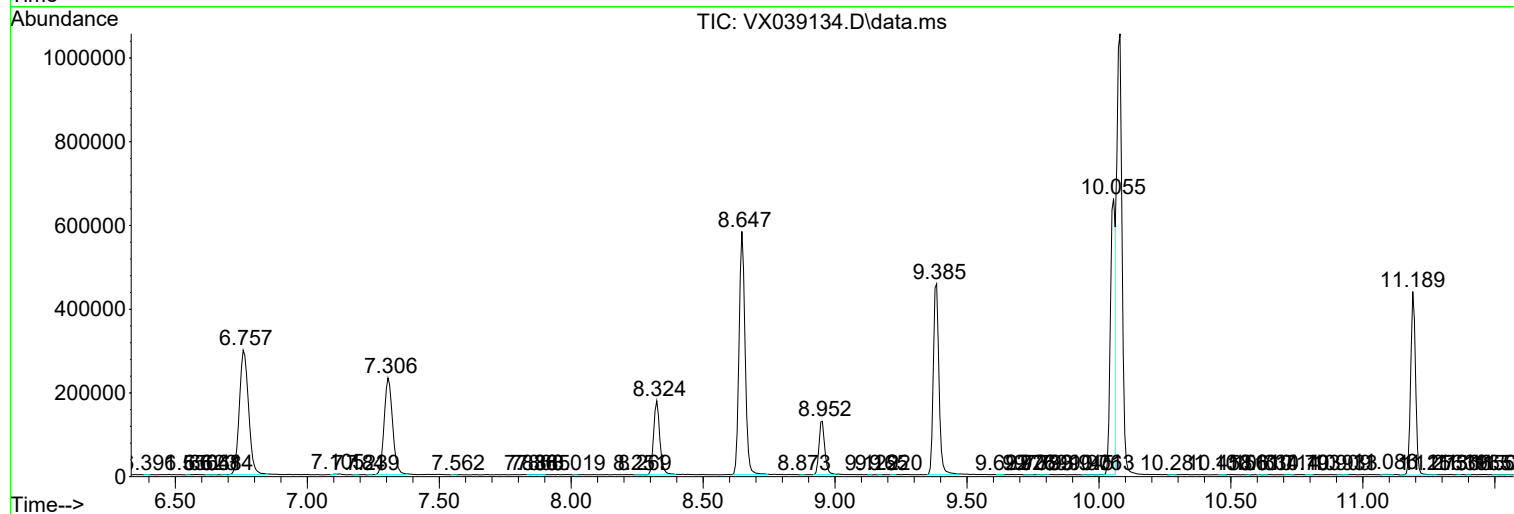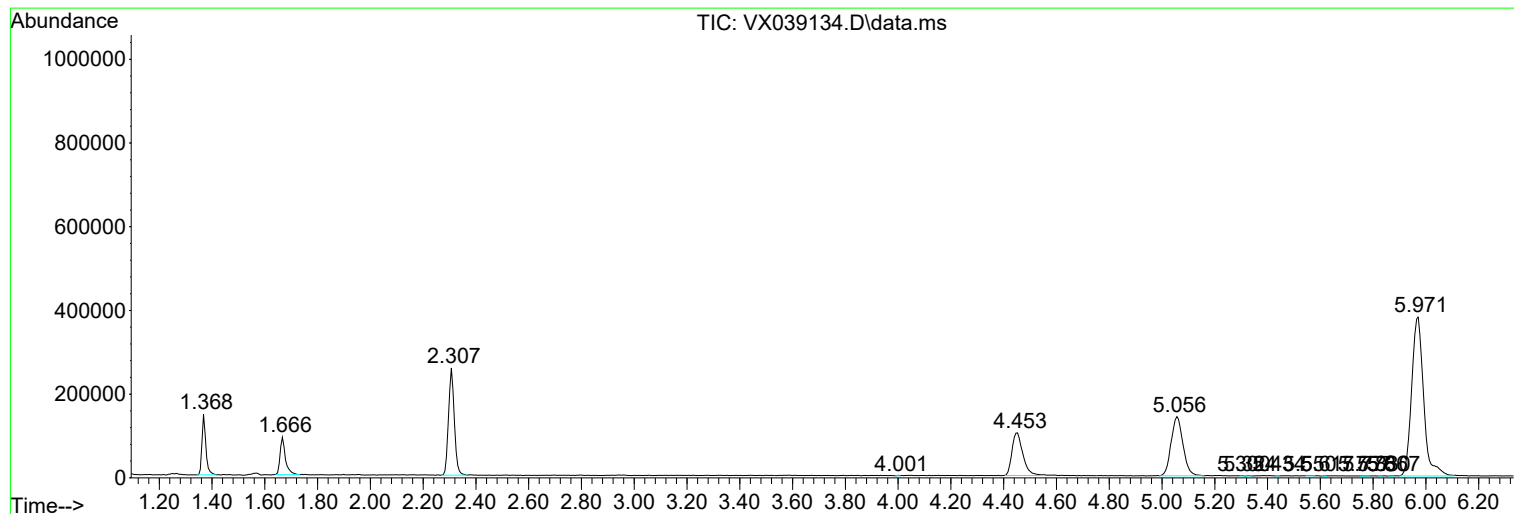

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039134.D
Acq On : 11 Dec 2023 11:33
Operator : JC/MD
Sample : 05646-11 40X
Misc : 3.70g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039134.D
Acq On : 11 Dec 2023 11:33
Operator : JC/MD
Sample : 05646-11 40X
Misc : 3.70g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc