

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039139.D
 Acq On : 11 Dec 2023 13:28
 Operator : JC/MD
 Sample : 05646-13MEDL 200X
 Misc : 0.90g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COAS0MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M

Title : VOC Analysis

Signal : TIC: VX039139.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	58	rVB	143325	147310	9.44%	1.387%
2	1.666	91	95	106	rBV	94436	131632	8.44%	1.239%
3	2.307	194	200	213	rVB	243587	378070	24.23%	3.558%
4	2.782	275	278	282	rBV4	809	1656	0.11%	0.016%
5	2.886	294	295	298	rBV	436	311	0.02%	0.003%
6	2.947	298	305	312	rVV4	2129	5337	0.34%	0.050%
7	3.099	329	330	332	rVB	605	277	0.02%	0.003%
8	3.184	341	344	346	rVB	447	438	0.03%	0.004%
9	3.203	346	347	349	rBV2	360	337	0.02%	0.003%
10	3.270	357	358	360	rBV	354	293	0.02%	0.003%
11	3.666	419	423	424	rBV2	555	646	0.04%	0.006%
12	3.733	432	434	437	rVB	343	279	0.02%	0.003%
13	3.983	473	475	476	rBV	537	398	0.03%	0.004%
14	4.038	481	484	486	rVV2	338	407	0.03%	0.004%
15	4.446	542	551	568	rBV	104909	305158	19.55%	2.872%
16	4.721	595	596	599	rVB	572	305	0.02%	0.003%
17	4.782	604	606	608	rVB2	495	337	0.02%	0.003%
18	4.891	622	624	627	rBV2	335	412	0.03%	0.004%
19	5.056	638	651	669	rBV2	140674	449784	28.82%	4.233%
20	5.178	669	671	673	rVB	458	303	0.02%	0.003%
21	5.373	701	703	704	rBV	573	590	0.04%	0.006%
22	5.550	729	732	733	rBV3	673	572	0.04%	0.005%
23	5.721	759	760	763	rBV2	522	437	0.03%	0.004%
24	5.970	788	801	811	rBV2	379999	1168677	74.89%	11.000%
25	6.214	839	841	843	rBV	574	401	0.03%	0.004%
26	6.312	856	857	859	rBV	418	327	0.02%	0.003%
27	6.556	894	897	899	rBV2	453	488	0.03%	0.005%
28	6.617	905	907	909	rBV2	489	428	0.03%	0.004%
29	6.641	909	911	914	rVB	364	298	0.02%	0.003%
30	6.690	918	919	921	rBV	372	275	0.02%	0.003%
31	6.757	921	930	948	rBV	284168	700167	44.87%	6.590%
32	7.111	984	988	996	rVB4	2290	4505	0.29%	0.042%
33	7.172	996	998	1002	rBV	507	445	0.03%	0.004%
34	7.306	1012	1020	1037	rBV	232787	516826	33.12%	4.864%
35	7.574	1062	1064	1067	rVB	403	315	0.02%	0.003%
36	7.610	1067	1070	1071	rBV2	309	338	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039139.D
 Acq On : 11 Dec 2023 13:28
 Operator : JC/MD
 Sample : 05646-13MEDL 200X
 Misc : 0.90g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COAS0MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.757	1093	1094	1096	rVB2	413	299	0.02%	0.003%
38	7.781	1096	1098	1099	rVB	576	411	0.03%	0.004%
39	7.927	1119	1122	1124	rBV	561	533	0.03%	0.005%
40	8.104	1148	1151	1154	rVB	418	436	0.03%	0.004%
41	8.165	1158	1161	1162	rBV2	442	402	0.03%	0.004%
42	8.324	1181	1187	1202	rBV	170816	285841	18.32%	2.690%
43	8.482	1211	1213	1214	rBV	400	305	0.02%	0.003%
44	8.574	1227	1228	1233	rVB2	417	451	0.03%	0.004%
45	8.647	1233	1240	1257	rBV	584649	923768	59.20%	8.695%
46	8.891	1278	1280	1282	rBV2	413	314	0.02%	0.003%
47	8.946	1284	1289	1299	rBV	123753	192082	12.31%	1.808%
48	9.275	1341	1343	1346	rVB	515	630	0.04%	0.006%
49	9.385	1355	1361	1375	rBV	475656	693922	44.47%	6.531%
50	9.702	1409	1413	1417	rVB3	1398	2159	0.14%	0.020%
51	9.769	1423	1424	1429	rBV2	329	369	0.02%	0.003%
52	9.805	1429	1430	1435	rVB2	413	433	0.03%	0.004%
53	9.848	1435	1437	1439	rBV	536	605	0.04%	0.006%
54	9.994	1459	1461	1463	rVB2	428	316	0.02%	0.003%
55	10.055	1465	1471	1473	rBV	623981	944336	60.51%	8.888%
56	10.439	1532	1534	1536	rVB	555	392	0.03%	0.004%
57	10.476	1538	1540	1541	rVV	360	273	0.02%	0.003%
58	10.799	1590	1593	1595	rBV2	324	394	0.03%	0.004%
59	10.903	1608	1610	1612	rBV	465	447	0.03%	0.004%
60	11.018	1627	1629	1632	rBV	335	346	0.02%	0.003%
61	11.092	1638	1641	1649	rVB3	1452	2033	0.13%	0.019%
62	11.189	1652	1657	1667	rVB	447807	555287	35.58%	5.226%
63	11.366	1683	1686	1690	rVB4	1365	1703	0.11%	0.016%
64	11.402	1690	1692	1696	rVB	483	586	0.04%	0.006%
65	11.433	1696	1697	1700	rBV	559	424	0.03%	0.004%
66	11.457	1700	1701	1704	rVB2	440	362	0.02%	0.003%
67	11.512	1708	1710	1712	rBV	532	491	0.03%	0.005%
68	11.707	1741	1742	1744	rBV	490	306	0.02%	0.003%
69	11.969	1780	1785	1788	rBV	22132	27689	1.77%	0.261%
70	12.024	1788	1794	1804	rVB2	703802	1560541	100.00%	14.688%
71	12.207	1823	1824	1825	rBV	484	271	0.02%	0.003%
72	12.317	1837	1842	1854	rBV	616233	854294	54.74%	8.041%
73	12.549	1878	1880	1885	rBV2	323	565	0.04%	0.005%
74	12.585	1885	1886	1890	rBV2	331	288	0.02%	0.003%
75	12.713	1905	1907	1909	rVB2	368	322	0.02%	0.003%
76	12.829	1924	1926	1928	rVB	515	296	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039139.D
 Acq On : 11 Dec 2023 13:28
 Operator : JC/MD
 Sample : 05646-13MEDL 200X
 Misc : 0.90g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AS0MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.902	1936	1938	1941	rVB2	505	522	0.03%	0.005%
78	12.927	1941	1942	1945	rBV	429	533	0.03%	0.005%
79	13.061	1959	1964	1970	rVB4	6030	11778	0.75%	0.111%
80	13.116	1970	1973	1978	rVB3	957	1314	0.08%	0.012%
81	13.177	1981	1983	1985	rBV	278	270	0.02%	0.003%
82	13.390	2015	2018	2020	rVB2	628	741	0.05%	0.007%
83	13.426	2022	2024	2026	rBV	407	340	0.02%	0.003%
84	13.585	2045	2050	2062	rBV	353906	453294	29.05%	4.266%
85	13.695	2066	2068	2071	rVB	378	353	0.02%	0.003%
86	13.756	2076	2078	2080	rBV	382	413	0.03%	0.004%
87	13.957	2106	2111	2122	rBV	157689	199573	12.79%	1.878%
88	14.079	2129	2131	2134	rVB	393	346	0.02%	0.003%
89	14.237	2155	2157	2158	rBV	314	289	0.02%	0.003%
90	14.323	2170	2171	2174	rVB2	514	440	0.03%	0.004%
91	14.420	2185	2187	2189	rBV	449	431	0.03%	0.004%
92	14.457	2192	2193	2198	rVB3	633	665	0.04%	0.006%
93	14.506	2198	2201	2203	rBV2	492	630	0.04%	0.006%
94	14.627	2218	2221	2224	rBV3	769	993	0.06%	0.009%
95	14.780	2240	2246	2253	rVB3	9205	16330	1.05%	0.154%
96	15.249	2318	2323	2329	rVB	41965	59922	3.84%	0.564%
97	15.804	2412	2414	2417	rBV2	542	511	0.03%	0.005%
98	15.957	2438	2439	2441	rBV	697	340	0.02%	0.003%
99	16.066	2455	2457	2459	rVB	701	497	0.03%	0.005%
100	16.725	2563	2565	2567	rBV2	422	297	0.02%	0.003%


Sum of corrected areas: 10624523

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039139.D
Acq On : 11 Dec 2023 13:28
Operator : JC/MD
Sample : 05646-13MEDL 200X
Misc : 0.90g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS0MEDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

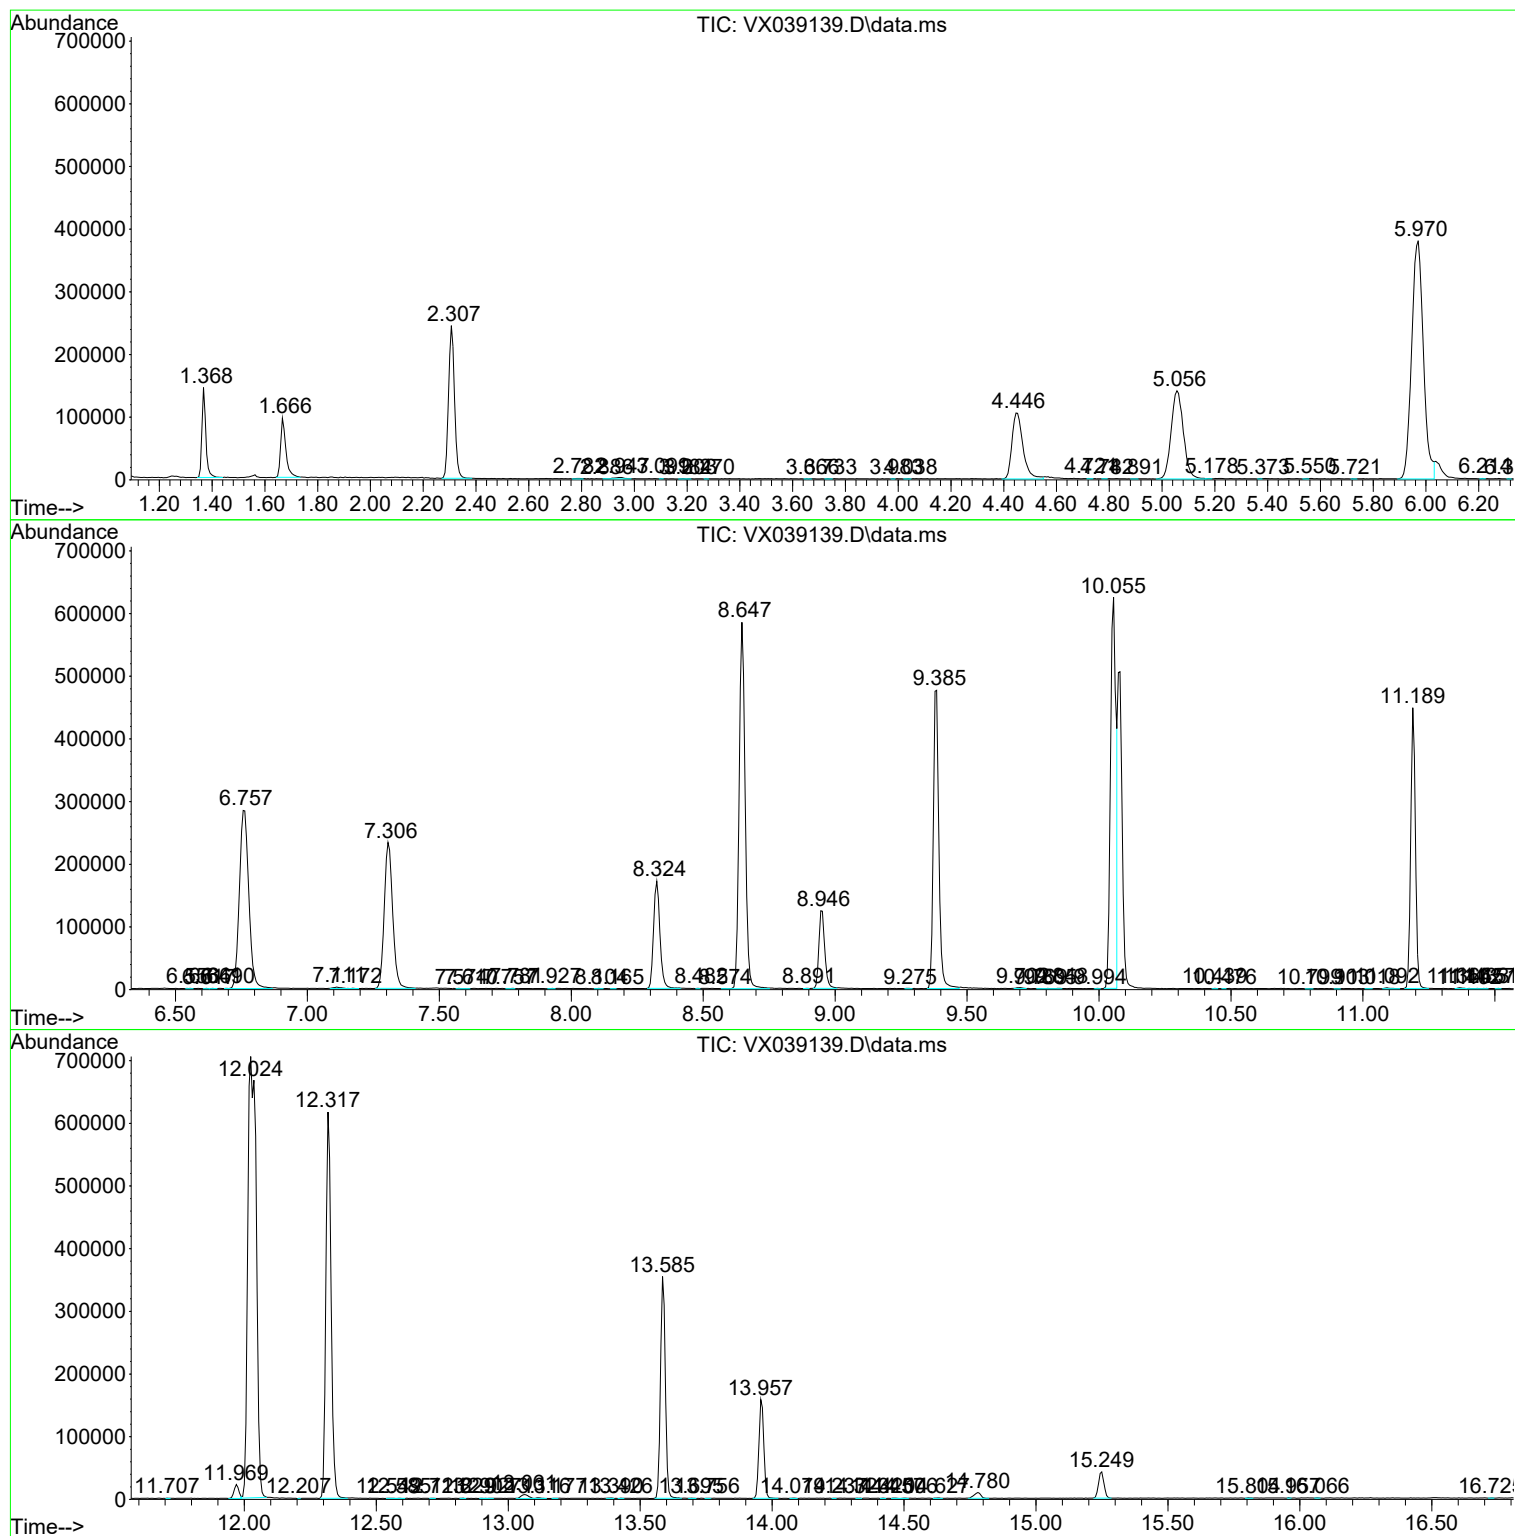

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039139.D
Acq On : 11 Dec 2023 13:28
Operator : JC/MD
Sample : 05646-13MEDL 200X
Misc : 0.90g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS0MEDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039139.D
Acq On : 11 Dec 2023 13:28
Operator : JC/MD
Sample : 05646-13MEDL 200X
Misc : 0.90g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS0MEDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc