

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039141.D
 Acq On : 11 Dec 2023 14:13
 Operator : JC/MD
 Sample : VIBLK625
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK625

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039141.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	56	rVB	135088	142234	12.76%	1.668%
2	1.672	91	96	105	rBV	87229	127443	11.43%	1.495%
3	2.306	194	200	214	rVB	236404	367128	32.93%	4.306%
4	4.452	543	552	578	rBV	99761	294850	26.45%	3.458%
5	5.056	640	651	668	rVB2	137224	427926	38.39%	5.019%
6	5.842	778	780	781	rBV	644	396	0.04%	0.005%
7	5.964	787	800	821	rBV2	363851	1114753	100.00%	13.075%
8	6.757	922	930	944	rBV	267847	649790	58.29%	7.622%
9	7.116	984	989	996	rVB3	1856	4712	0.42%	0.055%
10	7.171	996	998	999	rBV	377	256	0.02%	0.003%
11	7.220	1005	1006	1010	rVB2	532	389	0.03%	0.005%
12	7.305	1012	1020	1035	rVV	224445	500831	44.93%	5.874%
13	7.592	1065	1067	1068	rBV2	368	320	0.03%	0.004%
14	7.671	1079	1080	1083	rBV	378	193	0.02%	0.002%
15	7.775	1095	1097	1100	rBV2	427	448	0.04%	0.005%
16	7.799	1100	1101	1102	rVB	376	140	0.01%	0.002%
17	7.842	1106	1108	1110	rBV2	291	252	0.02%	0.003%
18	7.964	1127	1128	1130	rBV	598	310	0.03%	0.004%
19	8.104	1149	1151	1154	rBV	350	353	0.03%	0.004%
20	8.324	1181	1187	1200	rBV	165775	278819	25.01%	3.270%
21	8.647	1234	1240	1257	rBV	558443	876126	78.59%	10.276%
22	8.945	1284	1289	1301	rBV	120116	187254	16.80%	2.196%
23	9.269	1340	1342	1346	rBV2	370	626	0.06%	0.007%
24	9.378	1355	1360	1386	rBV	446457	669664	60.07%	7.855%
25	9.695	1407	1412	1417	rBV4	1070	1756	0.16%	0.021%
26	9.848	1435	1437	1438	rBV	261	205	0.02%	0.002%
27	9.903	1445	1446	1448	rBV	339	242	0.02%	0.003%
28	10.055	1465	1471	1490	rBV	558697	790201	70.89%	9.269%
29	10.409	1528	1529	1531	rBV	186	103	0.01%	0.001%
30	10.555	1552	1553	1555	rBV	253	191	0.02%	0.002%
31	10.866	1603	1604	1606	rBV	248	222	0.02%	0.003%
32	11.049	1633	1634	1636	rVB	347	196	0.02%	0.002%
33	11.091	1638	1641	1647	rBV2	1140	1452	0.13%	0.017%
34	11.189	1652	1657	1670	rVV	431821	543498	48.76%	6.375%
35	11.293	1672	1674	1675	rBV2	249	135	0.01%	0.002%
36	11.372	1685	1687	1689	rBV	225	231	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039141.D
 Acq On : 11 Dec 2023 14:13
 Operator : JC/MD
 Sample : VIBLK625
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK625

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	11.512	1709	1710	1711	rBV	282	116	0.01%	0.001%
38	11.567	1717	1719	1721	rBV2	181	207	0.02%	0.002%
39	11.610	1724	1726	1728	rBV	193	177	0.02%	0.002%
40	11.835	1761	1763	1766	rVB2	201	204	0.02%	0.002%
41	11.866	1766	1768	1771	rBV2	199	204	0.02%	0.002%
42	11.963	1783	1784	1788	rVB2	480	496	0.04%	0.006%
43	12.018	1788	1793	1803	rBV	565915	761473	68.31%	8.932%
44	12.317	1837	1842	1851	rBV	584209	758488	68.04%	8.897%
45	12.542	1878	1879	1882	rVB	199	141	0.01%	0.002%
46	12.737	1909	1911	1912	rBV2	203	209	0.02%	0.002%
47	12.811	1921	1923	1924	rBV	232	201	0.02%	0.002%
48	12.865	1929	1932	1936	rVB2	363	620	0.06%	0.007%
49	12.896	1936	1937	1939	rVB	314	199	0.02%	0.002%
50	12.932	1939	1943	1944	rBV2	330	413	0.04%	0.005%
51	12.993	1950	1953	1955	rBV2	187	229	0.02%	0.003%
52	13.030	1957	1959	1961	rVV	401	255	0.02%	0.003%
53	13.048	1961	1962	1963	rVV	187	116	0.01%	0.001%
54	13.091	1967	1969	1970	rVB2	176	103	0.01%	0.001%
55	13.140	1975	1977	1979	rBV	133	153	0.01%	0.002%
56	13.170	1979	1982	1983	rVV	195	170	0.02%	0.002%
57	13.207	1986	1988	1989	rBV2	270	202	0.02%	0.002%
58	13.274	1996	1999	2001	rVB2	317	336	0.03%	0.004%
59	13.304	2003	2004	2005	rVV	222	88	0.01%	0.001%
60	13.323	2005	2007	2008	rVV	133	105	0.01%	0.001%
61	13.536	2040	2042	2045	rVV2	200	217	0.02%	0.003%
62	13.591	2046	2051	2057	rVV3	4479	6281	0.56%	0.074%
63	13.652	2059	2061	2064	rVB2	249	259	0.02%	0.003%
64	13.688	2064	2067	2068	rVB	171	116	0.01%	0.001%
65	13.786	2080	2083	2085	rBV2	268	308	0.03%	0.004%
66	13.810	2085	2087	2092	rVB	215	225	0.02%	0.003%
67	13.865	2094	2096	2098	rBV2	272	276	0.02%	0.003%
68	13.896	2098	2101	2103	rBV	233	253	0.02%	0.003%
69	13.920	2103	2105	2106	rVB2	161	81	0.01%	0.001%
70	13.963	2106	2112	2117	rVB4	1303	1906	0.17%	0.022%
71	13.999	2117	2118	2120	rBV	189	126	0.01%	0.001%
72	14.018	2120	2121	2122	rBV	157	87	0.01%	0.001%
73	14.060	2127	2128	2129	rBV	298	134	0.01%	0.002%
74	14.091	2129	2133	2134	rVB3	230	263	0.02%	0.003%
75	14.109	2134	2136	2137	rBV	317	280	0.03%	0.003%
76	14.164	2144	2145	2149	rBV	225	289	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039141.D
 Acq On : 11 Dec 2023 14:13
 Operator : JC/MD
 Sample : VIBLK625
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK625

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	14.194	2149	2150	2151	rBV	166	112	0.01%	0.001%
78	14.249	2158	2159	2162	rVB2	247	227	0.02%	0.003%
79	14.280	2162	2164	2165	rBV2	205	128	0.01%	0.002%
80	14.329	2170	2172	2173	rVB	258	138	0.01%	0.002%
81	14.432	2187	2189	2190	rVB2	189	135	0.01%	0.002%
82	14.457	2191	2193	2194	rVB	281	154	0.01%	0.002%
83	14.475	2194	2196	2197	rBV	402	281	0.03%	0.003%
84	14.761	2241	2243	2245	rVB	343	195	0.02%	0.002%
85	14.957	2273	2275	2277	rVB2	408	235	0.02%	0.003%
86	15.078	2294	2295	2297	rBV2	377	287	0.03%	0.003%
87	15.225	2317	2319	2321	rBV2	264	229	0.02%	0.003%
88	15.249	2321	2323	2328	rVV4	563	708	0.06%	0.008%
89	15.286	2328	2329	2331	rVB	434	229	0.02%	0.003%
90	15.310	2331	2333	2335	rBV2	432	378	0.03%	0.004%
91	15.444	2353	2355	2356	rBV2	405	249	0.02%	0.003%
92	15.505	2364	2365	2368	rBV2	300	225	0.02%	0.003%
93	15.658	2388	2390	2391	rVB	386	193	0.02%	0.002%
94	15.688	2393	2395	2396	rBV	327	216	0.02%	0.003%
95	15.859	2421	2423	2425	rBV2	353	297	0.03%	0.003%
96	15.908	2430	2431	2432	rBV	282	141	0.01%	0.002%
97	16.097	2461	2462	2463	rBV	602	288	0.03%	0.003%
98	16.176	2473	2475	2476	rBV	385	265	0.02%	0.003%
99	16.212	2479	2481	2482	rBV	351	221	0.02%	0.003%
100	16.407	2512	2513	2515	rBV2	508	382	0.03%	0.004%




Sum of corrected areas: 8525564

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039141.D
Acq On : 11 Dec 2023 14:13
Operator : JC/MD
Sample : VIBLK625
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK625

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

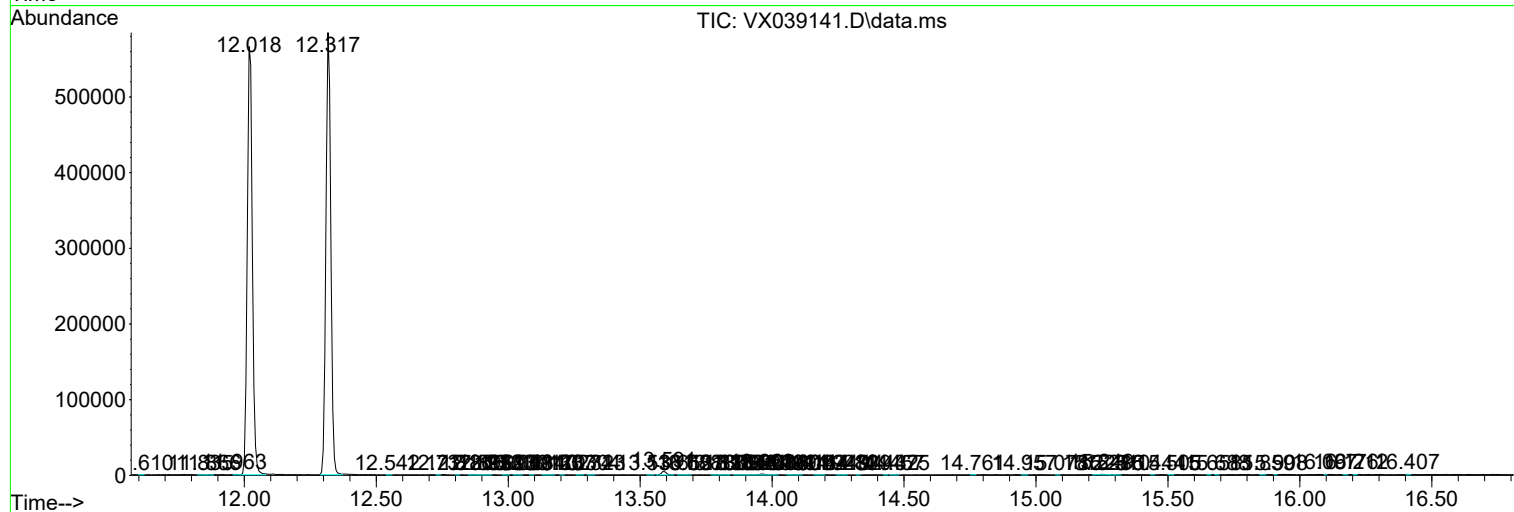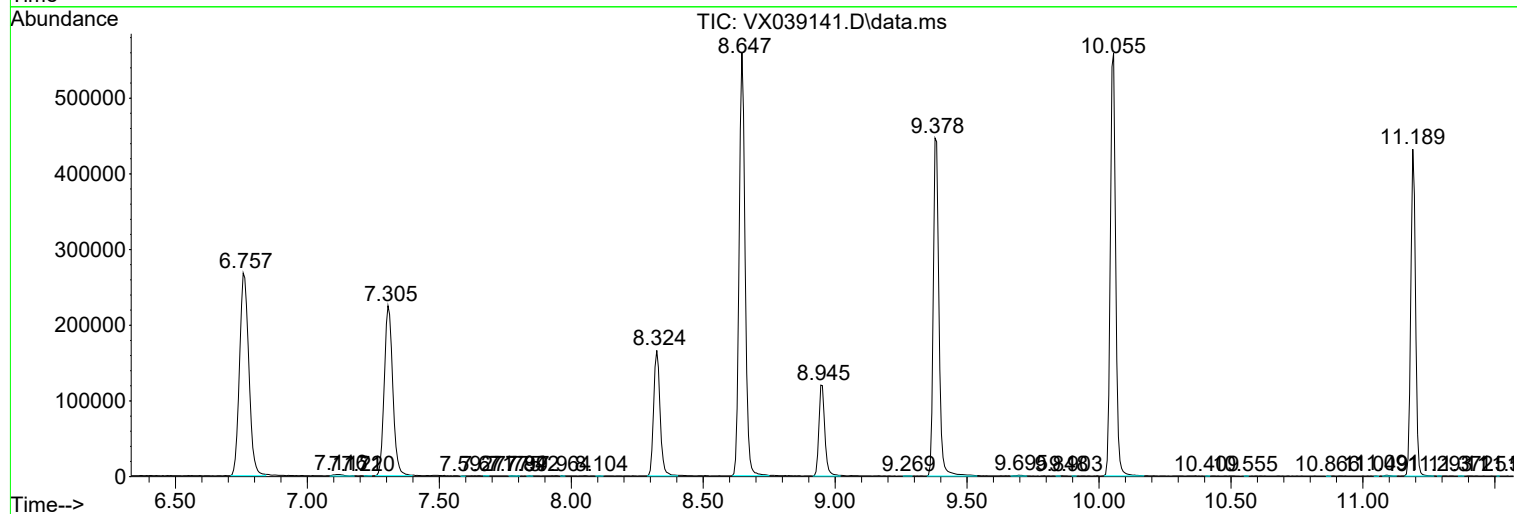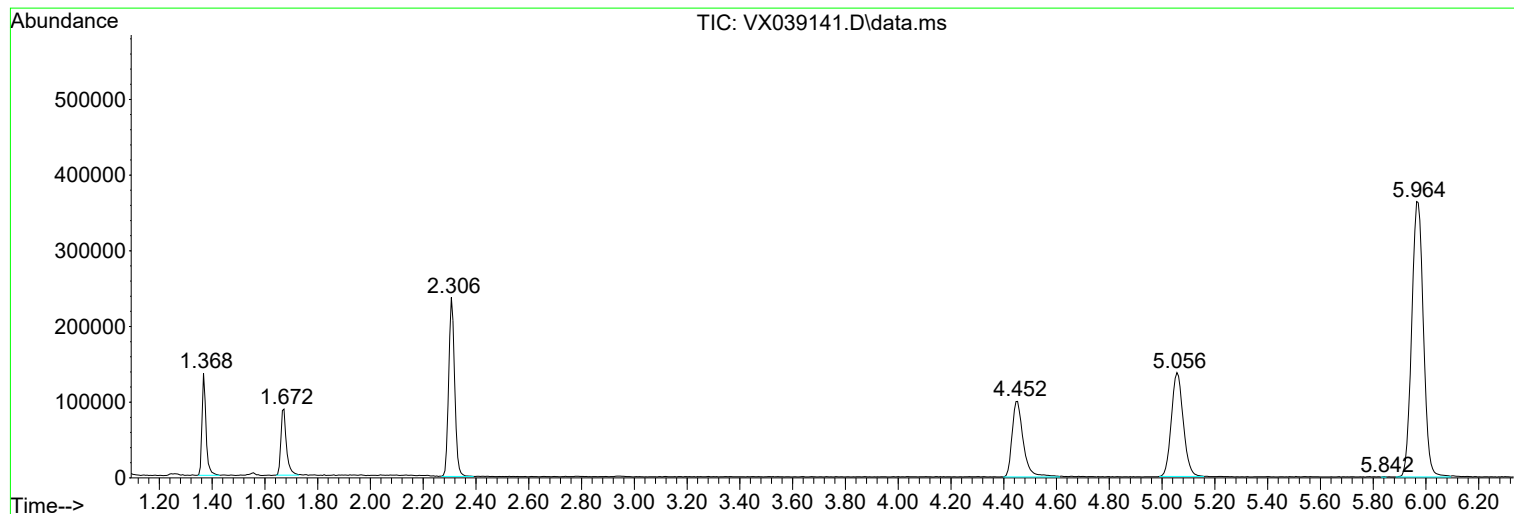

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039141.D
Acq On : 11 Dec 2023 14:13
Operator : JC/MD
Sample : VIBLK625
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK625

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039141.D
Acq On : 11 Dec 2023 14:13
Operator : JC/MD
Sample : VIBLK625
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK625

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc