

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039142.D
 Acq On : 11 Dec 2023 14:36
 Operator : JC/MD
 Sample : 05646-15DL 400X
 Misc : 1.75g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AS2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039142.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rBV	137785	144962	7.00%	1.298%
2	1.538	72	74	75	rBV	2058	1577	0.08%	0.014%
3	1.666	91	95	110	rBV	89217	129844	6.27%	1.163%
4	2.306	194	200	212	rVB	244068	378913	18.29%	3.394%
5	2.630	252	253	254	rBV	497	221	0.01%	0.002%
6	2.837	285	287	290	rBV	396	289	0.01%	0.003%
7	3.416	380	382	385	rBV	474	426	0.02%	0.004%
8	3.928	464	466	469	rBV	369	373	0.02%	0.003%
9	4.446	544	551	567	rBV	100121	290096	14.00%	2.598%
10	5.056	639	651	668	rBV	140038	442224	21.34%	3.961%
11	5.970	789	801	821	rBV2	369987	1137732	54.91%	10.190%
12	6.507	887	889	891	rBV	292	264	0.01%	0.002%
13	6.757	921	930	945	rBV	281346	675574	32.61%	6.051%
14	7.117	983	989	997	rVB4	2006	4672	0.23%	0.042%
15	7.184	999	1000	1001	rBV	359	213	0.01%	0.002%
16	7.306	1011	1020	1035	rBV	233701	515286	24.87%	4.615%
17	7.641	1074	1075	1076	rBV	421	160	0.01%	0.001%
18	7.940	1122	1124	1129	rBV2	320	594	0.03%	0.005%
19	8.104	1150	1151	1154	rBV2	388	329	0.02%	0.003%
20	8.214	1167	1169	1170	rBV	292	190	0.01%	0.002%
21	8.324	1180	1187	1201	rBV	165332	279664	13.50%	2.505%
22	8.647	1233	1240	1257	rBV	584902	905943	43.73%	8.114%
23	8.811	1265	1267	1268	rBV	473	365	0.02%	0.003%
24	8.952	1284	1290	1301	rBV	120451	189386	9.14%	1.696%
25	9.317	1348	1350	1351	rBV	276	185	0.01%	0.002%
26	9.378	1355	1360	1378	rBV	457814	671787	32.42%	6.017%
27	9.647	1401	1404	1405	rBV2	328	317	0.02%	0.003%
28	9.695	1410	1412	1419	rVB5	1112	1658	0.08%	0.015%
29	9.781	1425	1426	1429	rBV2	426	348	0.02%	0.003%
30	9.958	1453	1455	1457	rBV2	244	183	0.01%	0.002%
31	10.055	1465	1471	1486	rBV2	582844	946010	45.66%	8.473%
32	10.299	1509	1511	1513	rBV	245	152	0.01%	0.001%
33	10.464	1536	1538	1539	rBV	331	274	0.01%	0.002%
34	10.585	1555	1558	1563	rBV	314	622	0.03%	0.006%
35	10.677	1571	1573	1575	rBV	485	343	0.02%	0.003%
36	10.768	1586	1588	1589	rBV	199	154	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039142.D
 Acq On : 11 Dec 2023 14:36
 Operator : JC/MD
 Sample : 05646-15DL 400X
 Misc : 1.75g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AS2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	10.994	1624	1625	1626	rBV	362	207	0.01%	0.002%
38	11.030	1630	1631	1635	rVV2	352	387	0.02%	0.003%
39	11.091	1638	1641	1647	rVB4	900	1356	0.07%	0.012%
40	11.189	1652	1657	1667	rVB	434302	544474	26.28%	4.877%
41	11.348	1682	1683	1685	rBV	317	211	0.01%	0.002%
42	11.396	1689	1691	1692	rVV	433	234	0.01%	0.002%
43	11.463	1700	1702	1705	rVB2	321	254	0.01%	0.002%
44	11.555	1716	1717	1719	rBV	283	181	0.01%	0.002%
45	11.707	1740	1742	1743	rBV	400	283	0.01%	0.003%
46	11.835	1760	1763	1766	rBV2	218	329	0.02%	0.003%
47	11.969	1780	1785	1789	rBV	28401	37065	1.79%	0.332%
48	12.036	1789	1796	1806	rVB2	1080680	2071891	100.00%	18.558%
49	12.317	1837	1842	1854	rBV3	651786	993533	47.95%	8.899%
50	12.451	1862	1864	1869	rBV2	284	515	0.02%	0.005%
51	12.494	1869	1871	1873	rVV	418	350	0.02%	0.003%
52	12.536	1876	1878	1880	rVV	320	323	0.02%	0.003%
53	12.579	1883	1885	1887	rVB2	322	266	0.01%	0.002%
54	12.640	1893	1895	1896	rBV	251	193	0.01%	0.002%
55	12.683	1900	1902	1905	rVV	319	275	0.01%	0.002%
56	12.872	1931	1933	1936	rVV	218	200	0.01%	0.002%
57	12.994	1951	1953	1955	rBV2	255	248	0.01%	0.002%
58	13.061	1959	1964	1969	rVV4	3276	5835	0.28%	0.052%
59	13.164	1978	1981	1983	rBV2	162	217	0.01%	0.002%
60	13.201	1983	1987	1991	rVV3	783	1220	0.06%	0.011%
61	13.244	1991	1994	1997	rVV2	239	307	0.01%	0.003%
62	13.323	2006	2007	2011	rVB	258	209	0.01%	0.002%
63	13.372	2011	2015	2016	rBV2	252	298	0.01%	0.003%
64	13.384	2016	2017	2021	rVB	649	485	0.02%	0.004%
65	13.414	2021	2022	2024	rVB2	224	143	0.01%	0.001%
66	13.432	2024	2025	2026	rBV	403	175	0.01%	0.002%
67	13.475	2030	2032	2033	rBV2	294	211	0.01%	0.002%
68	13.493	2033	2035	2038	rVB2	334	256	0.01%	0.002%
69	13.542	2041	2043	2045	rBV2	222	247	0.01%	0.002%
70	13.585	2045	2050	2063	rVV	465541	583717	28.17%	5.228%
71	13.707	2067	2070	2072	rBV2	218	289	0.01%	0.003%
72	13.786	2082	2083	2085	rVB	415	274	0.01%	0.002%
73	13.871	2094	2097	2100	rBV2	260	353	0.02%	0.003%
74	13.957	2106	2111	2121	rVB	139017	173250	8.36%	1.552%
75	14.067	2127	2129	2130	rVB2	292	169	0.01%	0.002%
76	14.085	2130	2132	2133	rBV	231	140	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039142.D
 Acq On : 11 Dec 2023 14:36
 Operator : JC/MD
 Sample : 05646-15DL 400X
 Misc : 1.75g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AS2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	14.121	2136	2138	2142	rBV3	475	671	0.03%	0.006%
78	14.237	2156	2157	2159	rBV	307	288	0.01%	0.003%
79	14.353	2173	2176	2177	rBV	393	469	0.02%	0.004%
80	14.414	2184	2186	2187	rBV2	318	163	0.01%	0.001%
81	14.451	2191	2192	2195	rVB	265	185	0.01%	0.002%
82	14.475	2195	2196	2198	rBV	364	203	0.01%	0.002%
83	14.566	2208	2211	2212	rBV2	214	265	0.01%	0.002%
84	14.603	2215	2217	2220	rVB2	272	297	0.01%	0.003%
85	14.633	2220	2222	2223	rBV	250	235	0.01%	0.002%
86	14.670	2226	2228	2231	rVB2	391	290	0.01%	0.003%
87	14.780	2243	2246	2250	rVB3	1439	1770	0.09%	0.016%
88	14.896	2263	2265	2268	rVB2	334	270	0.01%	0.002%
89	15.103	2297	2299	2302	rBV2	272	253	0.01%	0.002%
90	15.213	2311	2317	2318	rBV2	555	827	0.04%	0.007%
91	15.249	2318	2323	2327	rVV2	10612	13922	0.67%	0.125%
92	15.499	2362	2364	2365	rBV2	291	163	0.01%	0.001%
93	15.597	2378	2380	2381	rVB	347	156	0.01%	0.001%
94	15.835	2418	2419	2423	rVB2	398	258	0.01%	0.002%
95	16.017	2446	2449	2451	rBV2	386	505	0.02%	0.005%
96	16.225	2481	2483	2488	rBV4	317	449	0.02%	0.004%
97	16.292	2492	2494	2495	rBV	274	197	0.01%	0.002%
98	16.499	2526	2528	2529	rBV2	486	292	0.01%	0.003%
99	16.548	2533	2536	2538	rBV2	384	389	0.02%	0.003%
100	16.767	2570	2572	2573	rBV	384	240	0.01%	0.002%




Sum of corrected areas: 11164657

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039142.D
Acq On : 11 Dec 2023 14:36
Operator : JC/MD
Sample : 05646-15DL 400X
Misc : 1.75g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

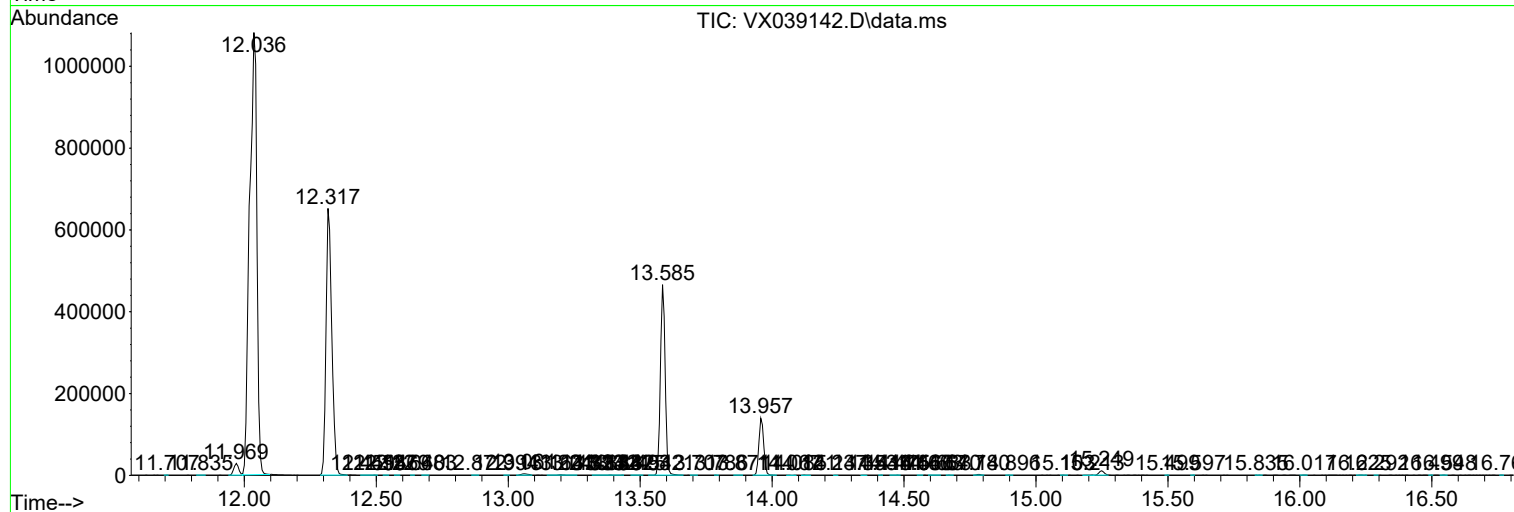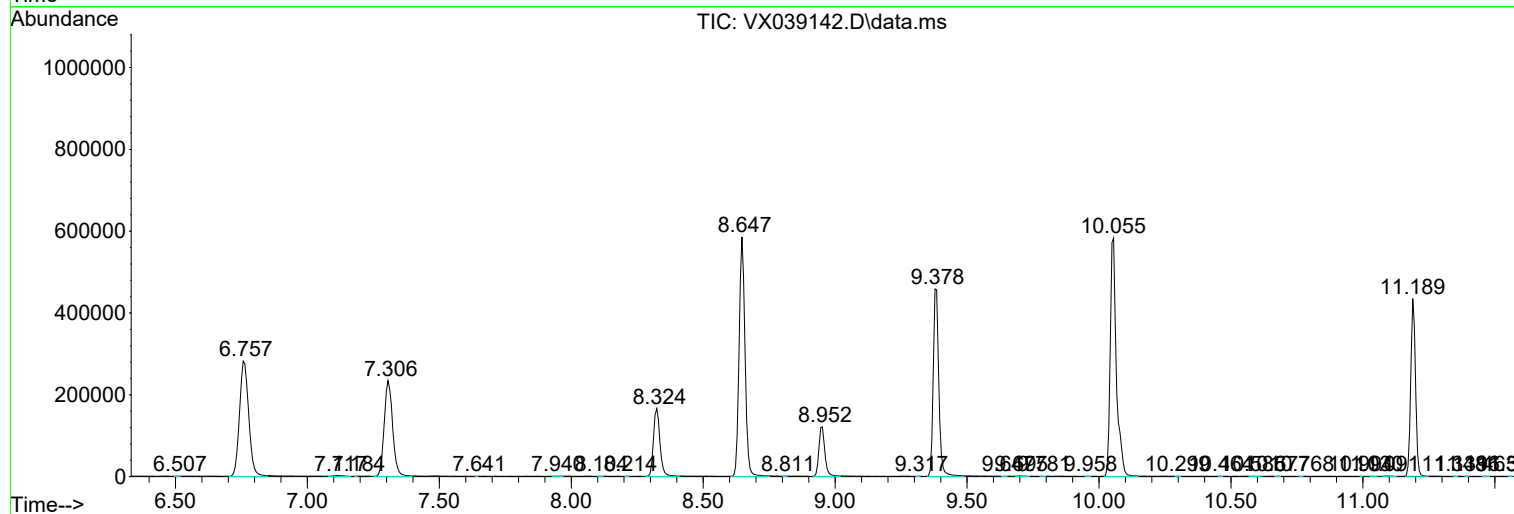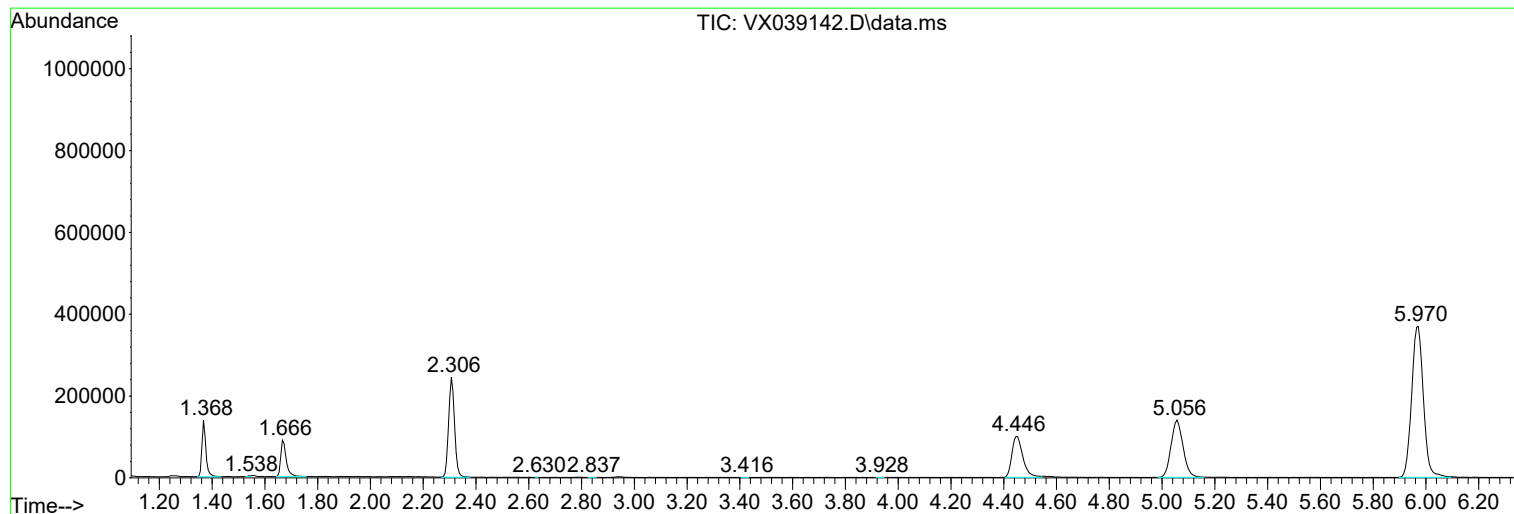

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039142.D
Acq On : 11 Dec 2023 14:36
Operator : JC/MD
Sample : 05646-15DL 400X
Misc : 1.75g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039142.D
Acq On : 11 Dec 2023 14:36
Operator : JC/MD
Sample : 05646-15DL 400X
Misc : 1.75g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------