

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039145.D
 Acq On : 11 Dec 2023 15:45
 Operator : JC/MD
 Sample : 05646-18DL 200X
 Misc : 2.88g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AS5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M

Title : VOC Analysis

Signal : TIC: VX039145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	32	rBV3	2813	6078	0.35%	0.057%
2	1.368	43	46	57	rVB	131673	138730	7.90%	1.308%
3	1.666	91	95	111	rBV	82547	126227	7.19%	1.190%
4	2.307	194	200	215	rVB	233908	363797	20.73%	3.430%
5	2.788	274	279	286	rBV3	838	1547	0.09%	0.015%
6	2.953	298	306	314	rBV2	1603	3958	0.23%	0.037%
7	3.087	327	328	331	rBV	250	248	0.01%	0.002%
8	3.520	396	399	400	rBV2	235	250	0.01%	0.002%
9	3.581	407	409	412	rVB	257	216	0.01%	0.002%
10	3.666	419	423	424	rBV	281	217	0.01%	0.002%
11	3.684	424	426	428	rBV2	225	221	0.01%	0.002%
12	3.800	441	445	450	rBV2	180	413	0.02%	0.004%
13	3.843	450	452	455	rBV	189	223	0.01%	0.002%
14	3.898	459	461	464	rBV	188	217	0.01%	0.002%
15	3.940	464	468	470	rBV2	264	276	0.02%	0.003%
16	3.995	474	477	478	rBV	312	340	0.02%	0.003%
17	4.062	485	488	490	rBV	313	281	0.02%	0.003%
18	4.117	493	497	500	rVB2	186	350	0.02%	0.003%
19	4.263	519	521	524	rVB2	305	337	0.02%	0.003%
20	4.294	524	526	529	rBV2	253	354	0.02%	0.003%
21	4.331	529	532	533	rVB	303	281	0.02%	0.003%
22	4.446	543	551	567	rBV	99945	284787	16.23%	2.685%
23	5.056	636	651	670	rVV	136281	433521	24.70%	4.087%
24	5.379	702	704	709	rBV2	336	521	0.03%	0.005%
25	5.568	733	735	738	rVB2	346	361	0.02%	0.003%
26	5.611	738	742	745	rBV2	191	340	0.02%	0.003%
27	5.653	747	749	753	rVB2	318	351	0.02%	0.003%
28	5.721	756	760	761	rBV	196	245	0.01%	0.002%
29	5.763	764	767	770	rBV2	217	295	0.02%	0.003%
30	5.794	770	772	776	rBV	161	227	0.01%	0.002%
31	5.873	783	785	787	rBV	301	241	0.01%	0.002%
32	5.970	788	801	824	rVV2	363910	1115415	63.55%	10.515%
33	6.464	879	882	883	rBV2	328	285	0.02%	0.003%
34	6.757	921	930	950	rVV	273276	656337	37.39%	6.187%
35	7.117	984	989	995	rVB5	1929	3863	0.22%	0.036%
36	7.220	1002	1006	1008	rBV2	184	225	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039145.D
 Acq On : 11 Dec 2023 15:45
 Operator : JC/MD
 Sample : 05646-18DL 200X
 Misc : 2.88g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AS5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.306	1011	1020	1037	rBV	228468	504224	28.73%	4.753%
38	7.610	1067	1070	1072	rVB2	239	267	0.02%	0.003%
39	7.641	1072	1075	1078	rBV2	158	216	0.01%	0.002%
40	7.848	1107	1109	1112	rVB	401	255	0.01%	0.002%
41	7.879	1112	1114	1117	rBV2	357	442	0.03%	0.004%
42	7.940	1121	1124	1125	rBV	387	290	0.02%	0.003%
43	8.324	1180	1187	1200	rBV	169473	279516	15.92%	2.635%
44	8.586	1226	1230	1233	rBV2	178	305	0.02%	0.003%
45	8.647	1234	1240	1257	rVV	555360	869364	49.53%	8.196%
46	8.946	1284	1289	1304	rBV	116892	184384	10.50%	1.738%
47	9.165	1322	1325	1328	rBV2	316	479	0.03%	0.005%
48	9.202	1328	1331	1334	rVV2	238	310	0.02%	0.003%
49	9.269	1339	1342	1346	rBV3	742	976	0.06%	0.009%
50	9.378	1355	1360	1384	rBV	434640	662779	37.76%	6.248%
51	9.702	1409	1413	1417	rVB3	1211	1580	0.09%	0.015%
52	9.848	1436	1437	1440	rVB	537	329	0.02%	0.003%
53	9.909	1446	1447	1452	rVB3	203	280	0.02%	0.003%
54	10.055	1465	1471	1489	rBV2	570619	931791	53.09%	8.784%
55	10.311	1511	1513	1515	rVB2	278	263	0.01%	0.002%
56	10.561	1553	1554	1558	rBV2	199	248	0.01%	0.002%
57	10.659	1568	1570	1573	rVB2	320	271	0.02%	0.003%
58	10.884	1605	1607	1609	rBV2	355	243	0.01%	0.002%
59	10.909	1609	1611	1614	rVB2	293	308	0.02%	0.003%
60	11.012	1625	1628	1632	rBV	212	245	0.01%	0.002%
61	11.092	1636	1641	1645	rBV4	835	1409	0.08%	0.013%
62	11.189	1651	1657	1668	rBV	419389	542718	30.92%	5.116%
63	11.305	1675	1676	1679	rBV	307	316	0.02%	0.003%
64	11.969	1781	1785	1788	rBV	24994	31097	1.77%	0.293%
65	12.036	1788	1796	1806	rVB2	846679	1755229	100.00%	16.547%
66	12.158	1814	1816	1821	rVB	435	523	0.03%	0.005%
67	12.317	1837	1842	1855	rBV2	605645	904752	51.55%	8.529%
68	12.542	1878	1879	1884	rBV	273	425	0.02%	0.004%
69	12.683	1899	1902	1904	rBV	287	278	0.02%	0.003%
70	12.860	1930	1931	1935	rVV2	298	357	0.02%	0.003%
71	12.908	1937	1939	1942	rBV	236	232	0.01%	0.002%
72	12.988	1948	1952	1955	rVB2	250	316	0.02%	0.003%
73	13.061	1958	1964	1969	rVV5	4032	7948	0.45%	0.075%
74	13.109	1970	1972	1978	rVB	816	919	0.05%	0.009%
75	13.378	2015	2016	2018	rBV2	343	272	0.02%	0.003%
76	13.585	2045	2050	2061	rVV	457209	555296	31.64%	5.235%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039145.D
 Acq On : 11 Dec 2023 15:45
 Operator : JC/MD
 Sample : 05646-18DL 200X
 Misc : 2.88g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AS5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.695	2065	2068	2071	rVB2	369	473	0.03%	0.004%
78	13.908	2099	2103	2104	rVB	230	277	0.02%	0.003%
79	13.957	2106	2111	2119	rBV	142183	184586	10.52%	1.740%
80	14.121	2132	2138	2140	rBV2	409	710	0.04%	0.007%
81	14.140	2140	2141	2143	rVV	537	242	0.01%	0.002%
82	14.347	2173	2175	2180	rVB	282	334	0.02%	0.003%
83	14.420	2183	2187	2190	rBV2	393	681	0.04%	0.006%
84	14.475	2193	2196	2199	rVB2	333	394	0.02%	0.004%
85	14.615	2217	2219	2224	rVB2	464	537	0.03%	0.005%
86	14.688	2230	2231	2234	rVB2	379	270	0.02%	0.003%
87	14.713	2234	2235	2237	rBV	326	252	0.01%	0.002%
88	14.780	2239	2246	2250	rVV4	4369	6647	0.38%	0.063%
89	14.823	2250	2253	2256	rVV2	256	366	0.02%	0.003%
90	15.213	2315	2317	2318	rBV2	352	291	0.02%	0.003%
91	15.249	2318	2323	2331	rVB	17299	25615	1.46%	0.241%
92	15.432	2351	2353	2354	rVB	686	379	0.02%	0.004%
93	15.457	2354	2357	2359	rBV2	340	402	0.02%	0.004%
94	15.652	2385	2389	2390	rBV2	353	435	0.02%	0.004%
95	15.700	2396	2397	2400	rBV2	282	226	0.01%	0.002%
96	15.737	2400	2403	2404	rBV2	246	208	0.01%	0.002%
97	15.859	2420	2423	2425	rBV	297	315	0.02%	0.003%
98	16.469	2521	2523	2526	rBV3	419	377	0.02%	0.004%
99	16.517	2529	2531	2534	rVB2	334	259	0.01%	0.002%
100	16.719	2563	2564	2567	rBV2	363	270	0.02%	0.003%




Sum of corrected areas: 10607573

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039145.D
Acq On : 11 Dec 2023 15:45
Operator : JC/MD
Sample : 05646-18DL 200X
Misc : 2.88g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

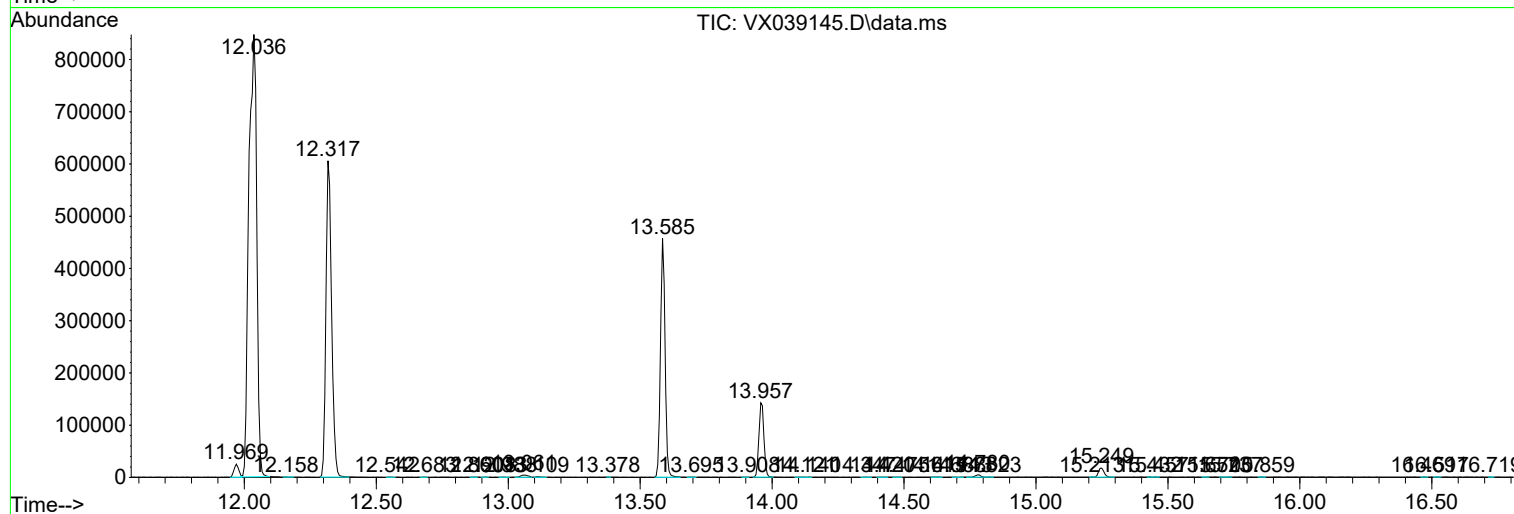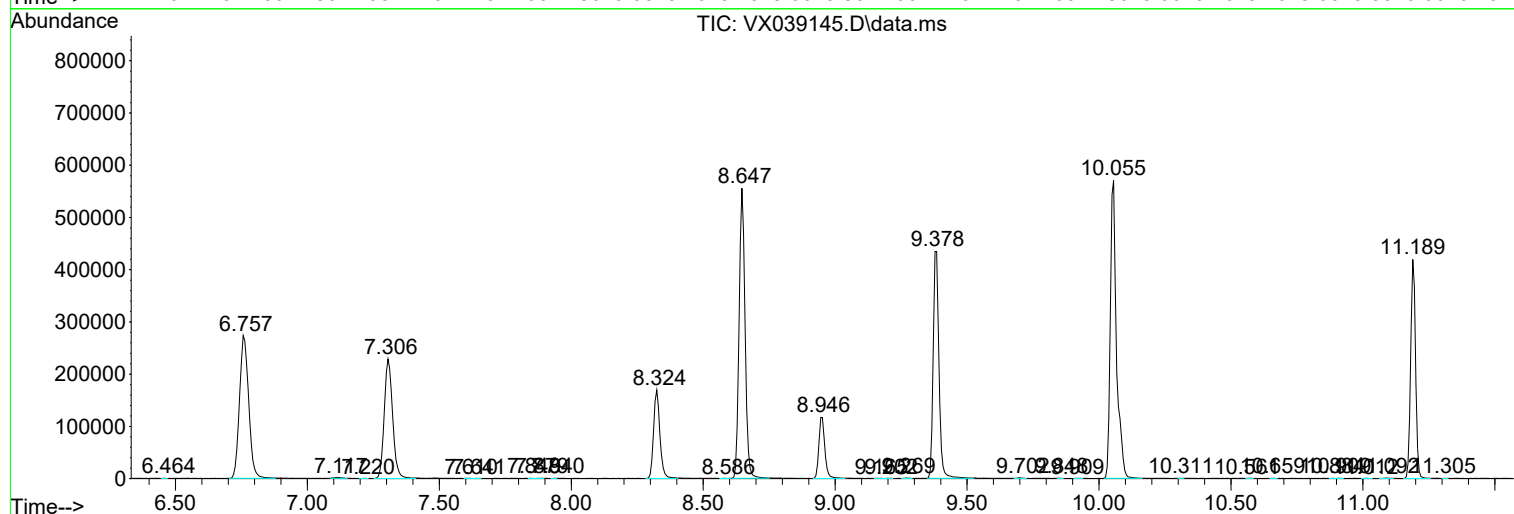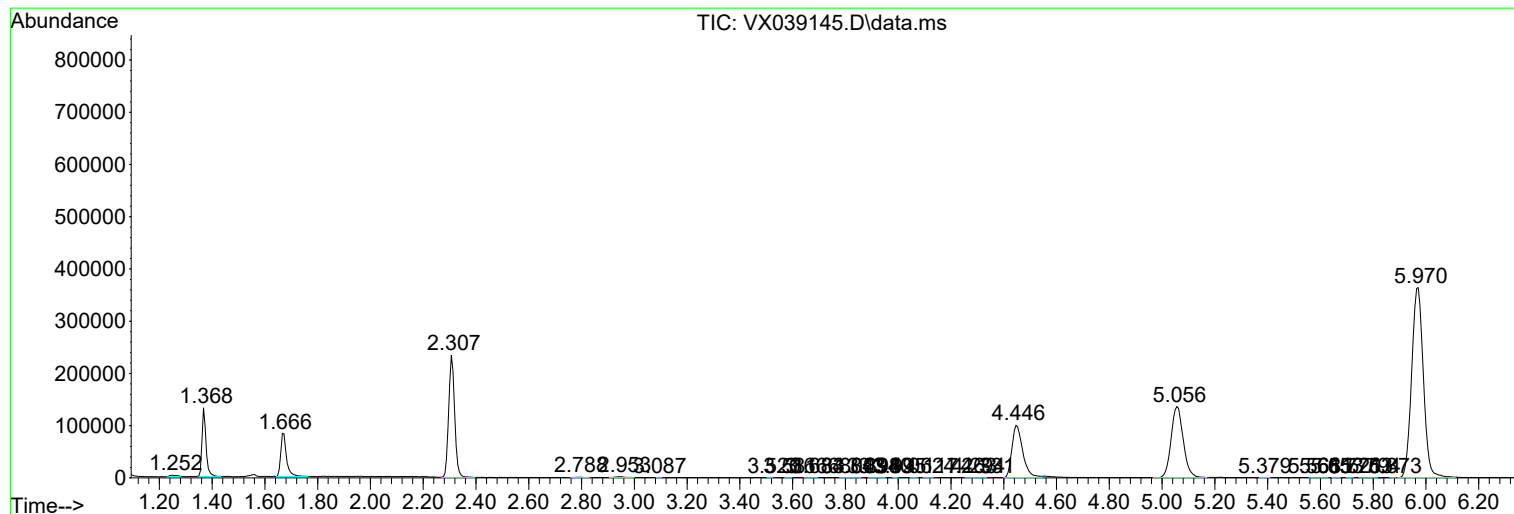

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039145.D
Acq On : 11 Dec 2023 15:45
Operator : JC/MD
Sample : 05646-18DL 200X
Misc : 2.88g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039145.D
Acq On : 11 Dec 2023 15:45
Operator : JC/MD
Sample : 05646-18DL 200X
Misc : 2.88g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AS5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc