

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039148.D
 Acq On : 11 Dec 2023 16:54
 Operator : JC/MD
 Sample : 05752-02 100X
 Misc : 2.41g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COATO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039148.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	28	rBV2	2627	3575	0.09%	0.025%
2	1.368	42	46	57	rVB	131018	136917	3.46%	0.940%
3	1.666	91	95	111	rVB	84225	124674	3.15%	0.856%
4	2.306	194	200	212	rBV	235554	354915	8.98%	2.436%
5	2.508	231	233	234	rBV	359	269	0.01%	0.002%
6	2.794	276	280	282	rBV3	1020	1220	0.03%	0.008%
7	2.946	298	305	311	rVB2	1310	3086	0.08%	0.021%
8	3.172	341	342	345	rBV2	218	221	0.01%	0.002%
9	3.233	350	352	353	rBV2	198	148	0.00%	0.001%
10	3.392	376	378	382	rVB2	322	245	0.01%	0.002%
11	3.513	396	398	399	rBV	263	178	0.00%	0.001%
12	3.593	409	411	413	rBV	204	150	0.00%	0.001%
13	3.727	430	433	434	rBV2	269	319	0.01%	0.002%
14	4.257	519	520	523	rVB2	213	203	0.01%	0.001%
15	4.336	531	533	535	rBV2	180	174	0.00%	0.001%
16	4.446	543	551	566	rBV	96352	274701	6.95%	1.885%
17	5.056	637	651	670	rBV	130165	418184	10.58%	2.870%
18	5.312	690	693	695	rBV2	279	236	0.01%	0.002%
19	5.385	703	705	709	rVB2	342	281	0.01%	0.002%
20	5.568	732	735	737	rBV2	359	296	0.01%	0.002%
21	5.726	759	761	763	rBV	209	159	0.00%	0.001%
22	5.745	763	764	766	rVB2	348	230	0.01%	0.002%
23	5.769	766	768	770	rBV	364	344	0.01%	0.002%
24	5.879	784	786	788	rBV	188	163	0.00%	0.001%
25	5.964	788	800	822	rBV2	352801	1074216	27.18%	7.373%
26	6.379	866	868	871	rBV2	216	259	0.01%	0.002%
27	6.458	878	881	882	rBV2	236	255	0.01%	0.002%
28	6.513	888	890	892	rBV2	213	207	0.01%	0.001%
29	6.690	918	919	921	rBV	247	203	0.01%	0.001%
30	6.757	921	930	952	rVV	276736	679540	17.19%	4.664%
31	6.958	962	963	967	rBV3	361	387	0.01%	0.003%
32	7.110	983	988	995	rVB5	1531	3334	0.08%	0.023%
33	7.214	1002	1005	1007	rVB2	232	209	0.01%	0.001%
34	7.238	1007	1009	1011	rBV2	179	177	0.00%	0.001%
35	7.305	1011	1020	1035	rBV	220790	485825	12.29%	3.334%
36	7.476	1046	1048	1049	rBV	693	422	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039148.D
 Acq On : 11 Dec 2023 16:54
 Operator : JC/MD
 Sample : 05752-02 100X
 Misc : 2.41g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COATO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	7.738	1089	1091	1093	rVB2	279	242	0.01%	0.002%
38	7.763	1093	1095	1099	rBV2	287	461	0.01%	0.003%
39	7.854	1109	1110	1113	rBV2	214	232	0.01%	0.002%
40	7.909	1118	1119	1121	rBV2	206	197	0.00%	0.001%
41	7.970	1127	1129	1131	rVB	369	260	0.01%	0.002%
42	8.208	1165	1168	1169	rBV	225	186	0.00%	0.001%
43	8.324	1181	1187	1198	rBV	161465	264621	6.70%	1.816%
44	8.567	1225	1227	1228	rBV	214	154	0.00%	0.001%
45	8.647	1234	1240	1253	rVV	535284	844067	21.36%	5.793%
46	8.878	1277	1278	1281	rVB2	264	169	0.00%	0.001%
47	8.952	1284	1290	1301	rBV	118224	180253	4.56%	1.237%
48	9.086	1310	1312	1314	rBV2	279	198	0.01%	0.001%
49	9.153	1320	1323	1325	rBV2	304	305	0.01%	0.002%
50	9.220	1333	1334	1337	rBV2	275	241	0.01%	0.002%
51	9.378	1355	1360	1377	rBV	436100	644308	16.30%	4.422%
52	9.701	1409	1413	1417	rVB4	1222	1935	0.05%	0.013%
53	10.055	1465	1471	1489	rBV2	597170	1040897	26.34%	7.144%
54	10.281	1505	1508	1511	rBV3	412	329	0.01%	0.002%
55	10.622	1562	1564	1568	rVB2	173	184	0.00%	0.001%
56	11.043	1631	1633	1635	rBV2	187	154	0.00%	0.001%
57	11.091	1638	1641	1645	rVB2	774	1026	0.03%	0.007%
58	11.189	1652	1657	1670	rVB	418402	523203	13.24%	3.591%
59	11.323	1675	1679	1682	rBV2	275	476	0.01%	0.003%
60	11.408	1691	1693	1694	rBV	270	178	0.00%	0.001%
61	11.457	1699	1701	1704	rVB2	280	284	0.01%	0.002%
62	11.543	1713	1715	1718	rVB2	224	224	0.01%	0.002%
63	11.689	1737	1739	1742	rVB2	178	178	0.00%	0.001%
64	11.914	1774	1776	1778	rVB2	218	137	0.00%	0.001%
65	11.969	1780	1785	1789	rBV	74603	94193	2.38%	0.646%
66	12.036	1789	1796	1811	rVB2	2464910	3952352	100.00%	27.127%
67	12.323	1837	1843	1851	rBV2	660993	1162925	29.42%	7.982%
68	12.487	1868	1870	1871	rBV2	323	229	0.01%	0.002%
69	12.701	1903	1905	1910	rBV2	428	518	0.01%	0.004%
70	12.750	1912	1913	1919	rBV3	294	535	0.01%	0.004%
71	12.920	1937	1941	1948	rVB2	6103	8398	0.21%	0.058%
72	13.061	1958	1964	1970	rBV2	12781	25582	0.65%	0.176%
73	13.109	1970	1972	1978	rVB5	2258	2620	0.07%	0.018%
74	13.195	1982	1986	1991	rVB	5151	6356	0.16%	0.044%
75	13.384	2011	2017	2022	rVB3	1982	3018	0.08%	0.021%
76	13.426	2022	2024	2026	rVB2	200	168	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039148.D
 Acq On : 11 Dec 2023 16:54
 Operator : JC/MD
 Sample : 05752-02 100X
 Misc : 2.41g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COATO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.463	2027	2030	2033	rVB	259	258	0.01%	0.002%
78	13.585	2045	2050	2061	rBV	1309686	1621176	41.02%	11.127%
79	13.859	2094	2095	2097	rBV	190	162	0.00%	0.001%
80	13.908	2100	2103	2106	rVV2	171	242	0.01%	0.002%
81	13.957	2106	2111	2124	rVV	416678	529713	13.40%	3.636%
82	14.134	2136	2140	2143	rVB2	537	585	0.01%	0.004%
83	14.194	2148	2150	2155	rVV2	227	248	0.01%	0.002%
84	14.231	2155	2156	2159	rVV2	253	164	0.00%	0.001%
85	14.262	2159	2161	2162	rVB	321	226	0.01%	0.002%
86	14.292	2164	2166	2167	rBV	288	143	0.00%	0.001%
87	14.402	2183	2184	2187	rBV2	183	208	0.01%	0.001%
88	14.548	2204	2208	2210	rBV2	315	475	0.01%	0.003%
89	14.597	2212	2216	2217	rVB2	179	172	0.00%	0.001%
90	14.627	2217	2221	2224	rBV3	581	714	0.02%	0.005%
91	14.780	2240	2246	2251	rBV2	11877	18580	0.47%	0.128%
92	14.853	2254	2258	2259	rBV2	251	296	0.01%	0.002%
93	14.926	2268	2270	2274	rVB3	374	275	0.01%	0.002%
94	15.249	2317	2323	2331	rBV	44526	65975	1.67%	0.453%
95	15.444	2351	2355	2358	rBV3	424	672	0.02%	0.005%
96	15.475	2358	2360	2363	rBV2	319	378	0.01%	0.003%
97	15.761	2405	2407	2409	rBV	361	421	0.01%	0.003%
98	15.816	2414	2416	2419	rVB2	345	382	0.01%	0.003%
99	16.365	2504	2506	2507	rVB2	455	218	0.01%	0.001%
100	16.383	2507	2509	2510	rBV	278	199	0.01%	0.001%




Sum of corrected areas: 14569797

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039148.D
Acq On : 11 Dec 2023 16:54
Operator : JC/MD
Sample : 05752-02 100X
Misc : 2.41g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0A70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

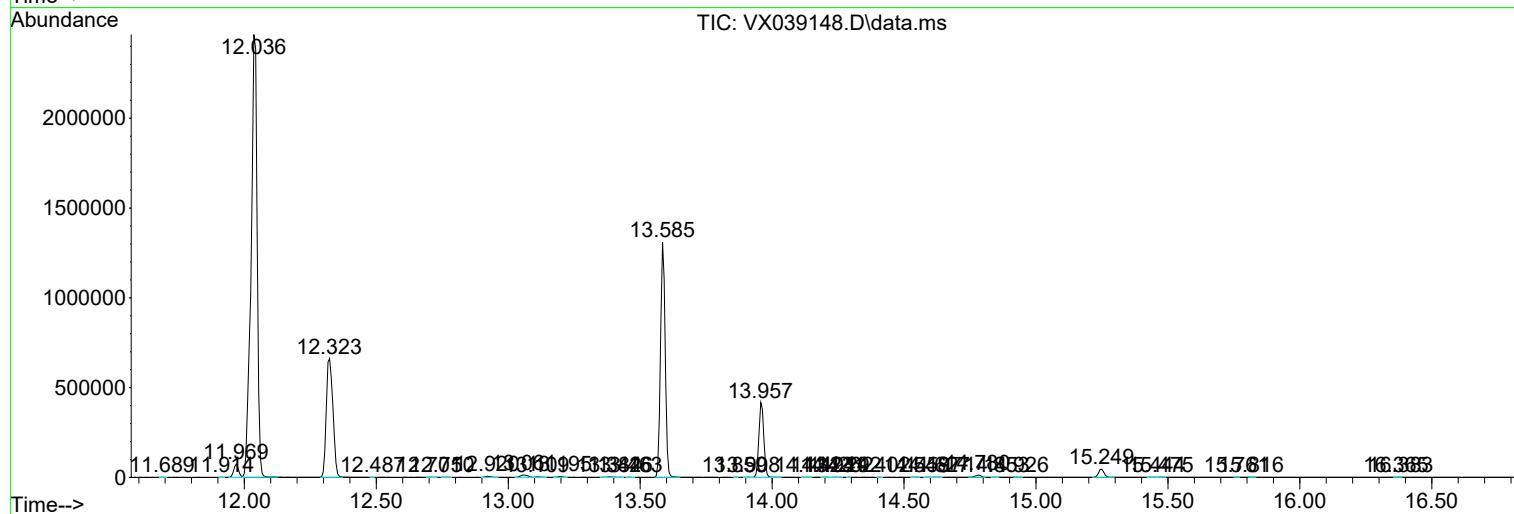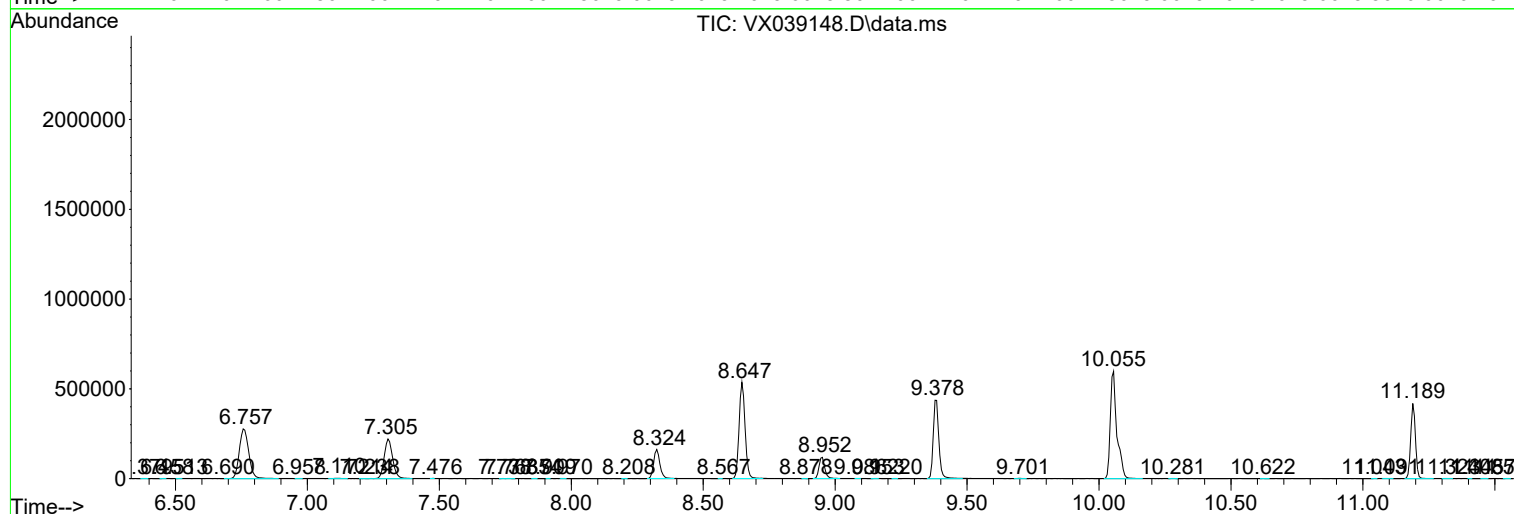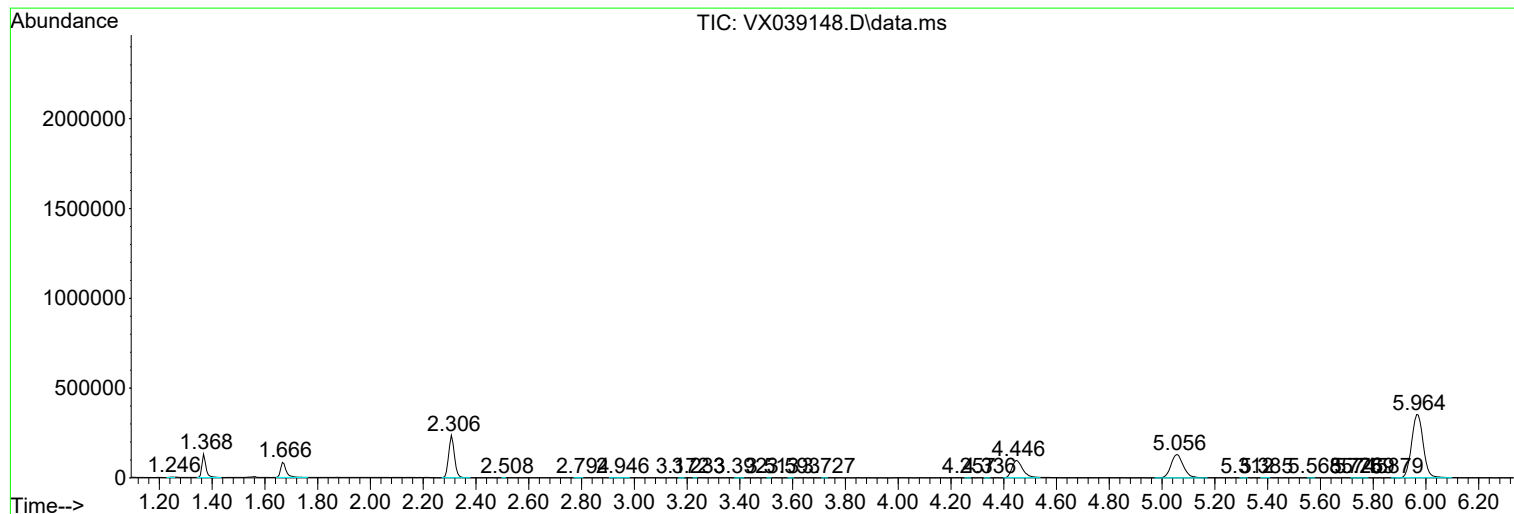

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039148.D
Acq On : 11 Dec 2023 16:54
Operator : JC/MD
Sample : 05752-02 100X
Misc : 2.41g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0A00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039148.D
Acq On : 11 Dec 2023 16:54
Operator : JC/MD
Sample : 05752-02 100X
Misc : 2.41g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc