

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039150.D
 Acq On : 11 Dec 2023 17:40
 Operator : JC/MD
 Sample : 05752-04 100X
 Misc : 2.04g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039150.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	28	rBV2	2994	4120	0.39%	0.048%
2	1.368	42	46	56	rVB	125113	130137	12.39%	1.516%
3	1.666	91	95	109	rVB	79175	114380	10.89%	1.332%
4	2.306	194	200	212	rVB	222499	347482	33.09%	4.048%
5	2.666	257	259	260	rBV	343	174	0.02%	0.002%
6	2.788	275	279	286	rVB2	1472	2483	0.24%	0.029%
7	2.880	293	294	296	rBV2	276	205	0.02%	0.002%
8	2.940	298	304	316	rVB	4226	8588	0.82%	0.100%
9	3.245	353	354	356	rBV2	230	178	0.02%	0.002%
10	3.453	386	388	389	rVB	297	168	0.02%	0.002%
11	3.635	416	418	421	rVB	220	211	0.02%	0.002%
12	3.666	421	423	426	rBV2	325	265	0.03%	0.003%
13	3.843	450	452	454	rVV	329	183	0.02%	0.002%
14	4.172	504	506	510	rBV2	379	472	0.04%	0.005%
15	4.202	510	511	513	rBV	180	164	0.02%	0.002%
16	4.349	533	535	537	rBV	243	160	0.02%	0.002%
17	4.446	543	551	565	rBV	93968	269709	25.68%	3.142%
18	4.684	589	590	591	rBV	498	256	0.02%	0.003%
19	5.056	637	651	673	rBV	135960	416875	39.70%	4.856%
20	5.343	696	698	699	rBV	225	157	0.01%	0.002%
21	5.385	699	705	710	rVV4	574	1270	0.12%	0.015%
22	5.550	728	732	733	rBV2	566	540	0.05%	0.006%
23	5.745	763	764	768	rBV2	193	225	0.02%	0.003%
24	5.970	789	801	815	rBV2	344748	1046094	99.61%	12.186%
25	6.239	843	845	847	rBV2	237	169	0.02%	0.002%
26	6.446	876	879	880	rBV	207	266	0.03%	0.003%
27	6.513	889	890	893	rBV	278	283	0.03%	0.003%
28	6.757	921	930	950	rBV	266366	648968	61.80%	7.560%
29	7.001	968	970	971	rVB	330	164	0.02%	0.002%
30	7.037	973	976	977	rBV2	296	296	0.03%	0.003%
31	7.110	982	988	996	rVB4	1865	4089	0.39%	0.048%
32	7.306	1011	1020	1036	rBV	214902	479642	45.67%	5.588%
33	7.604	1066	1069	1072	rBV2	185	190	0.02%	0.002%
34	7.897	1113	1117	1118	rBV2	211	273	0.03%	0.003%
35	8.055	1142	1143	1147	rVB	313	229	0.02%	0.003%
36	8.244	1168	1174	1176	rVB2	194	321	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039150.D
 Acq On : 11 Dec 2023 17:40
 Operator : JC/MD
 Sample : 05752-04 100X
 Misc : 2.04g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	8.324	1180	1187	1201	rBV	161976	264325	25.17%	3.079%
38	8.507	1215	1217	1221	rVB3	451	629	0.06%	0.007%
39	8.647	1234	1240	1255	rVV	542890	834366	79.45%	9.720%
40	8.946	1284	1289	1303	rBV	114258	176139	16.77%	2.052%
41	9.171	1324	1326	1328	rVB2	179	164	0.02%	0.002%
42	9.281	1340	1344	1347	rBV3	353	457	0.04%	0.005%
43	9.378	1355	1360	1373	rBV	423227	623802	59.40%	7.267%
44	9.695	1408	1412	1419	rVB3	1770	2713	0.26%	0.032%
45	9.775	1423	1425	1429	rBV3	287	454	0.04%	0.005%
46	9.903	1442	1446	1449	rBV2	269	395	0.04%	0.005%
47	10.049	1465	1470	1488	rBV	552360	802626	76.43%	9.350%
48	10.195	1490	1494	1496	rVB3	372	465	0.04%	0.005%
49	10.250	1501	1503	1504	rVB	300	173	0.02%	0.002%
50	10.268	1504	1506	1508	rVB	163	156	0.01%	0.002%
51	10.390	1523	1526	1528	rVV2	195	233	0.02%	0.003%
52	10.415	1528	1530	1531	rVB2	266	163	0.02%	0.002%
53	10.439	1531	1534	1535	rBV	194	197	0.02%	0.002%
54	10.683	1573	1574	1576	rBV	149	143	0.01%	0.002%
55	10.982	1622	1623	1626	rBV2	255	232	0.02%	0.003%
56	11.037	1630	1632	1633	rBV	210	178	0.02%	0.002%
57	11.098	1638	1642	1644	rVV4	620	716	0.07%	0.008%
58	11.189	1652	1657	1666	rVB	412088	515218	49.06%	6.002%
59	11.360	1683	1685	1687	rVB2	155	143	0.01%	0.002%
60	11.415	1692	1694	1696	rVV2	183	164	0.02%	0.002%
61	11.451	1698	1700	1702	rVB2	287	214	0.02%	0.002%
62	11.469	1702	1703	1707	rVB	312	289	0.03%	0.003%
63	11.512	1707	1710	1713	rBV2	168	226	0.02%	0.003%
64	11.543	1713	1715	1717	rBV	184	234	0.02%	0.003%
65	11.683	1737	1738	1740	rBV	207	143	0.01%	0.002%
66	11.707	1740	1742	1744	rBV	285	277	0.03%	0.003%
67	11.969	1781	1785	1788	rBV	5315	6411	0.61%	0.075%
68	12.024	1788	1794	1809	rVB2	597116	1050185	100.00%	12.234%
69	12.268	1832	1834	1837	rBV2	172	147	0.01%	0.002%
70	12.317	1837	1842	1854	rBV	590822	765454	72.89%	8.917%
71	12.488	1868	1870	1871	rBV	192	183	0.02%	0.002%
72	12.585	1884	1886	1890	rBV2	203	283	0.03%	0.003%
73	12.670	1893	1900	1901	rBV2	190	349	0.03%	0.004%
74	12.689	1901	1903	1905	rVB2	201	180	0.02%	0.002%
75	12.762	1912	1915	1920	rVV3	361	490	0.05%	0.006%
76	12.811	1922	1923	1926	rBV2	223	237	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
 Data File : VX039150.D
 Acq On : 11 Dec 2023 17:40
 Operator : JC/MD
 Sample : 05752-04 100X
 Misc : 2.04g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

77	12.920	1939	1941	1944	rBV2	176	280	0.03%	0.003%
78	13.061	1962	1964	1967	rBV2	307	342	0.03%	0.004%
79	13.091	1967	1969	1971	rVV2	212	147	0.01%	0.002%
80	13.237	1991	1993	1994	rBV	204	200	0.02%	0.002%
81	13.433	2024	2025	2027	rBV	295	175	0.02%	0.002%
82	13.585	2046	2050	2059	rBV2	25264	34385	3.27%	0.401%
83	13.713	2067	2071	2073	rVB2	160	230	0.02%	0.003%
84	13.890	2097	2100	2101	rVB2	209	194	0.02%	0.002%
85	13.908	2101	2103	2105	rBV2	231	190	0.02%	0.002%
86	13.963	2107	2112	2118	rBV2	8969	11578	1.10%	0.135%
87	14.134	2137	2140	2142	rVV	535	628	0.06%	0.007%
88	14.335	2170	2173	2175	rBV	283	315	0.03%	0.004%
89	14.396	2180	2183	2185	rBV2	223	245	0.02%	0.003%
90	14.487	2195	2198	2199	rBV2	371	421	0.04%	0.005%
91	14.560	2208	2210	2214	rVB2	188	240	0.02%	0.003%
92	14.609	2216	2218	2221	rVV2	317	283	0.03%	0.003%
93	14.658	2225	2226	2229	rBV2	220	225	0.02%	0.003%
94	15.182	2309	2312	2313	rBV2	355	383	0.04%	0.004%
95	15.249	2319	2323	2327	rBV3	2153	2724	0.26%	0.032%
96	15.487	2361	2362	2368	rVB2	472	591	0.06%	0.007%
97	15.798	2411	2413	2417	rVB2	380	508	0.05%	0.006%
98	16.194	2475	2478	2480	rBV2	400	486	0.05%	0.006%
99	16.383	2508	2509	2511	rVB2	325	184	0.02%	0.002%
100	16.432	2515	2517	2519	rBV2	416	301	0.03%	0.004%




Sum of corrected areas: 8584194

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039150.D
Acq On : 11 Dec 2023 17:40
Operator : JC/MD
Sample : 05752-04 100X
Misc : 2.04g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

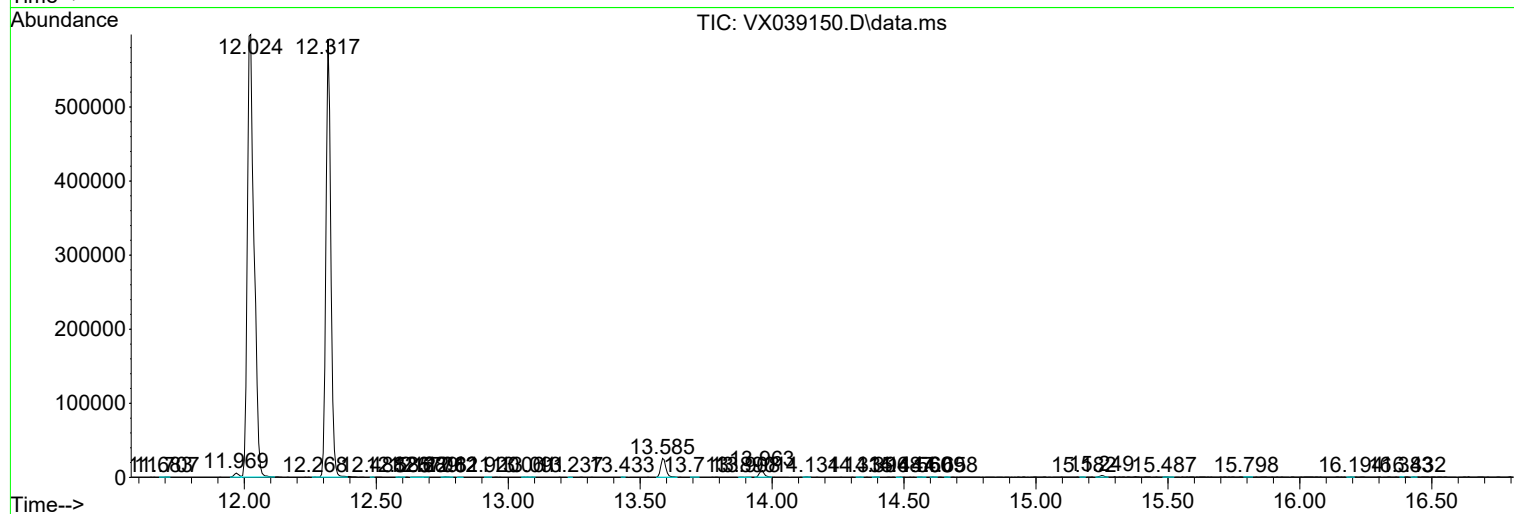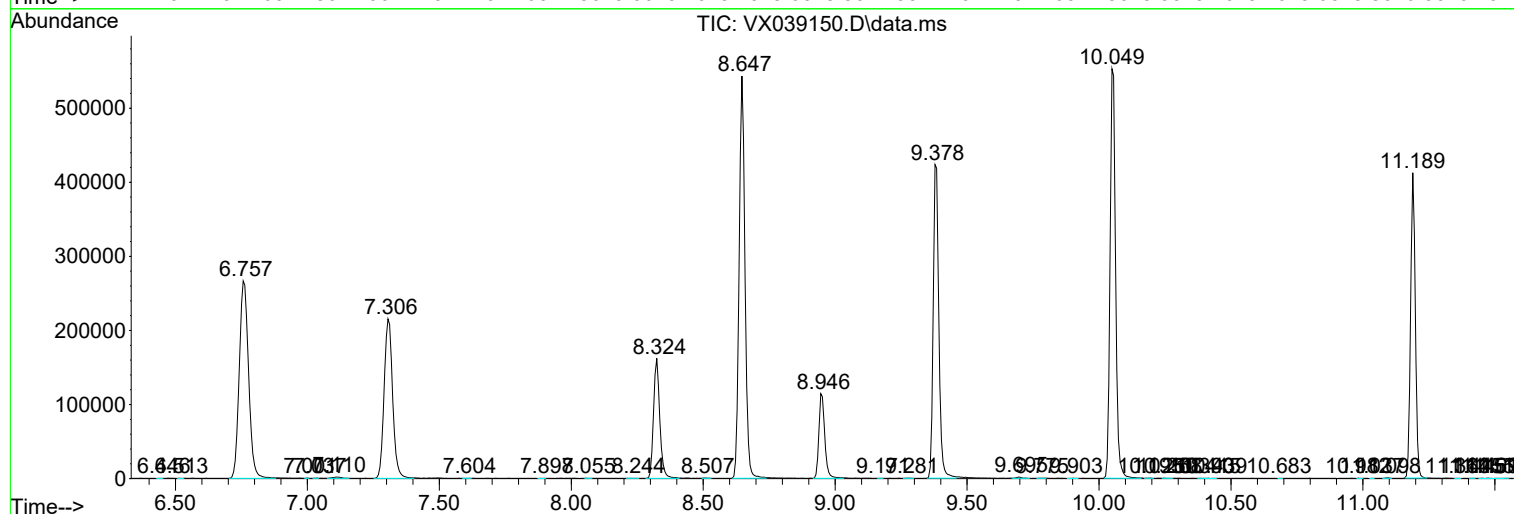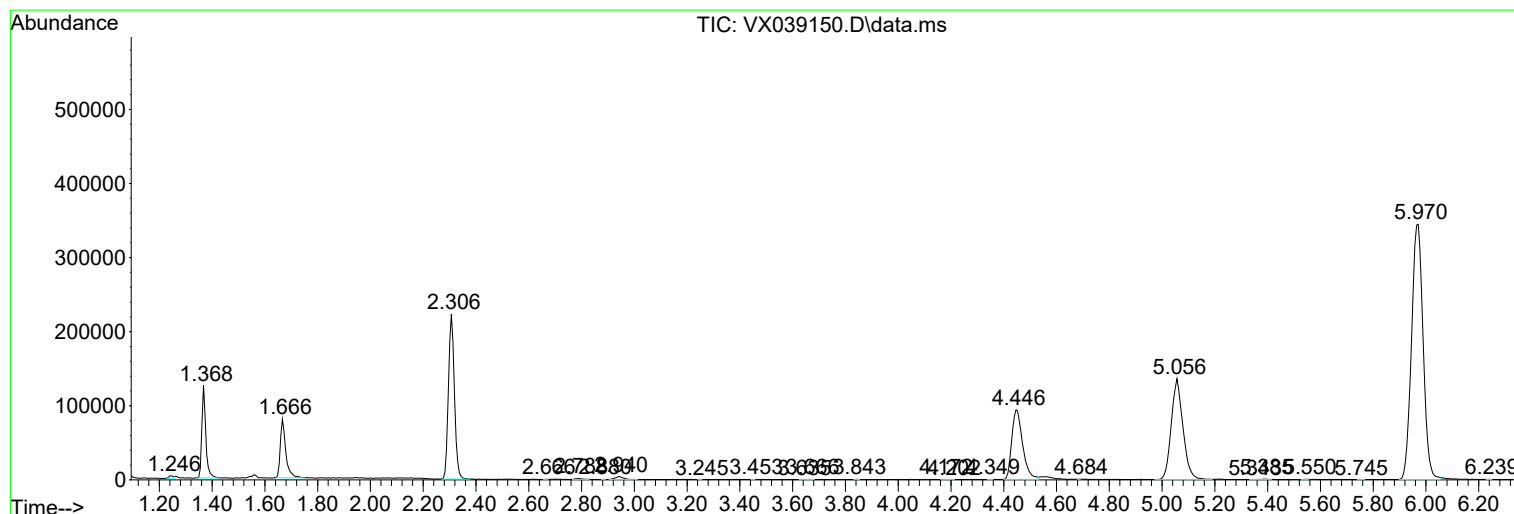

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039150.D
Acq On : 11 Dec 2023 17:40
Operator : JC/MD
Sample : 05752-04 100X
Misc : 2.04g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039150.D
Acq On : 11 Dec 2023 17:40
Operator : JC/MD
Sample : 05752-04 100X
Misc : 2.04g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc