
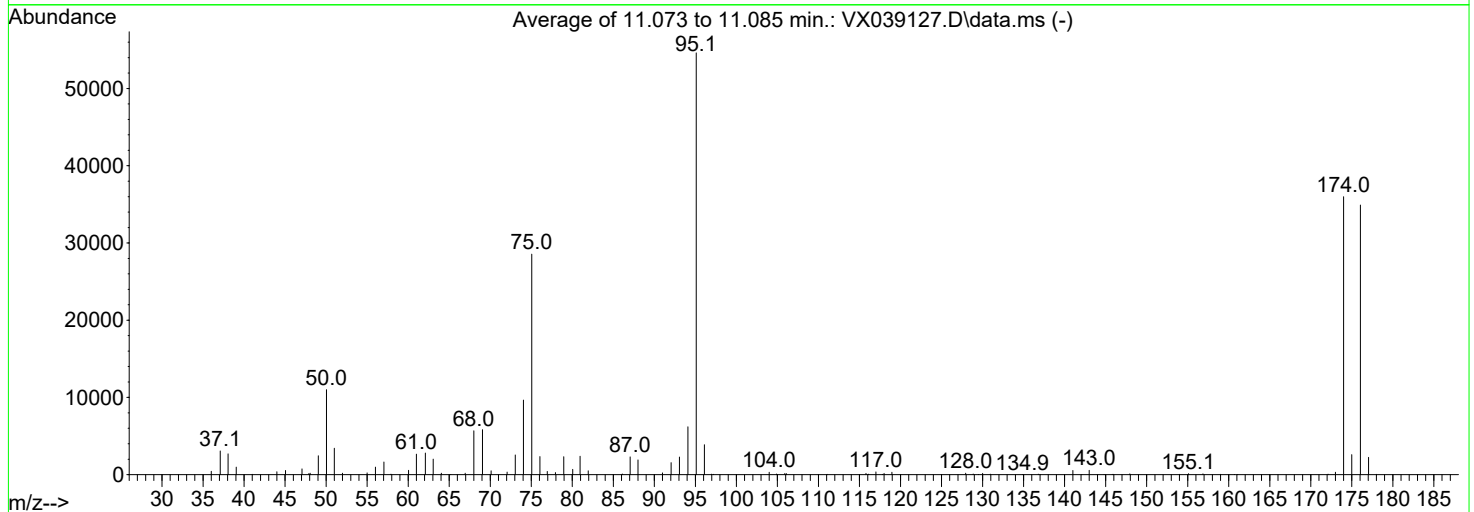


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121123\
Data File : VX039127.D
Acq On : 11 Dec 2023 08:29
Operator : JC/MD
Sample : BFB654
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB654

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Title : VOC Analysis
Last Update : Tue Dec 12 03:50:51 2023

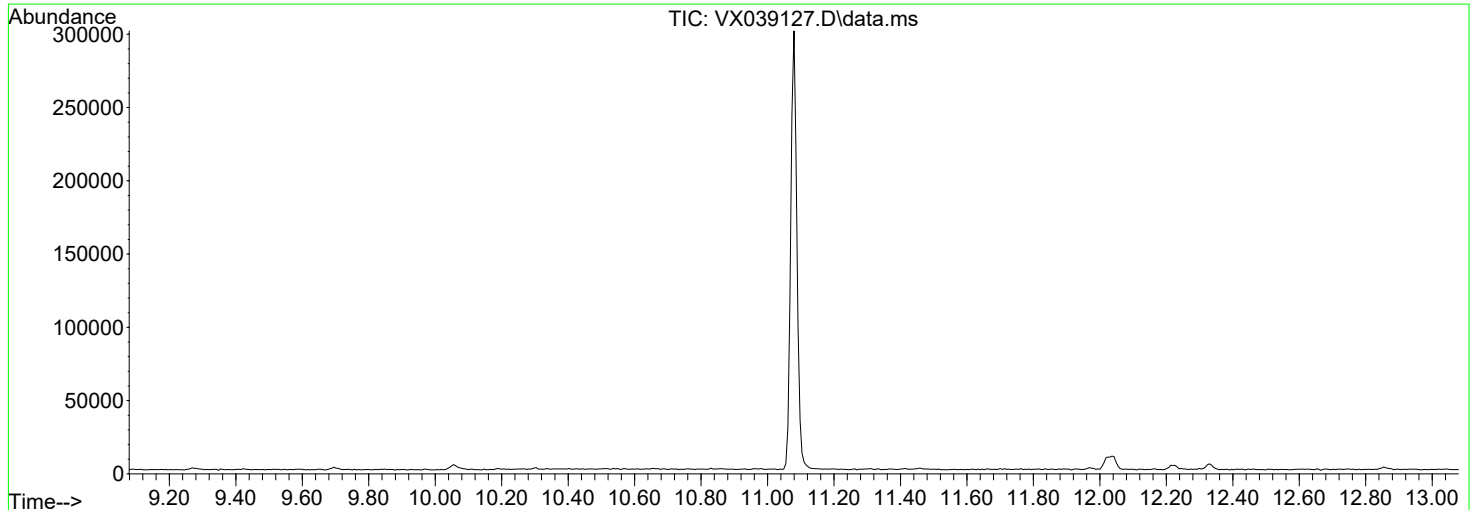

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	10996	PASS
75	95	30	80	52.3	28547	PASS
95	95	100	100	100.0	54621	PASS
96	95	5	9	7.1	3881	PASS
173	174	0.00	2	0.9	306	PASS
174	95	50	120	65.9	35997	PASS
175	174	5	9	7.2	2600	PASS
176	174	95	101	97.0	34923	PASS
177	176	5	9	6.4	2241	PASS

m/z	Abundance
36.00	249.0
37.80	77.0
40.00	2740.0
43.90	270.0

Instrument :
MSVOA_X
ClientSampleId :
BFB654

m/z	Abundance
36.00	768.0
37.10	3104.0
38.10	3007.0
39.00	1140.0
40.00	2675.0
44.00	574.0
45.10	444.0
47.10	930.0
47.90	452.0
49.10	2728.0
50.10	11924.0
51.00	3884.0
52.00	195.0
55.00	210.0
56.00	938.0
57.10	1660.0
57.90	116.0
60.20	570.0
61.00	2898.0
62.10	2959.0
63.00	2269.0
64.10	210.0
65.20	58.0
66.90	270.0
68.00	5895.0
69.00	5972.0
70.10	537.0
72.00	238.0
73.00	2466.0
74.10	9693.0
75.00	28408.0
76.10	2455.0
77.00	433.0
77.90	248.0
79.00	2454.0
80.00	635.0
81.00	2165.0
82.00	473.0
87.10	2103.0
88.00	1540.0
91.00	250.0
92.10	1516.0
93.00	2426.0
94.10	6092.0
95.10	53248.0
96.10	4048.0
97.00	75.0
103.90	306.0
105.00	90.0
105.90	261.0
111.00	56.0
116.10	169.0
117.00	400.0
117.80	142.0
119.00	344.0
127.90	195.0
128.90	85.0
129.50	60.0
130.10	108.0
131.00	78.0
136.80	73.0
141.00	490.0
143.00	474.0
145.80	143.0
147.90	92.0
154.00	64.0
155.10	58.0
156.90	125.0
172.10	107.0
173.00	223.0
174.00	30280.0
175.00	2210.0
176.00	28696.0
177.10	2179.0
178.00	51.0

Instrument :
MSVOA_X
ClientSampleId :
BFB654

m/z	Abundance
36.00	741.0
37.10	3669.0
38.00	3173.0
39.10	975.0
40.00	2683.0
41.00	99.0
44.10	809.0
45.10	712.0
47.10	864.0
48.10	329.0
49.00	2637.0
50.00	12641.0
51.00	4047.0
52.00	223.0
55.10	348.0
56.00	1152.0
57.00	1783.0
57.90	92.0
60.00	603.0
61.00	3141.0
62.10	3456.0
63.10	2229.0
63.90	159.0
67.00	142.0
68.00	6510.0
69.00	6690.0
70.10	600.0
72.10	411.0
73.10	2912.0
74.00	11058.0
75.10	34208.0
76.00	2704.0
77.00	406.0
77.90	355.0
79.00	2659.0
80.00	900.0
81.00	3093.0
82.00	629.0
86.10	160.0
87.00	2740.0
88.00	2249.0
91.00	264.0
92.10	1949.0
93.10	2358.0
94.10	7098.0
95.10	65064.0
96.10	4230.0
96.90	108.0
104.00	326.0
104.90	102.0
106.10	353.0
111.10	51.0
115.80	276.0
117.00	336.0
118.00	308.0
118.90	361.0
128.00	178.0
128.90	94.0
130.00	300.0
131.00	59.0
137.00	82.0
141.00	723.0
142.10	86.0
143.00	662.0
146.00	84.0
148.00	100.0
154.00	66.0
155.10	220.0
156.80	85.0
159.00	92.0
160.70	80.0
172.10	91.0
173.00	303.0
174.00	42792.0
175.00	3220.0
176.00	42288.0
177.10	2375.0
178.00	65.0

Instrument :
MSVOA_X
ClientSampleId :
BFB654

m/z	Abundance
36.00	523.0
37.10	2455.0
38.10	1924.0
39.00	827.0
40.00	2724.0
44.10	562.0
45.00	454.0
46.90	448.0
48.00	253.0
49.00	1949.0
50.10	8424.0
51.10	2316.0
52.00	127.0
54.90	130.0
56.00	815.0
57.10	1462.0
59.90	493.0
61.00	1895.0
62.00	2007.0
63.00	1555.0
64.10	184.0
66.90	137.0
68.00	4639.0
69.10	4779.0
70.00	340.0
72.00	340.0
73.10	2294.0
74.10	8217.0
75.10	23024.0
76.10	1892.0
76.90	416.0
78.00	210.0
78.90	1824.0
80.10	548.0
80.90	1911.0
81.90	395.0
86.10	83.0
87.10	2067.0
88.00	1928.0
91.00	194.0
92.00	1214.0
93.00	2038.0
94.10	5411.0
95.10	45552.0
96.10	3366.0
97.20	137.0
104.10	285.0
104.80	75.0
105.90	265.0
115.80	215.0
117.00	305.0
118.00	187.0
119.00	245.0
127.90	195.0
128.70	53.0
129.90	118.0
130.90	67.0
134.90	60.0
136.80	101.0
141.00	423.0
143.00	550.0
144.80	65.0
145.90	71.0
148.00	132.0
155.00	87.0
156.90	78.0
159.00	61.0
161.10	80.0
173.00	392.0
174.00	34920.0
175.00	2369.0
176.10	33784.0
177.00	2168.0

Instrument :
MSVOA_X
ClientSampleId :
BFB654