

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121125\
 Data File : VX048836.D
 Acq On : 11 Dec 2025 18:44
 Operator : JC/MD
 Sample : Q3828-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RMW-03B-90-120925

Quant Time: Dec 11 23:55:11 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 05 03:27:34 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.537	168	172815	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.744	114	291968	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	260001	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	125510	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.940	65	123876	53.406	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 106.820%			
35) Dibromofluoromethane	5.379	113	94752	47.133	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 94.260%			
50) Toluene-d8	8.634	98	340129	48.267	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 96.540%			
62) 4-Bromofluorobenzene	11.061	95	118676	48.839	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 97.680%			
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.148	85	555807	315.657	ug/l	98
3) Chloromethane	1.148	50	137235	61.764	ug/l #	42
4) Vinyl Chloride	1.380	62	14515	6.134	ug/l	97
7) Trichlorofluoromethane	2.142	101	8183	2.413	ug/l	99
8) Diethyl Ether	2.136	74	685	0.506	ug/l #	1
9) 1,1,2-Trichlorotrifluo...	2.337	101	3543073	1802.023	ug/l	98
12) 1,1-Dichloroethene	2.331	96	21657	10.792	ug/l #	76
13) Acrolein	2.142	56	179	40.593	ug/l #	15
16) Acetone	2.337	43	35746	40.257	ug/l	89
17) Carbon Disulfide	2.520	76	1384	0.237	ug/l #	79
20) Methylene Chloride	2.794	84	539	0.243	ug/l #	88
21) trans-1,2-Dichloroethene	3.093	96	3411	1.665	ug/l	96
24) 1,1-Dichloroethane	3.611	63	157265	44.788	ug/l	99
27) cis-1,2-Dichloroethene	4.483	96	3224871	1395.335	ug/l	95
31) Cyclohexane	5.525	56	3466	1.106	ug/l #	1
36) 1,1-Dichloropropene	5.537	75	13452	4.886	ug/l #	44
38) Carbon Tetrachloride	5.537	117	18150	5.820	ug/l #	13
39) Methylcyclohexane	7.110	83	30358	9.324	ug/l #	1
40) Benzene	6.025	78	26446	3.240	ug/l	100
42) 1,2-Dichloroethane	6.080	62	8717	3.017	ug/l	100
44) Trichloroethene	7.116	130	2557014	1200.604	ug/l	94
49) 1,4-Dioxane	7.653	88	232	6.731	ug/l #	73
51) 4-Methyl-2-Pentanone	8.628	43	1610	0.521	ug/l #	1
55) 1,1,2-Trichloroethane	9.140	97	808	0.408	ug/l #	82
60) Dibromochloromethane	9.256	129	13927	5.687	ug/l #	11
64) Tetrachloroethene	9.256	164	14381	7.588	ug/l	96
68) m/p-Xylenes	10.280	106	807	0.223	ug/l	74
69) o-Xylene	10.628	106	787	0.232	ug/l	84
76) 1,2,3-Trichloropropane	11.061	75	60041	25.684	ug/l #	30
81) trans-1,4-Dichloro-2-b...	11.061	75	60041	61.010	ug/l #	3
88) 1,4-Dichlorobenzene	12.018	146	1917	0.446	ug/l #	17
91) 1,2-Dichlorobenzene	12.317	146	2816	0.698	ug/l	96
95) Naphthalene	13.786	128	137	Below Cal	#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121125\
Data File : VX048836.D
Acq On : 11 Dec 2025 18:44
Operator : JC/MD
Sample : Q3828-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925

Quant Time: Dec 11 23:55:11 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 05 03:27:34 2025
Response via : Initial Calibration




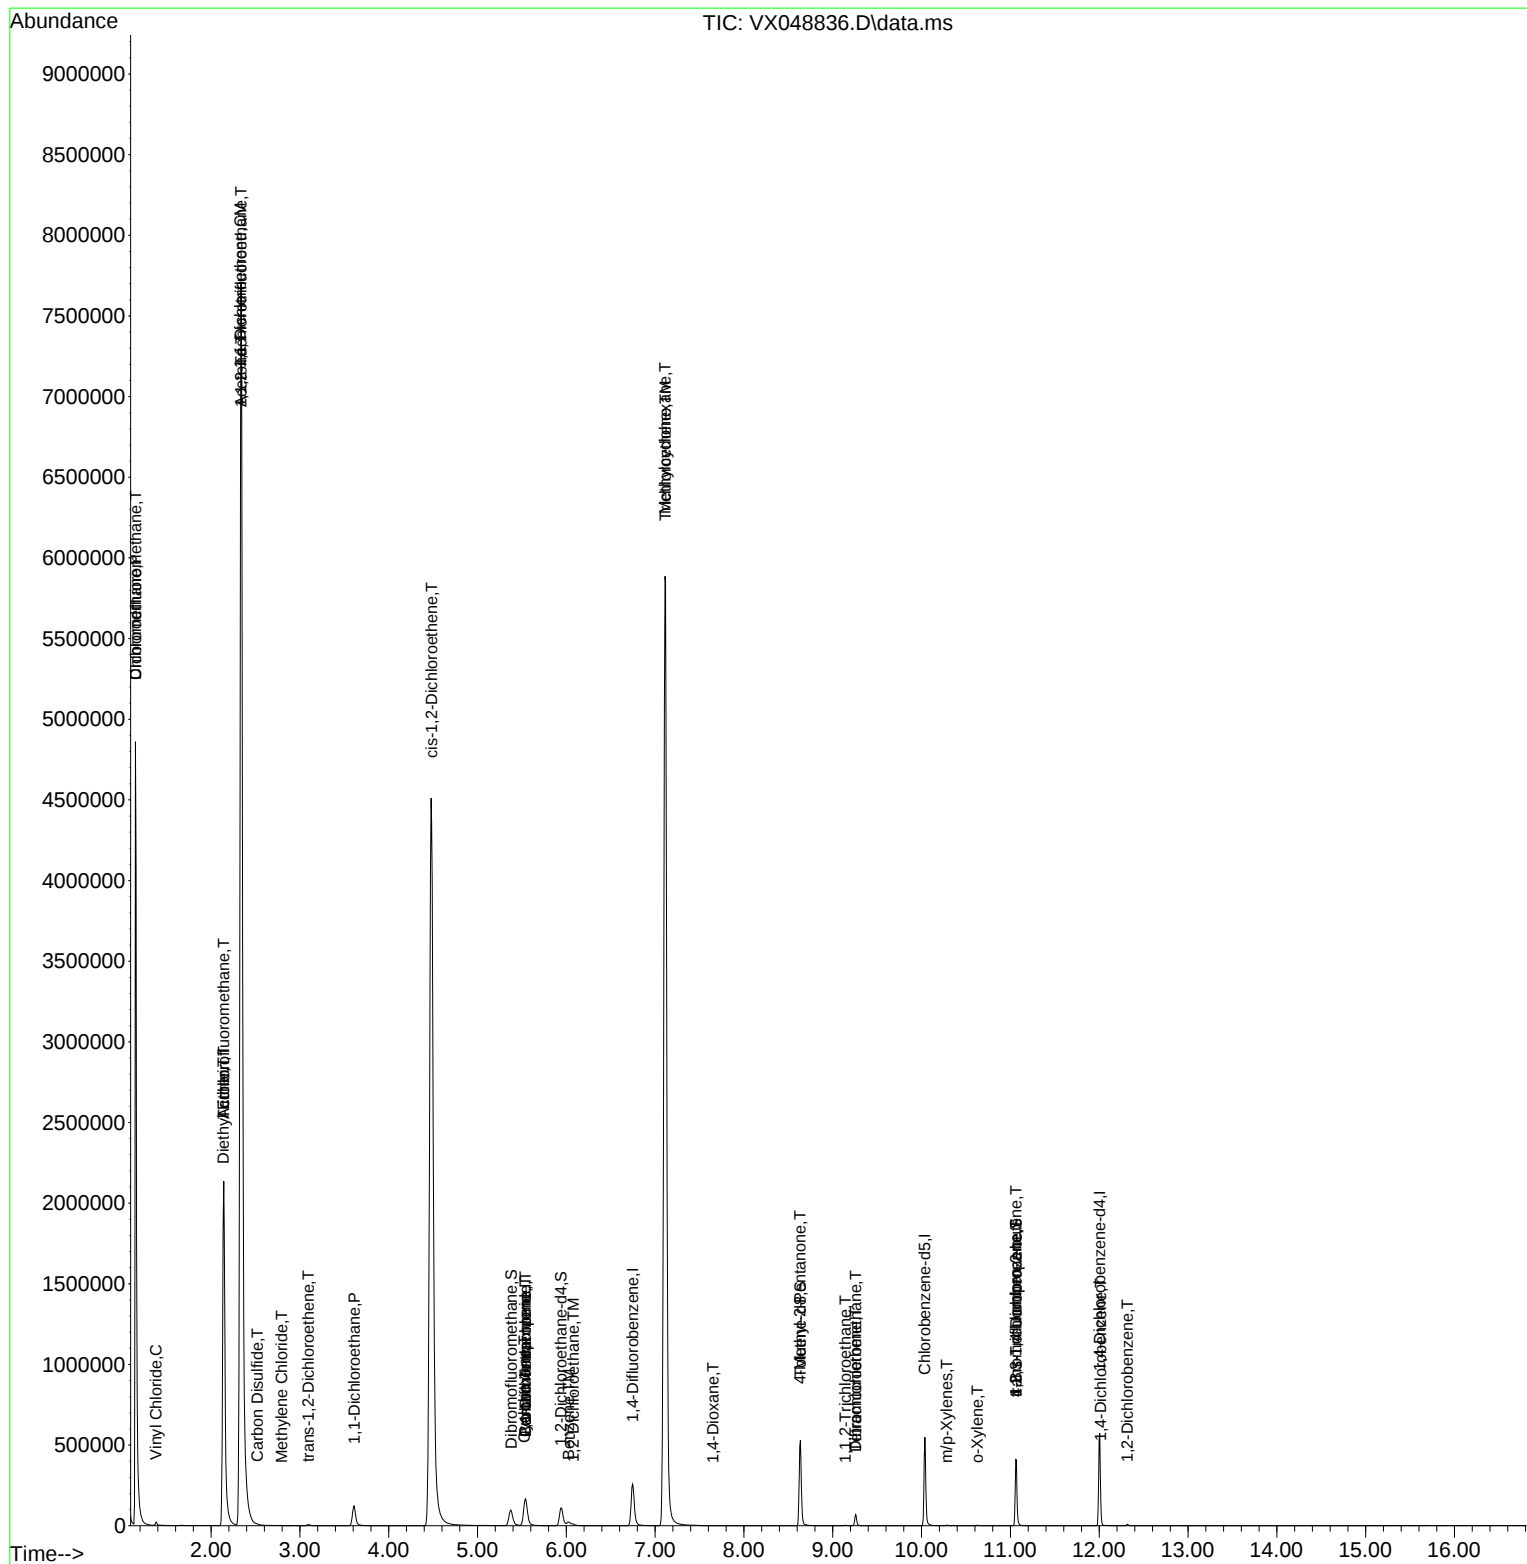




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.537 min Scan# 71
Delta R.T. -0.001 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44




Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925


Tgt Ion:168 Resp: 172815
Ion Ratio Lower Upper
168 100
99 59.0 44.2 66.4

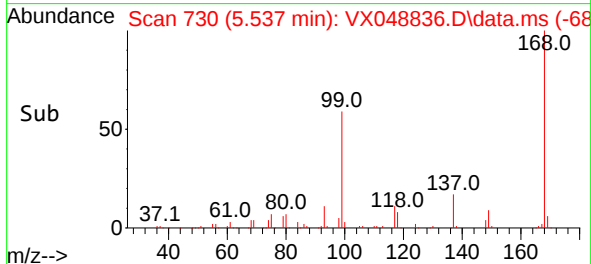

#2
Dichlorodifluoromethane
Concen: 315.657 ug/l
RT: 1.148 min Scan# 10
Delta R.T. -0.025 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Tgt Ion: 85 Resp: 555807
Ion Ratio Lower Upper
85 100
87 31.7 16.4 49.1

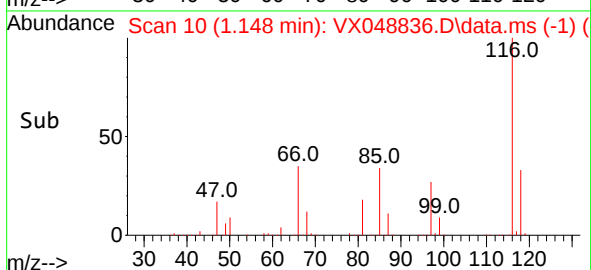

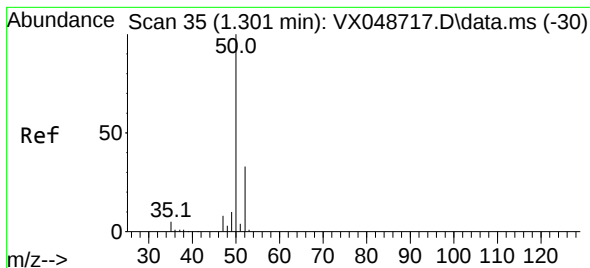

#3

Chloromethane

Concen: 61.764 ug/l

RT: 1.148 min Scan# 10

Delta R.T. -0.153 min

Lab File: VX048836.D

Acq: 11 Dec 2025 18:44

Instrument :

MSVOA_X

ClientSampleId :





RMW-03B-90-120925

Tgt Ion: 50 Resp: 137235

Ion Ratio Lower Upper

50 100

52 0.0 26.4 39.6#

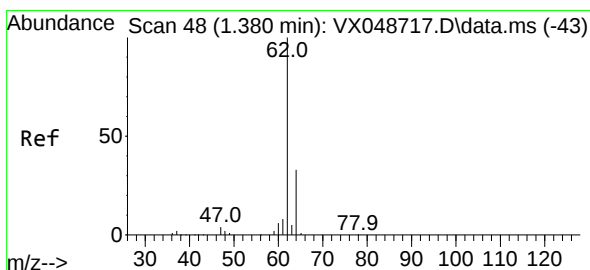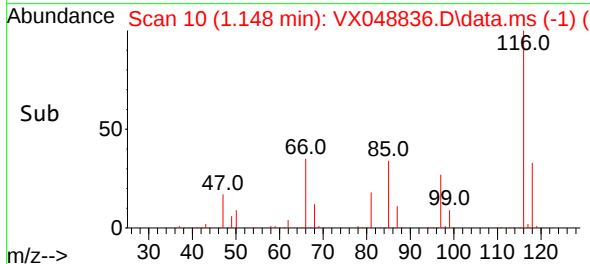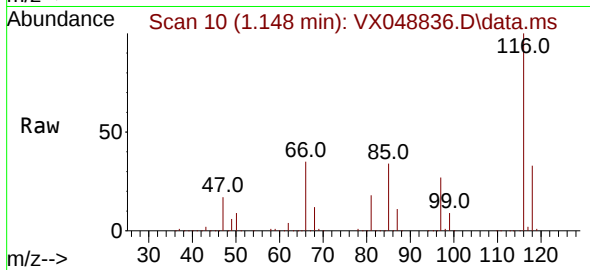

#4

Vinyl Chloride

Concen: 6.134 ug/l

RT: 1.380 min Scan# 48

Delta R.T. -0.000 min

Lab File: VX048836.D




Acq: 11 Dec 2025 18:44


Tgt Ion: 62 Resp: 14515

Ion Ratio Lower Upper

62 100

64 30.8 26.0 39.0


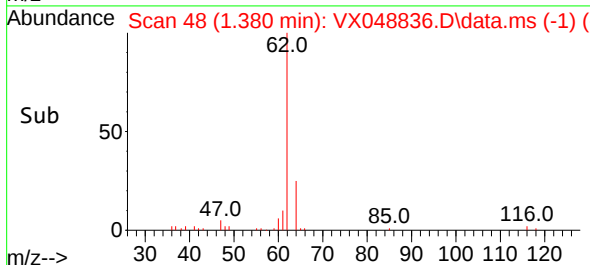

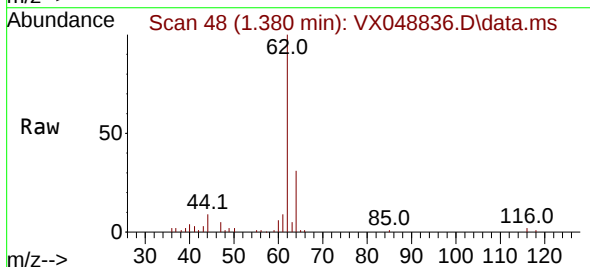




#7
Trichlorofluoromethane
Concen: 2.413 ug/l
RT: 2.142 min Scan# 11
Delta R.T. 0.244 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44




Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925


Tgt Ion:101 Resp: 8183
Ion Ratio Lower Upper
101 100
103 67.4 53.4 80.2

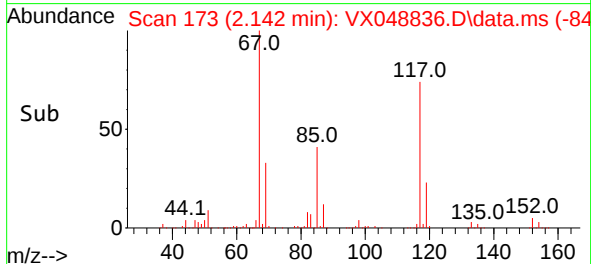

#8
Diethyl Ether
Concen: 0.506 ug/l
RT: 2.136 min Scan# 172
Delta R.T. -0.000 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Tgt Ion: 74 Resp: 685
Ion Ratio Lower Upper
74 100
45 207.7 48.9 146.8#







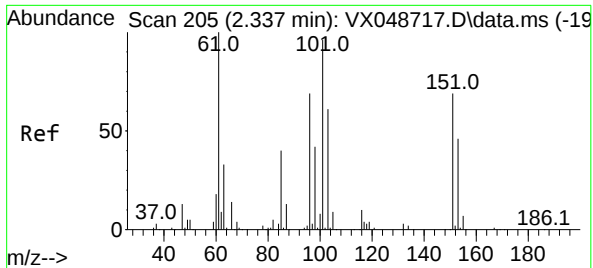

#9
1,1,2-Trichlorotrifluoroethane
Concen: 1802.023 ug/l
RT: 2.337 min Scan# 205
Delta R.T. -0.000 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44




Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925


Tgt Ion:101 Resp: 3543073
Ion Ratio Lower Upper
101 100
85 44.2 34.2 51.2
151 76.7 60.2 90.4

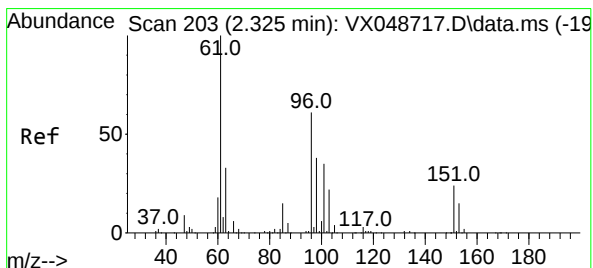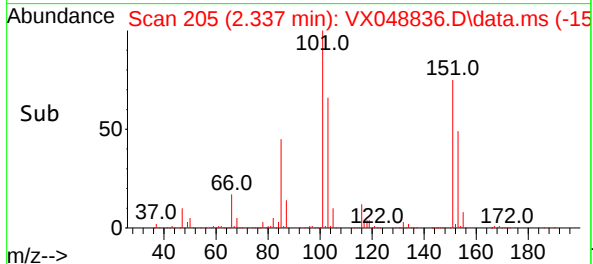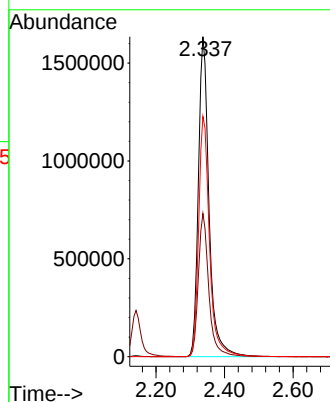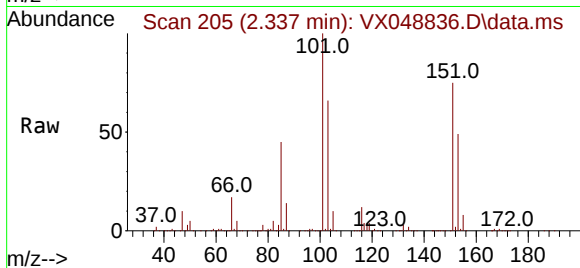

#12
1,1-Dichloroethene
Concen: 10.792 ug/l
RT: 2.331 min Scan# 204
Delta R.T. 0.006 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Tgt Ion: 96 Resp: 21657
Ion Ratio Lower Upper
96 100
61 125.3 130.7 196.1#
98 52.1 49.8 74.8


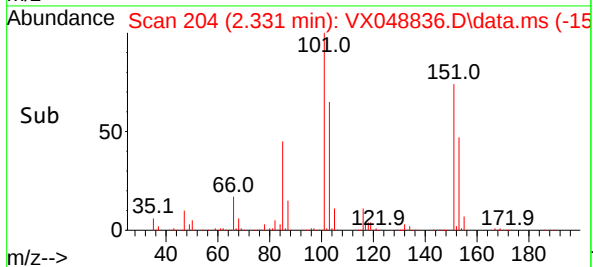
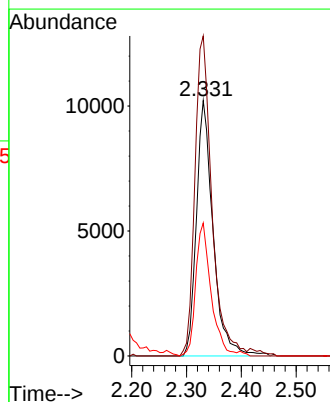
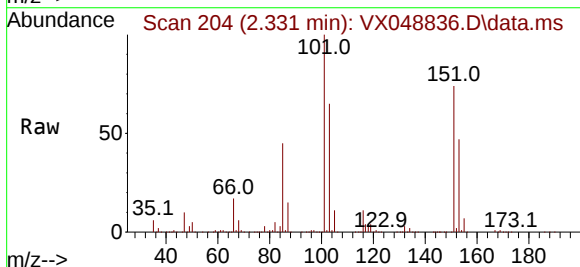




#13
Acrolein
Concen: 40.593 ug/l
RT: 2.142 min Scan# 11
Delta R.T. -0.092 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44




Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925


Tgt Ion: 56 Resp: 179
Ion Ratio Lower Upper
56 100
55 0.0 55.8 83.6#

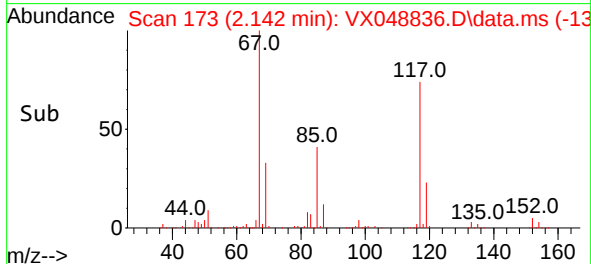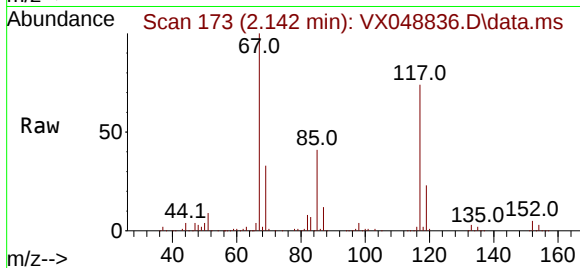

#16
Acetone
Concen: 40.257 ug/l
RT: 2.337 min Scan# 205
Delta R.T. -0.037 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Tgt Ion: 43 Resp: 35746
Ion Ratio Lower Upper
43 100
58 25.4 25.0 37.4




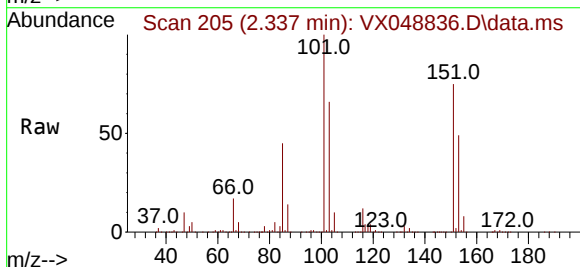




#17
Carbon Disulfide
Concen: 0.237 ug/l
RT: 2.520 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44




Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925


Tgt Ion: 76 Resp: 1384
Ion Ratio Lower Upper
76 100
78 17.1 7.4 11.2#

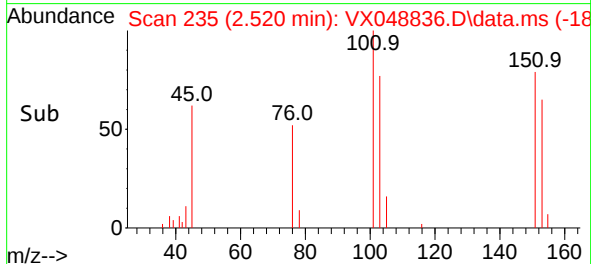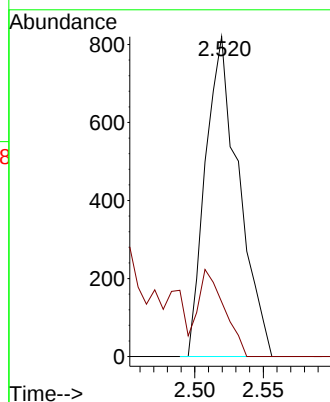

#20
Methylene Chloride
Concen: 0.243 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.006 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Tgt Ion: 84 Resp: 539
Ion Ratio Lower Upper
84 100
49 114.1 98.7 148.1
51 55.0 29.4 44.2#
86 58.1 52.5 78.7









#21
trans-1,2-Dichloroethene
Concen: 1.665 ug/l
RT: 3.093 min Scan# 31
Delta R.T. -0.000 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44




Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925


Tgt Ion: 96 Resp: 3411
Ion Ratio Lower Upper
96 100
61 147.5 112.8 169.2
98 63.3 51.0 76.4

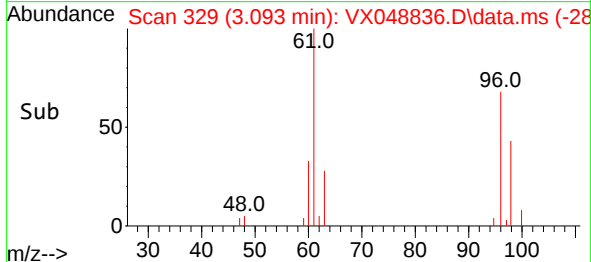

#24
1,1-Dichloroethane
Concen: 44.788 ug/l
RT: 3.611 min Scan# 414
Delta R.T. 0.006 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Tgt Ion: 63 Resp: 157265
Ion Ratio Lower Upper
63 100
98 6.6 3.5 10.6
100 4.6 2.5 7.4

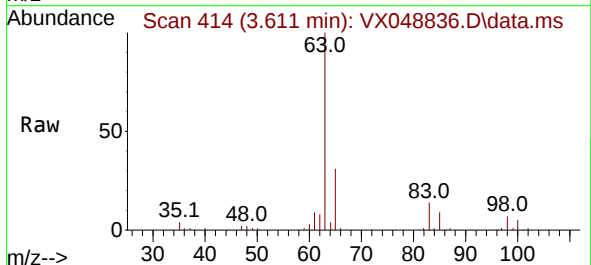







#27
 cis-1,2-Dichloroethene
 Concen: 1395.335 ug/l
 RT: 4.483 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: VX048836.D
 Acq: 11 Dec 2025 18:44

Instrument :
 MSVOA_X
 ClientSampleId :
 RMW-03B-90-120925

Tgt Ion: 96 Resp: 3224871




Ion	Ratio	Lower	Upper
96	100		
61	126.7	0.0	271.0
98	64.5	0.0	130.2

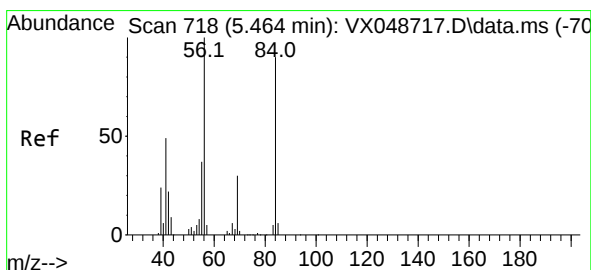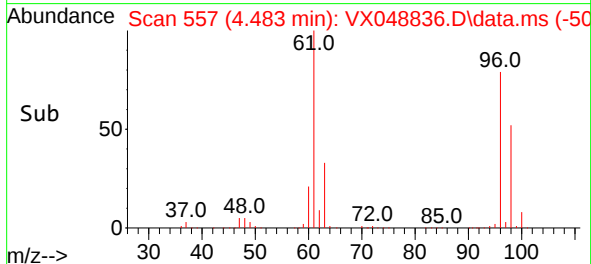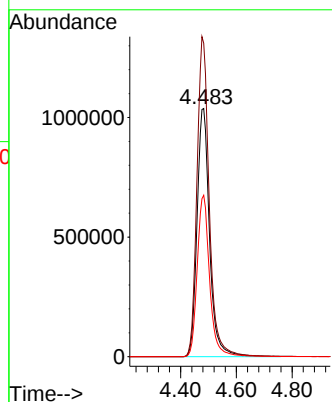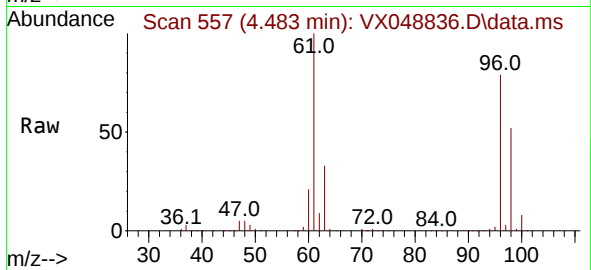


#31
 Cyclohexane
 Concen: 1.106 ug/l
 RT: 5.525 min Scan# 728
 Delta R.T. 0.061 min
 Lab File: VX048836.D
 Acq: 11 Dec 2025 18:44

Tgt Ion: 56 Resp: 3466

Ion	Ratio	Lower	Upper
56	100		
69	196.3	24.2	36.2#
84	124.1	72.1	108.1#

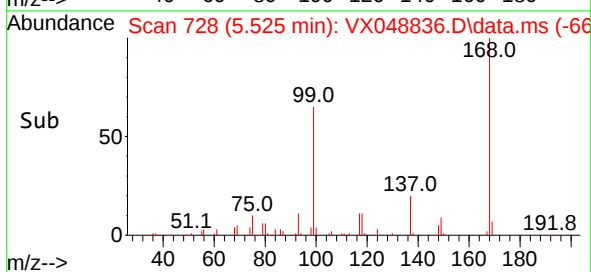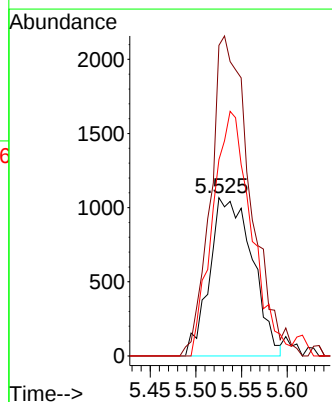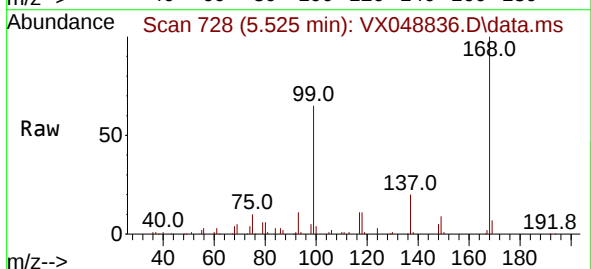



#33

1,2-Dichloroethane-d4

Concen: 53.406 ug/l

RT: 5.940 min Scan# 796

Delta R.T. -0.000 min

Lab File: VX048836.D

Acq: 11 Dec 2025 18:44

Instrument :

MSVOA_X

ClientSampleId :





RMW-03B-90-120925

Tgt Ion: 65 Resp: 123876

Ion Ratio Lower Upper

65 100

67 52.0 0.0 107.4

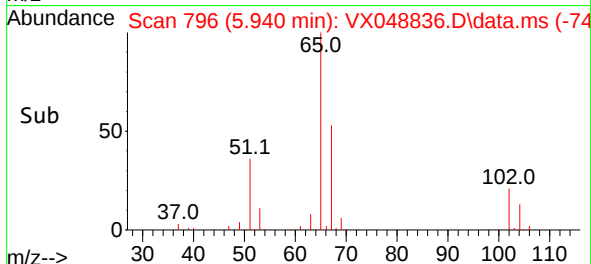

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.744 min Scan# 928

Delta R.T. -0.000 min

Lab File: VX048836.D

Acq: 11 Dec 2025 18:44




Tgt Ion: 114 Resp: 291968


Ion Ratio Lower Upper

114 100

63 20.8 0.0 39.0

88 15.6 0.0 31.8

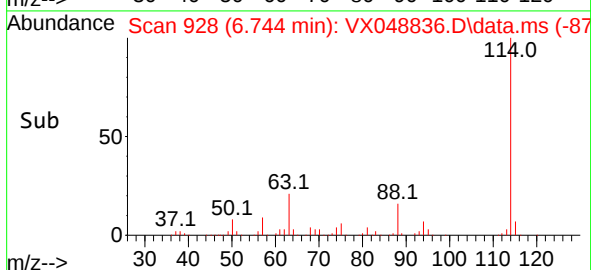

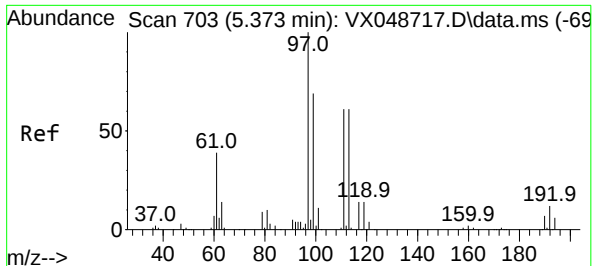

#35

Dibromofluoromethane

Concen: 47.133 ug/l

RT: 5.379 min Scan# 703

Delta R.T. 0.006 min

Lab File: VX048836.D


Acq: 11 Dec 2025 18:44

Instrument :




MSVOA_X

ClientSampleId :

RMW-03B-90-120925

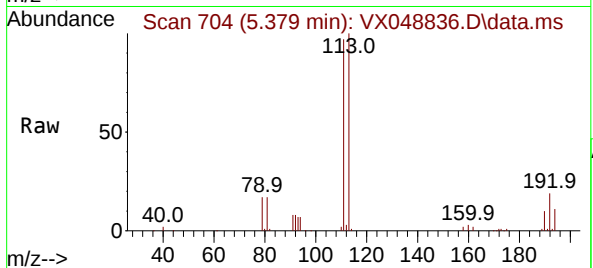

Tgt Ion:	113	Resp:	94752
Ion	Ratio	Lower	Upper
113	100		
111	103.9	79.5	119.3
192	19.4	16.1	24.1

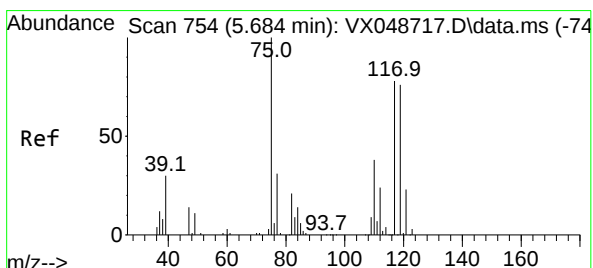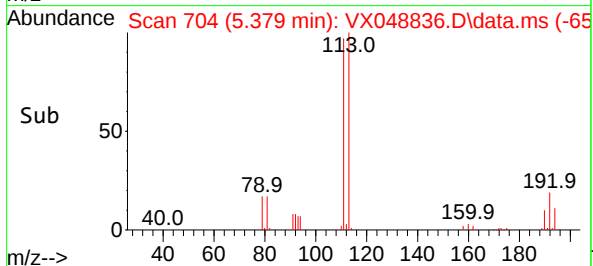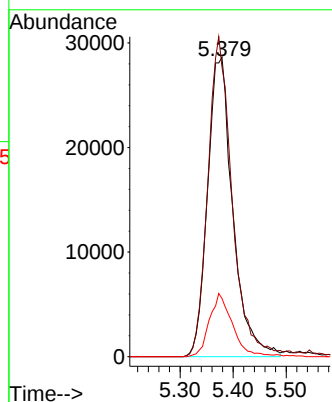

#36

1,1-Dichloropropene

Concen: 4.886 ug/l




RT: 5.537 min Scan# 730


Delta R.T. -0.147 min

Lab File: VX048836.D

Acq: 11 Dec 2025 18:44

Tgt Ion:	75	Resp:	13452
Ion	Ratio	Lower	Upper
75	100		
110	4.8	18.6	55.8#
77	0.0	25.3	37.9#


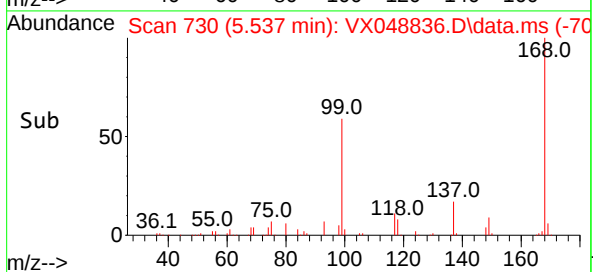
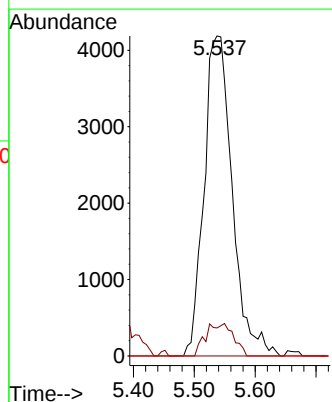
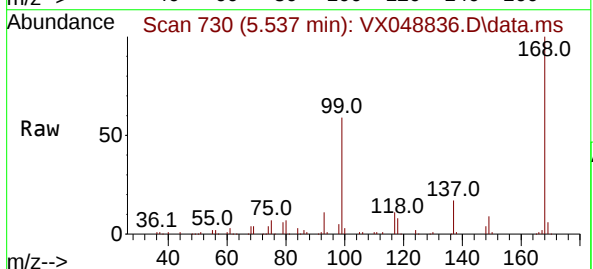




#38
Carbon Tetrachloride
Concen: 5.820 ug/l
RT: 5.537 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44




Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925


Tgt Ion:117 Resp: 18150
Ion Ratio Lower Upper
117 100
119 4.4 80.5 120.7#
121 0.0 25.4 38.0#

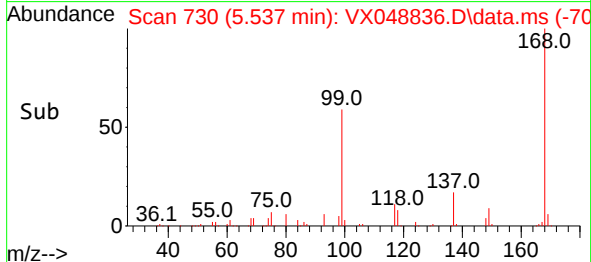

#39
Methylcyclohexane
Concen: 9.324 ug/l
RT: 7.110 min Scan# 988
Delta R.T. -0.256 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Tgt Ion: 83 Resp: 30358
Ion Ratio Lower Upper
83 100
55 0.0 60.6 90.8#
98 206.1 39.3 58.9#


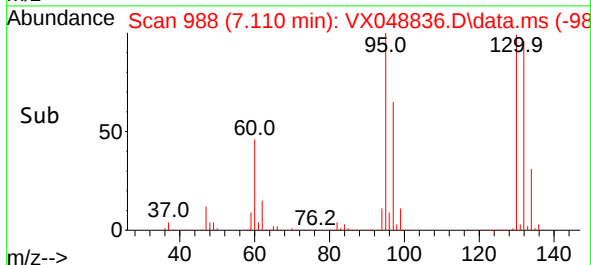
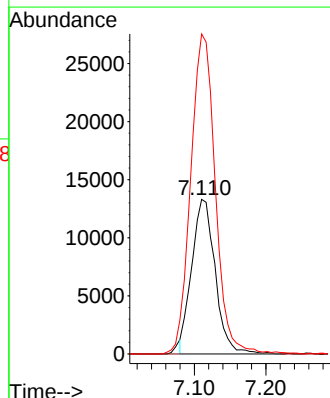
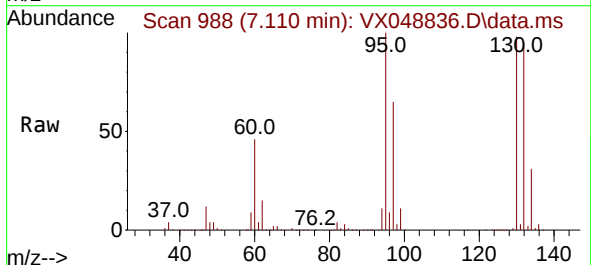




#40
Benzene
Concen: 3.240 ug/l
RT: 6.025 min Scan# 810
Delta R.T. -0.000 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44




Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925


Tgt Ion: 78 Resp: 26446
Ion Ratio Lower Upper
78 100
77 23.6 18.8 28.2

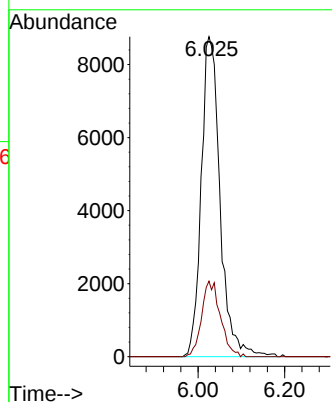

#42
1,2-Dichloroethane
Concen: 3.017 ug/l
RT: 6.080 min Scan# 819
Delta R.T. 0.006 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Tgt Ion: 62 Resp: 8717
Ion Ratio Lower Upper
62 100
98 9.9 0.0 20.2


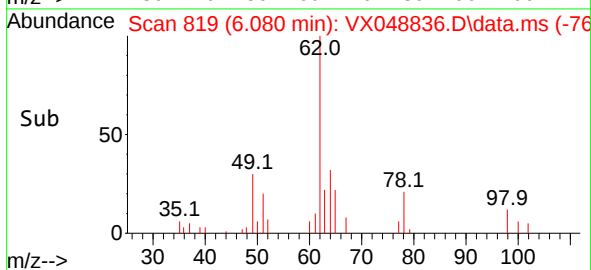
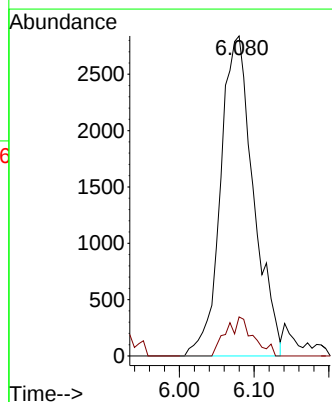





#44
Trichloroethene
Concen: 1200.604 ug/l
RT: 7.116 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44




Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925


Tgt Ion:130 Resp: 2557014
Ion Ratio Lower Upper
130 100
95 100.2 0.0 189.6

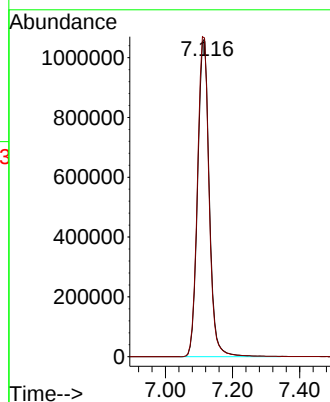

#49
1,4-Dioxane
Concen: 6.731 ug/l
RT: 7.653 min Scan# 1077
Delta R.T. 0.012 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Tgt Ion: 88 Resp: 232
Ion Ratio Lower Upper
88 100
43 35.3 28.6 43.0
58 38.8 58.0 87.0#


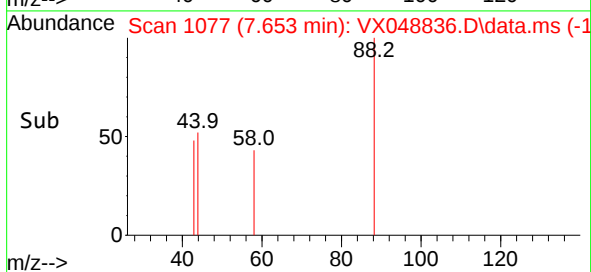
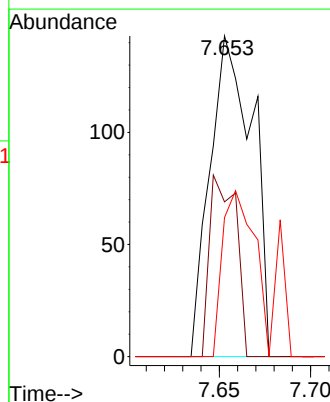
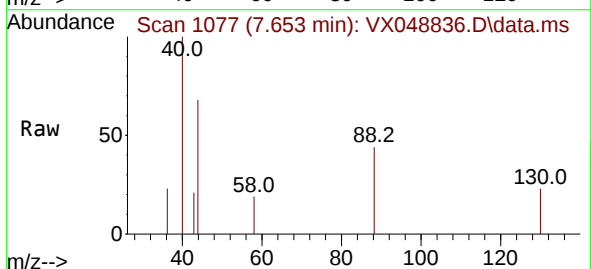




#50
Toluene-d8
Concen: 48.267 ug/l
RT: 8.634 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44




Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925


Tgt Ion: 98 Resp: 340129
Ion Ratio Lower Upper
98 100
100 65.2 53.4 80.0

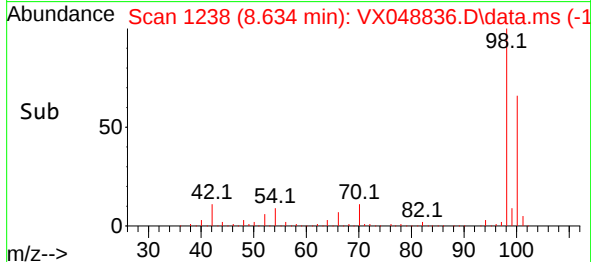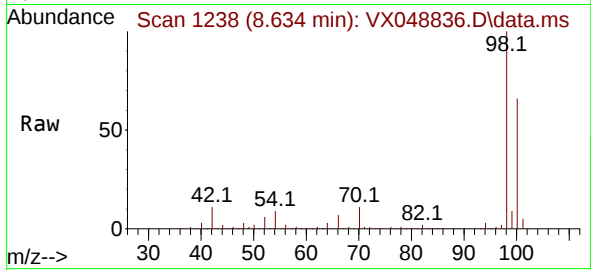

#51
4-Methyl-2-Pentanone
Concen: 0.521 ug/l
RT: 8.628 min Scan# 1237
Delta R.T. 0.073 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Tgt Ion: 43 Resp: 1610
Ion Ratio Lower Upper
43 100
58 167.6 32.2 48.4#

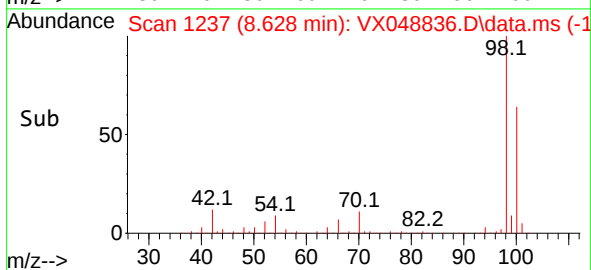

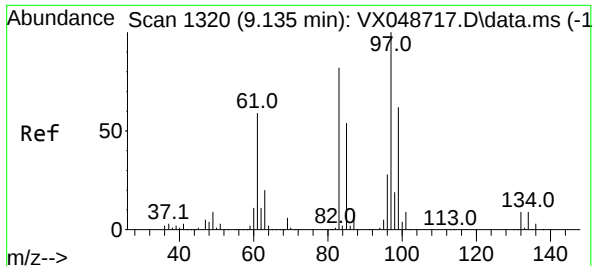

#55

1,1,2-Trichloroethane

Concen: 0.408 ug/l

RT: 9.140 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX048836.D

Acq: 11 Dec 2025 18:44

Instrument :

MSVOA_X

ClientSampleId :

RMW-03B-90-120925

Tgt Ion: 97 Resp: 808





Ion Ratio Lower Upper

97 100

83 75.0 66.0 99.0

85 87.1 43.2 64.8#

99 56.9 50.0 75.0

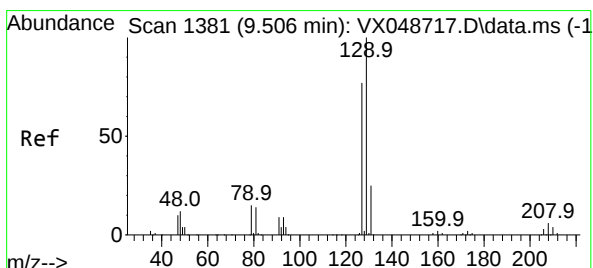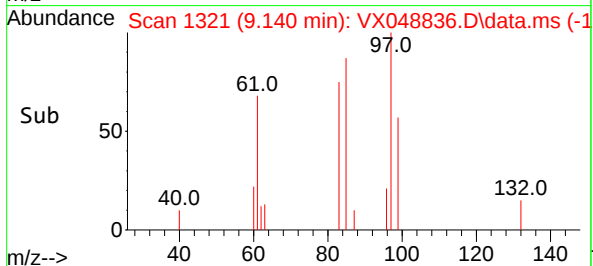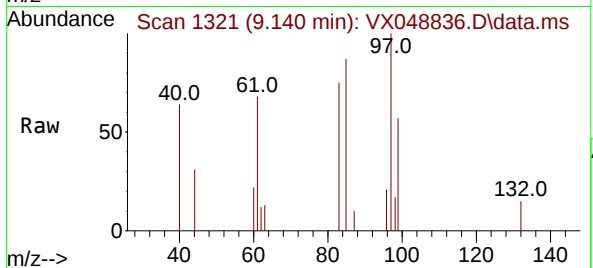

#60

Dibromochloromethane

Concen: 5.687 ug/l

RT: 9.256 min Scan# 1340

Delta R.T. -0.250 min

Lab File: VX048836.D




Acq: 11 Dec 2025 18:44


Tgt Ion: 129 Resp: 13927

Ion Ratio Lower Upper

129 100

127 0.0 38.3 114.9#


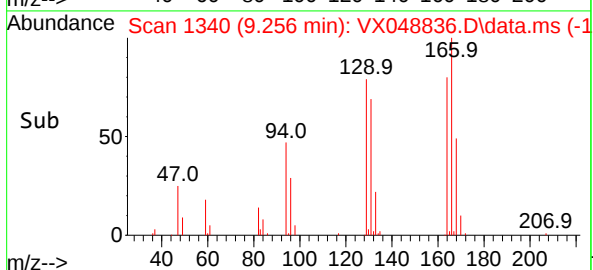

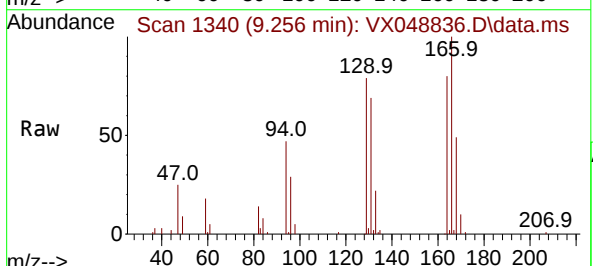




#62
4-Bromofluorobenzene
Concen: 48.839 ug/l
RT: 11.061 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44




Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925


Tgt Ion: 95 Resp: 118676
Ion Ratio Lower Upper
95 100
174 81.2 0.0 157.8
176 78.2 0.0 154.0

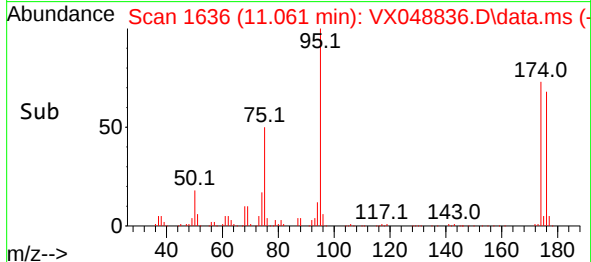

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Tgt Ion: 117 Resp: 260001
Ion Ratio Lower Upper
117 100
82 55.8 44.1 66.1
119 32.4 25.2 37.8

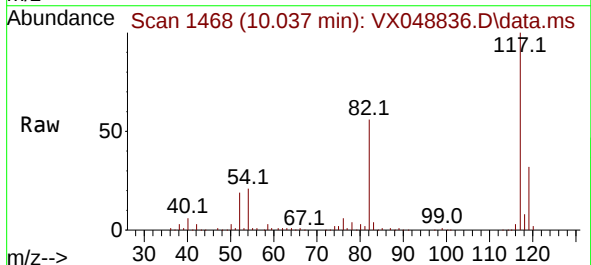







#64
Tetrachloroethene
Concen: 7.588 ug/l
RT: 9.256 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925

Tgt Ion:164 Resp: 14381




Ion	Ratio	Lower	Upper
164	100		
166	124.7	103.1	154.7
129	98.4	76.9	115.3
131	86.4	75.1	112.7

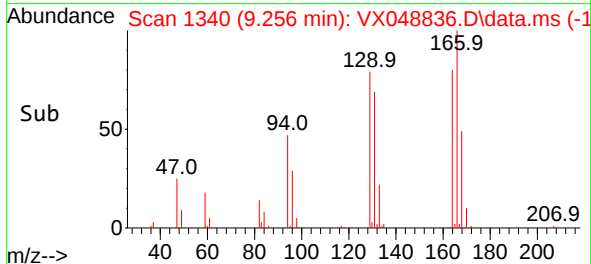


#68
m/p-Xylenes
Concen: 0.223 ug/l
RT: 10.280 min Scan# 1508
Delta R.T. -0.000 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Tgt Ion:106 Resp: 807

Ion	Ratio	Lower	Upper
106	100		
91	245.7	164.2	246.4









#69
o-Xylene
Concen: 0.232 ug/l
RT: 10.628 min Scan# 1564
Delta R.T. 0.006 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44




Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925


Tgt Ion:106 Resp: 787
Ion Ratio Lower Upper
106 100
91 241.8 108.1 324.3

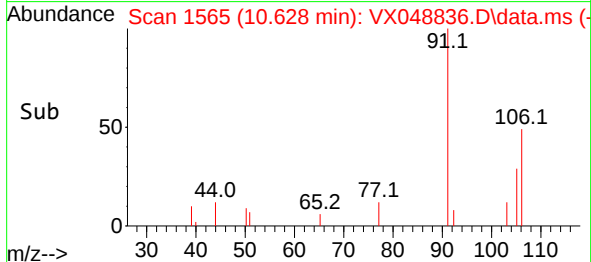

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Tgt Ion:152 Resp: 125510
Ion Ratio Lower Upper
152 100
115 58.8 42.1 126.4
150 158.7 0.0 347.8


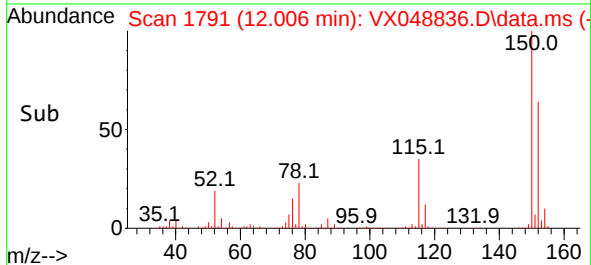






#76
1,2,3-Trichloropropane
Concen: 25.684 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.159 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44




Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925


Tgt Ion: 75 Resp: 60041
Ion Ratio Lower Upper
75 100
77 1.1 24.3 73.0#

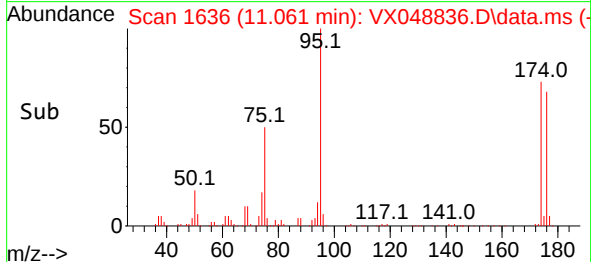

#81
trans-1,4-Dichloro-2-butene
Concen: 61.010 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. 0.061 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Tgt Ion: 75 Resp: 60041
Ion Ratio Lower Upper
75 100
53 0.0 79.9 119.9#
89 0.0 67.1 100.7#




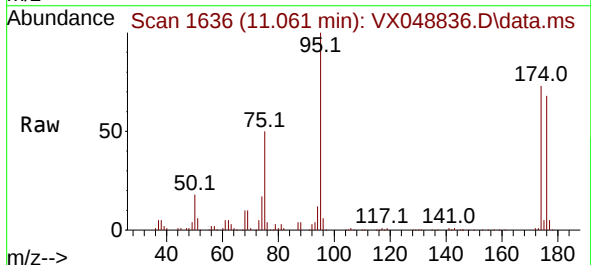




#88
1,4-Dichlorobenzene
Concen: 0.446 ug/l
RT: 12.018 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44




Instrument :
MSVOA_X
ClientSampleId :
RMW-03B-90-120925


Tgt Ion:146 Resp: 1917
Ion Ratio Lower Upper
146 100
111 133.6 19.6 58.7#
148 92.5 31.6 94.7

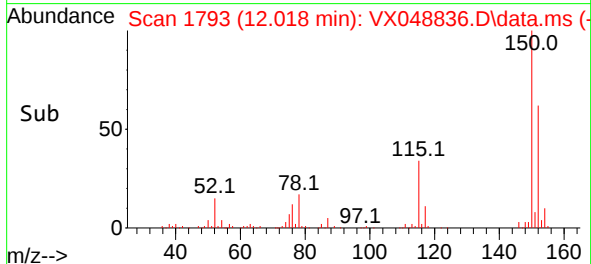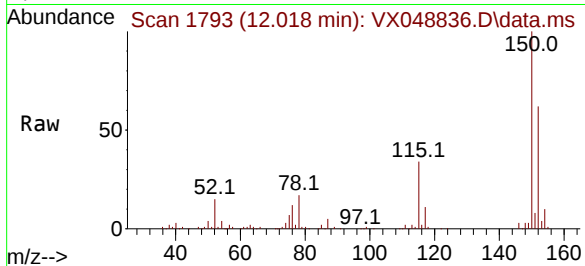

#91
1,2-Dichlorobenzene
Concen: 0.698 ug/l
RT: 12.317 min Scan# 1842
Delta R.T. -0.000 min
Lab File: VX048836.D
Acq: 11 Dec 2025 18:44

Tgt Ion:146 Resp: 2816
Ion Ratio Lower Upper
146 100
111 41.8 20.8 62.5
148 69.6 32.0 96.0

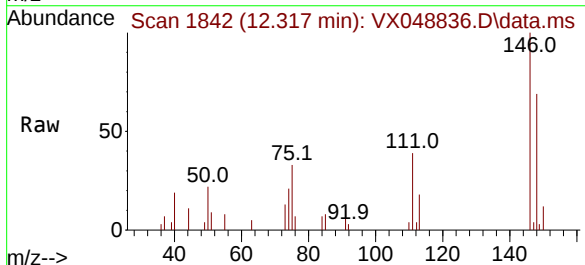



#95

Naphthalene

Concen: Below Cal

RT: 13.786 min Scan# 20

Delta R.T. 0.030 min

Lab File: VX048836.D


Acq: 11 Dec 2025 18:44

Instrument :

MSVOA_X

ClientSampleId :

RMW-03B-90-120925

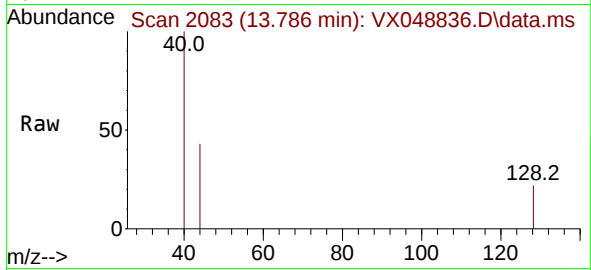

Tgt Ion:128 Resp: 137

Ion Ratio Lower Upper

128 100

127 0.0 10.2 15.2#

129 0.0 8.6 13.0#

