


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX121218\
Data File : VX006436.D
Acq On : 12 Dec 2018 09:53
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
Title : SW846 8260
Last Update : Fri Nov 30 03:55:33 2018

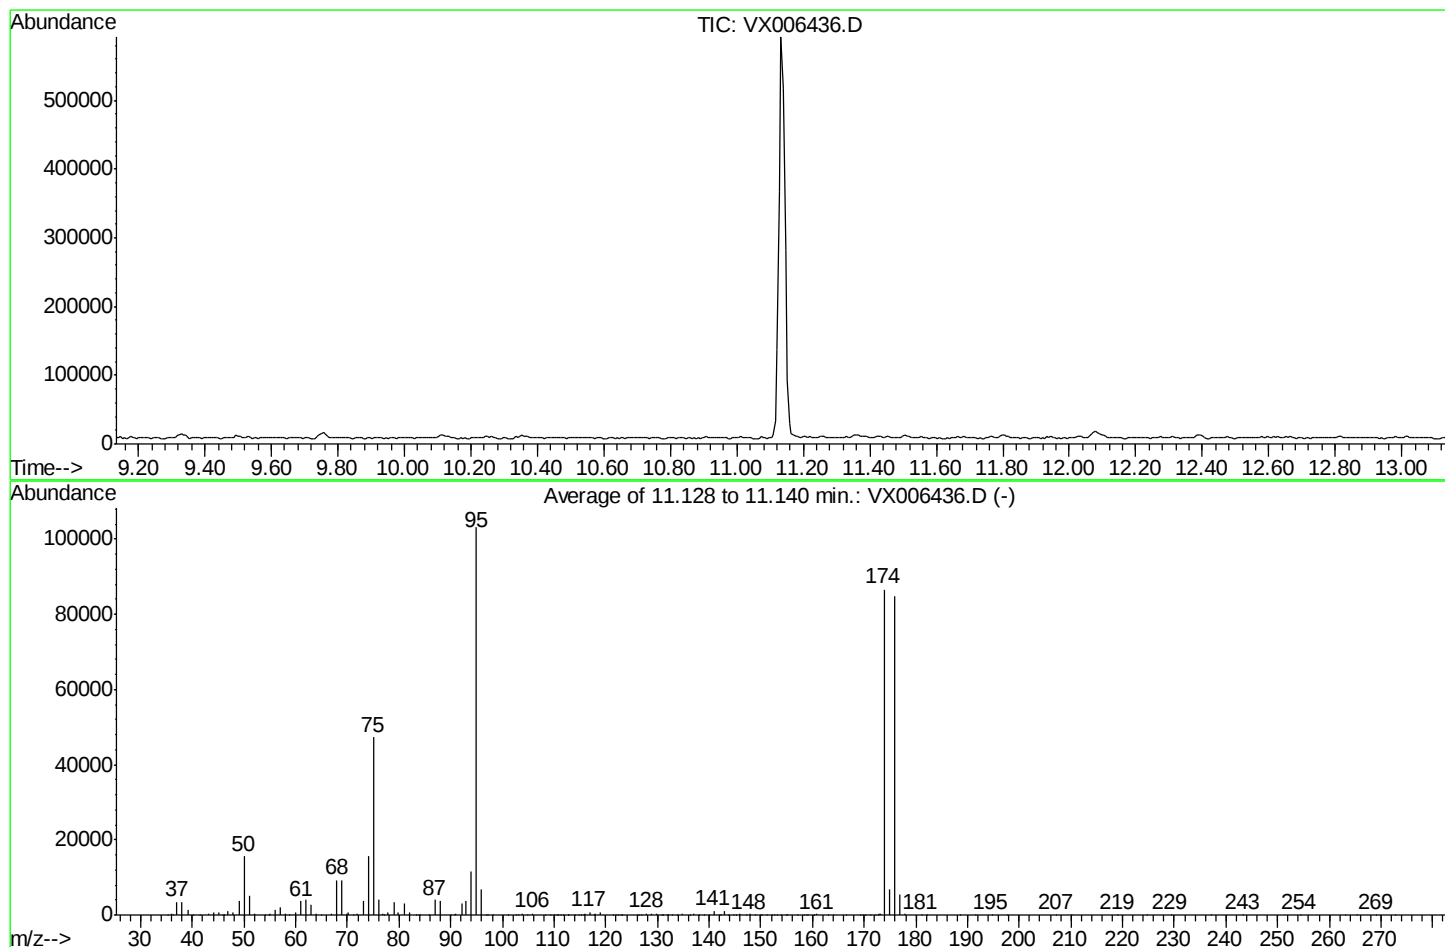

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	15623	PASS
75	95	30	60	45.7	47186	PASS
95	95	100	100	100.0	103146	PASS
96	95	5	9	6.7	6926	PASS
173	174	0.00	2	0.5	438	PASS
174	95	50	100	83.9	86549	PASS
175	174	5	9	7.8	6727	PASS
176	174	95	101	98.1	84941	PASS
177	176	5	9	6.6	5592	PASS