


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX121219\
 Data File : VX013990.D
 Acq On : 12 Dec 2019 21:48
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X121219W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Dec 13 01:35:34 2019

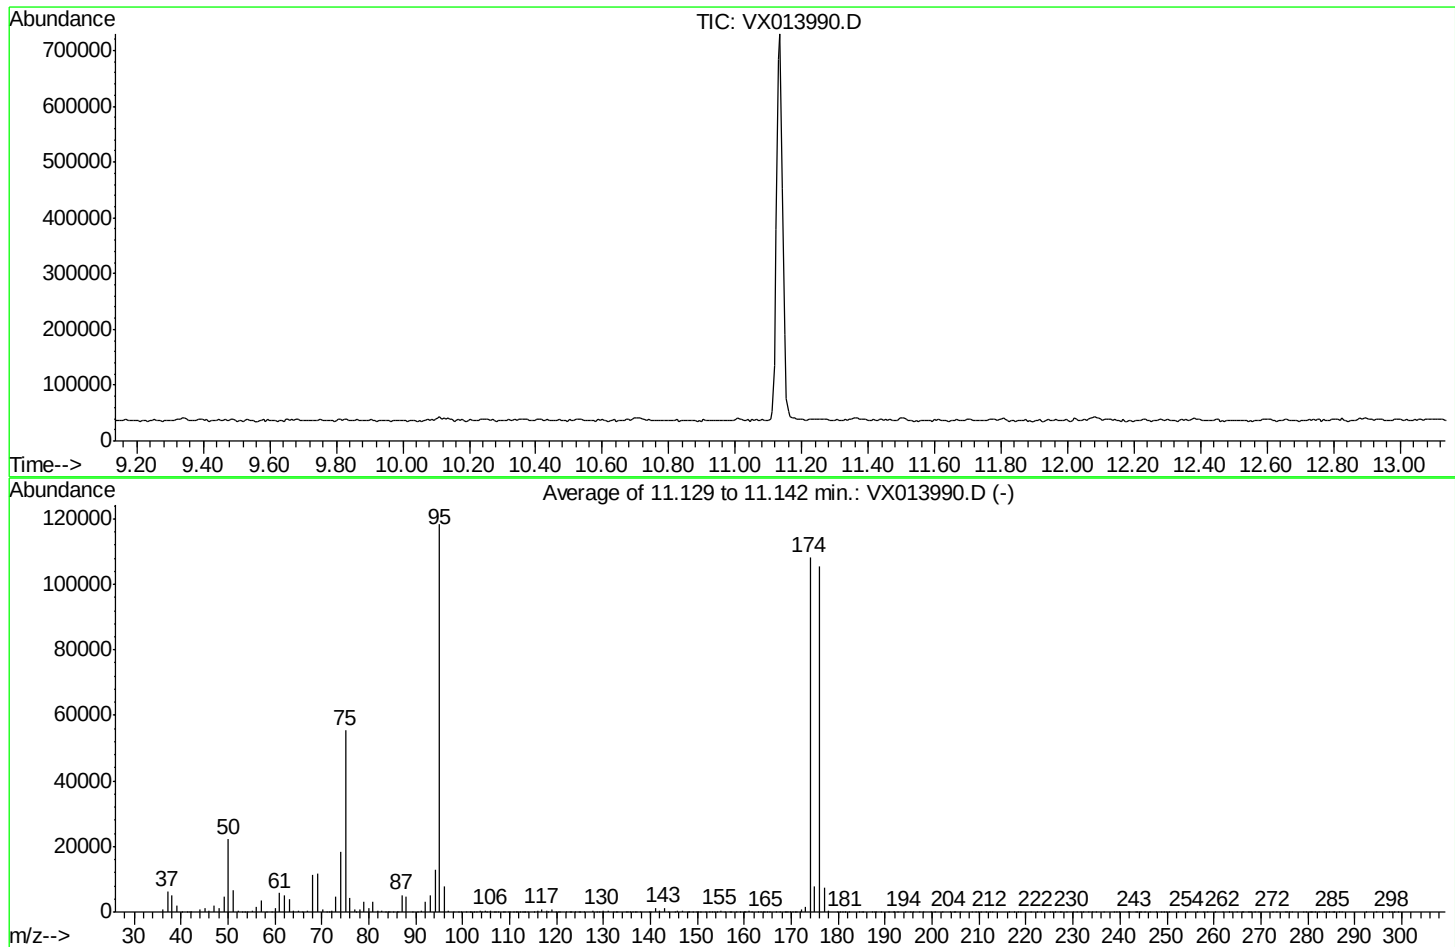

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1675

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	22162	PASS
75	95	30	60	46.7	55314	PASS
95	95	100	100	100.0	118319	PASS
96	95	5	9	6.6	7795	PASS
173	174	0.00	2	1.3	1448	PASS
174	95	50	100	91.3	108082	PASS
175	174	5	9	7.1	7639	PASS
176	174	95	101	97.5	105385	PASS
177	176	5	9	6.9	7289	PASS