
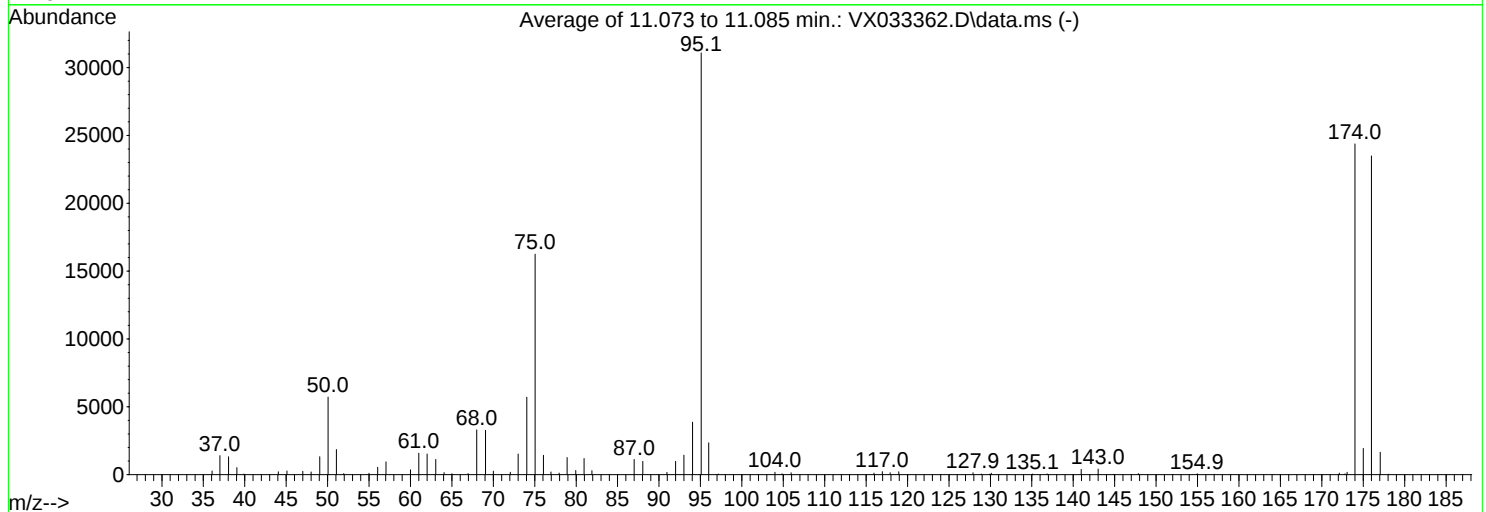


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121222\
 Data File : VX033362.D
 Acq On : 12 Dec 2022 10:08
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X121222W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Mon Dec 12 12:37:35 2022

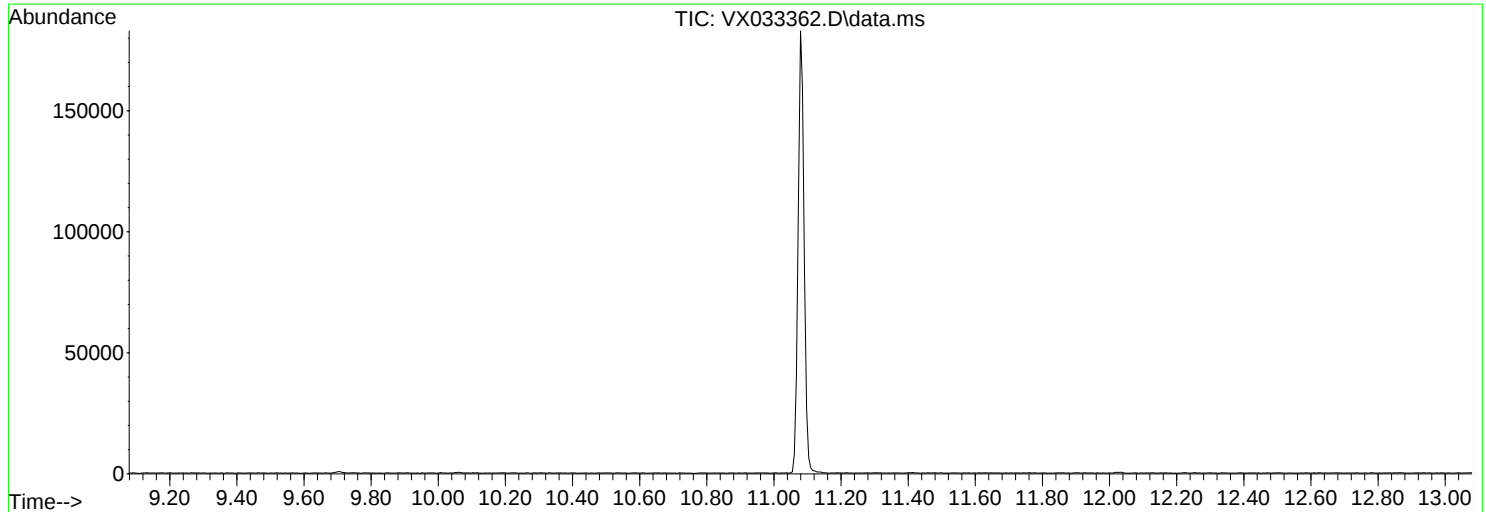

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	5720	PASS
75	95	30	60	52.3	16254	PASS
95	95	100	100	100.0	31085	PASS
96	95	5	9	7.5	2342	PASS
173	174	0.00	2	0.7	177	PASS
174	95	50	100	78.4	24370	PASS
175	174	5	9	8.0	1940	PASS
176	174	95	101	96.4	23492	PASS
177	176	5	9	7.0	1652	PASS