

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121223\
 Data File : VX039155.D
 Acq On : 12 Dec 2023 10:38
 Operator : JC/MD
 Sample : VX1212MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1212MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M

Title : SW846 8260

Signal : TIC: VX039155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.379	693	704	721	rBV	78184	228275	31.21%	5.634%
2	5.544	721	731	746	rVB2	119999	344488	47.10%	8.502%
3	5.952	788	798	814	rBV	93222	246088	33.65%	6.073%
4	6.757	920	930	951	rBV	217297	524744	71.75%	12.950%
5	8.647	1233	1240	1258	rBV	459641	731391	100.00%	18.050%
6	10.049	1465	1470	1487	rBV	502780	702221	96.01%	17.330%
7	11.079	1634	1639	1655	rBV	424841	545850	74.63%	13.471%
8	12.018	1788	1793	1812	rVB	537223	713918	97.61%	17.619%
9	13.585	2046	2050	2056	rVB2	5556	7410	1.01%	0.183%
10	13.780	2076	2082	2089	rVB	5602	7576	1.04%	0.187%




Sum of corrected areas: 4051961

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121223\
Data File : VX039155.D
Acq On : 12 Dec 2023 10:38
Operator : JC/MD
Sample : VX1212MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

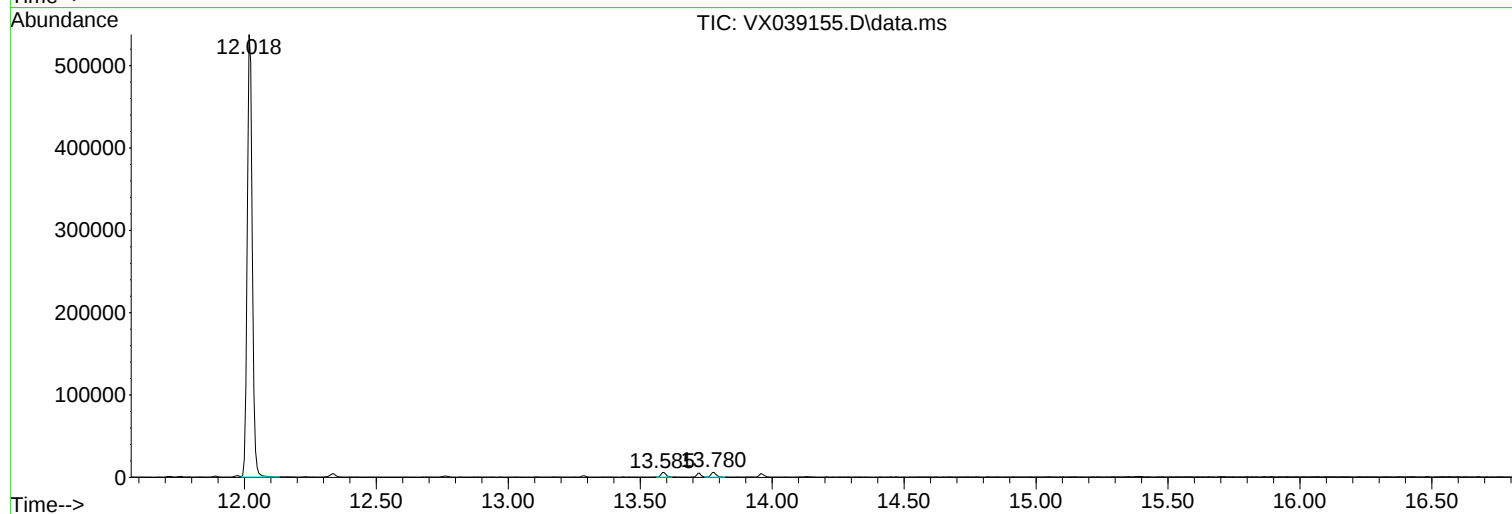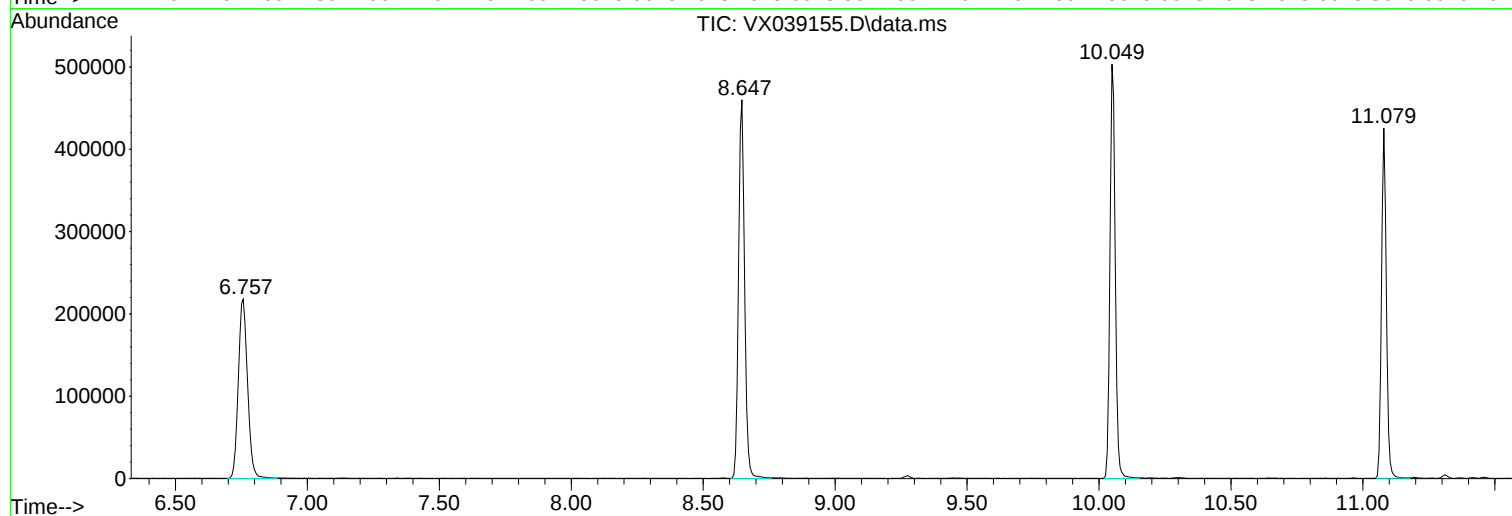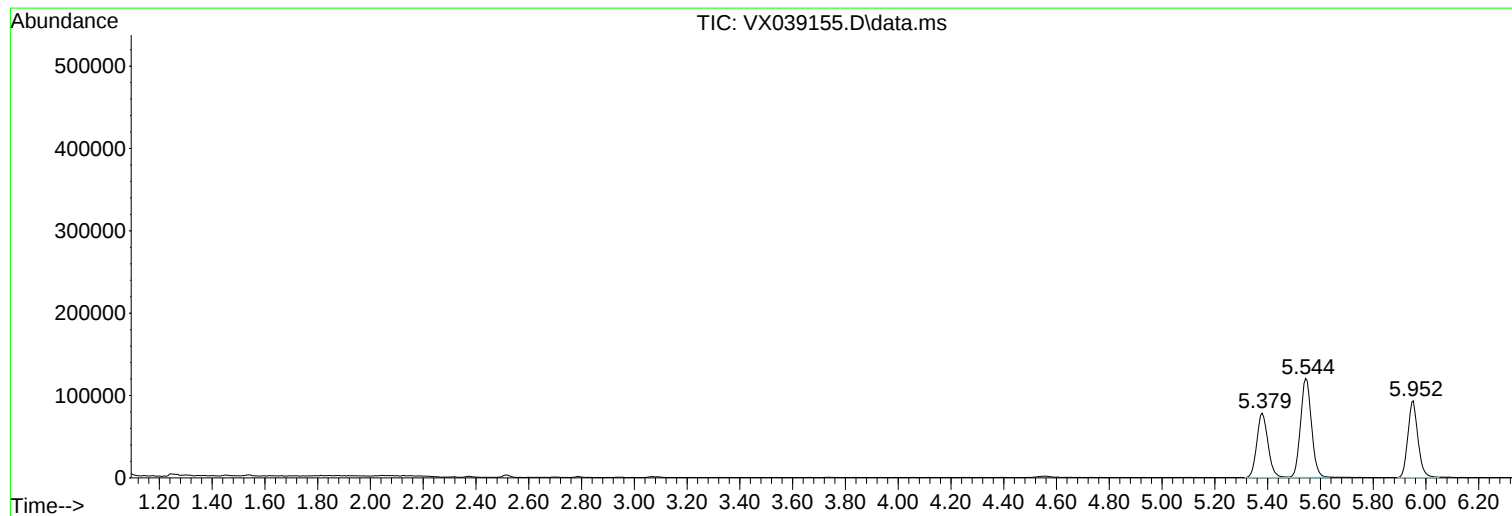

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121223\
Data File : VX039155.D
Acq On : 12 Dec 2023 10:38
Operator : JC/MD
Sample : VX1212MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121223\
Data File : VX039155.D
Acq On : 12 Dec 2023 10:38
Operator : JC/MD
Sample : VX1212MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc