
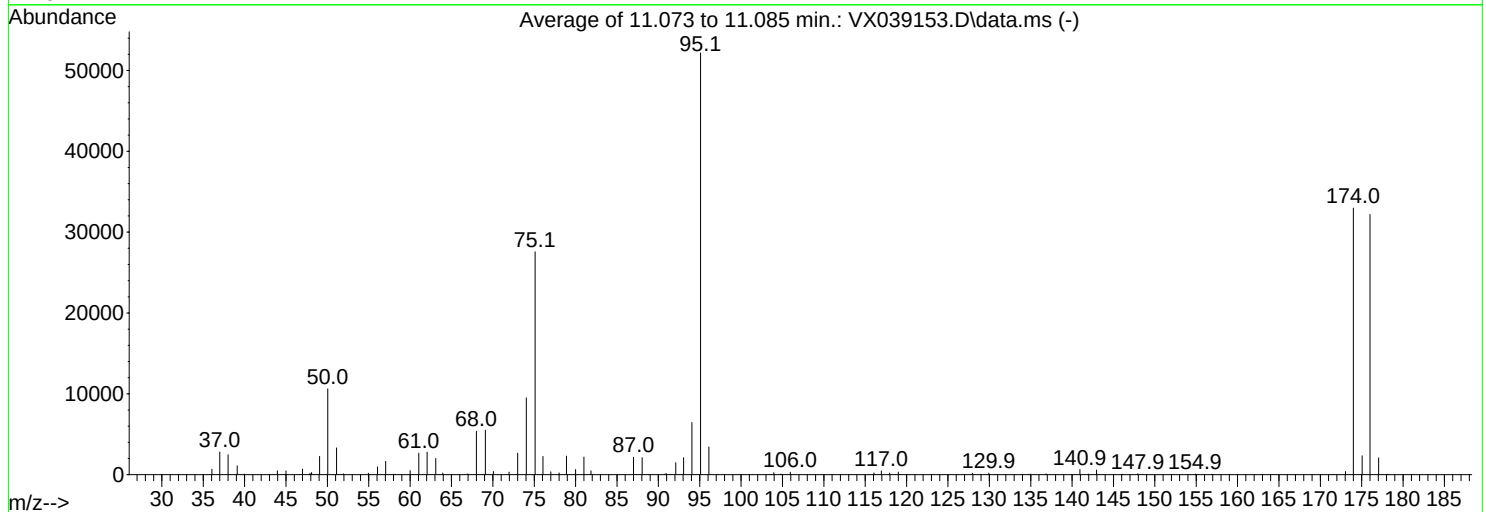


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121223\
Data File : VX039153.D
Acq On : 12 Dec 2023 08:22
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Title : SW846 8260
Last Update : Thu Nov 16 22:59:22 2023

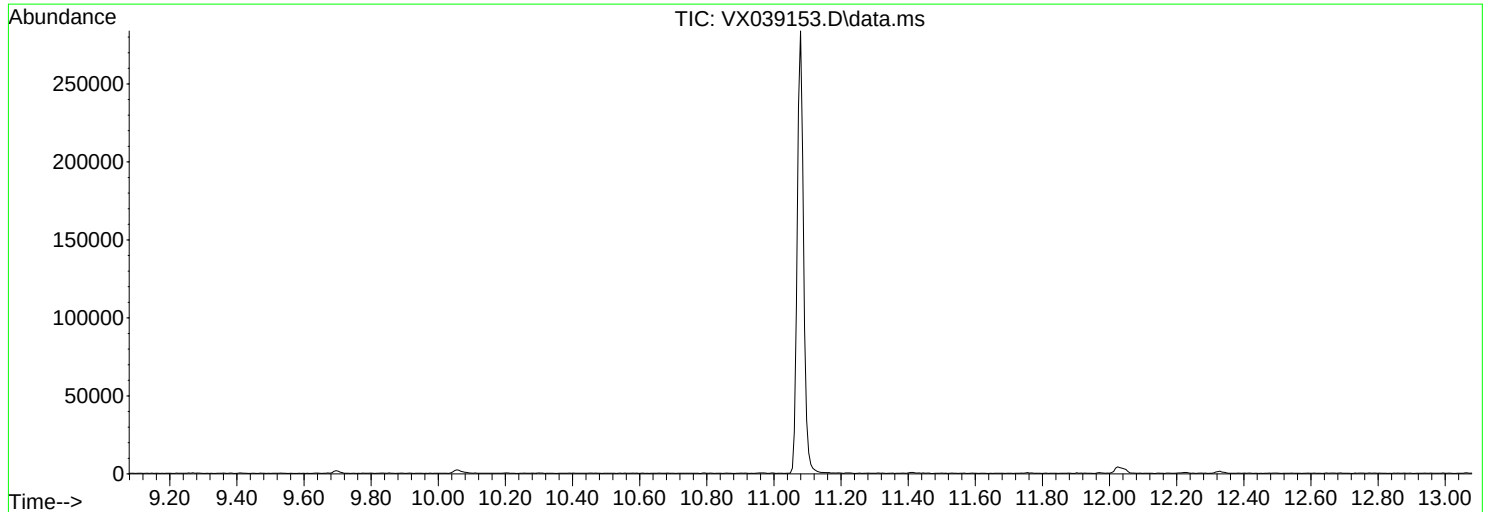

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.4	10621	PASS
75	95	30	60	52.9	27581	PASS
95	95	100	100	100.0	52181	PASS
96	95	5	9	6.6	3419	PASS
173	174	0.00	2	1.2	381	PASS
174	95	50	100	63.2	32973	PASS
175	174	5	9	7.1	2340	PASS
176	174	95	101	97.6	32184	PASS
177	176	5	9	6.4	2072	PASS