


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121224\
Data File : VX044239.D
Acq On : 12 Dec 2024 08:51
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Title : SW846 8260
Last Update : Thu Dec 12 04:28:14 2024

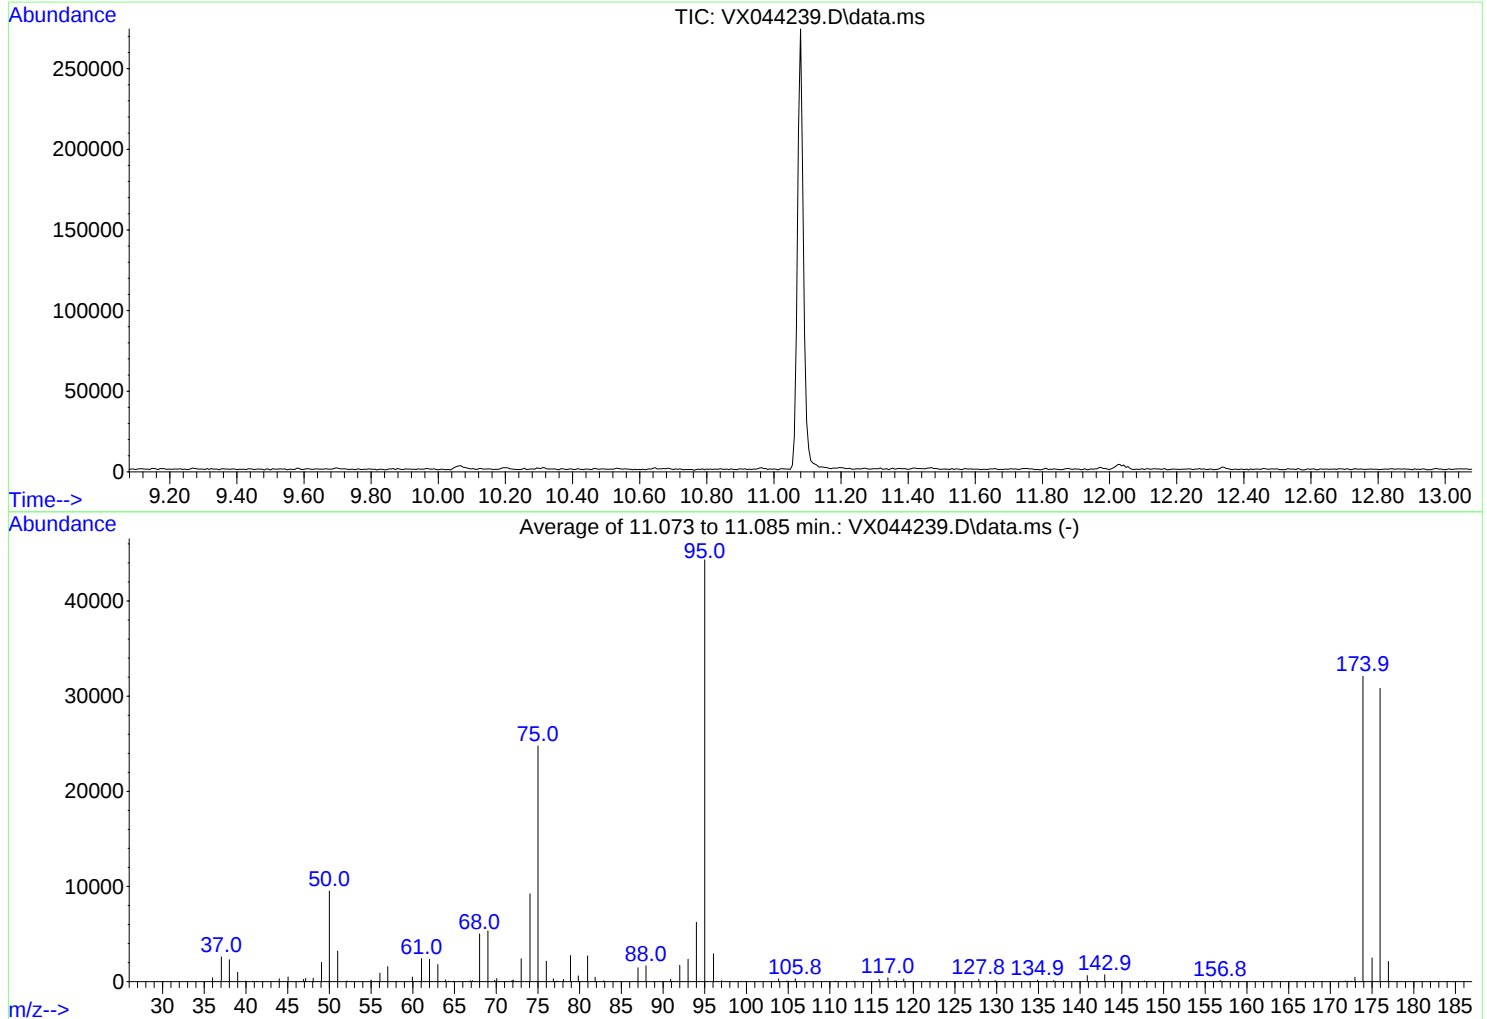

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.5	9525	PASS
75	95	30	60	55.9	24765	PASS
95	95	100	100	100.0	44328	PASS
96	95	5	9	6.6	2935	PASS
173	174	0.00	2	1.5	471	PASS
174	95	50	100	72.4	32085	PASS
175	174	5	9	7.8	2492	PASS
176	174	95	101	96.1	30821	PASS
177	176	5	9	6.9	2113	PASS