

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121225\
 Data File : VX048841.D
 Acq On : 12 Dec 2025 10:09
 Operator : JC/MD
 Sample : VX1212MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1212MBL01

Quant Time: Dec 12 22:08:30 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 05 03:27:34 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.532	168	128949	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.739	114	264334	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	285483	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	147205	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.934	65	90408	52.237	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 104.480%			
35) Dibromofluoromethane	5.367	113	84040	46.175	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 92.340%			
50) Toluene-d8	8.629	98	296092	46.411	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 92.820%			
62) 4-Bromofluorobenzene	11.061	95	126455	57.481	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 114.960%			
Target Compounds						Qvalue
5) Bromomethane	1.630	94	508	0.466	ug/l #	70
9) 1,1,2-Trichlorotrifluo...	2.337	101	365	0.249	ug/l #	75
10) Methyl Iodide	2.471	142	1648	0.789	ug/l #	86
13) Acrolein	2.233	56	329	41.201	ug/l #	79
15) Acrylonitrile	3.056	53	479	0.550	ug/l #	81
16) Acetone	2.368	43	964	1.455	ug/l #	77
17) Carbon Disulfide	2.514	76	1911	0.439	ug/l #	83
18) Methyl Acetate	2.691	43	937	0.503	ug/l #	56
23) Vinyl Acetate	3.715	43	1563	0.396	ug/l #	70
25) 2-Butanone	4.562	43	454	0.464	ug/l #	46
29) Tetrahydrofuran	4.995	42	278	0.372	ug/l #	30
31) Cyclohexane	5.532	56	2411	1.031	ug/l #	18
36) 1,1-Dichloropropene	5.538	75	10320	4.140	ug/l #	48
38) Carbon Tetrachloride	5.532	117	12977	4.596	ug/l #	14
44) Trichloroethene	7.098	130	1081	0.561	ug/l	78
49) 1,4-Dioxane	7.659	88	48	1.538	ug/l #	22
51) 4-Methyl-2-Pentanone	8.562	43	868	0.310	ug/l #	71
58) 2-Chloroethyl Vinyl ether	8.226	63	612	0.403	ug/l #	77
59) 2-Hexanone	9.427	43	561	0.285	ug/l	67
76) 1,2,3-Trichloropropane	11.061	75	64289	23.448	ug/l #	30
81) trans-1,4-Dichloro-2-b...	11.061	75	64289	55.699	ug/l #	3
87) 1,3-Dichlorobenzene	11.951	146	1229	0.252	ug/l	93
88) 1,4-Dichlorobenzene	11.951	146	1229	0.244	ug/l	91
89) n-Butylbenzene	12.317	91	2400	0.292	ug/l	96
90) Hexachloroethane	12.518	117	398	0.222	ug/l	96
91) 1,2-Dichlorobenzene	12.317	146	1078	0.228	ug/l	94
93) 1,2,4-Trichlorobenzene	13.573	180	2197	0.703	ug/l	97
94) Hexachlorobutadiene	13.707	225	877	0.678	ug/l	93
95) Naphthalene	13.762	128	3505	Below Cal		99
96) 1,2,3-Trichlorobenzene	13.945	180	2068	0.717	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121225\
Data File : VX048841.D
Acq On : 12 Dec 2025 10:09
Operator : JC/MD
Sample : VX1212MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01

Quant Time: Dec 12 22:08:30 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 05 03:27:34 2025
Response via : Initial Calibration




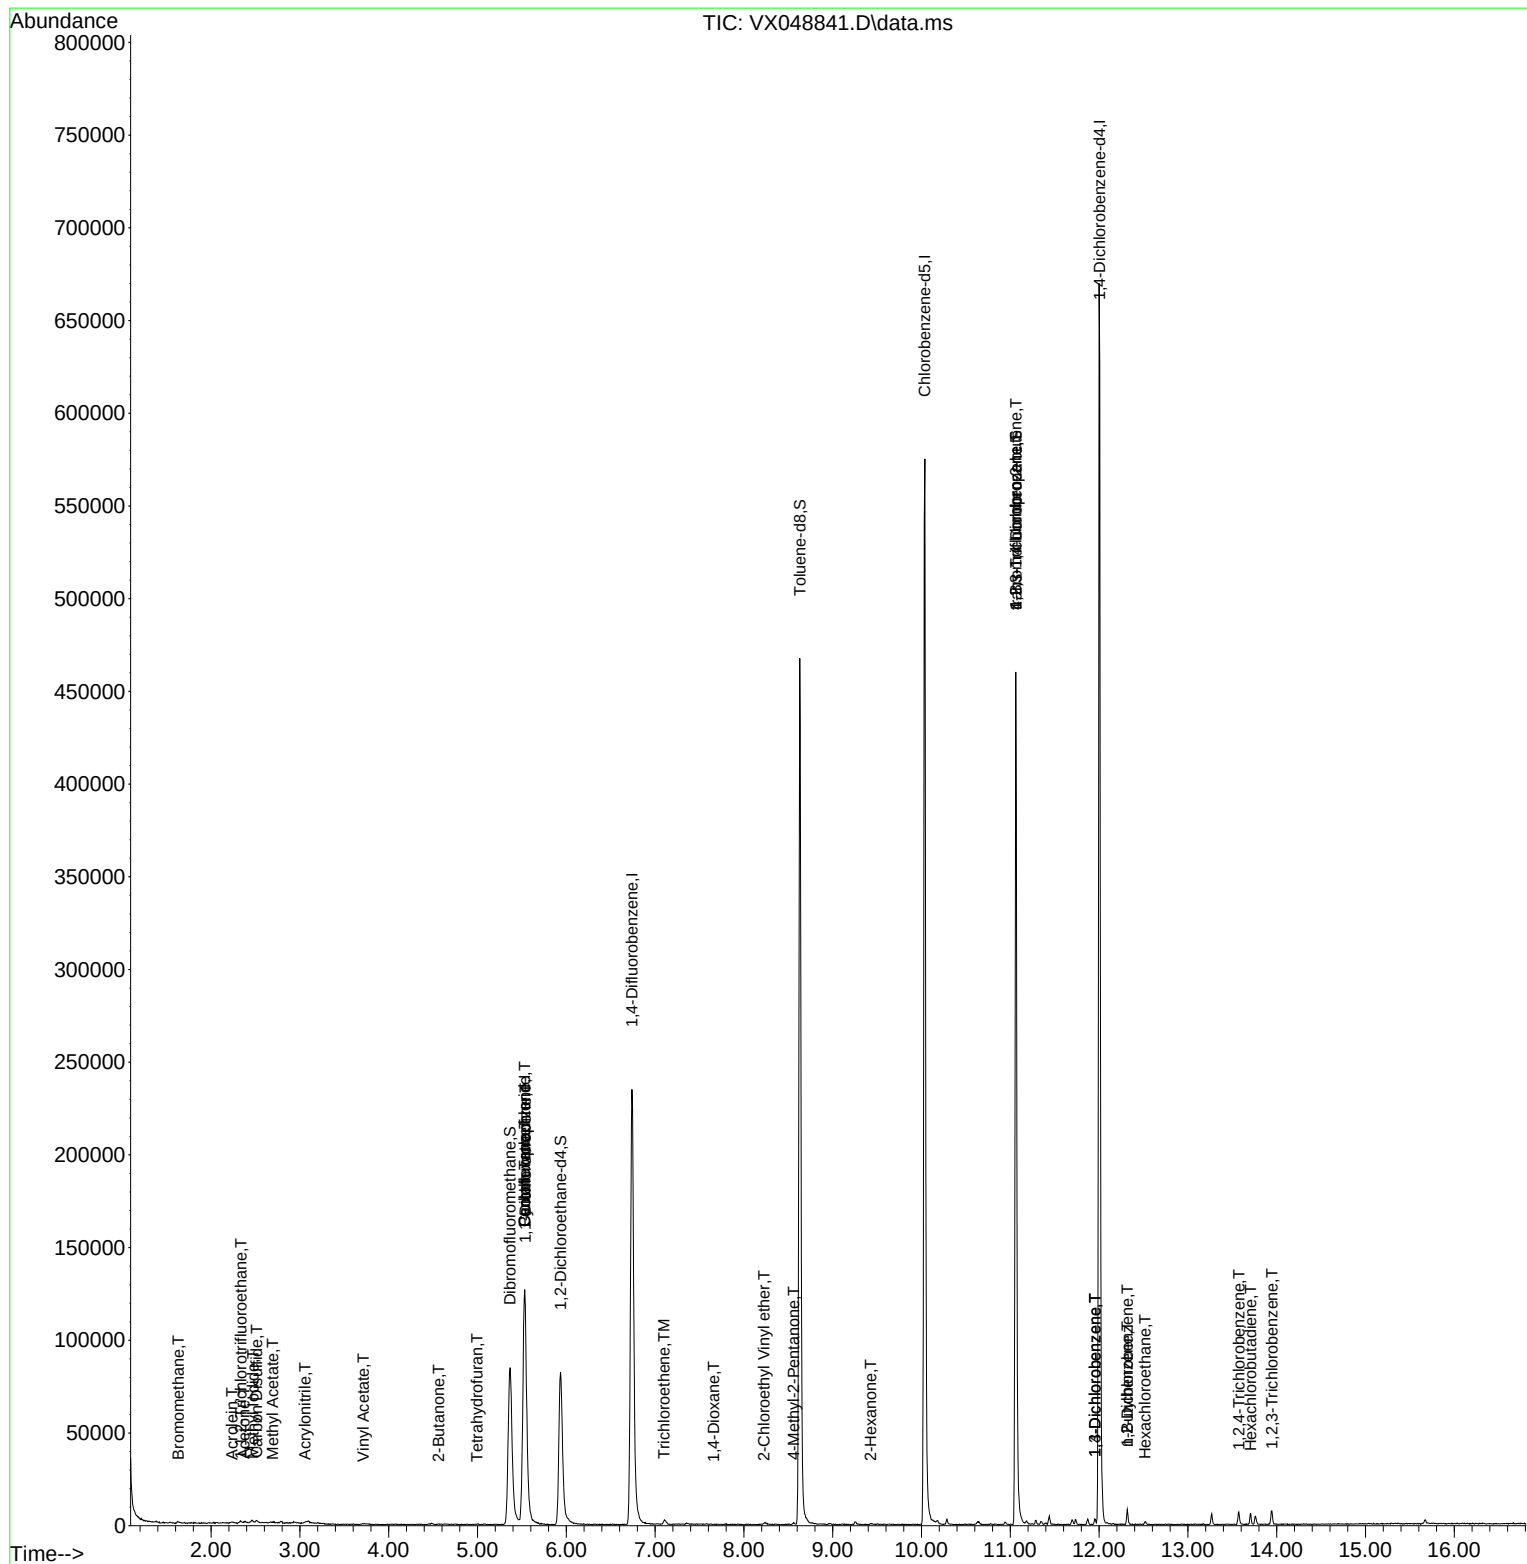




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.532 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09




Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01


Tgt Ion:168 Resp: 128949
Ion Ratio Lower Upper
168 100
99 60.7 44.2 66.4



#5
Bromomethane
Concen: 0.466 ug/l
RT: 1.630 min Scan# 89
Delta R.T. 0.012 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09

Tgt Ion: 94 Resp: 508
Ion Ratio Lower Upper
94 100
96 65.4 75.2 112.8#


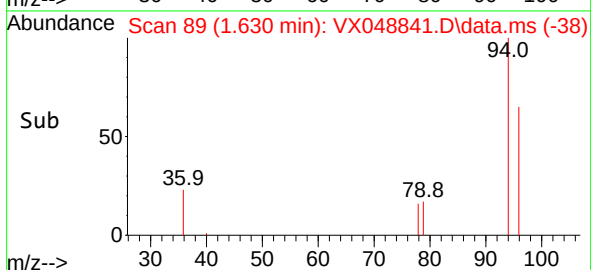




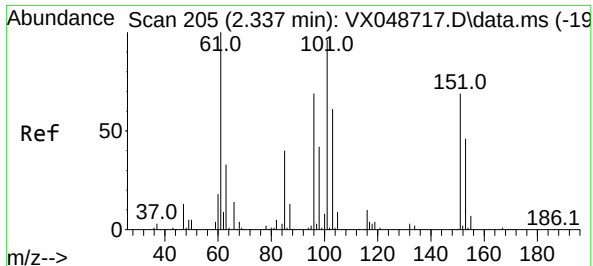

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.249 ug/l
RT: 2.337 min Scan# 205
Delta R.T. 0.000 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09




Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01


Tgt Ion:101 Resp: 365
Ion Ratio Lower Upper
101 100
85 14.8 34.2 51.2#
151 87.7 60.2 90.4

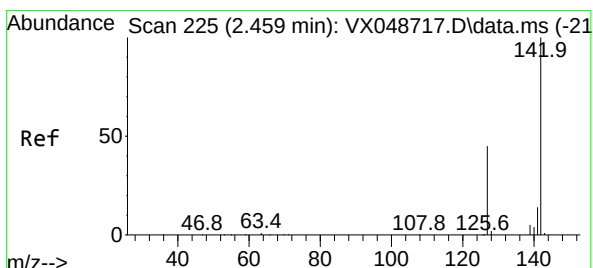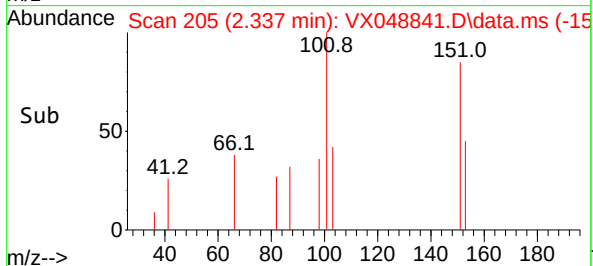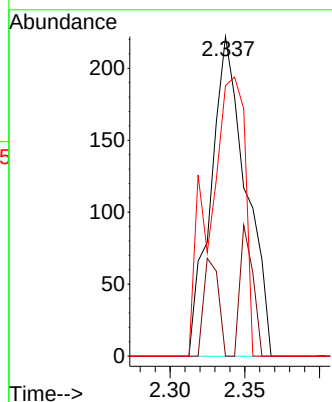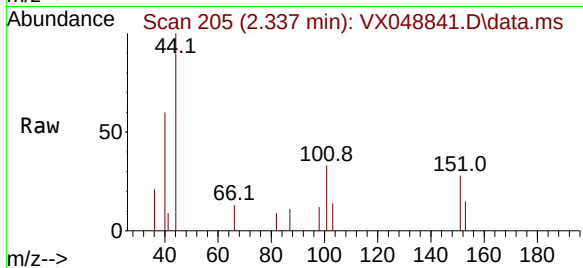

#10
Methyl Iodide
Concen: 0.789 ug/l
RT: 2.471 min Scan# 227
Delta R.T. 0.012 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09

Tgt Ion:142 Resp: 1648
Ion Ratio Lower Upper
142 100
127 55.5 35.8 53.6#
141 11.6 11.1 16.7


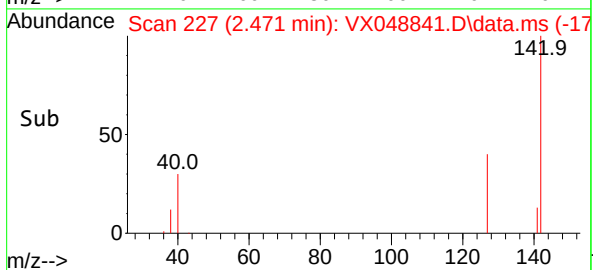
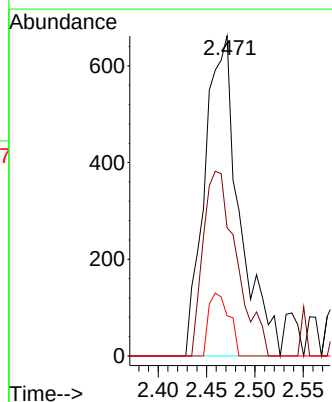
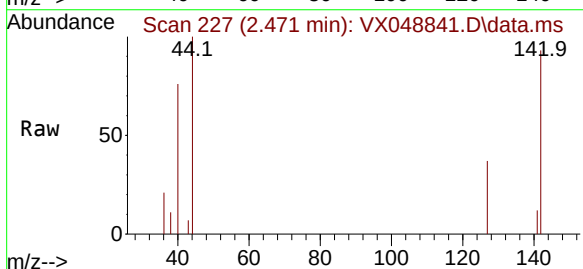




#13
Acrolein
Concen: 41.201 ug/l
RT: 2.233 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09




Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01


Tgt Ion: 56 Resp: 329
Ion Ratio Lower Upper
56 100
55 87.2 55.8 83.6#

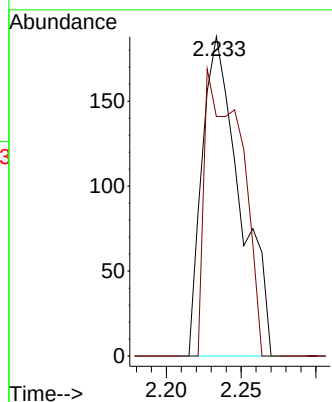

#15
Acrylonitrile
Concen: 0.550 ug/l
RT: 3.056 min Scan# 323
Delta R.T. 0.000 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09

Tgt Ion: 53 Resp: 479
Ion Ratio Lower Upper
53 100
52 105.8 66.3 99.5#
51 33.8 28.7 43.1


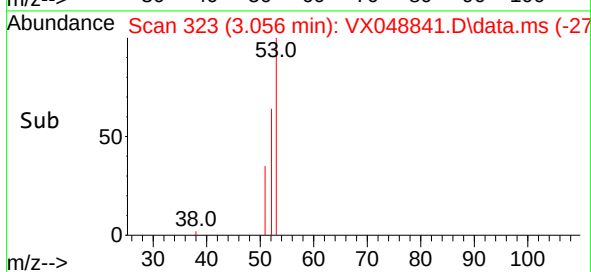
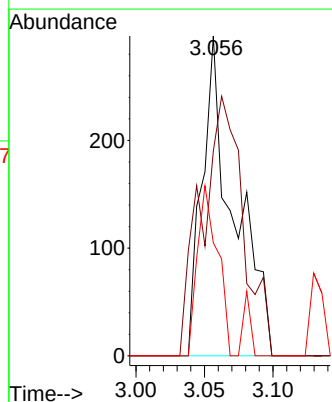



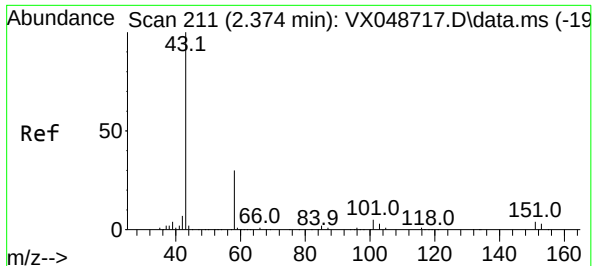

#16
Acetone
Concen: 1.455 ug/l
RT: 2.368 min Scan# 211
Delta R.T. -0.006 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09




Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01


Tgt Ion: 43 Resp: 964
Ion Ratio Lower Upper
43 100
58 18.7 25.0 37.4#

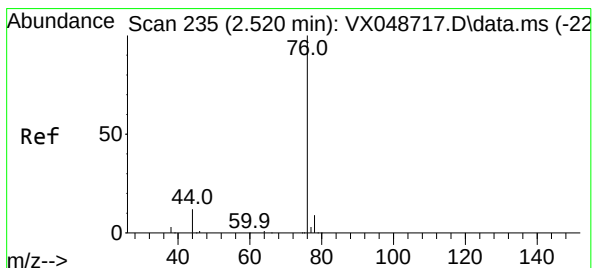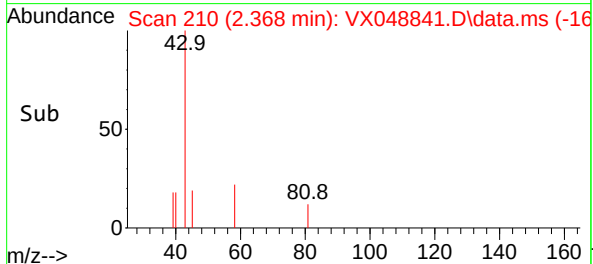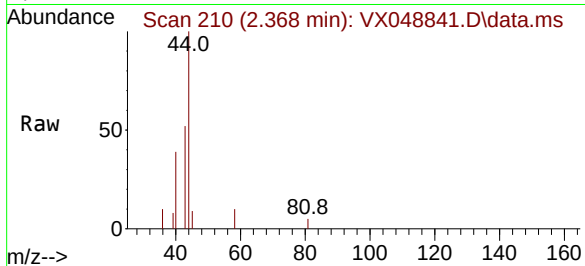

#17
Carbon Disulfide
Concen: 0.439 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.006 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09

Tgt Ion: 76 Resp: 1911
Ion Ratio Lower Upper
76 100
78 15.5 7.4 11.2#


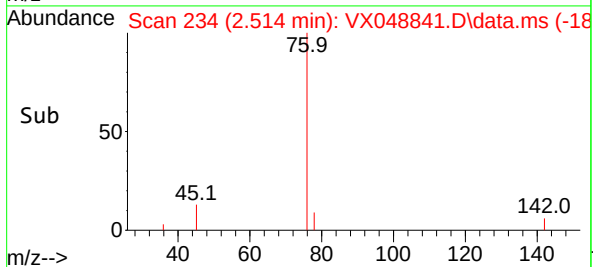

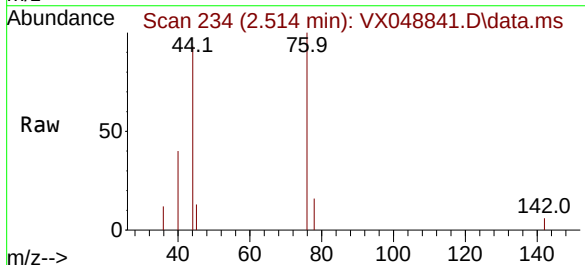




#18
Methyl Acetate
Concen: 0.503 ug/l
RT: 2.691 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09




Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01


Tgt Ion: 43 Resp: 937
Ion Ratio Lower Upper
43 100
74 2.5 19.2 28.8#

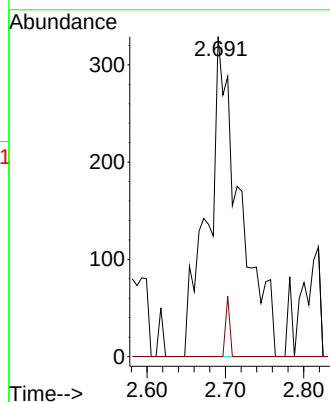

#23
Vinyl Acetate
Concen: 0.396 ug/l
RT: 3.715 min Scan# 431
Delta R.T. 0.000 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09

Tgt Ion: 43 Resp: 1563
Ion Ratio Lower Upper
43 100
86 0.0 9.2 13.8#









#25
2-Butanone
Concen: 0.464 ug/l
RT: 4.562 min Scan# 51
Delta R.T. 0.024 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09




Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01


Tgt Ion: 43 Resp: 454
Ion Ratio Lower Upper
43 100
72 0.0 22.6 34.0#

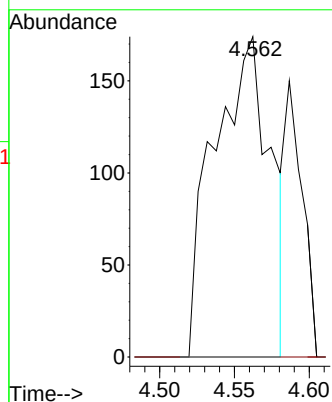

#29
Tetrahydrofuran
Concen: 0.372 ug/l
RT: 4.995 min Scan# 641
Delta R.T. 0.012 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09

Tgt Ion: 42 Resp: 278
Ion Ratio Lower Upper
42 100
72 0.0 39.4 59.2#
71 0.0 35.8 53.6#


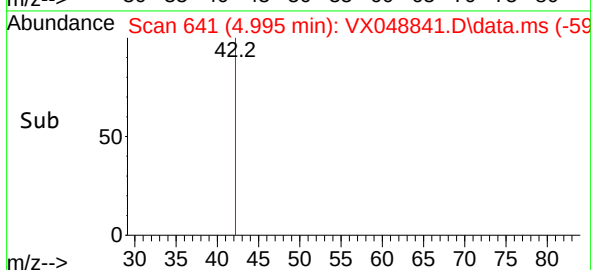






#31
Cyclohexane
Concen: 1.031 ug/l
RT: 5.532 min Scan# 718
Delta R.T. 0.067 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09




Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01


Tgt Ion: 56 Resp: 2411
Ion Ratio Lower Upper
56 100
69 150.4 24.2 36.2#
84 123.4 72.1 108.1#

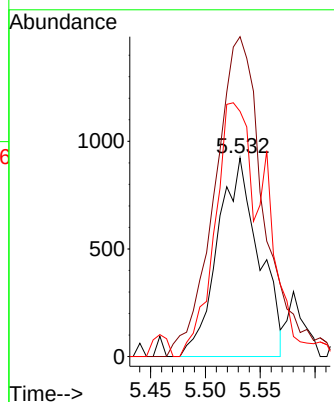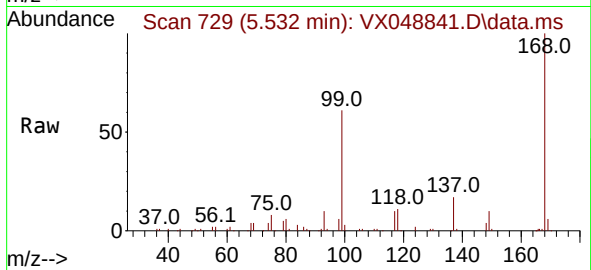

#33
1,2-Dichloroethane-d4
Concen: 52.237 ug/l
RT: 5.934 min Scan# 795
Delta R.T. -0.006 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09

Tgt Ion: 65 Resp: 90408
Ion Ratio Lower Upper
65 100
67 51.0 0.0 107.4


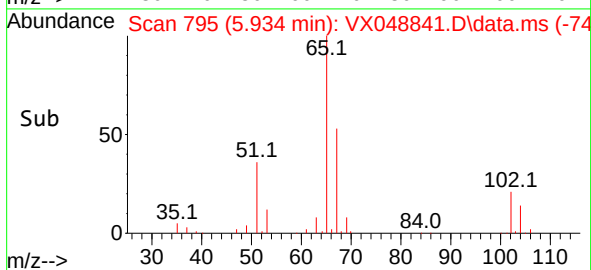
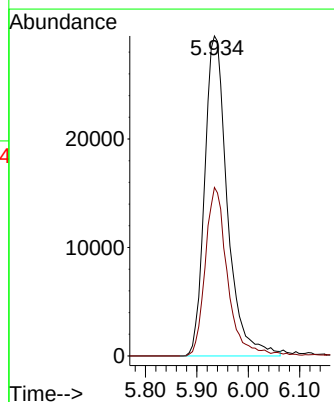
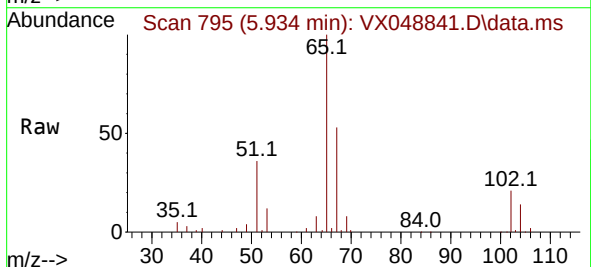




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.739 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09




Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01


Tgt Ion:114 Resp: 264334
Ion Ratio Lower Upper
114 100
63 20.9 0.0 39.0
88 16.3 0.0 31.8

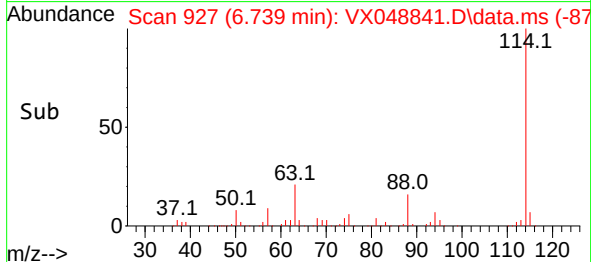

#35
Dibromofluoromethane
Concen: 46.175 ug/l
RT: 5.367 min Scan# 702
Delta R.T. -0.006 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09

Tgt Ion:113 Resp: 84040
Ion Ratio Lower Upper
113 100
111 102.0 79.5 119.3
192 19.1 16.1 24.1


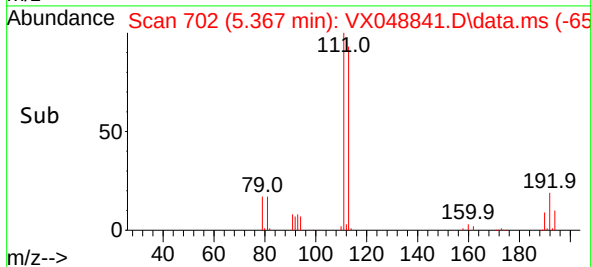

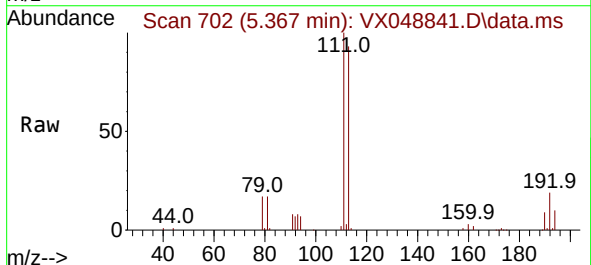




#36
 1,1-Dichloropropene
 Concen: 4.140 ug/l
 RT: 5.538 min Scan# 712
 Delta R.T. -0.146 min
 Lab File: VX048841.D
 Acq: 12 Dec 2025 10:09




Instrument :
 MSVOA_X
 ClientSampleId :
 VX1212MBL01


Tgt Ion: 75 Resp: 10320
 Ion Ratio Lower Upper
 75 100
 110 8.9 18.6 55.8#
 77 0.0 25.3 37.9#

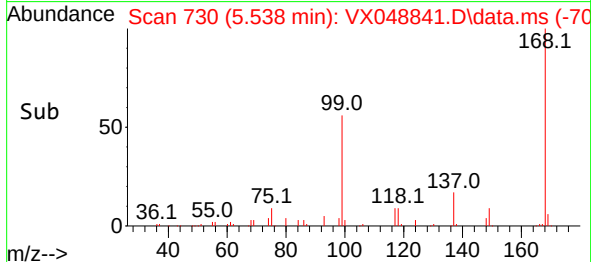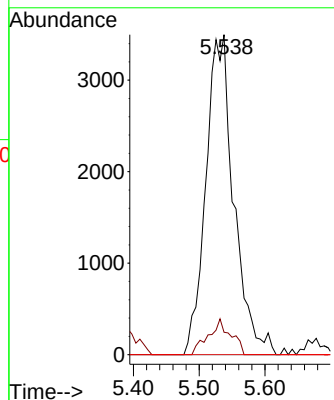

#38
 Carbon Tetrachloride
 Concen: 4.596 ug/l
 RT: 5.532 min Scan# 729
 Delta R.T. -0.134 min
 Lab File: VX048841.D
 Acq: 12 Dec 2025 10:09

Tgt Ion: 117 Resp: 12977
 Ion Ratio Lower Upper
 117 100
 119 4.6 80.5 120.7#
 121 0.0 25.4 38.0#


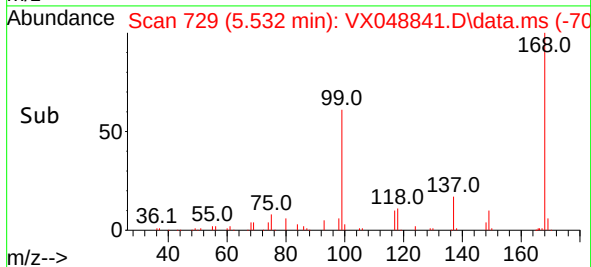
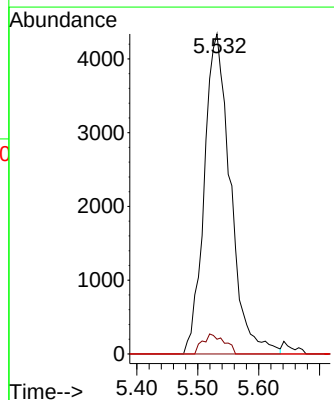
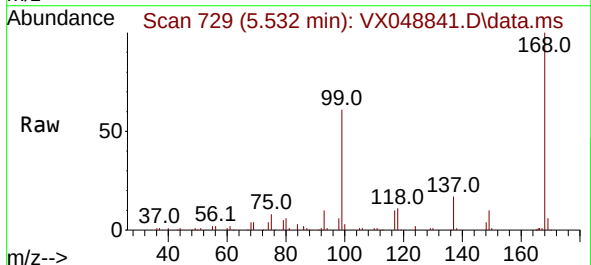




#44
Trichloroethene
Concen: 0.561 ug/l
RT: 7.098 min Scan# 91
Delta R.T. -0.012 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09




Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01


Tgt Ion:130 Resp: 1081
Ion Ratio Lower Upper
130 100
95 73.2 0.0 189.6

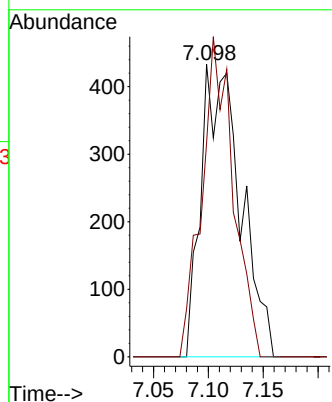

#49
1,4-Dioxane
Concen: 1.538 ug/l
RT: 7.659 min Scan# 1078
Delta R.T. 0.018 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09

Tgt Ion: 88 Resp: 48
Ion Ratio Lower Upper
88 100
43 0.0 28.6 43.0#
58 0.0 58.0 87.0#


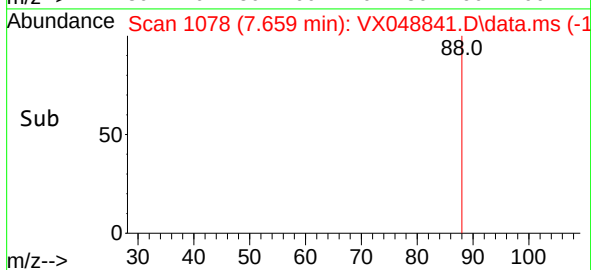






#50
Toluene-d8
Concen: 46.411 ug/l
RT: 8.629 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09




Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01


Tgt Ion: 98 Resp: 296092
Ion Ratio Lower Upper
98 100
100 65.5 53.4 80.0



#51
4-Methyl-2-Pentanone
Concen: 0.310 ug/l
RT: 8.562 min Scan# 1226
Delta R.T. 0.006 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09

Tgt Ion: 43 Resp: 868
Ion Ratio Lower Upper
43 100
58 22.2 32.2 48.4#


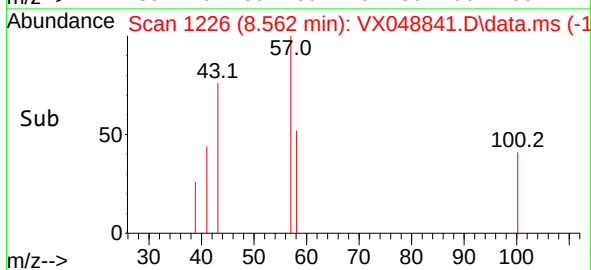

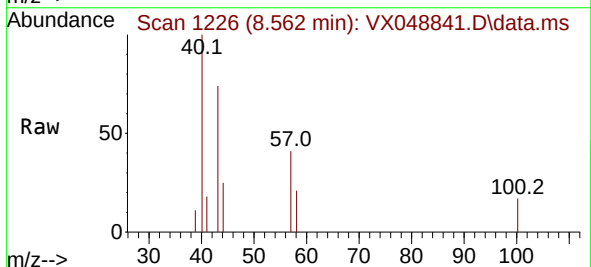




#58
 2-Chloroethyl Vinyl ether
 Concen: 0.403 ug/l
 RT: 8.226 min Scan# 1171
 Delta R.T. 0.000 min
 Lab File: VX048841.D
 Acq: 12 Dec 2025 10:09




Instrument :
 MSVOA_X
 ClientSampleId :
 VX1212MBL01


Tgt Ion: 63 Resp: 612
 Ion Ratio Lower Upper
 63 100
 106 17.0 23.4 35.2#



#59
 2-Hexanone
 Concen: 0.285 ug/l
 RT: 9.427 min Scan# 1368
 Delta R.T. 0.012 min
 Lab File: VX048841.D
 Acq: 12 Dec 2025 10:09

Tgt Ion: 43 Resp: 561
 Ion Ratio Lower Upper
 43 100
 58 31.6 27.8 83.4


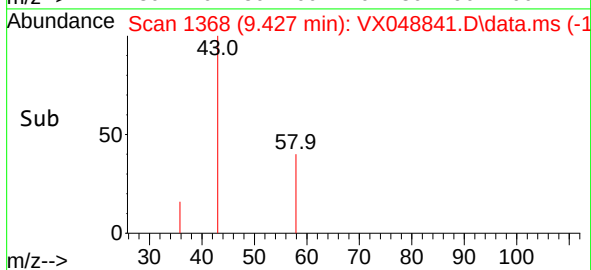

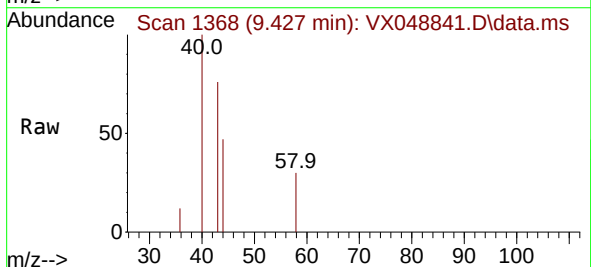




#62
4-Bromofluorobenzene
Concen: 57.481 ug/l
RT: 11.061 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09




Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01


Tgt Ion: 95 Resp: 126455
Ion Ratio Lower Upper
95 100
174 80.5 0.0 157.8
176 77.5 0.0 154.0

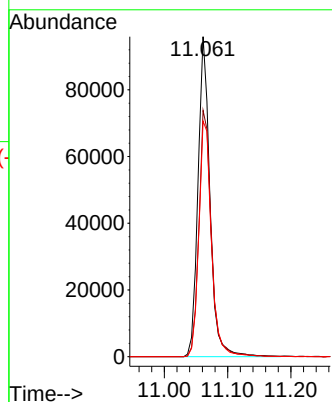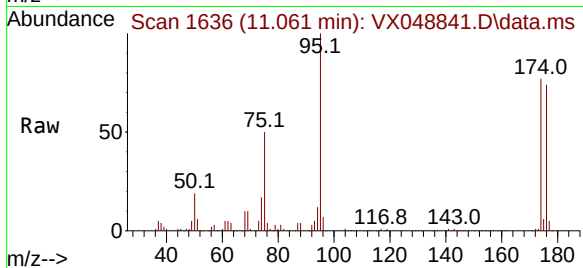

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. 0.000 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09

Tgt Ion: 117 Resp: 285483
Ion Ratio Lower Upper
117 100
82 54.3 44.1 66.1
119 32.3 25.2 37.8


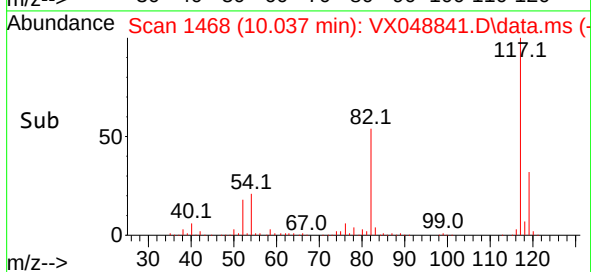
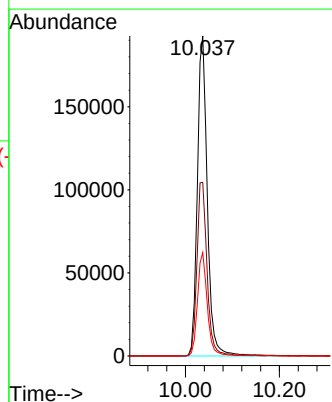
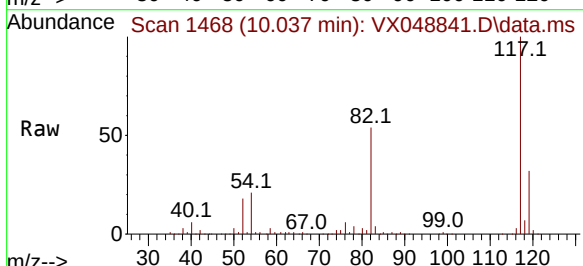




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.006 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX048841.D
 Acq: 12 Dec 2025 10:09




Instrument :
 MSVOA_X
 ClientSampleId :
 VX1212MBL01


Tgt Ion:152 Resp: 147205
 Ion Ratio Lower Upper
 152 100
 115 60.4 42.1 126.4
 150 158.2 0.0 347.8

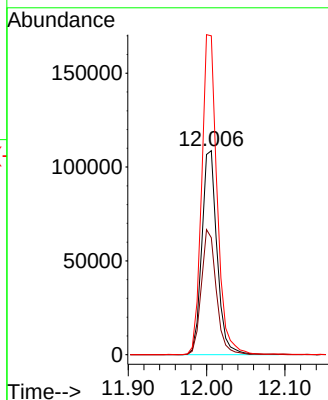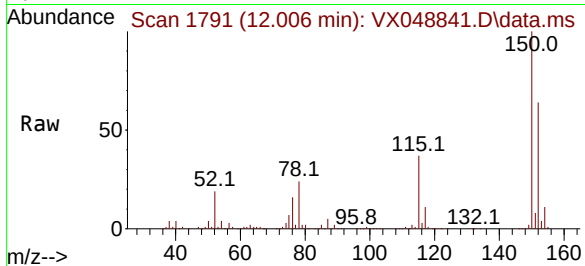

#76
 1,2,3-Trichloropropane
 Concen: 23.448 ug/l
 RT: 11.061 min Scan# 1636
 Delta R.T. -0.158 min
 Lab File: VX048841.D
 Acq: 12 Dec 2025 10:09

Tgt Ion: 75 Resp: 64289
 Ion Ratio Lower Upper
 75 100
 77 0.9 24.3 73.0#


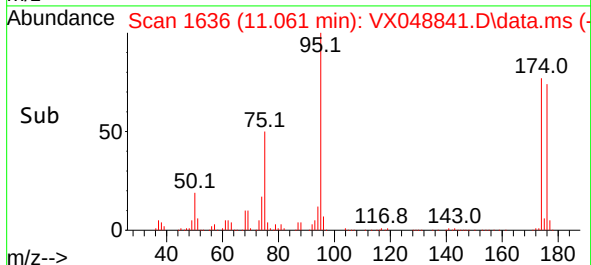
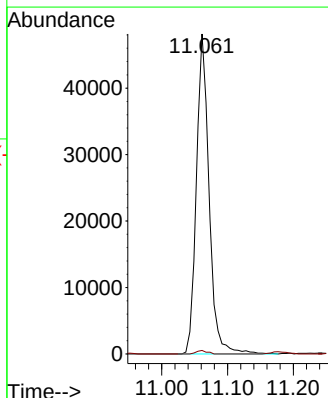
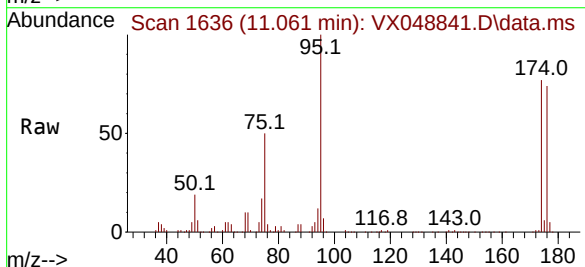




#81
trans-1,4-Dichloro-2-butene
Concen: 55.699 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. 0.061 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09




Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01


Tgt Ion: 75 Resp: 64289
Ion Ratio Lower Upper
75 100
53 0.1 79.9 119.9#
89 0.0 67.1 100.7#

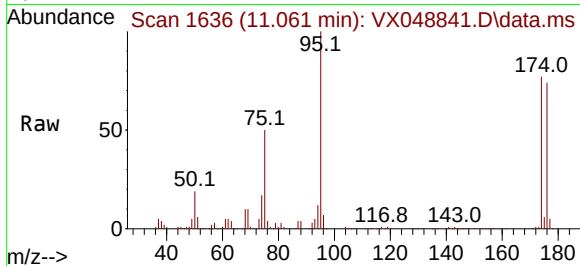

#87
1,3-Dichlorobenzene
Concen: 0.252 ug/l
RT: 11.951 min Scan# 1782
Delta R.T. 0.000 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09

Tgt Ion:146 Resp: 1229
Ion Ratio Lower Upper
146 100
111 42.4 20.3 60.8
148 71.7 32.1 96.5

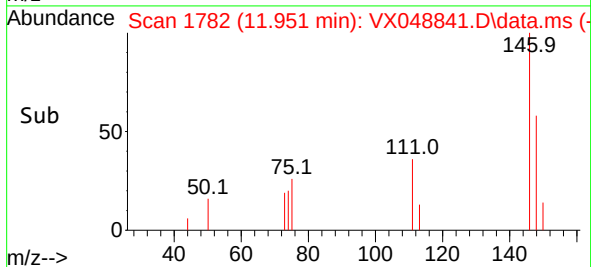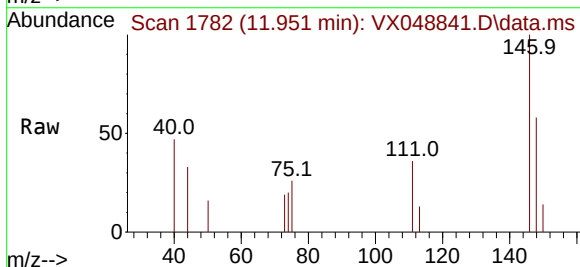



#88

1,4-Dichlorobenzene

Concen: 0.244 ug/l

RT: 11.951 min Scan# 11

Delta R.T. -0.073 min

Lab File: VX048841.D

Acq: 12 Dec 2025 10:09

Instrument :

MSVOA_X

ClientSampleId :

VX1212MBL01





Tgt Ion:146 Resp: 1229

Ion Ratio Lower Upper

146 100

111 42.4 19.6 58.7

148 71.7 31.6 94.7

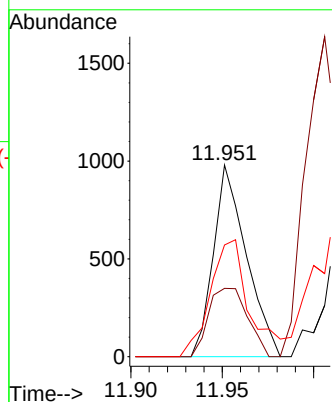

#89

n-Butylbenzene

Concen: 0.292 ug/l

RT: 12.317 min Scan# 1842

Delta R.T. 0.006 min

Lab File: VX048841.D

Acq: 12 Dec 2025 10:09




Tgt Ion: 91 Resp: 2400


Ion Ratio Lower Upper

91 100

92 52.1 27.1 81.3

134 28.5 12.9 38.6


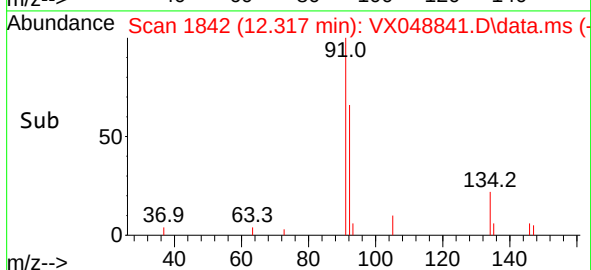






#90
Hexachloroethane
Concen: 0.222 ug/l
RT: 12.518 min Scan# 1875
Delta R.T. 0.000 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09




Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01


Tgt Ion:117 Resp: 398
Ion Ratio Lower Upper
117 100
201 69.6 36.4 109.1

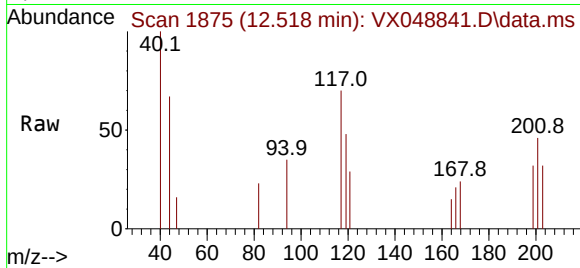

#91
1,2-Dichlorobenzene
Concen: 0.228 ug/l
RT: 12.317 min Scan# 1842
Delta R.T. 0.000 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09

Tgt Ion:146 Resp: 1078
Ion Ratio Lower Upper
146 100
111 44.3 20.8 62.5
148 58.0 32.0 96.0

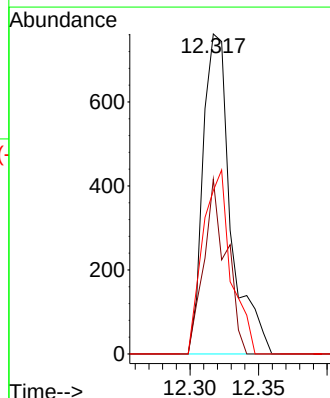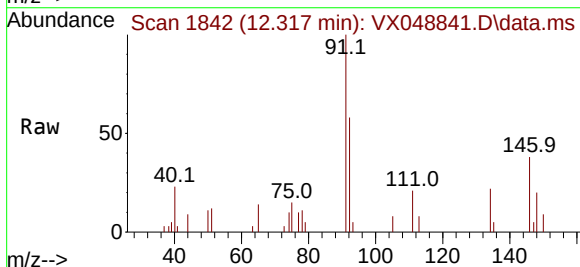



#93

1,2,4-Trichlorobenzene

Concen: 0.703 ug/l

RT: 13.573 min Scan# 2047

Delta R.T. 0.006 min

Lab File: VX048841.D

Acq: 12 Dec 2025 10:09

Instrument :

MSVOA_X

ClientSampleId :

VX1212MBL01





Tgt Ion:180 Resp: 2197

Ion Ratio Lower Upper

180 100

182 90.0 46.9 140.8

145 31.2 15.1 45.3

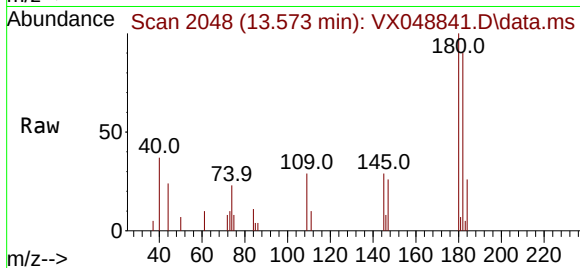

#94

Hexachlorobutadiene

Concen: 0.678 ug/l

RT: 13.707 min Scan# 2070

Delta R.T. 0.000 min

Lab File: VX048841.D

Acq: 12 Dec 2025 10:09




Tgt Ion:225 Resp: 877


Ion Ratio Lower Upper

225 100

223 72.4 33.0 98.9


227 70.4 32.9 98.7

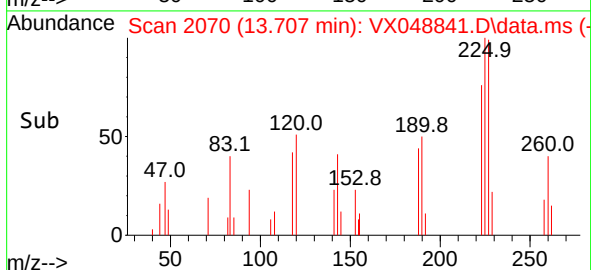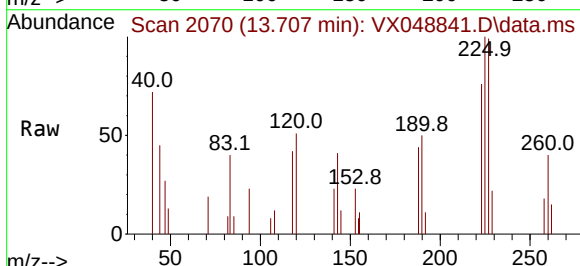






#95
Naphthalene
Concen: Below Cal
RT: 13.762 min Scan# 2109
Delta R.T. 0.006 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09

Instrument :
MSVOA_X
ClientSampleId :
VX1212MBL01



Tgt Ion:128 Resp: 3505

Ion	Ratio	Lower	Upper
128	100		
127	12.3	10.2	15.2
129	10.4	8.6	13.0



#96
1,2,3-Trichlorobenzene
Concen: 0.717 ug/l
RT: 13.945 min Scan# 2109
Delta R.T. 0.006 min
Lab File: VX048841.D
Acq: 12 Dec 2025 10:09

Tgt Ion:180 Resp: 2068

Ion	Ratio	Lower	Upper
180	100		
182	100.1	48.0	144.2
145	35.0	16.6	49.8

