

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121225\
 Data File : VX048855.D
 Acq On : 12 Dec 2025 15:20
 Operator : JC/MD
 Sample : Q3848-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-18B-57.5-121125-FD

Quant Time: Dec 12 22:14:06 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 05 03:27:34 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.538	168	156804	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.745	114	318047	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	339965	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	178735	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.940	65	108303	51.460	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 102.920%			
35) Dibromofluoromethane	5.367	113	95151	43.450	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 86.900%			
50) Toluene-d8	8.629	98	323713	42.171	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 84.340%#			
62) 4-Bromofluorobenzene	11.061	95	141751	53.552	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 107.100%			
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.148	85	4476	2.802	ug/l	92
3) Chloromethane	1.301	50	433	0.215	ug/l	90
4) Vinyl Chloride	1.380	62	116081	54.063	ug/l	100
8) Diethyl Ether	2.148	74	277	0.226	ug/l	85
9) 1,1,2-Trichlorotrifluo...	2.337	101	13304	7.457	ug/l	98
12) 1,1-Dichloroethene	2.325	96	14378	7.896	ug/l	96
13) Acrolein	2.246	56	721	42.022	ug/l #	57
16) Acetone	2.374	43	9233	11.460	ug/l	91
17) Carbon Disulfide	2.514	76	8400	1.589	ug/l #	92
18) Methyl Acetate	2.697	43	1409	0.622	ug/l #	72
20) Methylene Chloride	2.788	84	706	0.351	ug/l	94
21) trans-1,2-Dichloroethene	3.093	96	6123	3.295	ug/l	97
24) 1,1-Dichloroethane	3.599	63	26087	8.188	ug/l	96
25) 2-Butanone	4.550	43	732	0.616	ug/l #	54
27) cis-1,2-Dichloroethene	4.477	96	1657994	790.630	ug/l	94
29) Tetrahydrofuran	5.001	42	6149	6.772	ug/l #	85
31) Cyclohexane	5.532	56	3140	1.104	ug/l #	4
36) 1,1-Dichloropropene	5.532	75	12470	4.158	ug/l #	49
37) Ethyl Acetate	4.550	43	732	0.204	ug/l #	71
38) Carbon Tetrachloride	5.532	117	15455	4.549	ug/l #	13
39) Methylcyclohexane	7.111	83	8076	2.277	ug/l #	1
40) Benzene	6.031	78	7472	0.840	ug/l	96
41) Methacrylonitrile	5.007	41	3481	2.135	ug/l #	39
42) 1,2-Dichloroethane	6.074	62	3997	1.270	ug/l	91
44) Trichloroethene	7.111	130	687987	296.545	ug/l	96
49) 1,4-Dioxane	7.653	88	95	2.530	ug/l #	48
60) Dibromochloromethane	9.256	129	8115	3.042	ug/l #	11
64) Tetrachloroethene	9.256	164	8611	3.475	ug/l	94
76) 1,2,3-Trichloropropane	11.061	75	73581	22.103	ug/l #	30
81) trans-1,4-Dichloro-2-b...	11.061	75	73581	52.504	ug/l #	3
95) Naphthalene	13.762	128	598	Below Cal	#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121225\
Data File : VX048855.D
Acq On : 12 Dec 2025 15:20
Operator : JC/MD
Sample : Q3848-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-121125-FD

Quant Time: Dec 12 22:14:06 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 05 03:27:34 2025
Response via : Initial Calibration




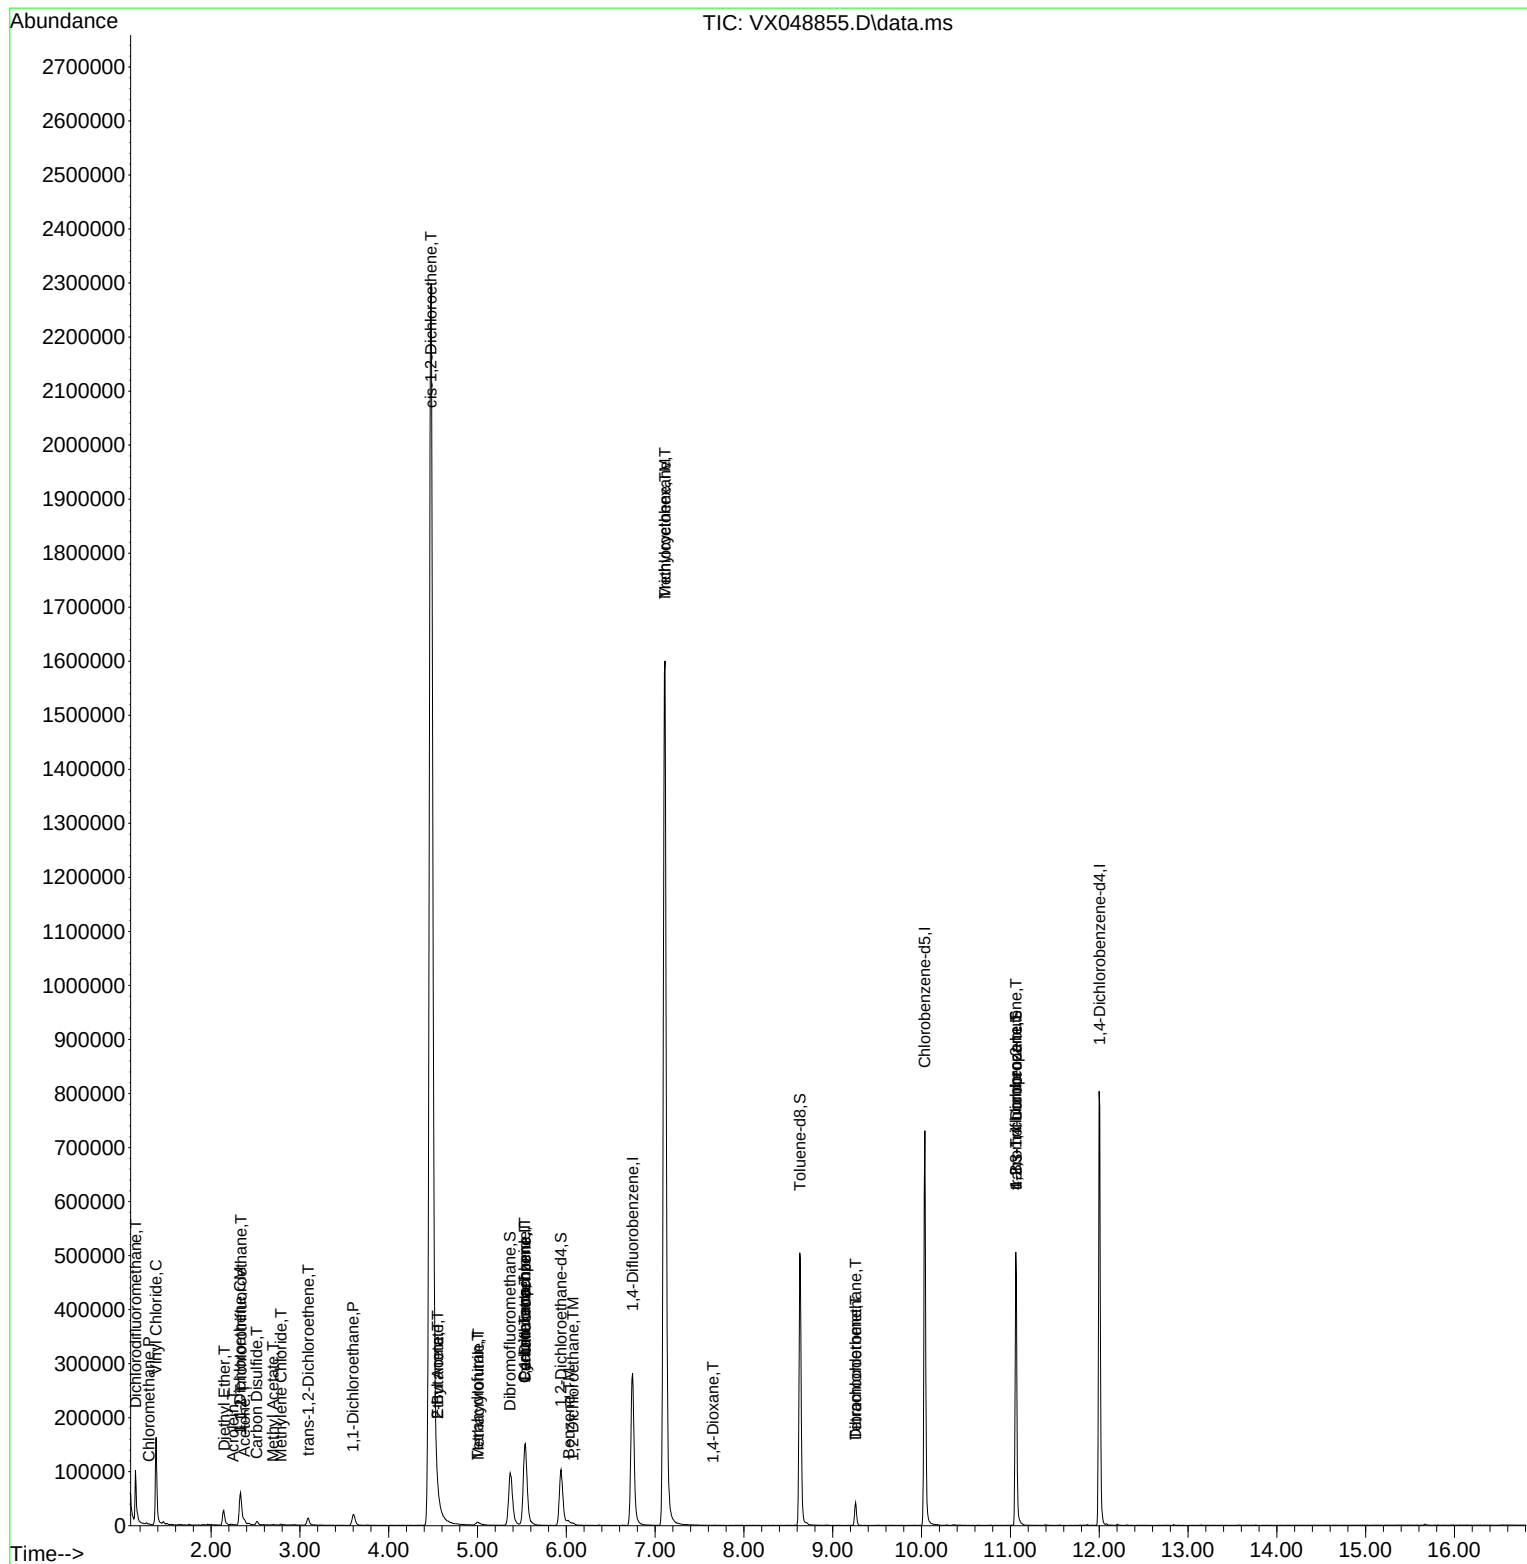




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.538 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-121125-FD


Tgt Ion:168 Resp: 156804
Ion Ratio Lower Upper
168 100
99 58.3 44.2 66.4

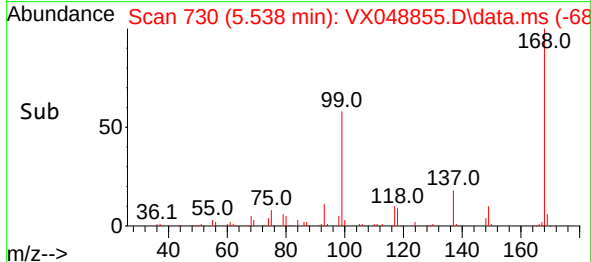

#2
Dichlorodifluoromethane
Concen: 2.802 ug/l
RT: 1.148 min Scan# 10
Delta R.T. -0.024 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20

Tgt Ion: 85 Resp: 4476
Ion Ratio Lower Upper
85 100
87 37.5 16.4 49.1

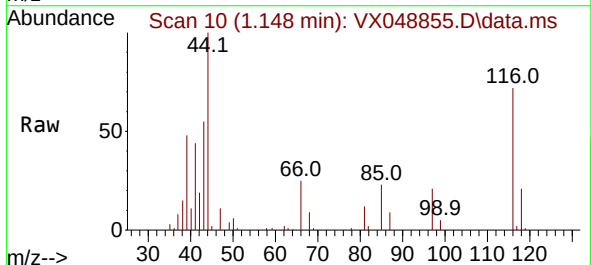

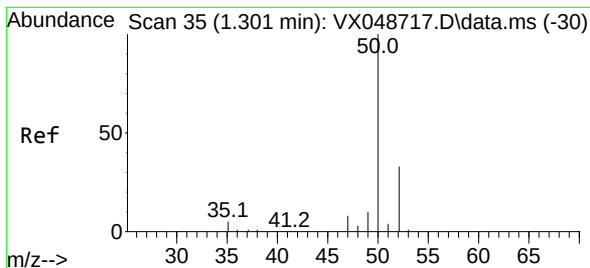

#3

Chloromethane

Concen: 0.215 ug/l

RT: 1.301 min Scan# 35

Delta R.T. 0.000 min

Lab File: VX048855.D

Acq: 12 Dec 2025 15:20

Instrument :

MSVOA_X

ClientSampleId :





MW-18B-57.5-121125-FD

Tgt Ion: 50 Resp: 433

Ion Ratio Lower Upper

50 100

52 27.1 26.4 39.6

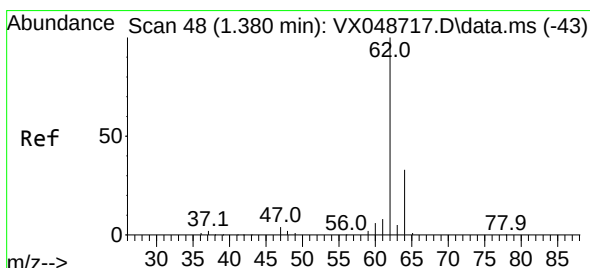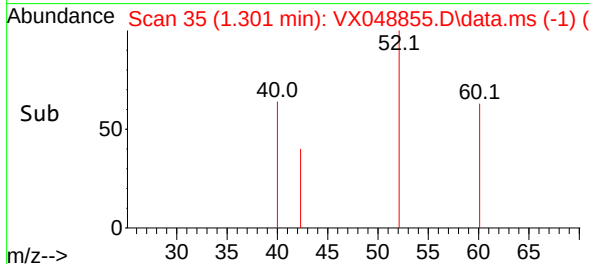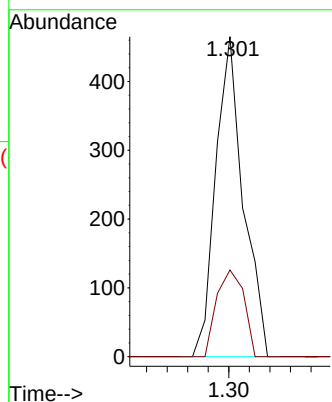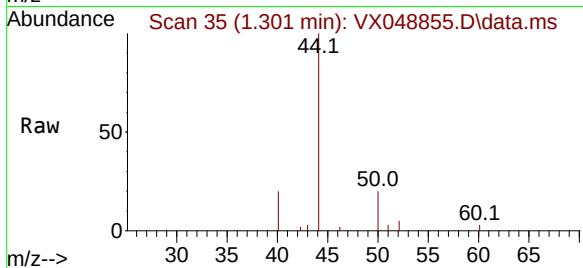

#4

Vinyl Chloride

Concen: 54.063 ug/l

RT: 1.380 min Scan# 48

Delta R.T. 0.000 min

Lab File: VX048855.D




Acq: 12 Dec 2025 15:20


Tgt Ion: 62 Resp: 116081

Ion Ratio Lower Upper

62 100

64 32.5 26.0 39.0


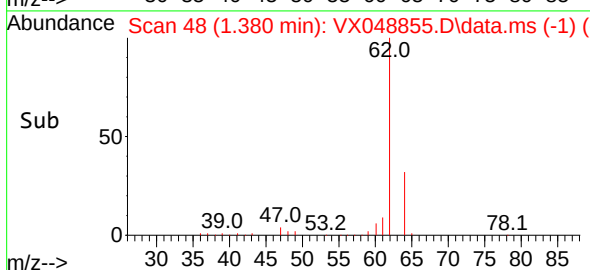

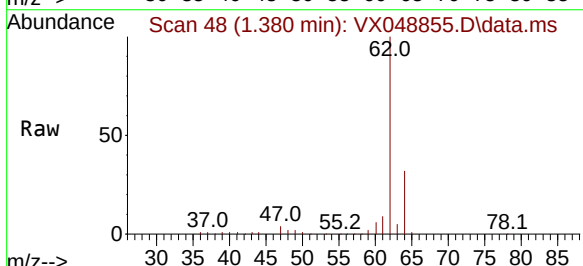




#8
Diethyl Ether
Concen: 0.226 ug/l
RT: 2.148 min Scan# 11
Delta R.T. 0.012 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-121125-FD


Tgt Ion: 74 Resp: 277
Ion Ratio Lower Upper
74 100
45 112.6 48.9 146.8

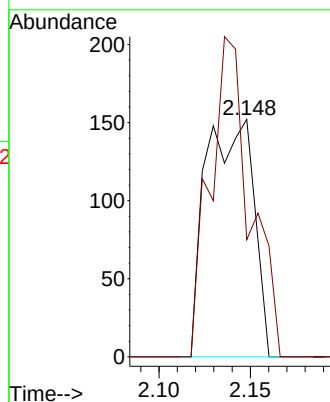

#9
1,1,2-Trichlorotrifluoroethane
Concen: 7.457 ug/l
RT: 2.337 min Scan# 205
Delta R.T. 0.000 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20

Tgt Ion: 101 Resp: 13304
Ion Ratio Lower Upper
101 100
85 43.7 34.2 51.2
151 77.6 60.2 90.4





#12

1,1-Dichloroethene

Concen: 7.896 ug/l

RT: 2.325 min Scan# 203

Delta R.T. 0.000 min

Lab File: VX048855.D

Acq: 12 Dec 2025 15:20

Instrument :

MSVOA_X

ClientSampleId :

MW-18B-57.5-121125-FD





Tgt Ion: 96 Resp: 14378

Ion Ratio Lower Upper

96 100

61 160.4 130.7 196.1

98 67.9 49.8 74.8



#13

Acrolein

Concen: 42.022 ug/l

RT: 2.246 min Scan# 190

Delta R.T. 0.012 min

Lab File: VX048855.D




Acq: 12 Dec 2025 15:20


Tgt Ion: 56 Resp: 721

Ion Ratio Lower Upper

56 100

55 104.6 55.8 83.6#


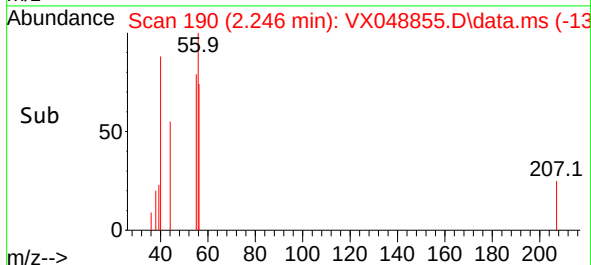
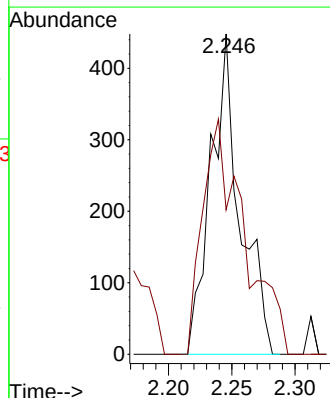





#16
Acetone
Concen: 11.460 ug/l
RT: 2.374 min Scan# 211
Delta R.T. 0.000 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-121125-FD


Tgt Ion: 43 Resp: 9233
Ion Ratio Lower Upper
43 100
58 26.5 25.0 37.4

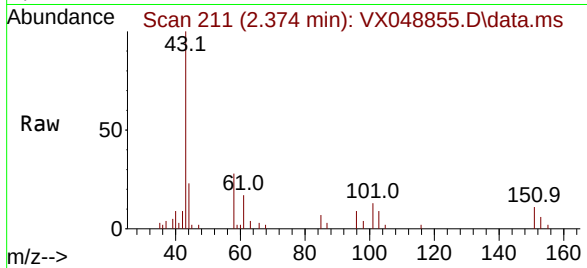

#17
Carbon Disulfide
Concen: 1.589 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.006 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20

Tgt Ion: 76 Resp: 8400
Ion Ratio Lower Upper
76 100
78 6.5 7.4 11.2#


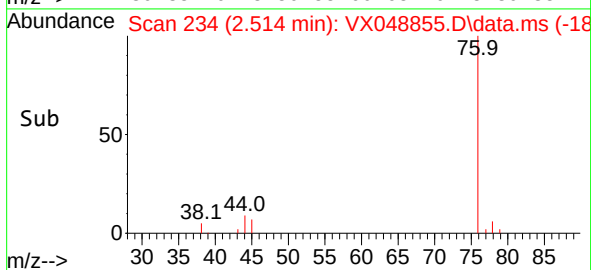

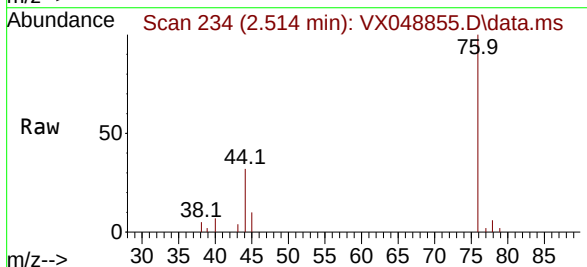




#18
Methyl Acetate
Concen: 0.622 ug/l
RT: 2.697 min Scan# 20
Delta R.T. 0.000 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-121125-FD


Tgt Ion: 43 Resp: 1409
Ion Ratio Lower Upper
43 100
74 10.4 19.2 28.8#

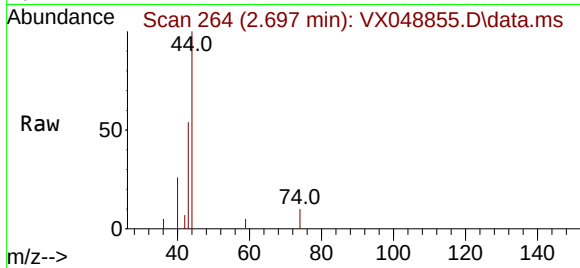

#20
Methylene Chloride
Concen: 0.351 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20

Tgt Ion: 84 Resp: 706
Ion Ratio Lower Upper
84 100
49 126.0 98.7 148.1
51 30.6 29.4 44.2
86 58.4 52.5 78.7


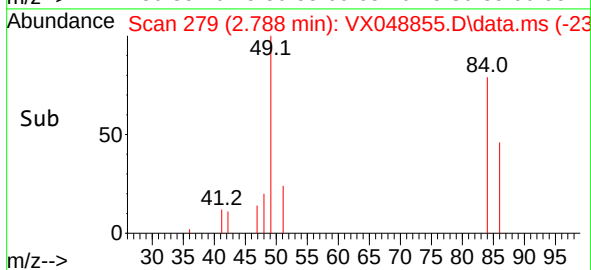

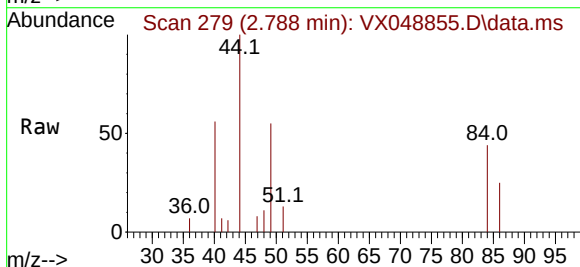




#21
trans-1,2-Dichloroethene
Concen: 3.295 ug/l
RT: 3.093 min Scan# 31
Delta R.T. 0.000 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-121125-FD


Tgt Ion: 96 Resp: 6123
Ion Ratio Lower Upper
96 100
61 137.4 112.8 169.2
98 66.2 51.0 76.4

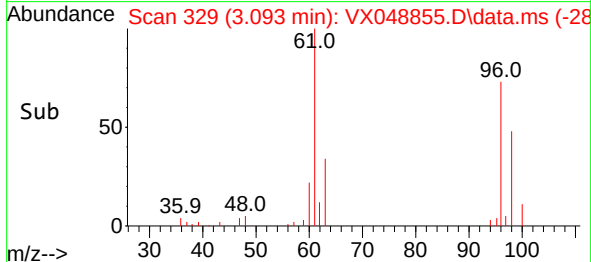

#24
1,1-Dichloroethane
Concen: 8.188 ug/l
RT: 3.599 min Scan# 412
Delta R.T. -0.006 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20

Tgt Ion: 63 Resp: 26087
Ion Ratio Lower Upper
63 100
98 8.2 3.5 10.6
100 3.5 2.5 7.4


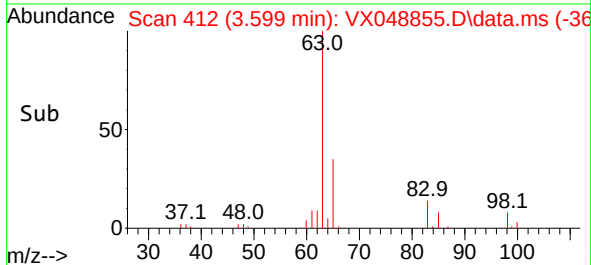






#25
2-Butanone
Concen: 0.616 ug/l
RT: 4.550 min Scan# 50
Delta R.T. 0.012 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-121125-FD


Tgt Ion: 43 Resp: 732
Ion Ratio Lower Upper
43 100
72 52.4 22.6 34.0#



#27
cis-1,2-Dichloroethene
Concen: 790.630 ug/l
RT: 4.477 min Scan# 556
Delta R.T. -0.006 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20

Tgt Ion: 96 Resp: 1657994
Ion Ratio Lower Upper
96 100
61 126.2 0.0 271.0
98 64.0 0.0 130.2

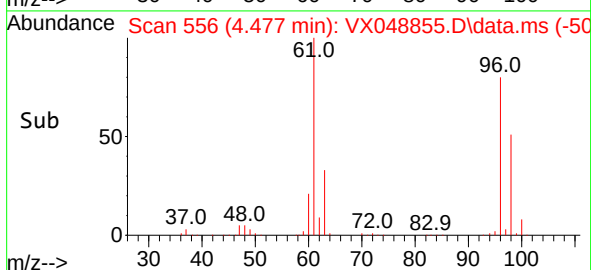



#29

Tetrahydrofuran

Concen: 6.772 ug/l

RT: 5.001 min Scan# 642

Delta R.T. 0.018 min

Lab File: VX048855.D

Acq: 12 Dec 2025 15:20

Instrument :

MSVOA_X

ClientSampleId :

MW-18B-57.5-121125-FD





Tgt Ion: 42 Resp: 6149

Ion Ratio Lower Upper

42 100

72 39.6 39.4 59.2

71 34.9 35.8 53.6#

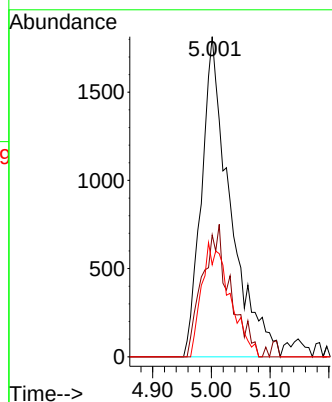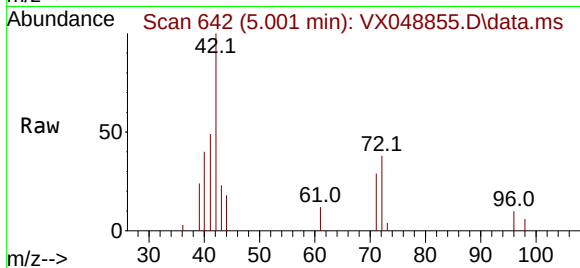

#31

Cyclohexane

Concen: 1.104 ug/l

RT: 5.532 min Scan# 729

Delta R.T. 0.067 min

Lab File: VX048855.D

Acq: 12 Dec 2025 15:20




Tgt Ion: 56 Resp: 3140


Ion Ratio Lower Upper

56 100

69 158.5 24.2 36.2#

84 136.9 72.1 108.1#


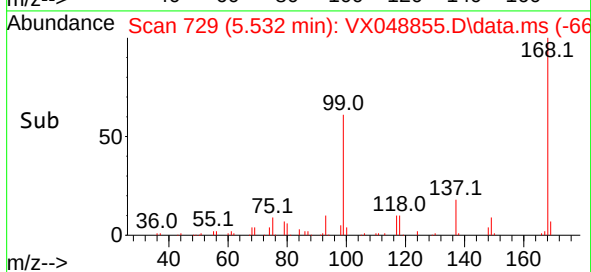
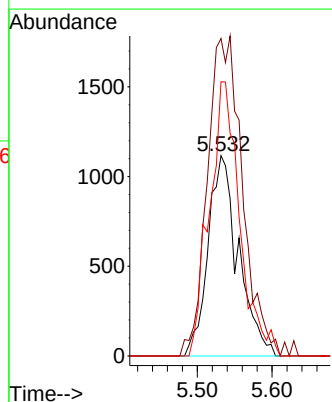
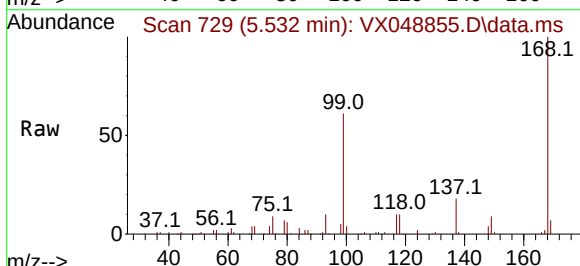




#33
 1,2-Dichloroethane-d4
 Concen: 51.460 ug/l
 RT: 5.940 min Scan# 796
 Delta R.T. 0.000 min
 Lab File: VX048855.D
 Acq: 12 Dec 2025 15:20




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-18B-57.5-121125-FD


Tgt Ion: 65 Resp: 108303
 Ion Ratio Lower Upper
 65 100
 67 52.6 0.0 107.4

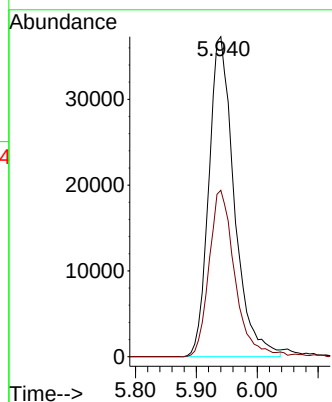

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.745 min Scan# 928
 Delta R.T. 0.000 min
 Lab File: VX048855.D
 Acq: 12 Dec 2025 15:20

Tgt Ion: 114 Resp: 318047
 Ion Ratio Lower Upper
 114 100
 63 21.1 0.0 39.0
 88 16.0 0.0 31.8







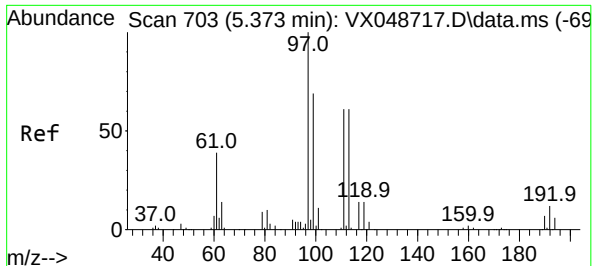

#35
Dibromofluoromethane
Concen: 43.450 ug/l
RT: 5.367 min Scan# 703
Delta R.T. -0.006 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-121125-FD


Tgt Ion:113 Resp: 95151
Ion Ratio Lower Upper
113 100
111 104.4 79.5 119.3
192 19.0 16.1 24.1

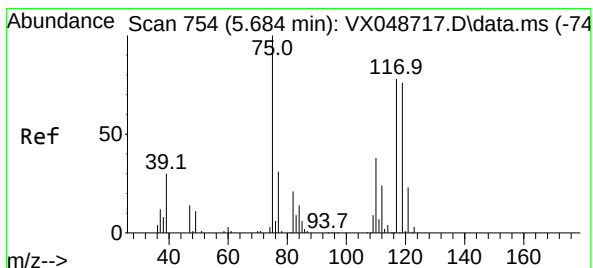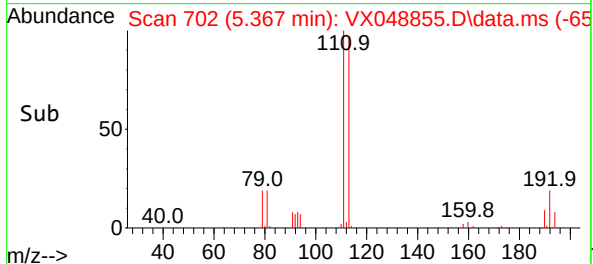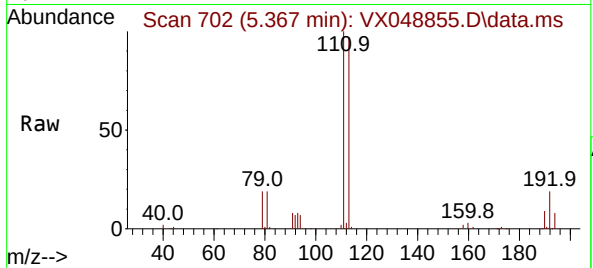

#36
1,1-Dichloropropene
Concen: 4.158 ug/l
RT: 5.532 min Scan# 729
Delta R.T. -0.152 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20

Tgt Ion: 75 Resp: 12470
Ion Ratio Lower Upper
75 100
110 9.5 18.6 55.8#
77 0.0 25.3 37.9#

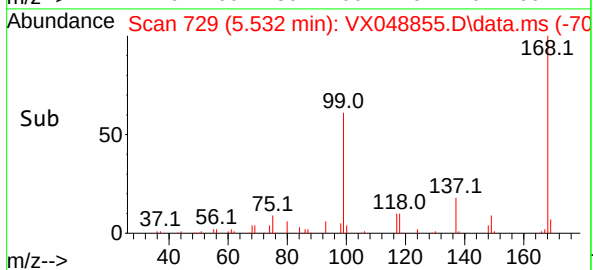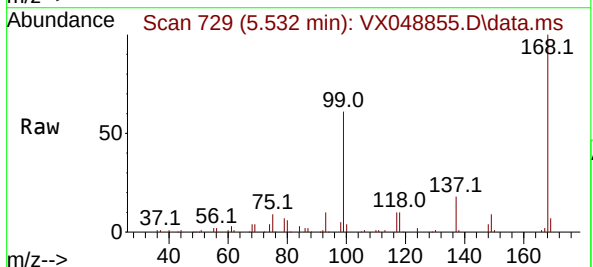



#37

Ethyl Acetate

Concen: 0.204 ug/l

RT: 4.550 min Scan# 5

Delta R.T. -0.146 min

Lab File: VX048855.D

Acq: 12 Dec 2025 15:20

Instrument :

MSVOA_X

ClientSampleId :

MW-18B-57.5-121125-FD





Tgt Ion: 43 Resp: 732

Ion Ratio Lower Upper

43 100

61 0.0 9.7 14.5#

70 0.0 8.2 12.4#

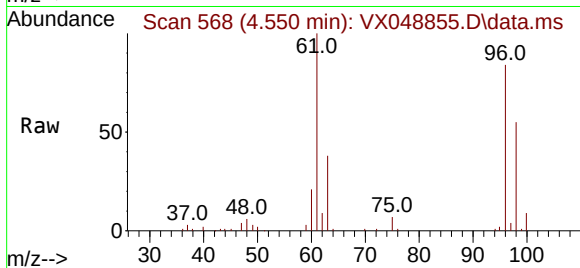

#38

Carbon Tetrachloride

Concen: 4.549 ug/l

RT: 5.532 min Scan# 729

Delta R.T. -0.134 min

Lab File: VX048855.D

Acq: 12 Dec 2025 15:20




Tgt Ion: 117 Resp: 15455


Ion Ratio Lower Upper

117 100

119 4.1 80.5 120.7#

121 0.0 25.4 38.0#

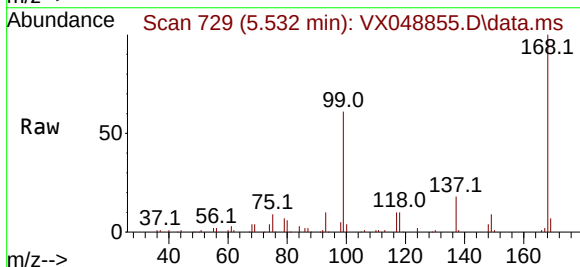

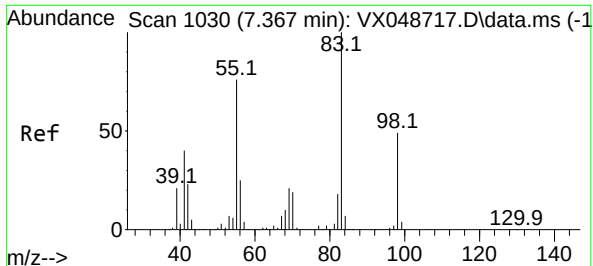

#39

Methylcyclohexane

Concen: 2.277 ug/l

RT: 7.111 min Scan# 98

Delta R.T. -0.256 min

Lab File: VX048855.D

Acq: 12 Dec 2025 15:20

Instrument :

MSVOA_X

ClientSampleId :

MW-18B-57.5-121125-FD





Tgt Ion: 83 Resp: 8076

Ion Ratio Lower Upper

83 100

55 0.0 60.6 90.8#

98 189.8 39.3 58.9#

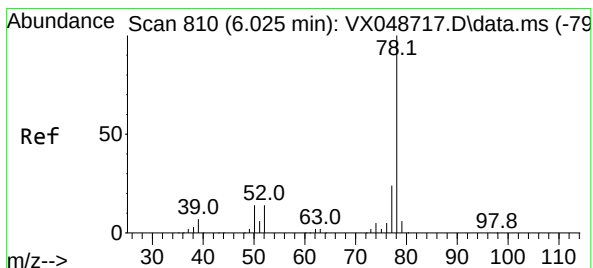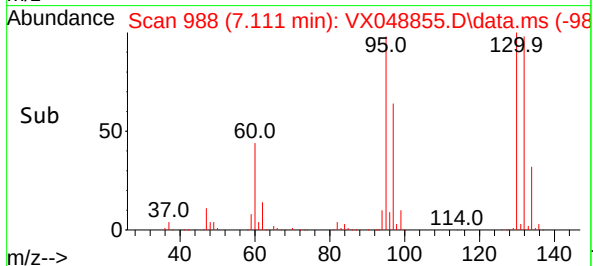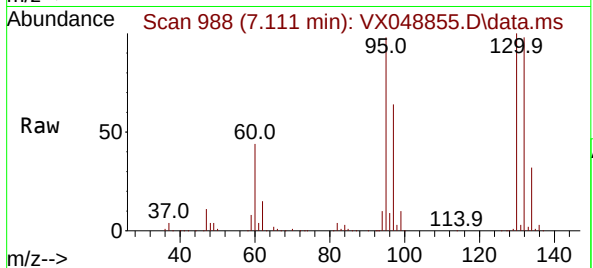

#40

Benzene

Concen: 0.840 ug/l

RT: 6.031 min Scan# 811

Delta R.T. 0.006 min

Lab File: VX048855.D




Acq: 12 Dec 2025 15:20


Tgt Ion: 78 Resp: 7472

Ion Ratio Lower Upper

78 100

77 21.8 18.8 28.2


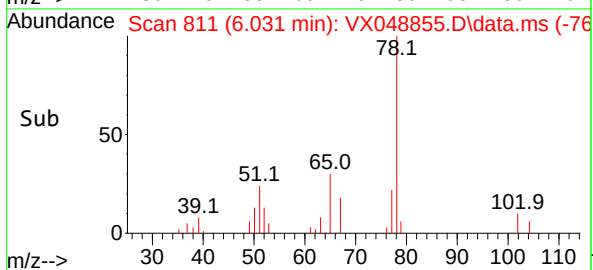

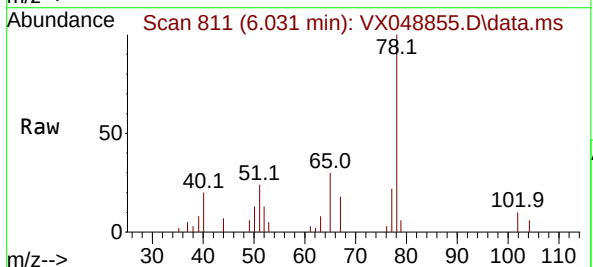




#41
Methacrylonitrile
Concen: 2.135 ug/l
RT: 5.007 min Scan# 643
Delta R.T. 0.104 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-121125-FD


Tgt Ion: 41	Resp: 3481
Ion Ratio	Lower Upper
41 100	
39 43.1	42.3 63.5
67 0.0	66.6 100.0#
52 0.0	23.9 35.9#

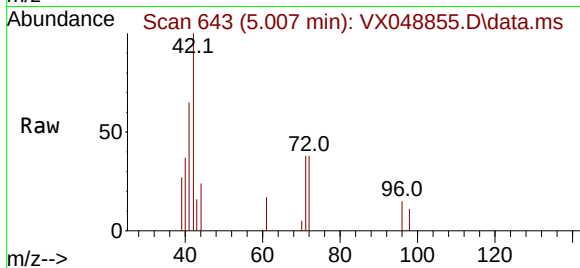

#42
1,2-Dichloroethane
Concen: 1.270 ug/l
RT: 6.074 min Scan# 818
Delta R.T. 0.000 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20

Tgt Ion: 62	Resp: 3997
Ion Ratio	Lower Upper
62 100	
98 6.9	0.0 20.2




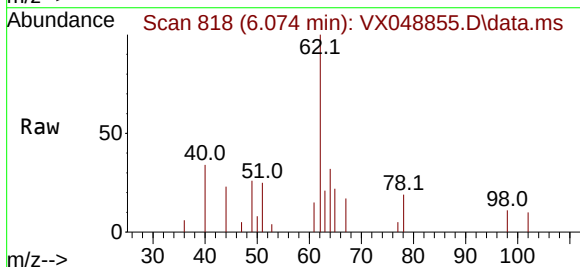




#44
Trichloroethene
Concen: 296.545 ug/l
RT: 7.111 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-121125-FD


Tgt Ion:130 Resp: 687987
Ion Ratio Lower Upper
130 100
95 98.3 0.0 189.6

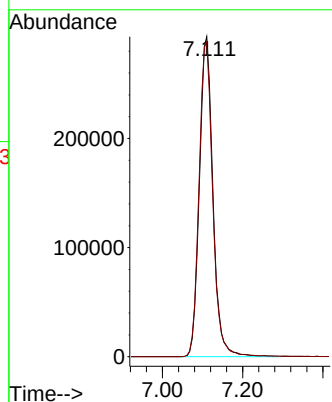

#49
1,4-Dioxane
Concen: 2.530 ug/l
RT: 7.653 min Scan# 1077
Delta R.T. 0.012 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20

Tgt Ion: 88 Resp: 95
Ion Ratio Lower Upper
88 100
43 118.9 28.6 43.0#
58 78.9 58.0 87.0


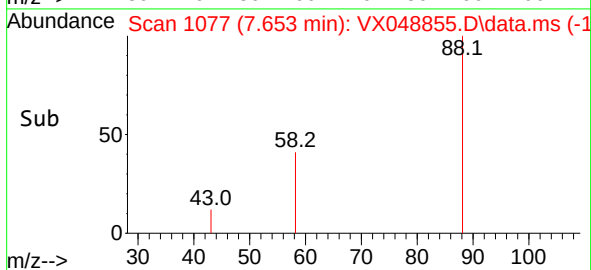






#50
Toluene-d8
Concen: 42.171 ug/l
RT: 8.629 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-121125-FD


Tgt Ion: 98 Resp: 323713
Ion Ratio Lower Upper
98 100
100 65.2 53.4 80.0

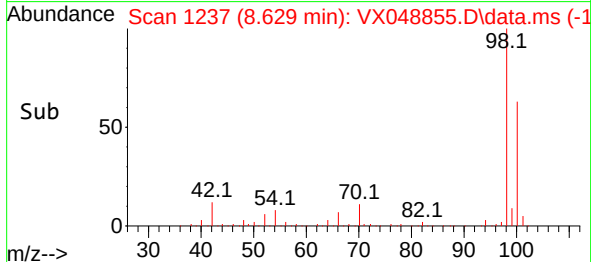

#60
Dibromochloromethane
Concen: 3.042 ug/l
RT: 9.256 min Scan# 1340
Delta R.T. -0.250 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20

Tgt Ion: 129 Resp: 8115
Ion Ratio Lower Upper
129 100
127 0.0 38.3 114.9#




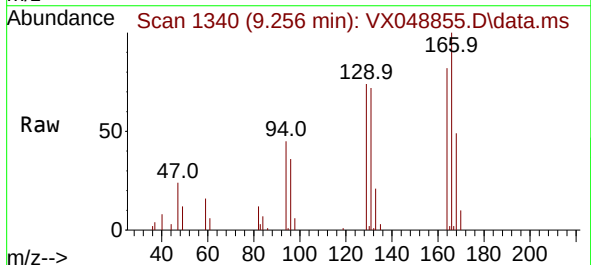




#62
4-Bromofluorobenzene
Concen: 53.552 ug/l
RT: 11.061 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-121125-FD


Tgt Ion: 95 Resp: 141751
Ion Ratio Lower Upper
95 100
174 80.8 0.0 157.8
176 77.7 0.0 154.0



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. 0.000 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20

Tgt Ion: 117 Resp: 339965
Ion Ratio Lower Upper
117 100
82 56.6 44.1 66.1
119 32.0 25.2 37.8


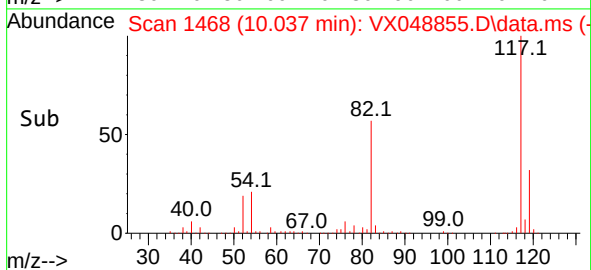






#64
Tetrachloroethene
Concen: 3.475 ug/l
RT: 9.256 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-121125-FD


Tgt Ion:164	Resp:	8611
Ion	Ratio	Lower Upper
164	100	
166	122.0	103.1 154.7
129	90.4	76.9 115.3
131	87.4	75.1 112.7



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. 0.000 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20

Tgt Ion:152	Resp:	178735
Ion	Ratio	Lower Upper
152	100	
115	59.3	42.1 126.4
150	158.7	0.0 347.8


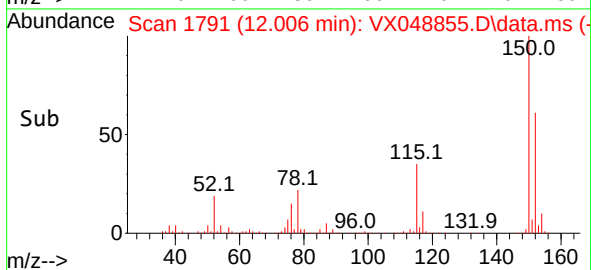






#76
1,2,3-Trichloropropane
Concen: 22.103 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.158 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20




Instrument :
MSVOA_X
ClientSampleId :
MW-18B-57.5-121125-FD


Tgt Ion: 75 Resp: 73581
Ion Ratio Lower Upper
75 100
77 1.0 24.3 73.0#

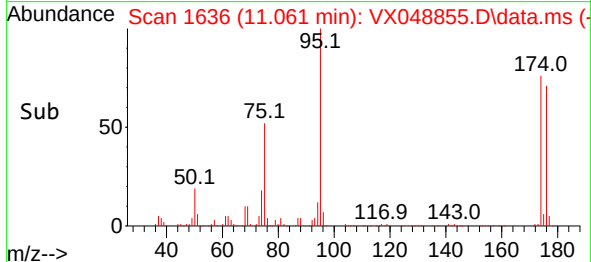

#81
trans-1,4-Dichloro-2-butene
Concen: 52.504 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. 0.061 min
Lab File: VX048855.D
Acq: 12 Dec 2025 15:20

Tgt Ion: 75 Resp: 73581
Ion Ratio Lower Upper
75 100
53 0.1 79.9 119.9#
89 0.0 67.1 100.7#

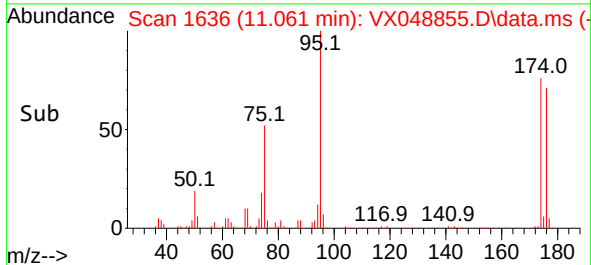



#95

Naphthalene

Concen: Below Cal

RT: 13.762 min Scan# 20

Delta R.T. 0.006 min

Lab File: VX048855.D


Acq: 12 Dec 2025 15:20

Instrument :

MSVOA_X

ClientSampleId :

MW-18B-57.5-121125-FD

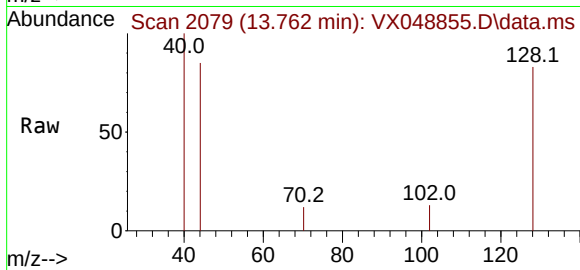

Tgt Ion:128 Resp: 598

Ion Ratio Lower Upper

128 100

127 0.0 10.2 15.2#

129 0.0 8.6 13.0#

