

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121225\
 Data File : VX048854.D
 Acq On : 12 Dec 2025 14:58
 Operator : JC/MD
 Sample : Q3835-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-01-7-121025

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M

Title : SW846 8260

Signal : TIC: VX048854.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.337	200	205	211	rBV4	4991	10396	1.19%	0.190%
2	4.477	546	556	567	rBV2	43580	132401	15.19%	2.419%
3	5.373	690	703	719	rBV	86250	277911	31.88%	5.077%
4	5.537	719	730	747	rVB	116099	357970	41.07%	6.540%
5	5.940	786	796	815	rBV	89635	264770	30.38%	4.837%
6	6.745	917	928	945	rBV	230195	588862	67.56%	10.758%
7	7.110	979	988	1008	rBV	322593	778673	89.33%	14.225%
8	8.634	1231	1238	1255	rBV	452508	752977	86.39%	13.756%
9	10.037	1462	1468	1481	rBV	588203	834248	95.71%	15.241%
10	11.061	1631	1636	1651	rBV	432859	604043	69.30%	11.035%
11	12.006	1785	1791	1803	rBV	648540	871637	100.00%	15.924%




Sum of corrected areas: 5473888

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121225\
Data File : VX048854.D
Acq On : 12 Dec 2025 14:58
Operator : JC/MD
Sample : Q3835-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-01-7-121025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

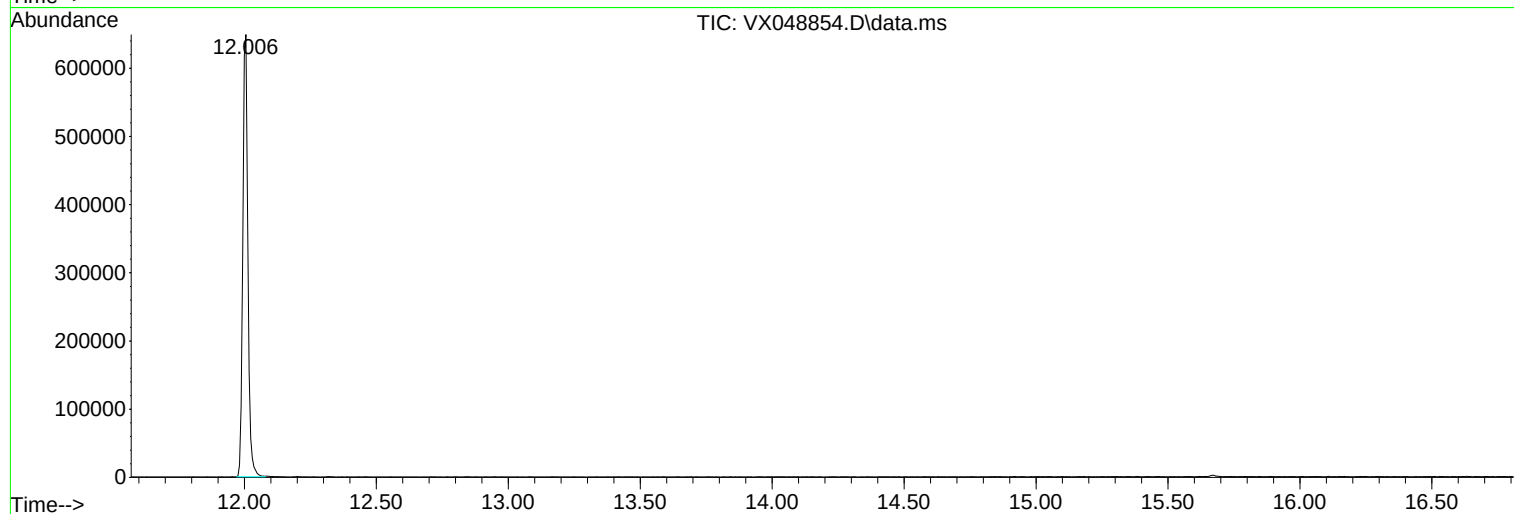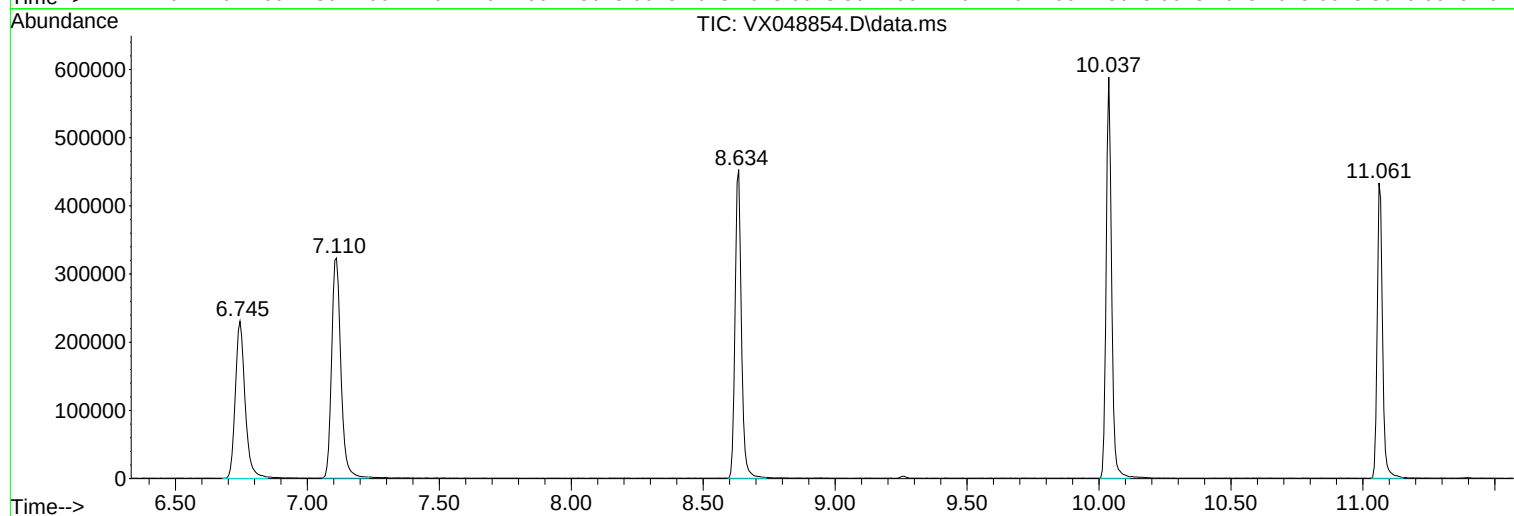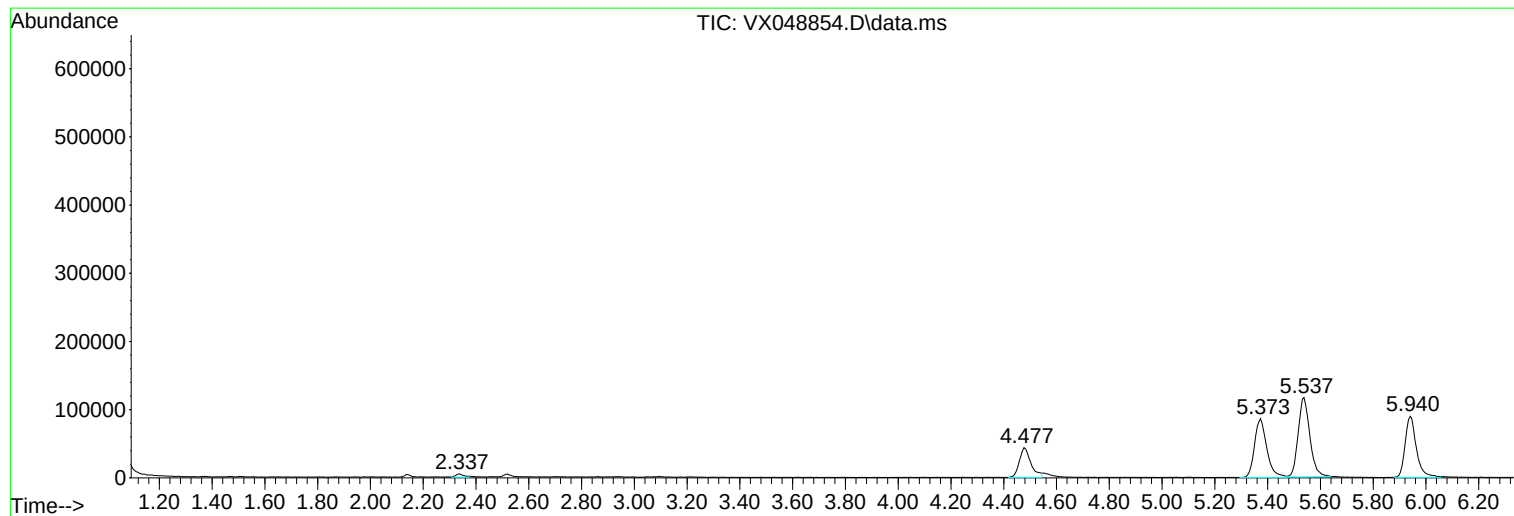

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121225\
Data File : VX048854.D
Acq On : 12 Dec 2025 14:58
Operator : JC/MD
Sample : Q3835-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-01-7-121025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121225\
Data File : VX048854.D
Acq On : 12 Dec 2025 14:58
Operator : JC/MD
Sample : Q3835-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-01-7-121025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120425W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc