

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX121318\
 Data File : VX006506.D
 Acq On : 13 Dec 2018 20:10
 Operator : JC/MD
 Sample : J6373-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-A-FRAME

Quant Time: Dec 14 00:19:44 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 30 03:55:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	635550	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	1032966	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	960858	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	466860	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	350944	54.09	ug/l	0.00
Spiked Amount			Recovery	=	108.18%	
35) Dibromofluoromethane	5.50	113	305064	45.61	ug/l	0.00
Spiked Amount			Recovery	=	91.22%	
50) Toluene-d8	8.71	98	1223390	50.29	ug/l	0.00
Spiked Amount			Recovery	=	100.58%	
62) 4-Bromofluorobenzene	11.13	95	458316	50.00	ug/l	0.00
Spiked Amount			Recovery	=	100.00%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Chloroethane	1.72	64	1617	0.383	ug/l #	67
11) Tert butyl alcohol	3.02	59	3942	2.222	ug/l #	76
13) Acrolein	2.31	56	660	0.681	ug/l #	31
14) Allyl chloride	2.85	41	45233	3.982	ug/l #	27
16) Acetone	2.44	43	16413	5.391	ug/l	96
18) Methyl Acetate	2.78	43	30037	2.950	ug/l #	87
20) Methylene Chloride	2.86	84	1324827	204.450	ug/l	93
36) 1,1-Dichloropropene	5.66	75	44119	5.072	ug/l #	49
38) Carbon Tetrachloride	5.67	117	61156	5.976	ug/l #	17
43) Isopropyl Acetate	6.46	43	35163	2.165	ug/l	99
48) Methyl methacrylate	7.69	41	18027	2.282	ug/l #	23
49) 1,4-Dioxane	7.75	88	108	0.555	ug/l #	1
51) 4-Methyl-2-Pentanone	8.62	43	169643	17.942	ug/l #	48
52) Toluene	8.79	92	8284	0.483	ug/l	99
54) cis-1,3-Dichloropropene	8.62	75	89589	7.966	ug/l #	60
57) 1,3-Dichloropropane	9.54	76	20387	1.851	ug/l #	44
59) 2-Hexanone	9.54	43	242107	33.516	ug/l #	52
68) m/p-Xylenes	10.36	106	3859	0.284	ug/l	91
74) N-amyl acetate	10.69	43	25232	1.817	ug/l #	54
76) 1,2,3-Trichloropropane	11.13	75	206916	22.962	ug/l #	37
80) 1,3,5-Trimethylbenzene	11.51	105	12006	0.448	ug/l	99
81) trans-1,4-Dichloro-2-buten	11.13	75	206916	53.886	ug/l #	15
84) 1,2,4-Trimethylbenzene	11.80	105	21190	0.765	ug/l	97
89) n-Butylbenzene	12.38	91	5330	0.213	ug/l #	59
95) Naphthalene	13.83	128	342208	9.543	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX121318\
Data File : VX006506.D
Acq On : 13 Dec 2018 20:10
Operator : JC/MD
Sample : J6373-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-A-FRAME

Quant Time: Dec 14 00:19:44 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 30 03:55:33 2018
Response via : Initial Calibration

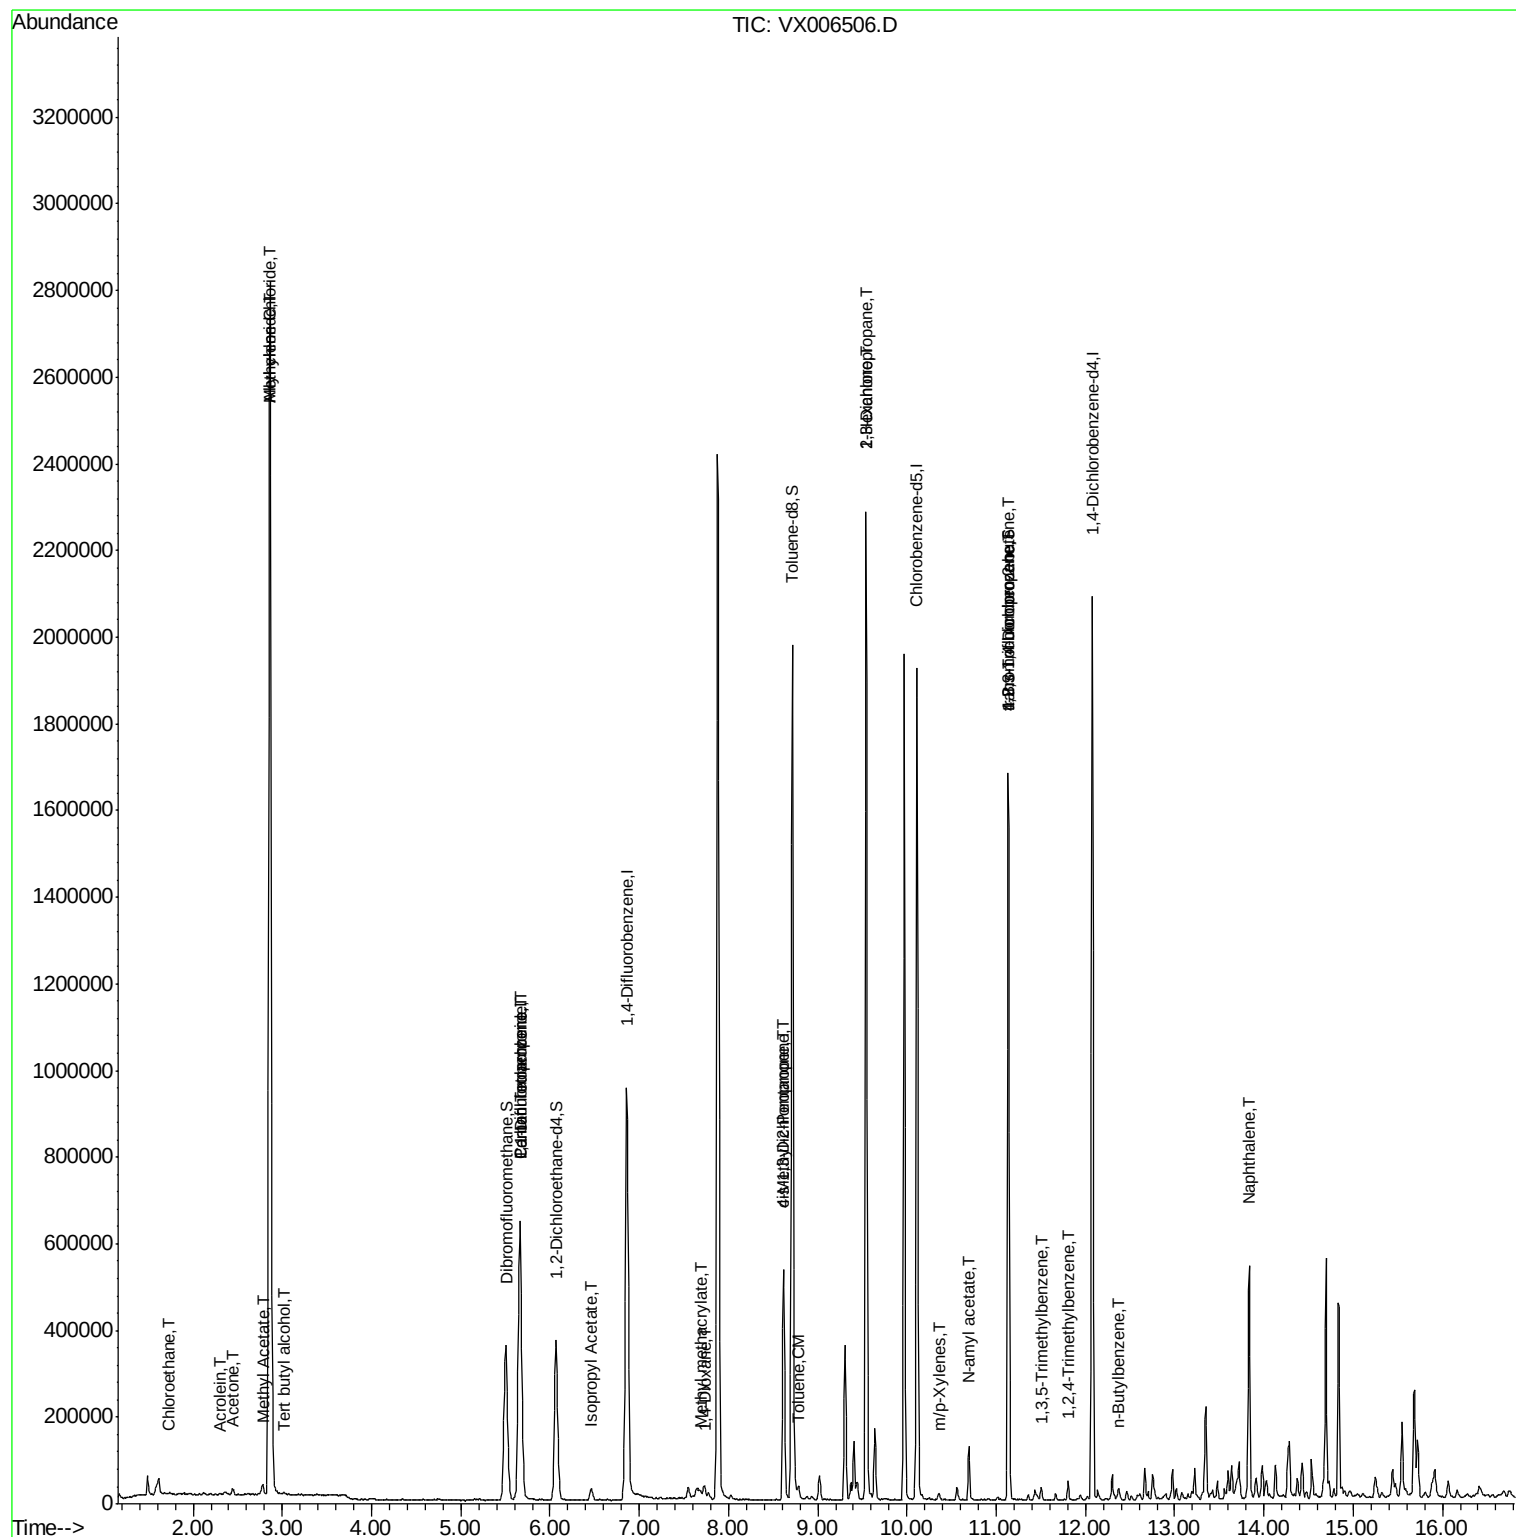



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX006506.D

Acq: 13 Dec 2018 20:10

Instrument :

MSVOA_X

ClientSampleId :


TP-A-FRAME

Tot Ion:168 Resp: 635550

Ion Ratio Lower Upper




168 100

99 53.9 37.8 56.8



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

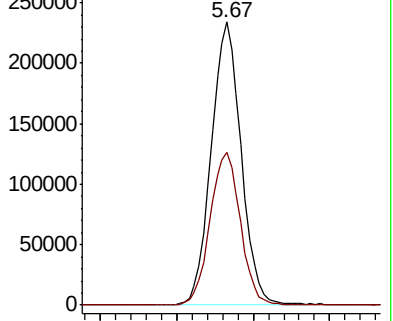

#6

Chloroethane

Concen: 0.383 ug/l

RT: 1.72 min Scan# 93

Delta R.T. 0.00 min

Lab File: VX006506.D


Acq: 13 Dec 2018 20:10

Tgt Ion: 64 Resp: 1617

Ion Ratio Lower Upper



64 100


66 14.1 25.9 38.9#



Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0




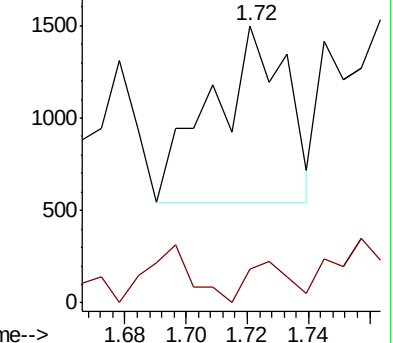


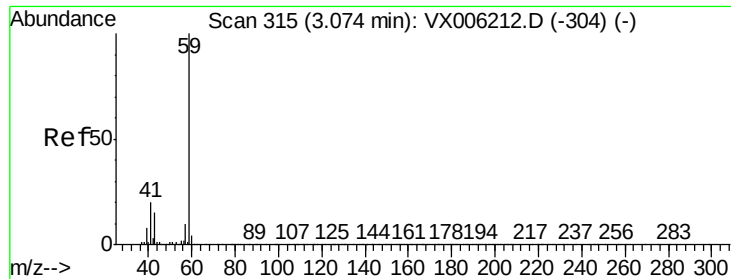

#11
Tert butyl alcohol
Concen: 2.222 ug/l
RT: 3.02 min Scan# 306
Delta R.T. -0.05 min
Lab File: VX006506.D
Acq: 13 Dec 2018 20:10




Instrument :
MSVOA_X
ClientSampled :
TP-A-FRAME


Tot Ion: 59 Resp: 3942
Ion Ratio Lower Upper
59 100
57 1.2 8.2 12.2#

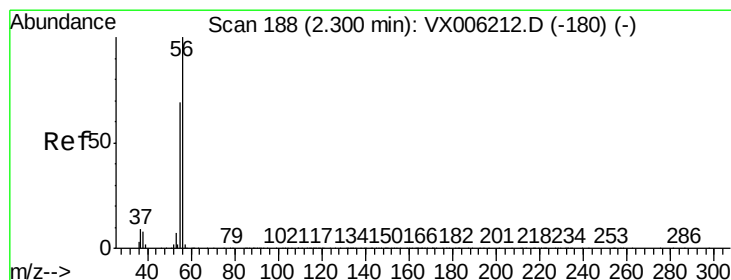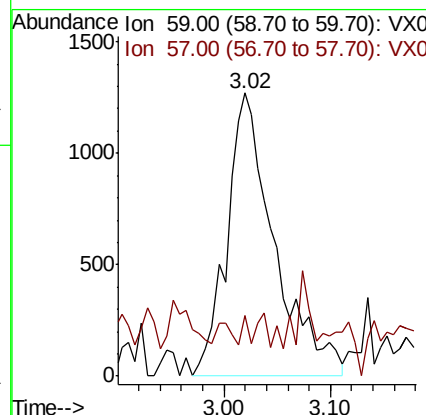

#13
Acrolein
Concen: 0.681 ug/l
RT: 2.31 min Scan# 189
Delta R.T. 0.01 min
Lab File: VX006506.D
Acq: 13 Dec 2018 20:10

Tgt Ion: 56 Resp: 660
Ion Ratio Lower Upper
56 100
55 14.4 57.8 86.6#


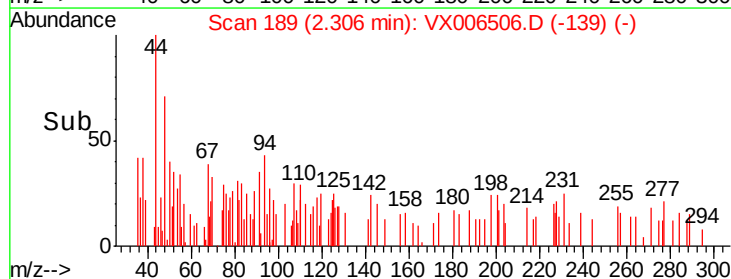
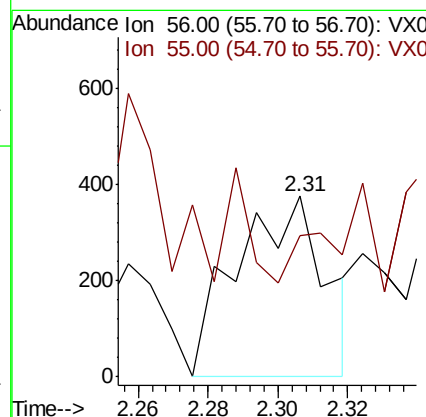
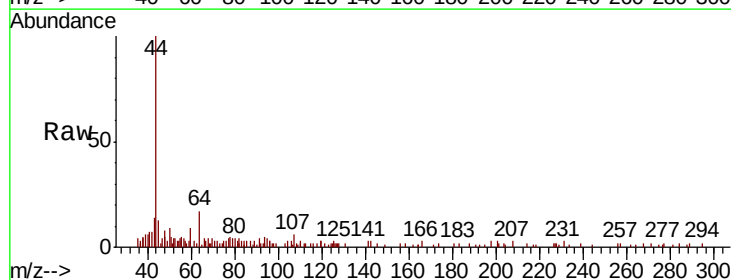


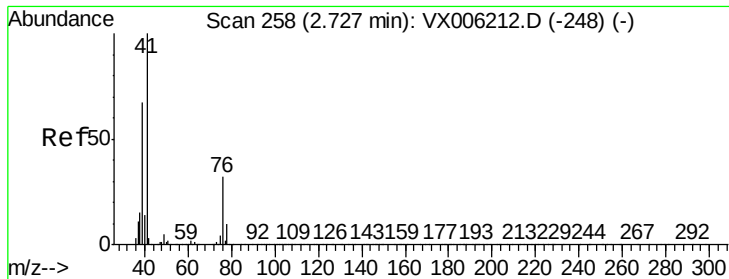

#14
Allvl chloride
Concen: 3.982 ug/l
RT: 2.85 min Scan# 279
Delta R.T. 0.13 min
Lab File: VX006506.D
Acq: 13 Dec 2018 20:10




Instrument :
MSVOA_X
ClientSampleId :
TP-A-FRAME


Tot Ion: 41 Resp: 45233
Ion Ratio Lower Upper
41 100
39 1.5 52.4 78.6#
76 0.3 25.4 38.0#

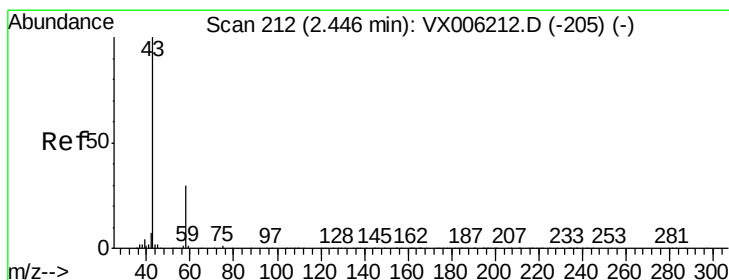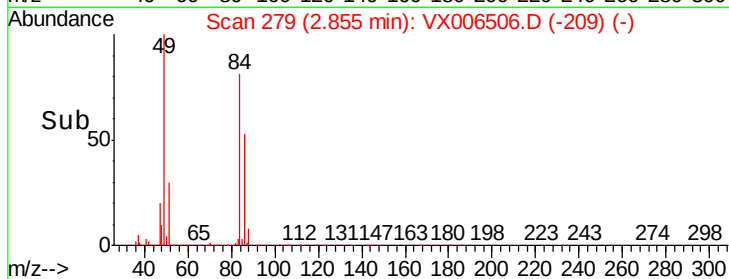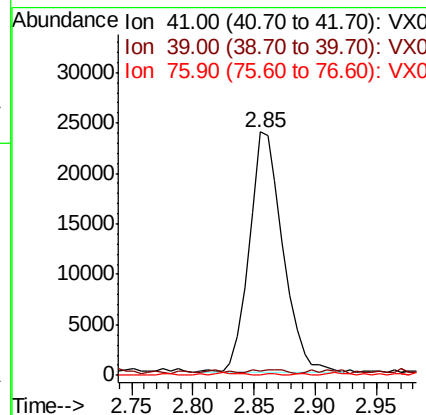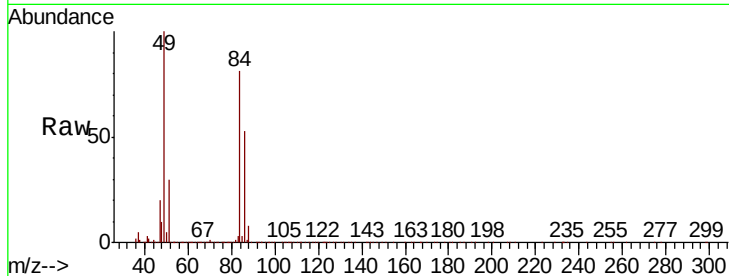

#16
Acetone
Concen: 5.391 ug/l
RT: 2.44 min Scan# 211
Delta R.T. -0.01 min
Lab File: VX006506.D
Acq: 13 Dec 2018 20:10

Tgt Ion: 43 Resp: 16413
Ion Ratio Lower Upper
43 100
58 32.0 24.0 36.0


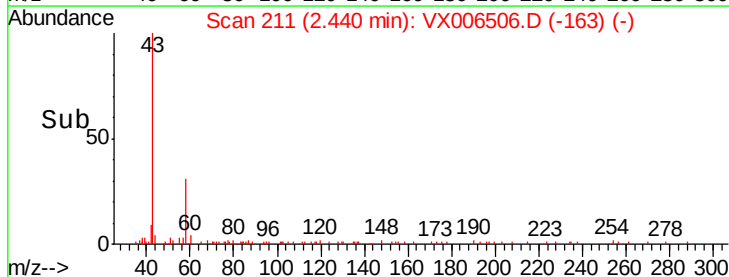
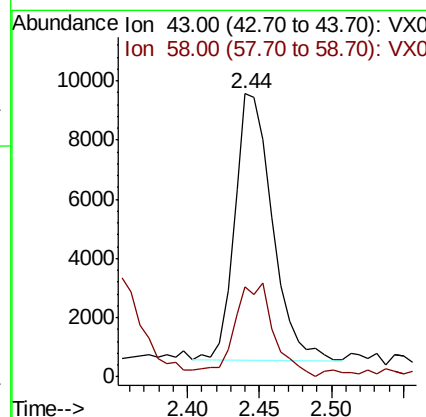
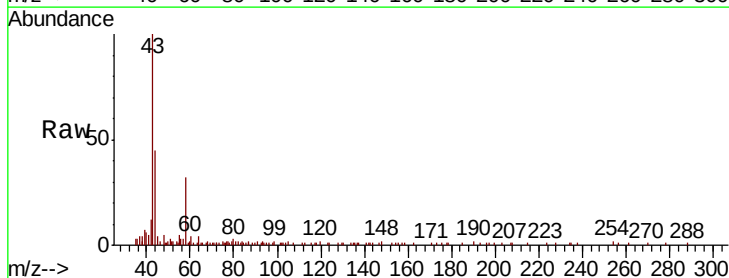




#18
Methyl Acetate
Concen: 2.950 ug/l
RT: 2.78 min Scan# 267
Delta R.T. 0.00 min
Lab File: VX006506.D
Acq: 13 Dec 2018 20:10




Instrument :
MSVOA_X
ClientSampleId :
TP-A-FRAME


Tot Ion: 43 Resp: 30037
Ion Ratio Lower Upper
43 100
74 28.6 17.9 26.9#

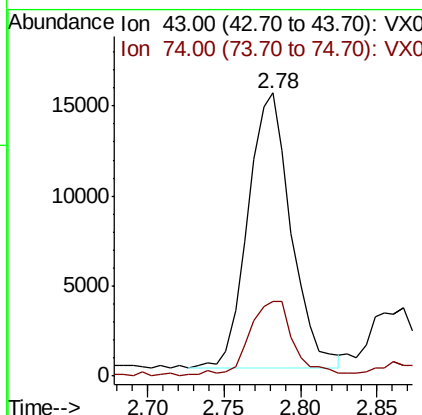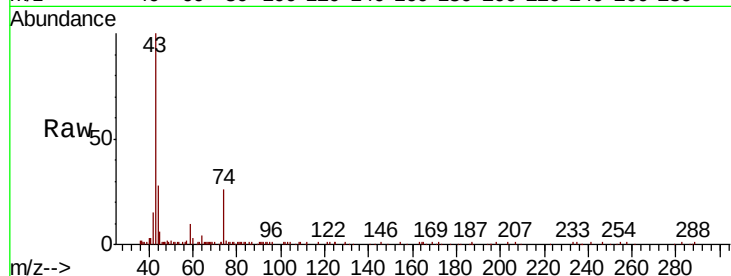

#20
Methylene Chloride
Concen: 204.450 ug/l
RT: 2.86 min Scan# 280
Delta R.T. 0.00 min
Lab File: VX006506.D
Acq: 13 Dec 2018 20:10

Tgt Ion: 84 Resp: 1324827
Ion Ratio Lower Upper
84 100
49 117.3 102.2 153.4
51 36.9 31.1 46.7
86 64.0 53.7 80.5



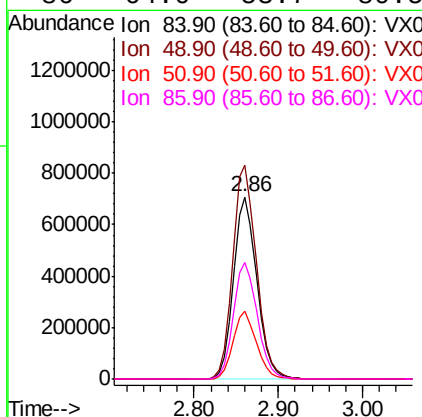





#33
 1,2-Dichloroethane-d4
 Concen: 54.092 ug/l
 RT: 6.07 min Scan# 806
 Delta R.T. 0.00 min
 Lab File: VX006506.D
 Acq: 13 Dec 2018 20:10




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-A-FRAME


Tot Ion: 65 Resp: 350944
 Ion Ratio Lower Upper
 65 100
 67 53.0 0.0 107.2

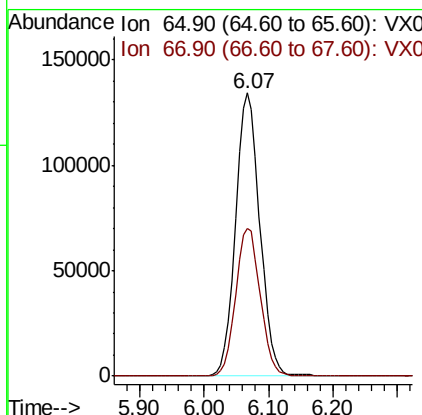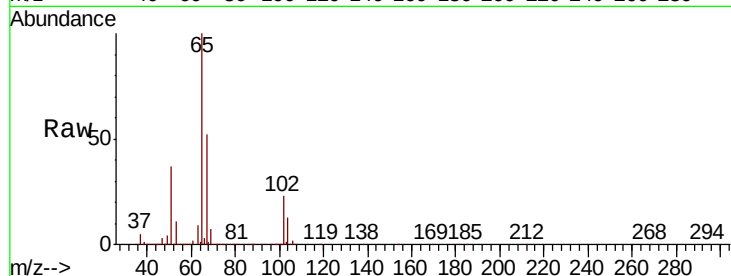

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. 0.00 min
 Lab File: VX006506.D
 Acq: 13 Dec 2018 20:10

Tgt Ion: 114 Resp: 1032966
 Ion Ratio Lower Upper
 114 100
 63 17.6 0.0 36.6
 88 14.4 0.0 29.0

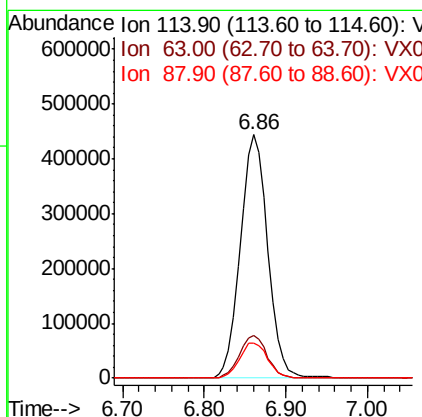

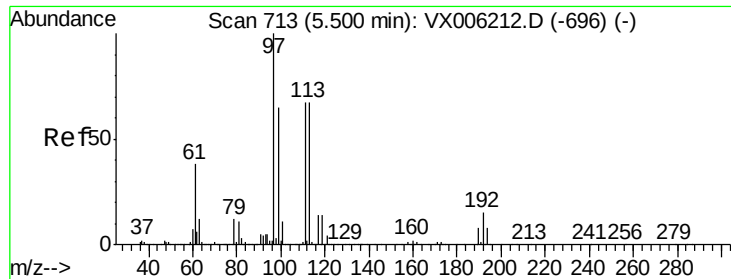

#35

Dibromofluoromethane

Concen: 45.613 ug/l

RT: 5.50 min Scan# 713

Delta R.T. 0.00 min

Lab File: VX006506.D

Acq: 13 Dec 2018 20:10

Instrument :

MSVOA_X

ClientSampleId :

TP-A-FRAME


Tot Ion:113 Resp: 305064

Ion Ratio Lower Upper

113 100

111 103.3 81.1 121.7




192 20.1 18.2 27.2

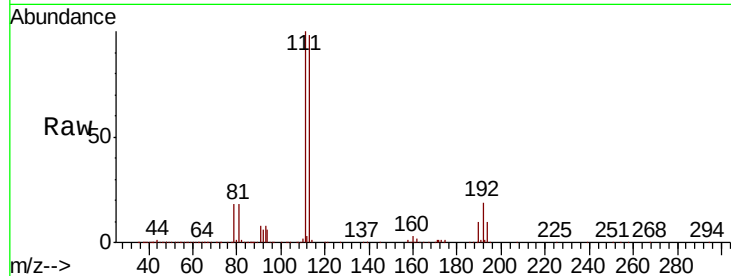

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

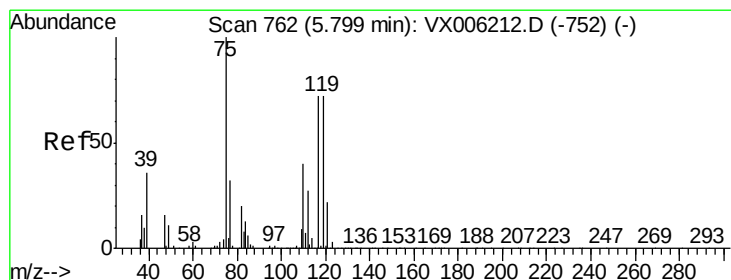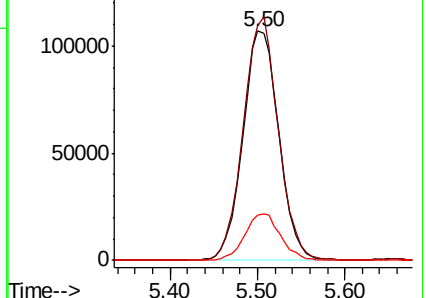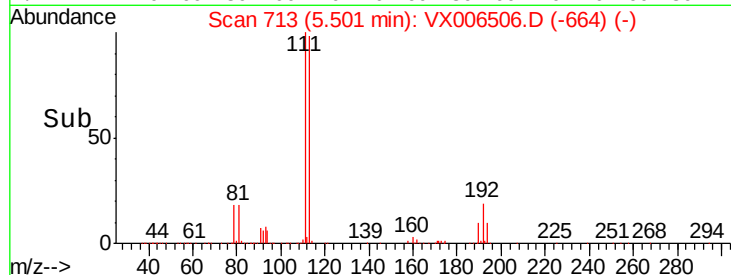

#36

1,1-Dichloropropene

Concen: 5.072 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.14 min

Lab File: VX006506.D

Acq: 13 Dec 2018 20:10


Tgt Ion: 75 Resp: 44119

Ion Ratio Lower Upper

75 100

110 10.4 20.4 61.3#



77 1.3 24.9 37.3#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

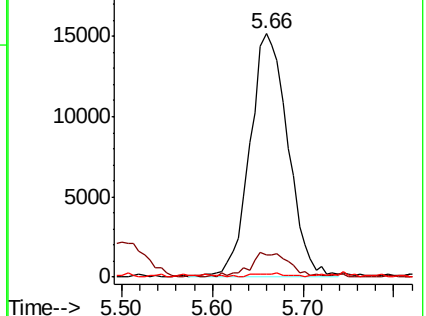



#38

Carbon Tetrachloride

Concen: 5.976 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.12 min

Lab File: VX006506.D

Acq: 13 Dec 2018 20:10

Instrument :

MSVOA_X

ClientSampleId :

TP-A-FRAME


Tot Ion:117 Resp: 61156

Ion Ratio Lower Upper

117 100

119 5.3 75.8 113.8#




121 0.0 24.6 37.0#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

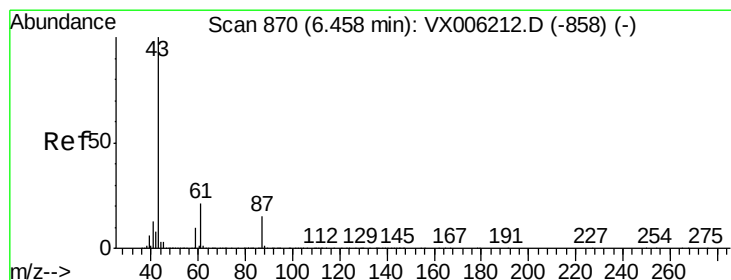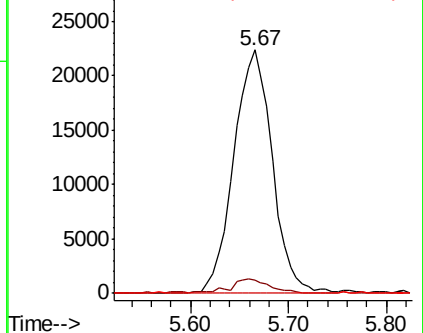

#43

Isopropyl Acetate

Concen: 2.165 ug/l

RT: 6.46 min Scan# 871

Delta R.T. 0.01 min

Lab File: VX006506.D

Acq: 13 Dec 2018 20:10


Tgt Ion: 43 Resp: 35163

Ion Ratio Lower Upper

43 100

61 21.7 16.8 25.2



87 15.1 11.9 17.9




Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0




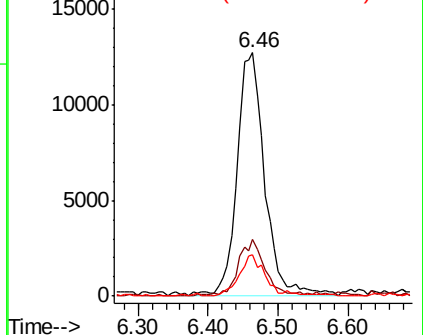




#48
Methvl methacrylate
Concen: 2.282 ug/l
RT: 7.69 min Scan# 1072
Delta R.T. -0.09 min
Lab File: VX006506.D
Acq: 13 Dec 2018 20:10




Instrument :
MSVOA_X
ClientSampleId :
TP-A-FRAME


Tot Ion: 41 Resp: 18027
Ion Ratio Lower Upper
41 100
69 0.0 70.3 105.5#
39 19.5 45.3 67.9#

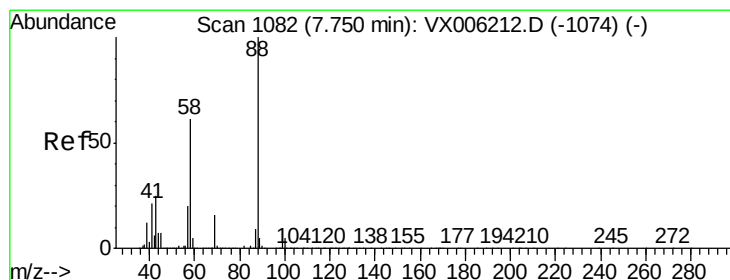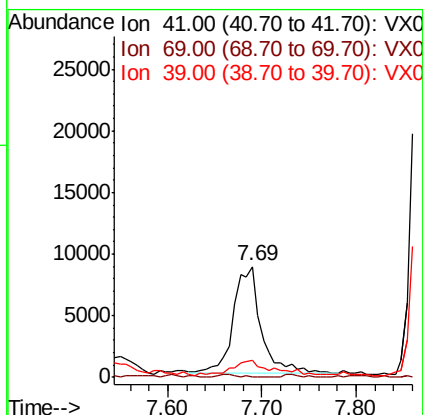

#49
1,4-Dioxane
Concen: 0.555 ug/l
RT: 7.75 min Scan# 1082
Delta R.T. 0.00 min
Lab File: VX006506.D
Acq: 13 Dec 2018 20:10

Tgt Ion: 88 Resp: 108
Ion Ratio Lower Upper
88 100
43 0.0 23.2 34.8#
58 1534.3 51.4 77.0#

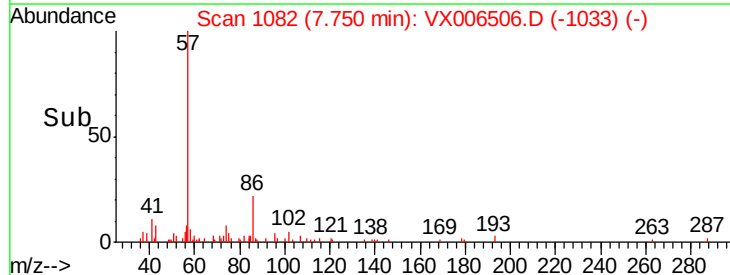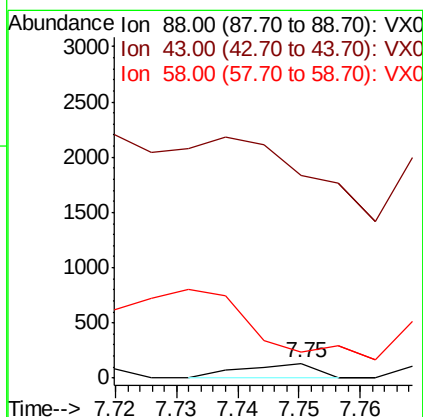

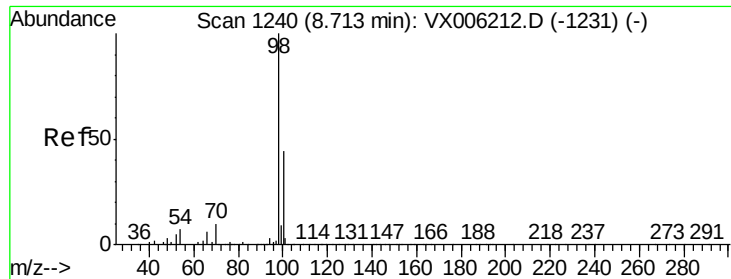

#50

Toluene-d8

Concen: 50.289 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX006506.D

Acq: 13 Dec 2018 20:10

Instrument :

MSVOA_X

ClientSampleId :





TP-A-FRAME

Tot Ion: 98 Resp: 1223390

Ion Ratio Lower Upper

98 100

100 65.2 52.2 78.2

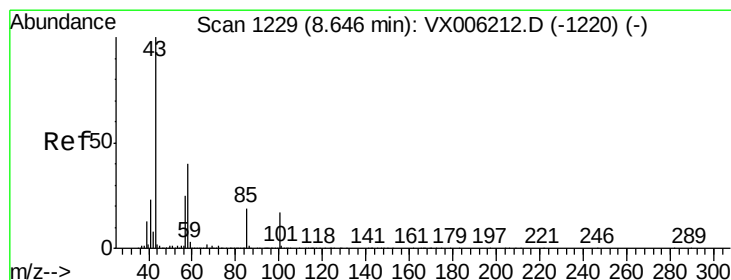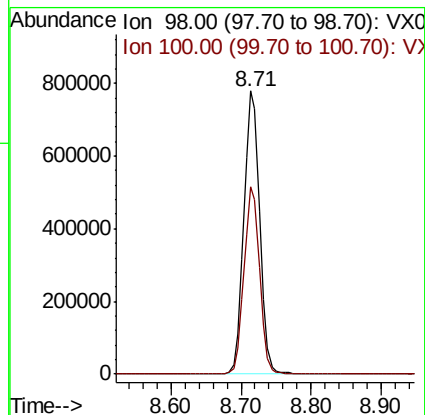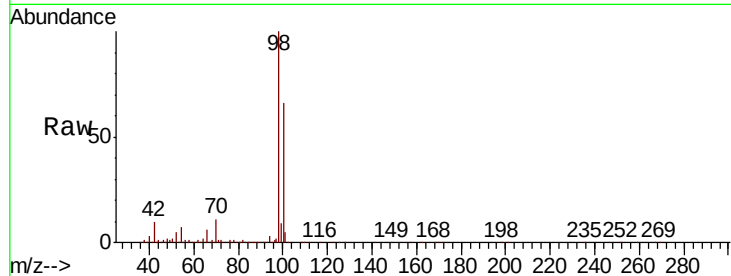

#51

4-Methyl-2-Pentanone

Concen: 17.942 ug/l

RT: 8.62 min Scan# 1224

Delta R.T. -0.03 min

Lab File: VX006506.D




Acq: 13 Dec 2018 20:10


Tgt Ion: 43 Resp: 169643

Ion Ratio Lower Upper

43 100

58 7.5 31.3 46.9#

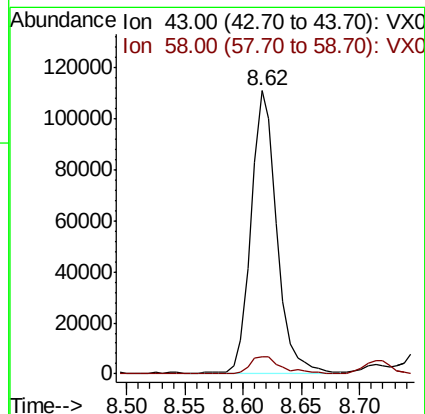



#52

Toluene

Concen: 0.483 ug/l

RT: 8.79 min Scan# 1252

Delta R.T. 0.00 min

Lab File: VX006506.D

Acq: 13 Dec 2018 20:10

Instrument :

MSVOA_X

ClientSampled :


TP-A-FRAME

Tot Ion: 92 Resp: 8284

Ion Ratio Lower Upper




92 100

91 175.5 139.2 208.8

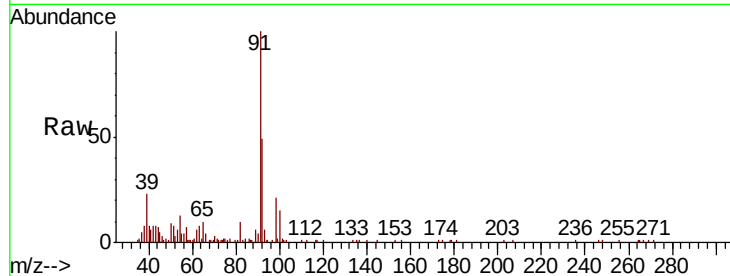

Abundance Ion 92.00 (91.70 to 92.70): VX0

Ion 91.00 (90.70 to 91.70): VX0

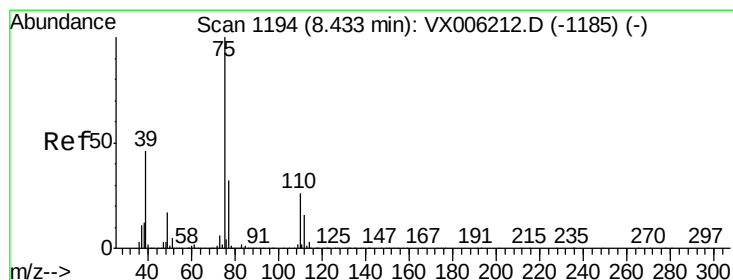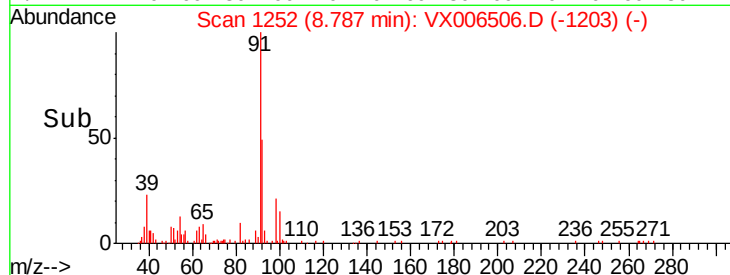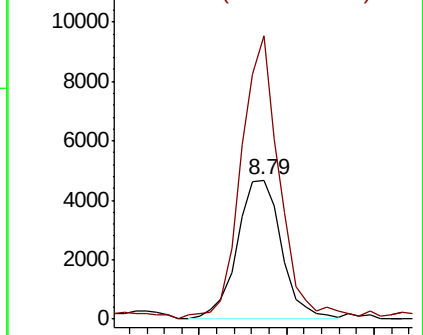

#54

cis-1,3-Dichloropropene

Concen: 7.966 ug/l

RT: 8.62 min Scan# 1224

Delta R.T. 0.18 min

Lab File: VX006506.D

Acq: 13 Dec 2018 20:10


Tgt Ion: 75 Resp: 89589

Ion Ratio Lower Upper

75 100

77 0.1 25.6 38.4#



39 27.7 36.5 54.7#

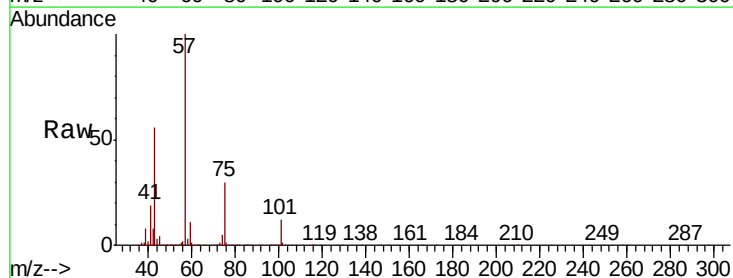


Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 76.90 (76.60 to 77.60): VX0

Ion 39.00 (38.70 to 39.70): VX0



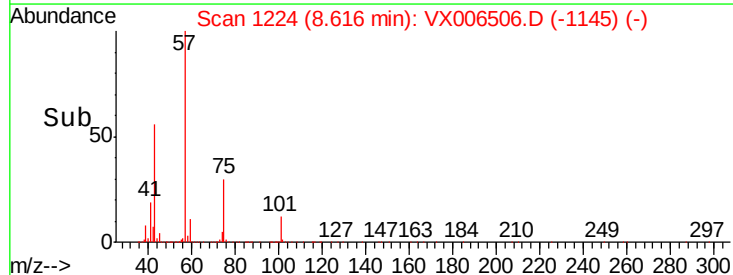
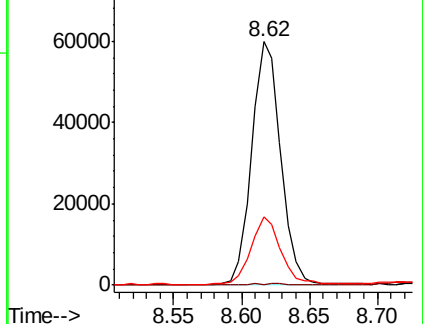


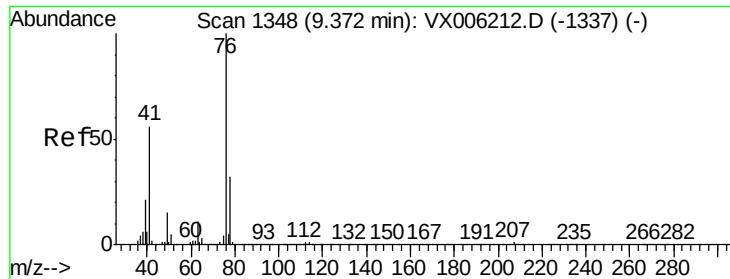

#57
 1,3-Dichloropropane
 Concen: 1.851 ug/l
 RT: 9.54 min Scan# 1376
 Delta R.T. 0.17 min
 Lab File: VX006506.D
 Acq: 13 Dec 2018 20:10




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-A-FRAME


Tot Ion: 76 Resp: 20387
 Ion Ratio Lower Upper
 76 100
 78 1.0 26.1 39.1#

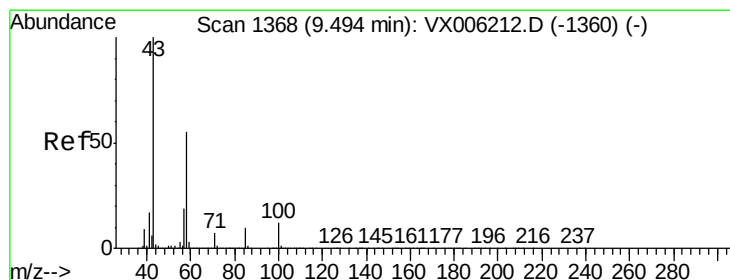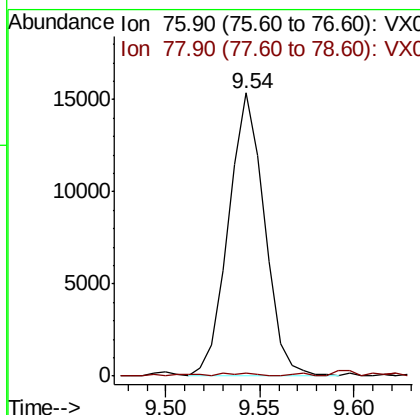

#59
 2-Hexanone
 Concen: 33.516 ug/l
 RT: 9.54 min Scan# 1376
 Delta R.T. 0.05 min
 Lab File: VX006506.D
 Acq: 13 Dec 2018 20:10

Tgt Ion: 43 Resp: 242107
 Ion Ratio Lower Upper
 43 100
 58 20.4 27.7 83.1#

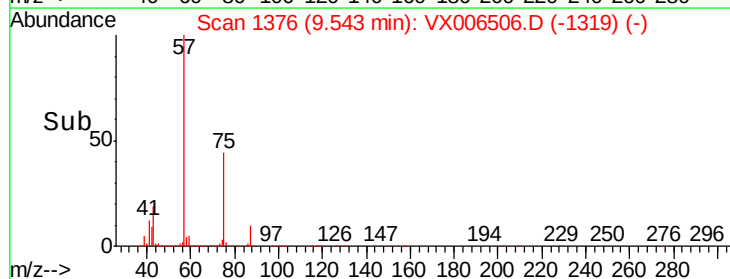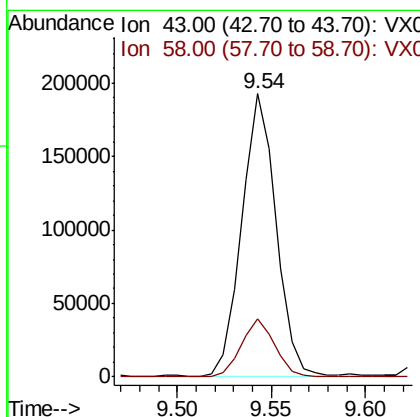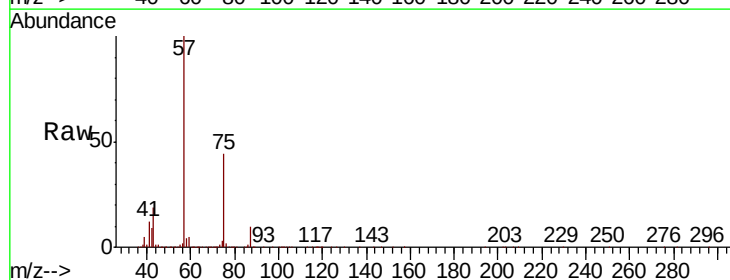

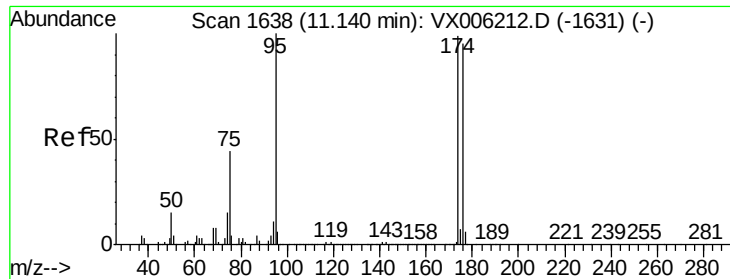

#62

4-Bromofluorobenzene

Concen: 49.995 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.01 min

Lab File: VX006506.D

Acq: 13 Dec 2018 20:10

Instrument :

MSVOA_X

ClientSampleId :

TP-A-FRAME


Tot Ion: 95 Resp: 458316

Ion Ratio Lower Upper

95 100

174 85.9 0.0 187.0

176 82.2 0.0 181.8

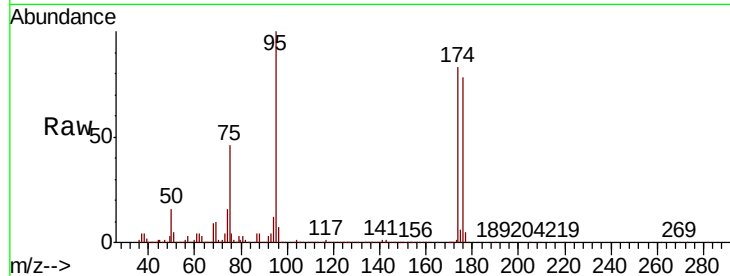


Abundance Ion 94.90 (94.60 to 95.60): VX006506.D (-1589) (-)

Ion 173.80 (173.50 to 174.50): VX006506.D (-1589) (-)

Ion 175.80 (175.50 to 176.50): VX006506.D (-1589) (-)

Time-->

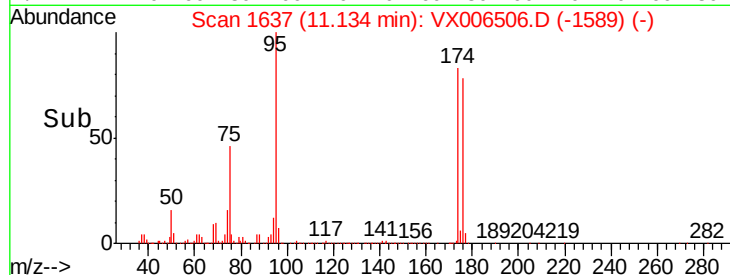


Abundance

Ion 94.90 (94.60 to 95.60): VX006506.D (-1589) (-)

Ion 173.80 (173.50 to 174.50): VX006506.D (-1589) (-)

Ion 175.80 (175.50 to 176.50): VX006506.D (-1589) (-)

Time-->



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. -0.01 min

Lab File: VX006506.D

Acq: 13 Dec 2018 20:10


Tgt Ion: 117 Resp: 960858

Ion Ratio Lower Upper

117 100

82 52.3 39.6 59.4

119 31.7 26.3 39.5




Abundance Ion 116.90 (116.60 to 117.60): VX006506.D (-1421) (-)

Ion 82.00 (81.70 to 82.70): VX006506.D (-1421) (-)

Ion 118.90 (118.60 to 119.60): VX006506.D (-1421) (-)

Time-->




Abundance

Ion 116.90 (116.60 to 117.60): VX006506.D (-1421) (-)

Ion 82.00 (81.70 to 82.70): VX006506.D (-1421) (-)

Ion 118.90 (118.60 to 119.60): VX006506.D (-1421) (-)





Time-->



#68
m/p-Xvlenes
Concen: 0.284 ug/l
RT: 10.36 min Scan# 1510
Delta R.T. 0.00 min
Lab File: VX006506.D
Acq: 13 Dec 2018 20:10




Instrument :
MSVOA_X
ClientSampleId :
TP-A-FRAME


Tot Ion:106 Resp: 3859
Ion Ratio Lower Upper
106 100
91 180.6 155.2 232.8

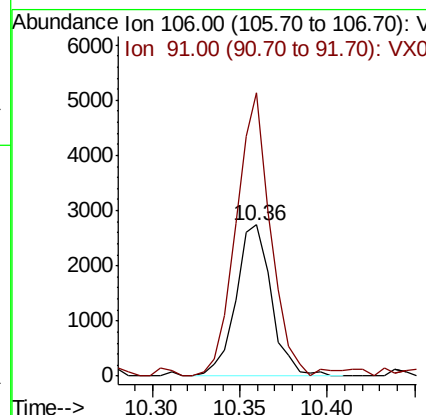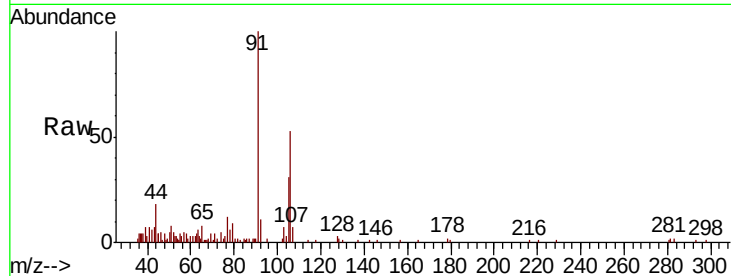

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX006506.D
Acq: 13 Dec 2018 20:10

Tgt Ion:152 Resp: 466860
Ion Ratio Lower Upper
152 100
115 56.3 39.0 116.9
150 156.0 0.0 345.8

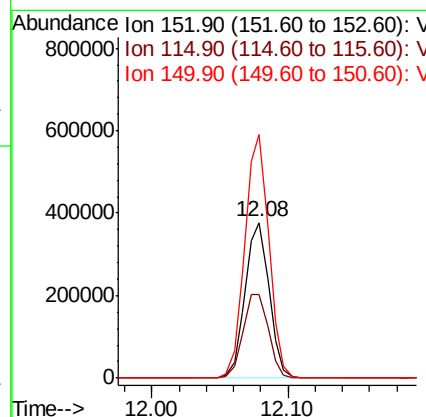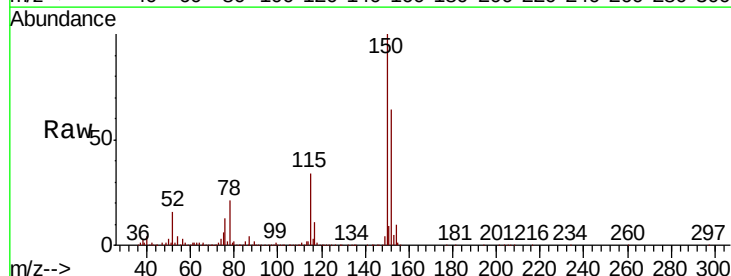



#74

N-amvl acetate

Concen: 1.817 ug/l

RT: 10.69 min Scan# 1565

Delta R.T. -0.20 min

Lab File: VX006506.D

Acq: 13 Dec 2018 20:10

Instrument :

MSVOA_X

ClientSampleId :

TP-A-FRAME

Tot Ion: 43 Resp: 25232


Ion Ratio Lower Upper

43 100

70 2.2 34.1 51.1#

55 4.3 17.8 26.8#

61 13.1 19.7 29.5#



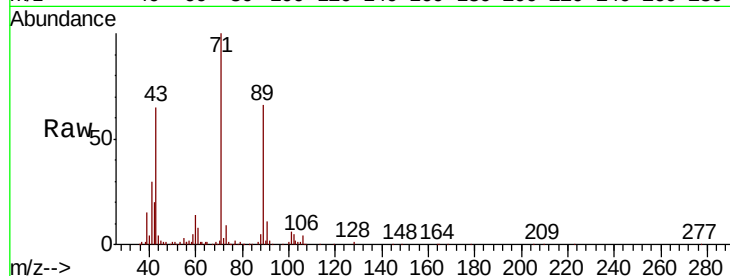


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

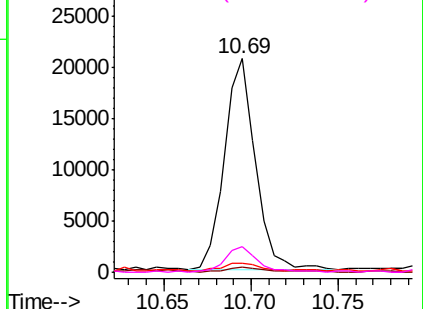

#76

1,2,3-Trichloropropane

Concen: 22.962 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.16 min

Lab File: VX006506.D


Acq: 13 Dec 2018 20:10

Tgt Ion: 75 Resp: 206916

Ion Ratio Lower Upper



75 100


77 1.3 19.9 59.7#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0



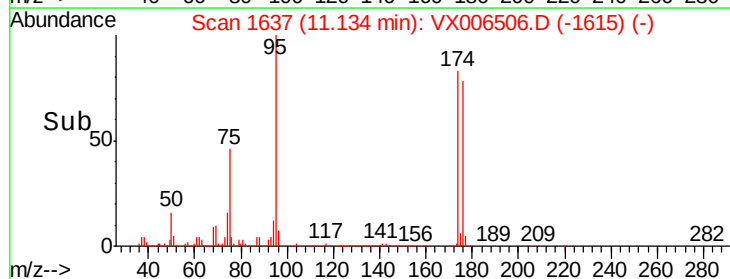
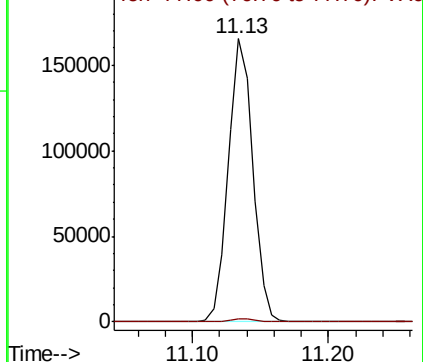


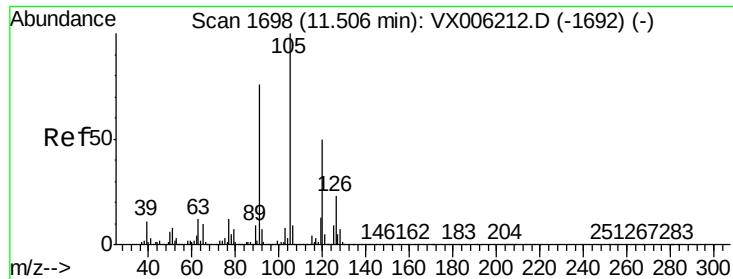

#80
 1,3,5-Trimethylbenzene
 Concen: 0.448 ug/l
 RT: 11.51 min Scan# 1698
 Delta R.T. 0.00 min
 Lab File: VX006506.D
 Acq: 13 Dec 2018 20:10




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-A-FRAME


Tot Ion:105 Resp: 12006
 Ion Ratio Lower Upper
 105 100
 120 50.1 25.4 76.0

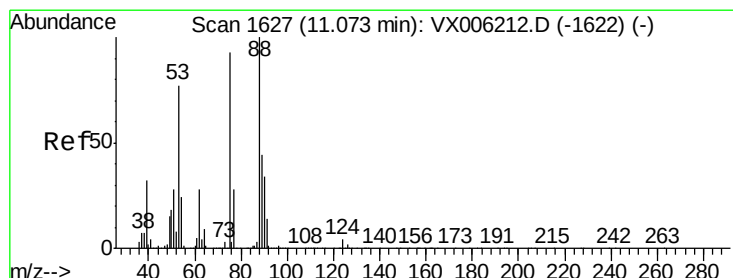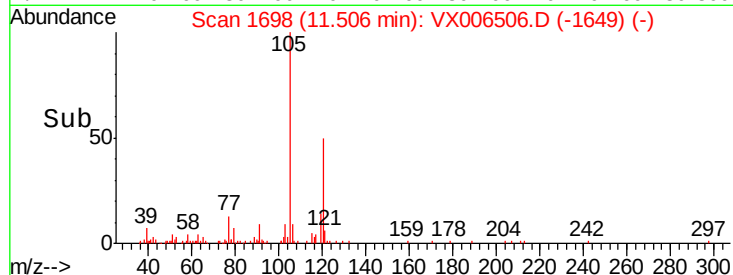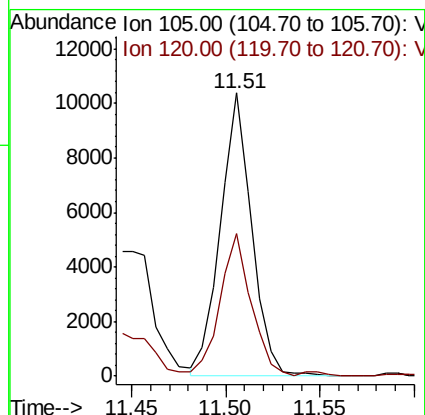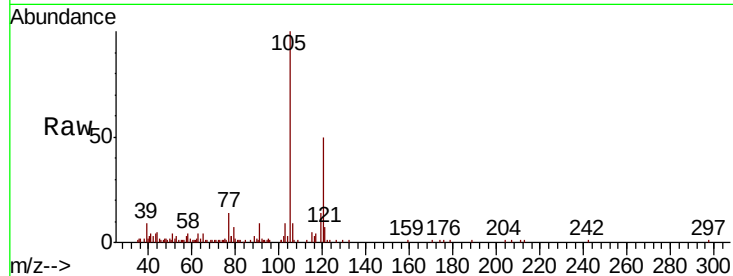

#81
 trans-1,4-Dichloro-2-butene
 Concen: 53.886 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. 0.06 min
 Lab File: VX006506.D
 Acq: 13 Dec 2018 20:10

Tgt Ion: 75 Resp: 206916
 Ion Ratio Lower Upper
 75 100
 53 0.1 64.4 96.6#
 89 0.0 44.2 66.4#

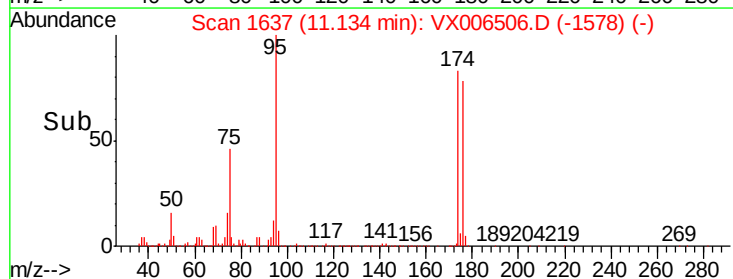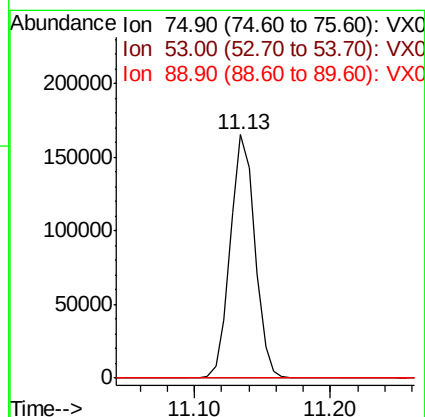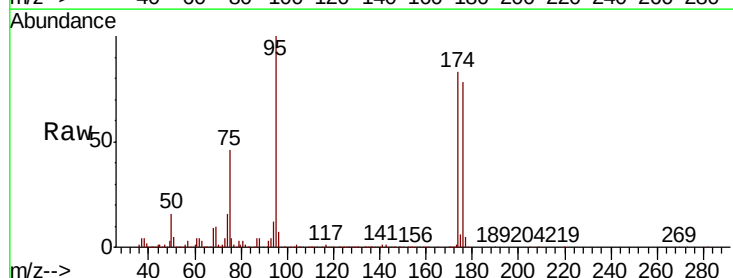



#84

1,2,4-Trimethylbenzene

Concen: 0.765 ug/l

RT: 11.80 min Scan# 1747

Delta R.T. 0.00 min

Lab File: VX006506.D

Acq: 13 Dec 2018 20:10

Instrument :

MSVOA_X

ClientSampleId :





TP-A-FRAME

Tot Ion:105 Resp: 21190

Ion Ratio Lower Upper

105 100

120 44.4 23.4 70.0

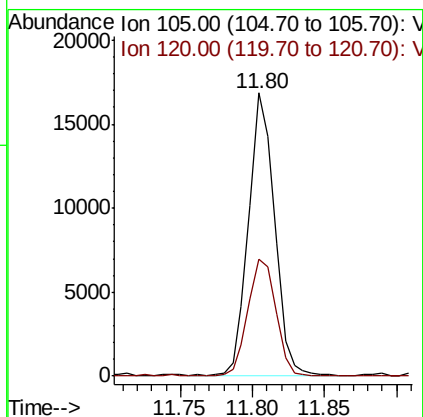

#89

n-Butylbenzene

Concen: 0.213 ug/l

RT: 12.38 min Scan# 1842

Delta R.T. -0.01 min

Lab File: VX006506.D

Acq: 13 Dec 2018 20:10




Tgt Ion: 91 Resp: 5330


Ion Ratio Lower Upper

91 100

92 45.9 26.6 79.8

134 81.4 14.8 44.3#

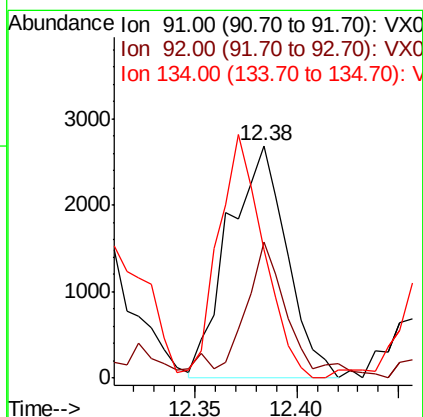




#95
Naphthalene
Concen: 9.543 ug/l
RT: 13.83 min Scan# 2080
Delta R.T. 0.00 min
Lab File: VX006506.D
Acq: 13 Dec 2018 20:10

Instrument :
MSVOA_X
ClientSampleId :
TP-A-FRAME

Tot Ion	Ratio	Lower	Upper
128	100		
127	13.3	10.2	15.4
129	11.2	8.9	13.3



Abundance

Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

