


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX121319\  
Data File : VX014005.D  
Acq On : 13 Dec 2019 12:35  
Operator : JC/SP  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X121319W.M  
Title : SW846 8260  
Last Update : Tue Dec 17 03:01:07 2019

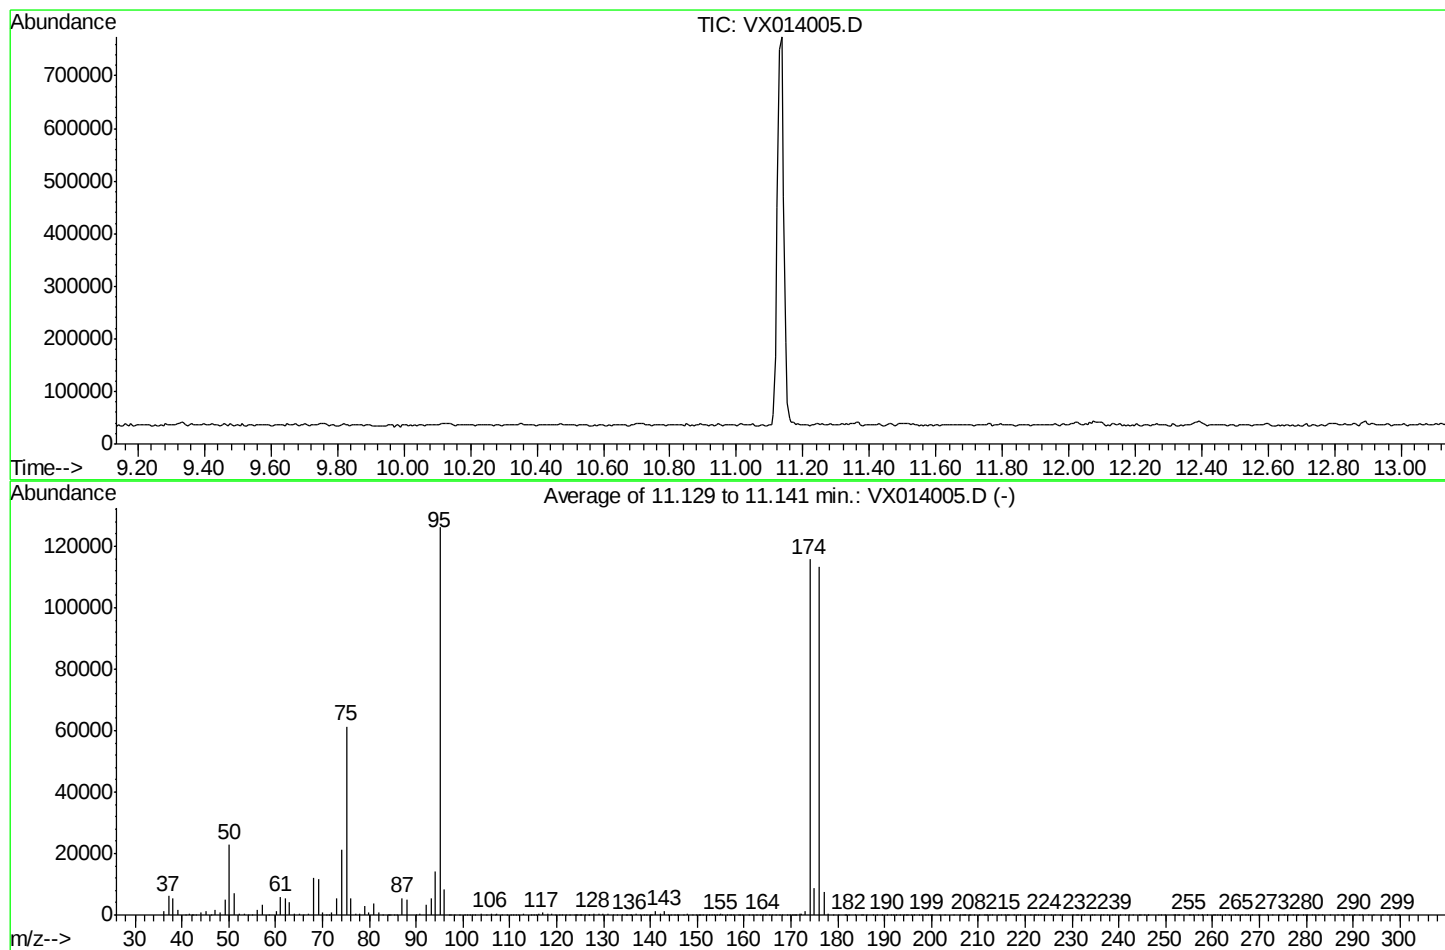

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1670

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 18.1      | 22875   | PASS             |
| 75          | 95           | 30           | 60           | 48.7      | 61429   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 126223  | PASS             |
| 96          | 95           | 5            | 9            | 6.5       | 8227    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.1       | 1287    | PASS             |
| 174         | 95           | 50           | 100          | 91.7      | 115781  | PASS             |
| 175         | 174          | 5            | 9            | 7.4       | 8574    | PASS             |
| 176         | 174          | 95           | 101          | 97.9      | 113312  | PASS             |
| 177         | 176          | 5            | 9            | 6.5       | 7381    | PASS             |