
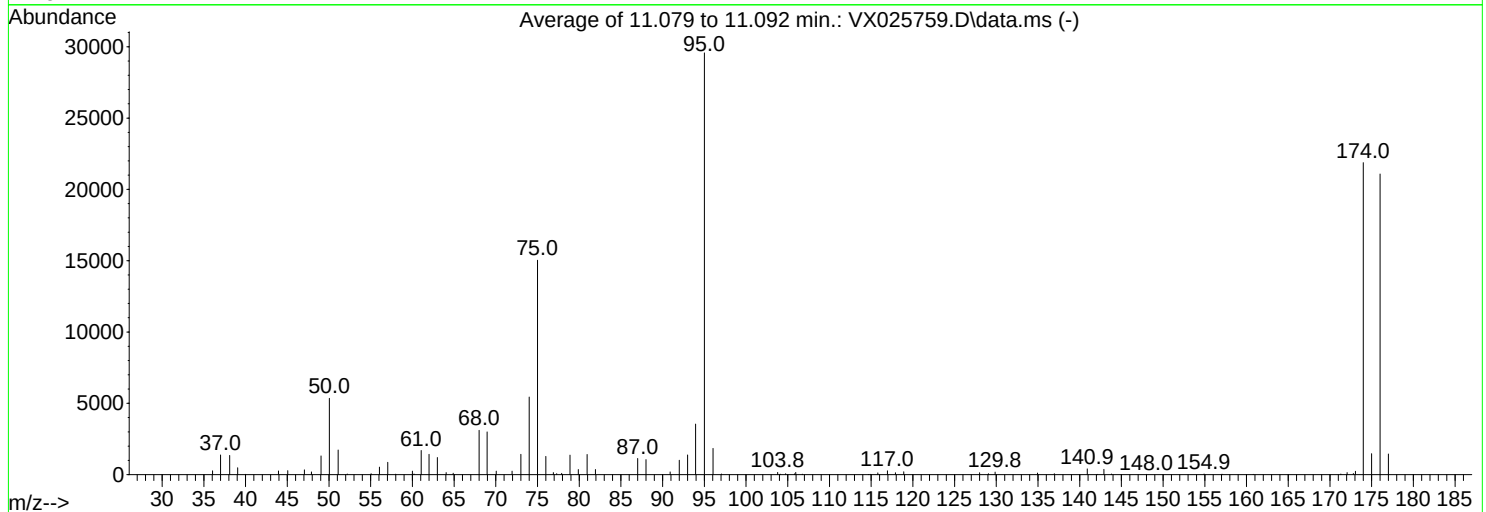


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121321\
Data File : VX025759.D
Acq On : 13 Dec 2021 18:07
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121321W.M
Title : SW846 8260
Last Update : Tue Dec 14 07:02:11 2021

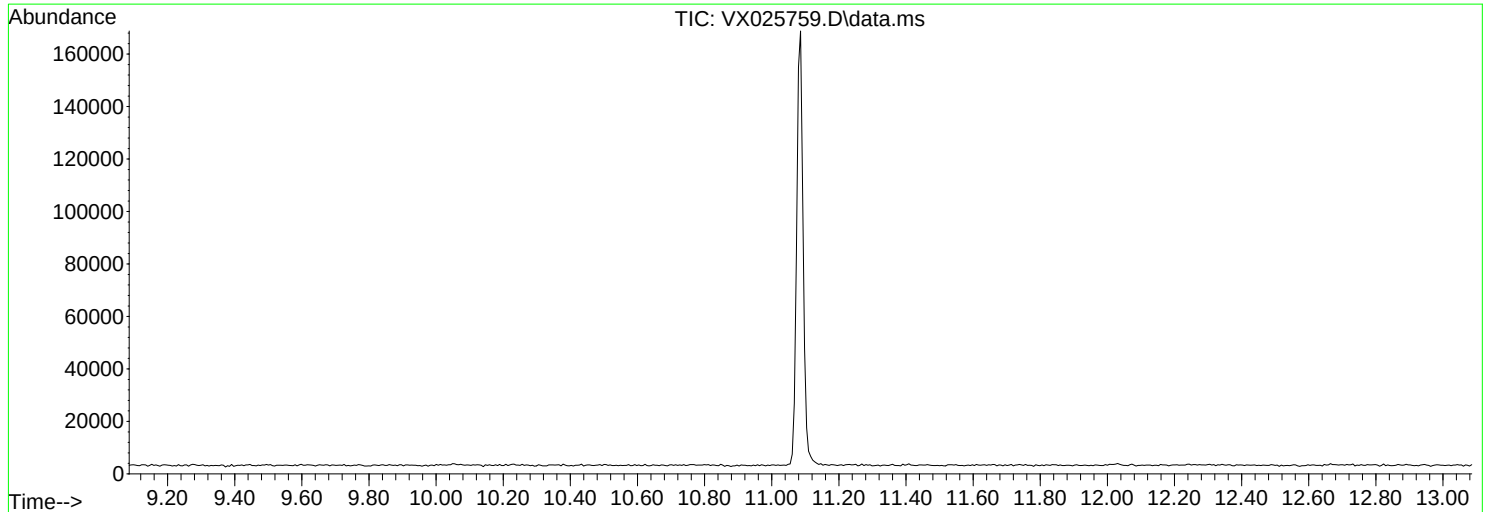

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	5353	PASS
75	95	30	60	50.8	15033	PASS
95	95	100	100	100.0	29573	PASS
96	95	5	9	6.2	1841	PASS
173	174	0.00	2	1.1	235	PASS
174	95	50	100	74.0	21880	PASS
175	174	5	9	6.7	1468	PASS
176	174	95	101	96.3	21075	PASS
177	176	5	9	6.9	1452	PASS