

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121322\
 Data File : VX033398.D
 Acq On : 13 Dec 2022 17:26
 Operator : JC/MD
 Sample : N6001-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-12

Quant Time: Dec 14 05:40:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 07 12:43:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	122976	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	196491	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	180890	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	85330	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	38024	48.197	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	96.400%		
35) Dibromofluoromethane	5.385	113	42448	48.030	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.060%		
50) Toluene-d8	8.647	98	89634	48.482	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	96.960%		
62) 4-Bromofluorobenzene	11.079	95	70847	50.117	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	100.240%		
Target Compounds					Qvalue	
3) Chloromethane	1.246	50	973	0.980	ug/l #	43
6) Chloroethane	1.752	64	620	0.721	ug/l #	42
11) Tert butyl alcohol	2.947	59	255	1.057	ug/l #	72
13) Acrolein	2.221	56	187	0.715	ug/l #	1
14) Allyl chloride	2.788	41	2374	1.333	ug/l #	62
15) Acrylonitrile	3.099	53	123	0.206	ug/l #	26
16) Acetone	2.343	43	1253	2.146	ug/l #	45
18) Methyl Acetate	2.782	43	5163	3.055	ug/l #	51
31) Cyclohexane	5.477	56	3336	1.779	ug/l	85
36) 1,1-Dichloropropene	5.550	75	9191	5.334	ug/l #	51
38) Carbon Tetrachloride	5.550	117	12448	6.448	ug/l #	14
39) Methylcyclohexane	7.385	83	1362	0.706	ug/l #	78
40) Benzene	6.037	78	64569	12.852	ug/l	99
42) 1,2-Dichloroethane	6.044	62	527	0.264	ug/l #	77
43) Isopropyl Acetate	6.251	43	3236	1.235	ug/l #	61
51) 4-Methyl-2-Pentanone	8.507	43	675	0.407	ug/l #	36
52) Toluene	8.720	92	2643	0.814	ug/l	100
55) 1,1,2-Trichloroethane	9.104	97	582	0.426	ug/l #	15
59) 2-Hexanone	9.244	43	310	0.254	ug/l	78
67) Ethyl Benzene	10.195	91	126688	19.852	ug/l	99
68) m/p-Xylenes	10.305	106	3890	1.567	ug/l	95
69) o-Xylene	10.640	106	1156	0.471	ug/l	81
73) Isopropylbenzene	10.963	105	9912	1.603	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	36495	21.022	ug/l #	37
78) n-propylbenzene	11.305	91	13544	1.961	ug/l	99
79) 2-Chlorotoluene	11.305	91	13544	3.173	ug/l #	41
81) trans-1,4-Dichloro-2-b...	11.079	75	36495	65.392	ug/l #	6
82) 4-Chlorotoluene	11.305	91	13544	2.729	ug/l #	45
90) Hexachloroethane	12.646	117	906	1.032	ug/l #	12
95) Naphthalene	13.780	128	10233	1.796	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121322\
Data File : VX033398.D
Acq On : 13 Dec 2022 17:26
Operator : JC/MD
Sample : N6001-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-12

Quant Time: Dec 14 05:40:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 07 12:43:54 2022
Response via : Initial Calibration




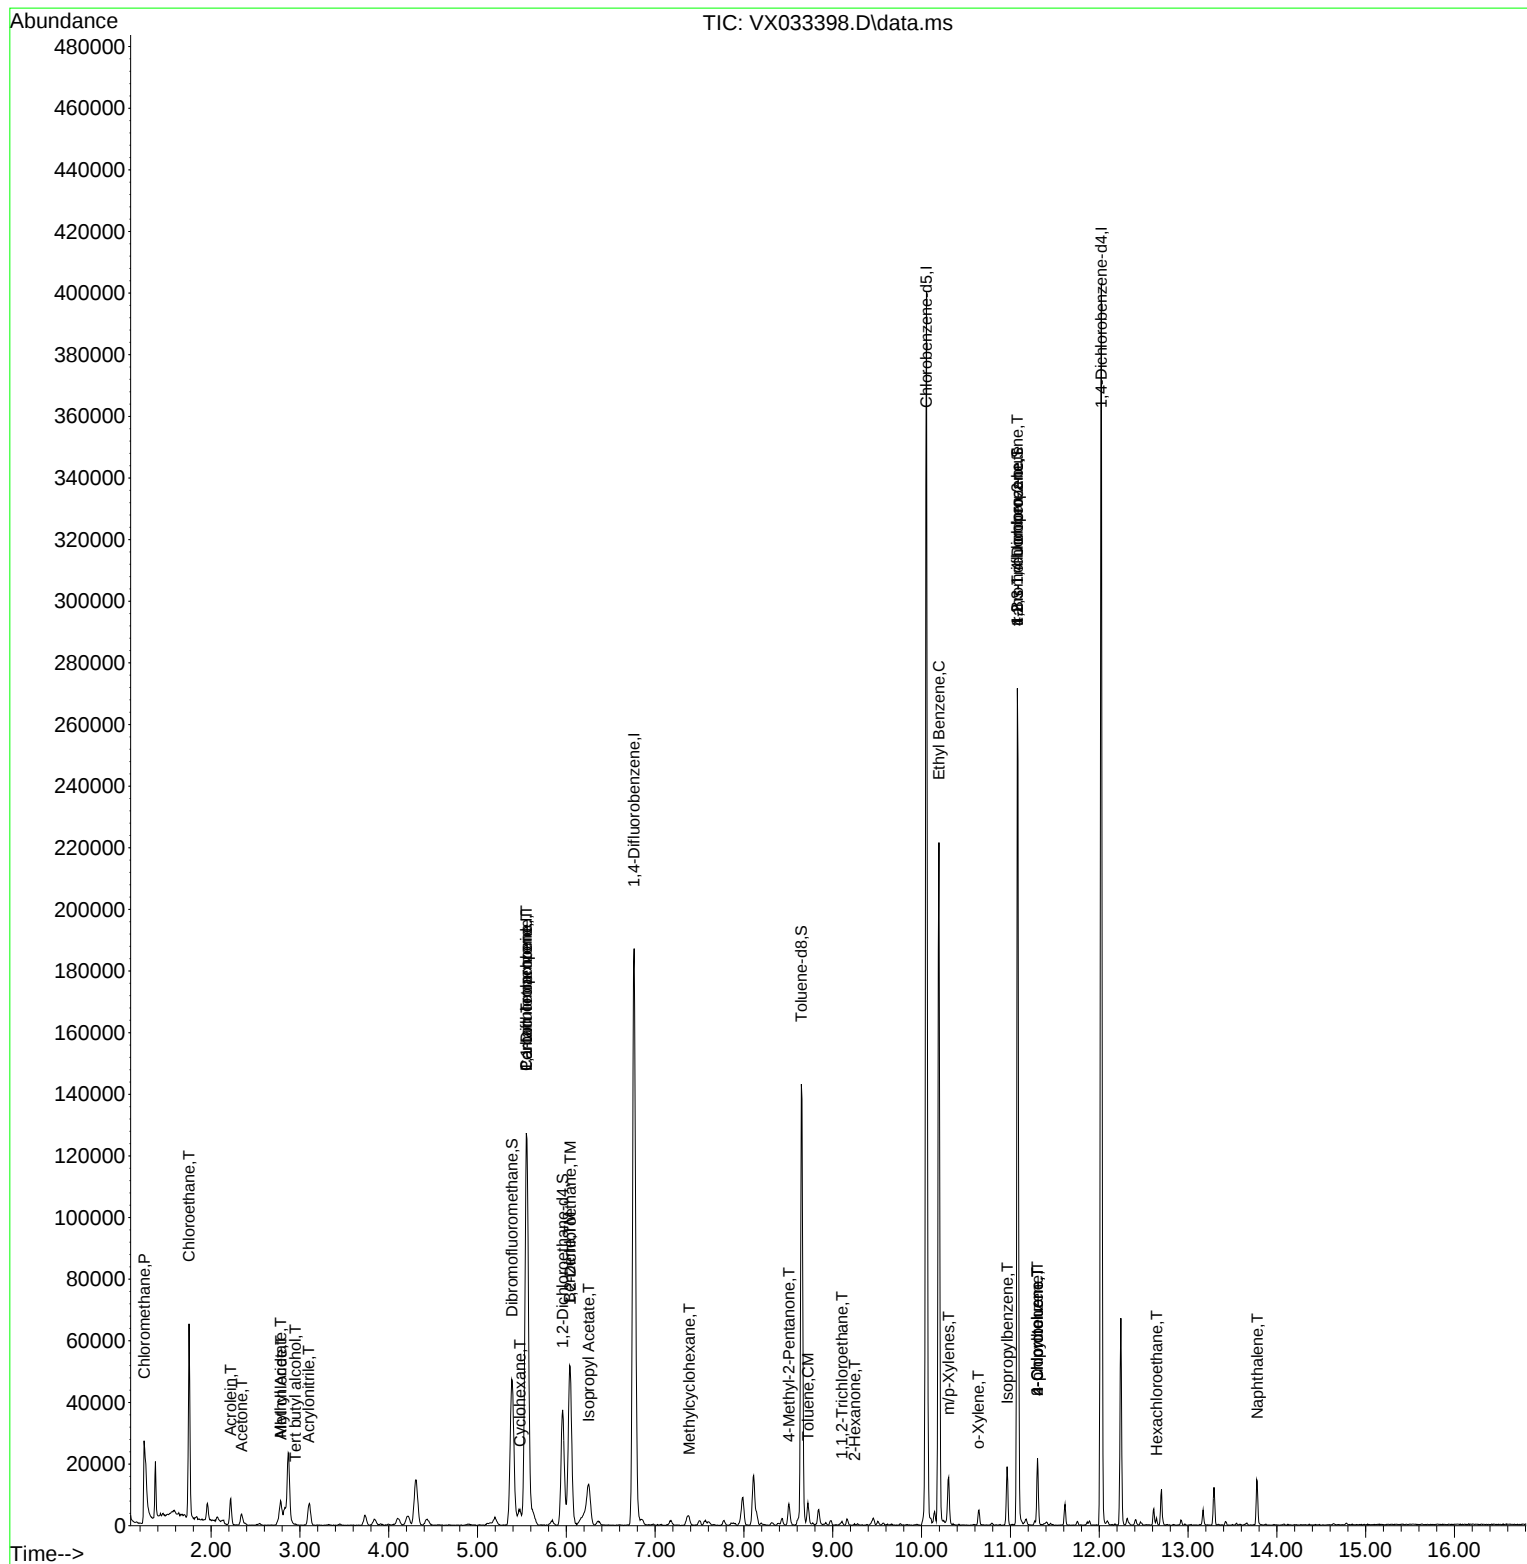




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26




Instrument :
MSVOA_X
ClientSampleId :
MW-12


Tgt Ion:168 Resp: 122976
Ion Ratio Lower Upper
168 100
99 57.8 46.1 69.1

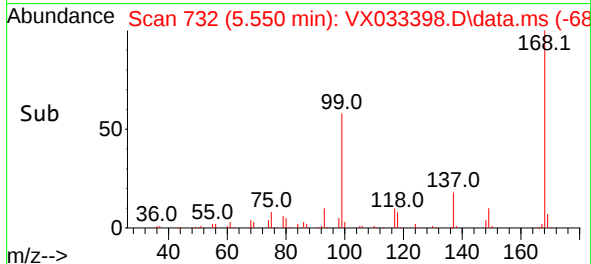

#3
Chloromethane
Concen: 0.980 ug/l
RT: 1.246 min Scan# 26
Delta R.T. -0.048 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26

Tgt Ion: 50 Resp: 973
Ion Ratio Lower Upper
50 100
52 0.0 25.4 38.2#







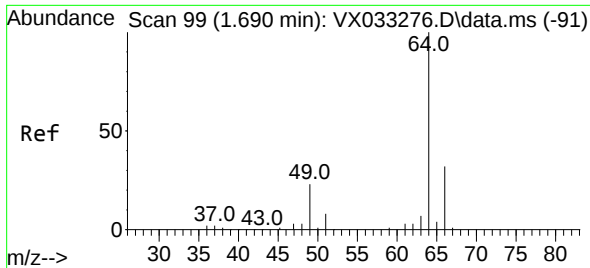

#6
Chloroethane
Concen: 0.721 ug/l
RT: 1.752 min Scan# 109
Delta R.T. 0.061 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26




Instrument :
MSVOA_X
ClientSampleId :
MW-12


Tgt Ion: 64 Resp: 620
Ion Ratio Lower Upper
64 100
66 0.0 26.0 39.0#

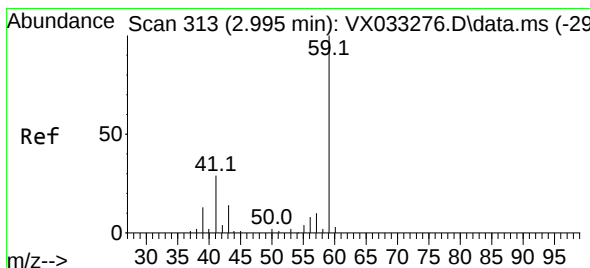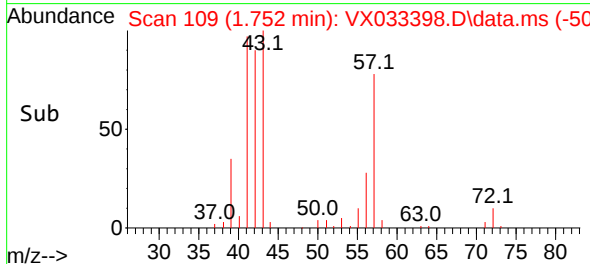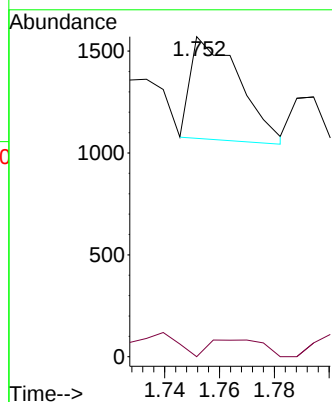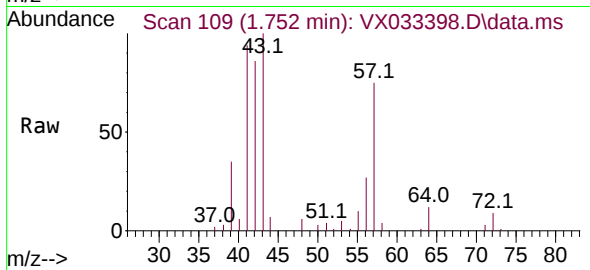

#11
Tert butyl alcohol
Concen: 1.057 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.048 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26

Tgt Ion: 59 Resp: 255
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

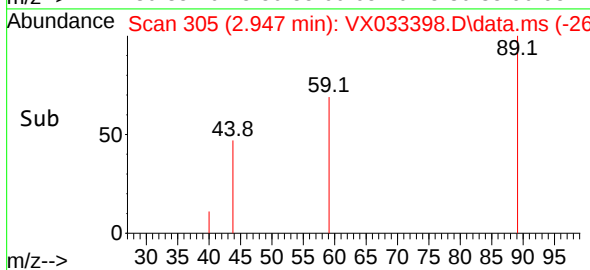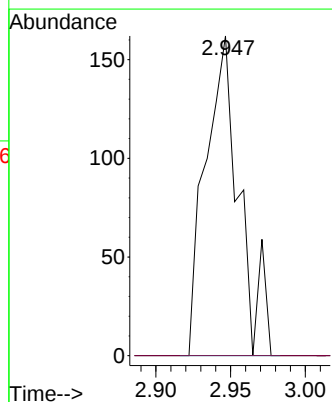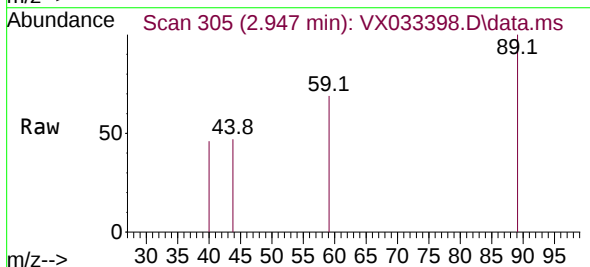

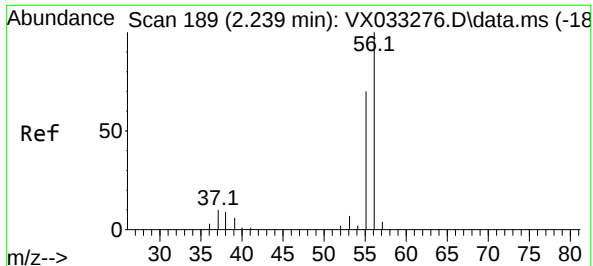

#13

Acrolein

Concen: 0.715 ug/l

RT: 2.221 min Scan# 187

Delta R.T. -0.018 min

Lab File: VX033398.D

Acq: 13 Dec 2022 17:26

Instrument :

MSVOA_X

ClientSampleId :





MW-12

Tgt Ion: 56 Resp: 187

Ion Ratio Lower Upper

56 100

55 2403.2 56.9 85.3#

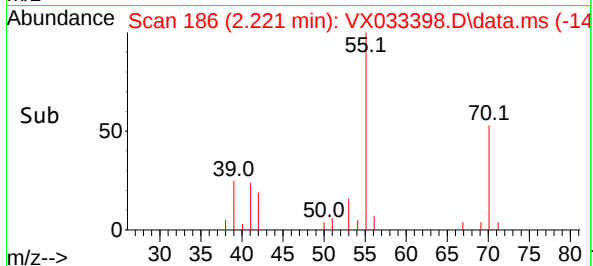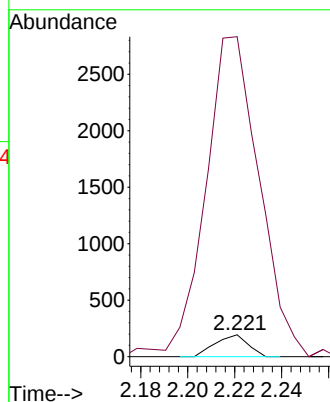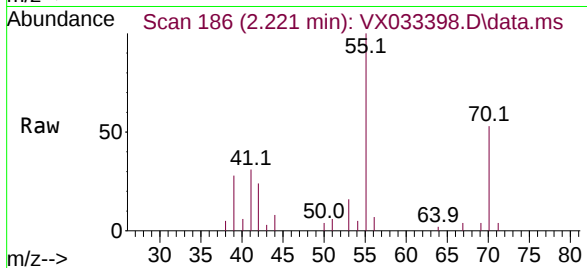

#14

Allyl chloride

Concen: 1.333 ug/l

RT: 2.788 min Scan# 279

Delta R.T. 0.122 min

Lab File: VX033398.D

Acq: 13 Dec 2022 17:26




Tgt Ion: 41 Resp: 2374


Ion Ratio Lower Upper

41 100

39 53.1 61.4 92.2#

76 0.0 29.2 43.8#

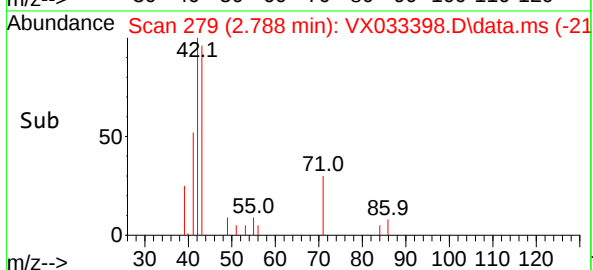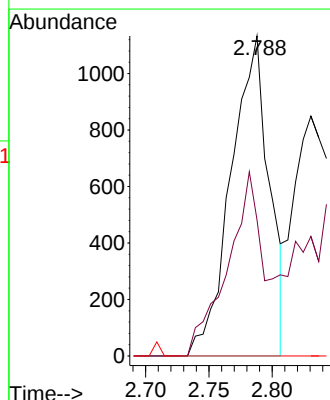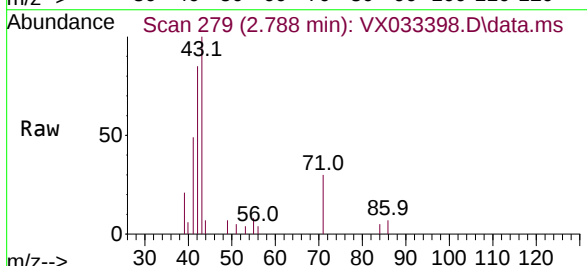

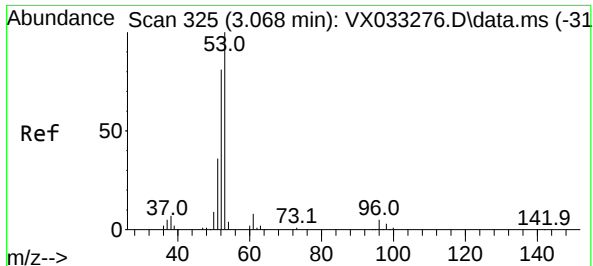

#15

Acrylonitrile

Concen: 0.206 ug/l

RT: 3.099 min Scan# 31

Delta R.T. 0.031 min

Lab File: VX033398.D

Acq: 13 Dec 2022 17:26

Instrument :

MSVOA_X

ClientSampleId :

MW-12





Tgt Ion: 53 Resp: 123

Ion Ratio Lower Upper

53 100

52 0.0 67.4 101.0#

51 17.9 30.3 45.5#

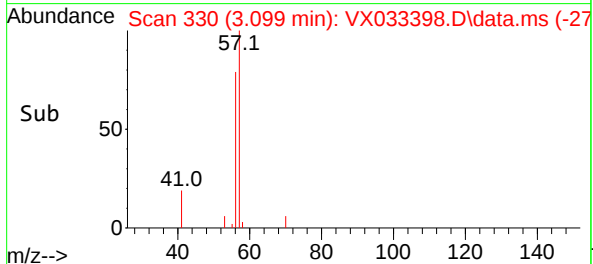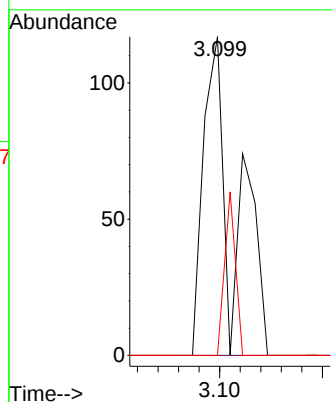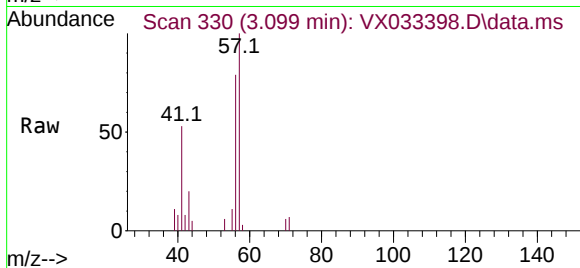

#16

Acetone

Concen: 2.146 ug/l

RT: 2.343 min Scan# 206

Delta R.T. -0.048 min

Lab File: VX033398.D




Acq: 13 Dec 2022 17:26


Tgt Ion: 43 Resp: 1253

Ion Ratio Lower Upper

43 100

58 0.0 23.8 35.8#

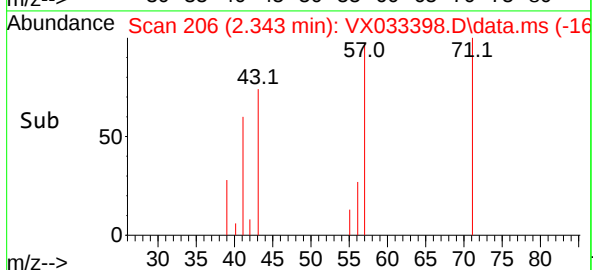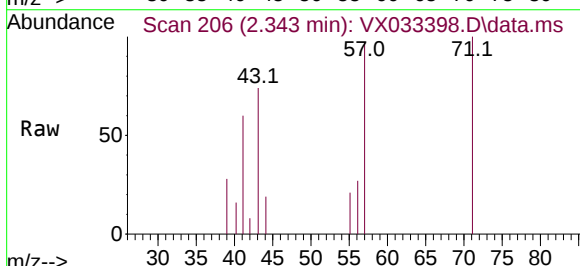



#18

Methyl Acetate

Concen: 3.055 ug/l

RT: 2.782 min Scan# 21

Delta R.T. 0.073 min

Lab File: VX033398.D

Acq: 13 Dec 2022 17:26

Instrument :

MSVOA_X

ClientSampleId :





MW-12

Tgt Ion: 43 Resp: 5163

Ion Ratio Lower Upper

43 100

74 0.0 19.4 29.0#

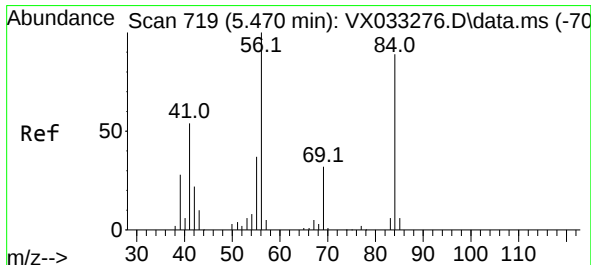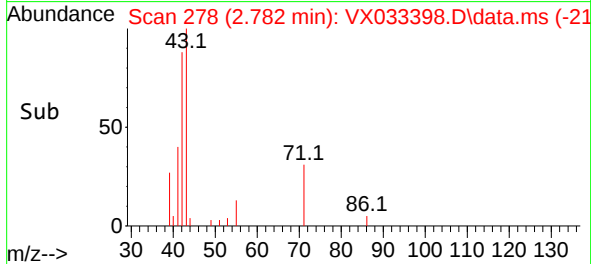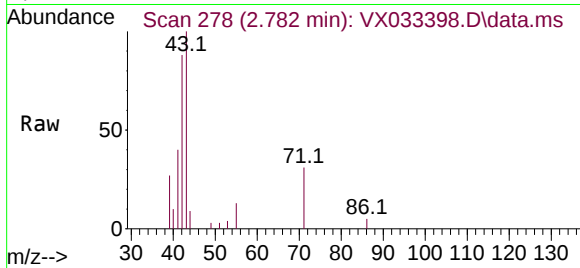

#31

Cyclohexane

Concen: 1.779 ug/l

RT: 5.477 min Scan# 720

Delta R.T. 0.006 min

Lab File: VX033398.D

Acq: 13 Dec 2022 17:26




Tgt Ion: 56 Resp: 3336


Ion Ratio Lower Upper

56 100

69 34.5 24.1 36.1

84 99.2 66.9 100.3

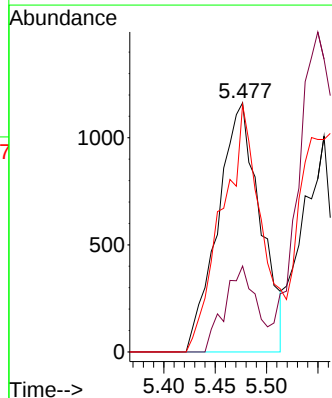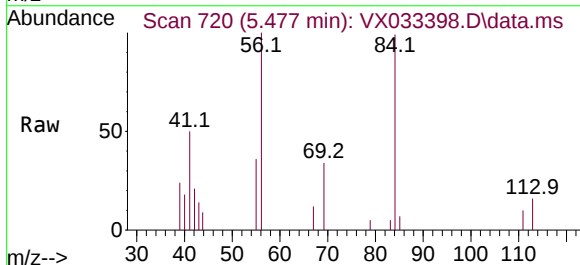

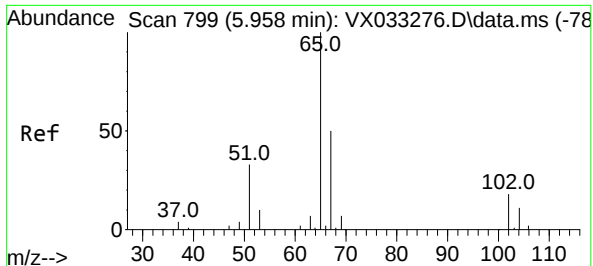

#33

1,2-Dichloroethane-d4

Concen: 48.197 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX033398.D

Acq: 13 Dec 2022 17:26

Instrument :

MSVOA_X

ClientSampleId :





MW-12

Tgt Ion: 65 Resp: 38024

Ion Ratio Lower Upper

65 100

67 51.3 0.0 101.8

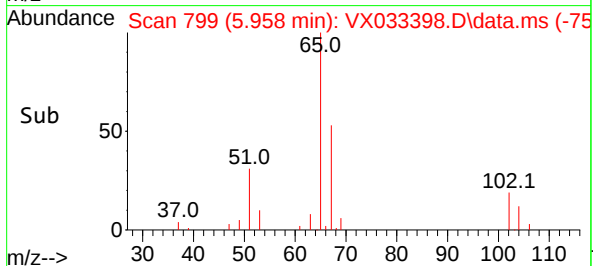

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX033398.D

Acq: 13 Dec 2022 17:26




Tgt Ion: 114 Resp: 196491


Ion Ratio Lower Upper

114 100

63 18.5 0.0 41.6

88 15.0 0.0 33.4

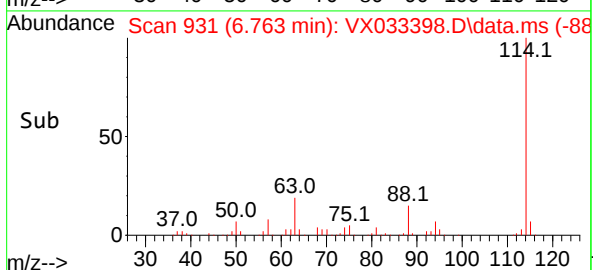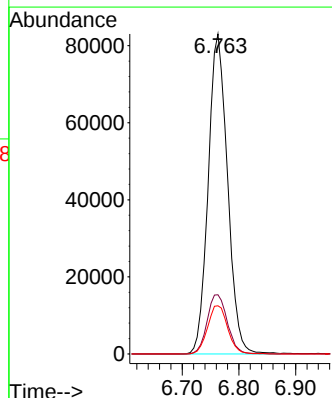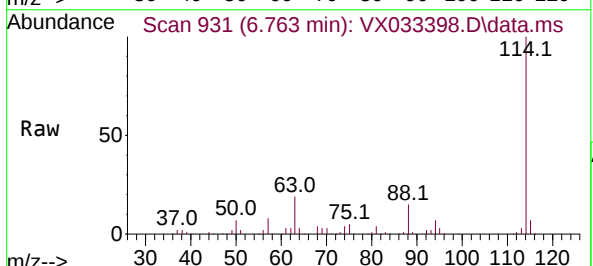

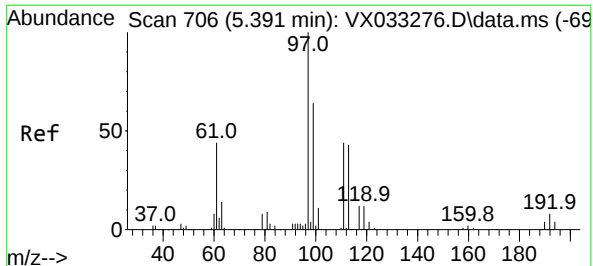

#35

Dibromofluoromethane

Concen: 48.030 ug/l

RT: 5.385 min Scan# 706

Delta R.T. -0.006 min

Lab File: VX033398.D

Acq: 13 Dec 2022 17:26

Instrument :

MSVOA_X

ClientSampleId :

MW-12





Tgt Ion:113 Resp: 42448

Ion Ratio Lower Upper

113 100

111 102.5 82.4 123.6

192 19.7 15.4 23.2

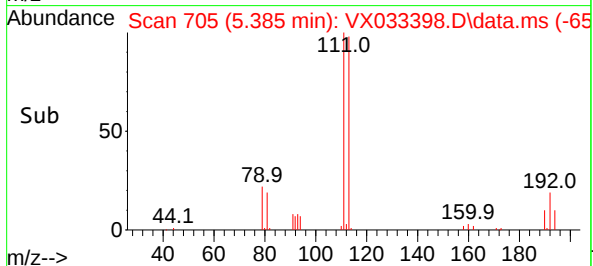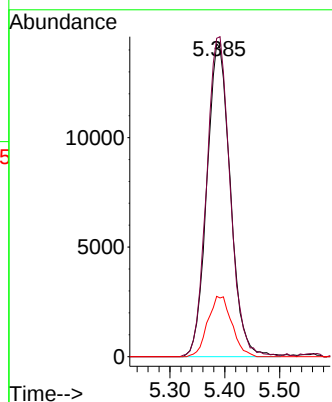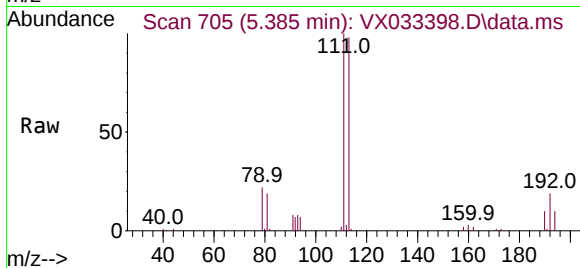

#36

1,1-Dichloropropene

Concen: 5.334 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.146 min

Lab File: VX033398.D

Acq: 13 Dec 2022 17:26




Tgt Ion: 75 Resp: 9191


Ion Ratio Lower Upper

75 100

110 11.3 18.4 55.2#

77 0.0 24.5 36.7#


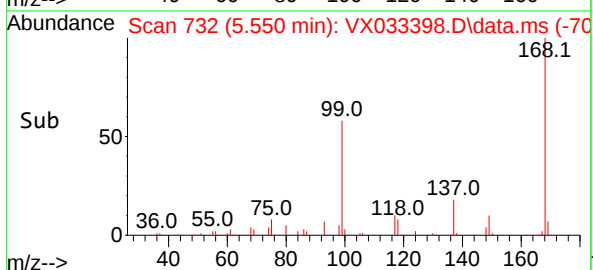

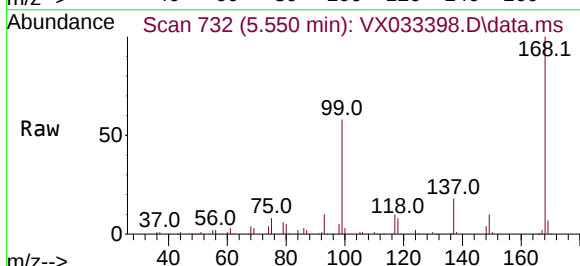


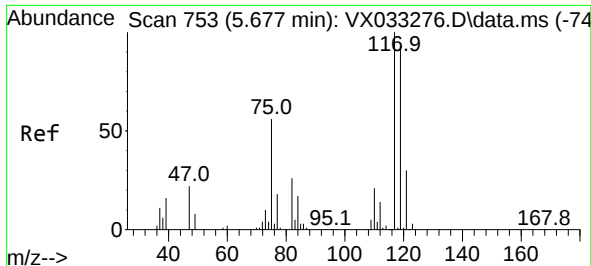

#38
Carbon Tetrachloride
Concen: 6.448 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26




Instrument :
MSVOA_X
ClientSampleId :
MW-12


Tgt Ion:117 Resp: 12448
Ion Ratio Lower Upper
117 100
119 3.2 77.2 115.8#
121 0.0 25.8 38.6#

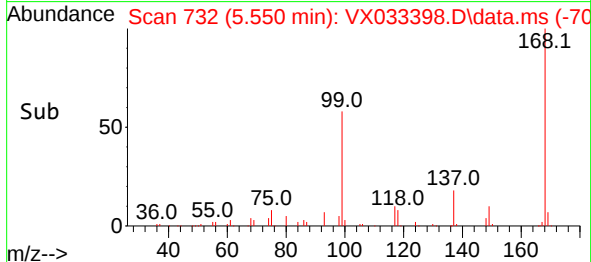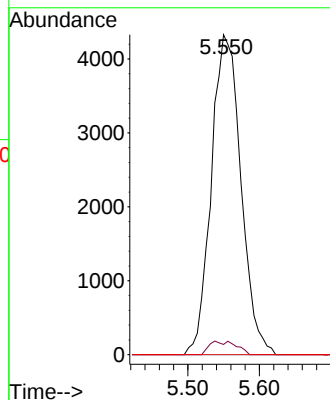

#39
Methylcyclohexane
Concen: 0.706 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. 0.000 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26

Tgt Ion: 83 Resp: 1362
Ion Ratio Lower Upper
83 100
55 59.6 58.4 87.6
98 26.4 37.2 55.8#



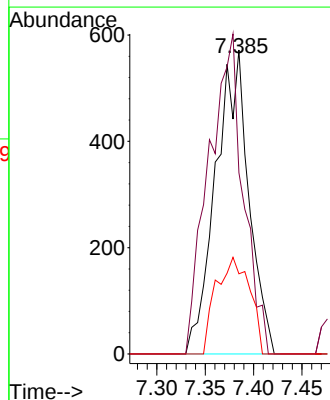
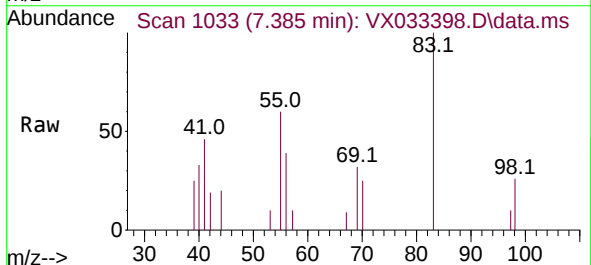


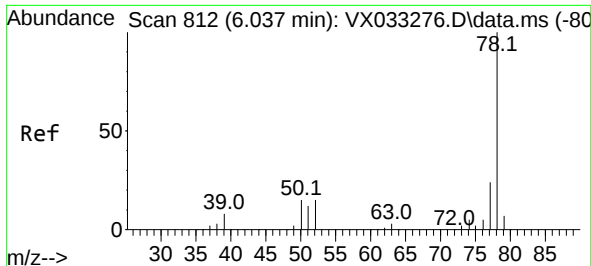

#40
Benzene
Concen: 12.852 ug/l
RT: 6.037 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26




Instrument :
MSVOA_X
ClientSampleId :
MW-12


Tgt Ion: 78 Resp: 64569
Ion Ratio Lower Upper
78 100
77 23.4 19.0 28.4

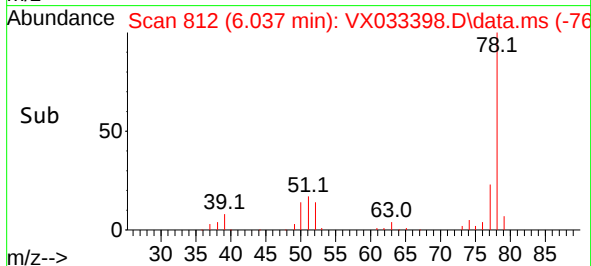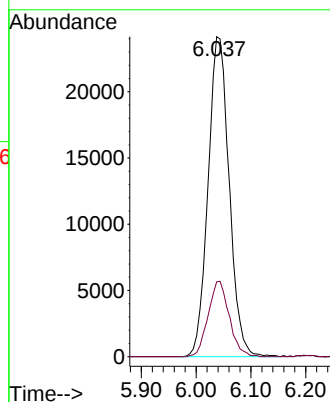

#42
1,2-Dichloroethane
Concen: 0.264 ug/l
RT: 6.044 min Scan# 813
Delta R.T. -0.048 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26

Tgt Ion: 62 Resp: 527
Ion Ratio Lower Upper
62 100
98 0.0 0.0 16.0


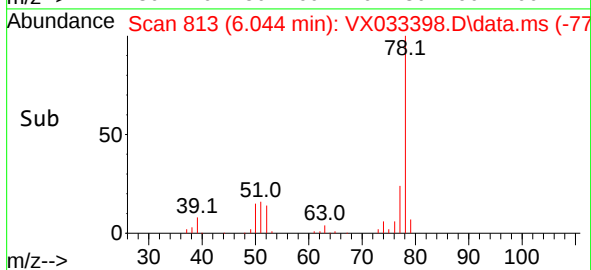
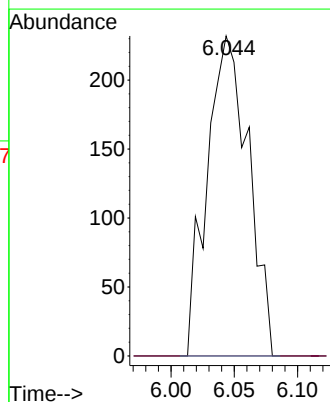



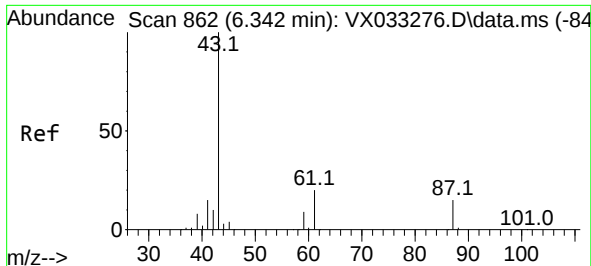

#43
Isopropyl Acetate
Concen: 1.235 ug/l
RT: 6.251 min Scan# 84
Delta R.T. -0.091 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26




Instrument :
MSVOA_X
ClientSampleId :
MW-12


Tgt Ion: 43 Resp: 3236
Ion Ratio Lower Upper
43 100
61 0.0 15.4 23.0#
87 0.0 10.8 16.2#

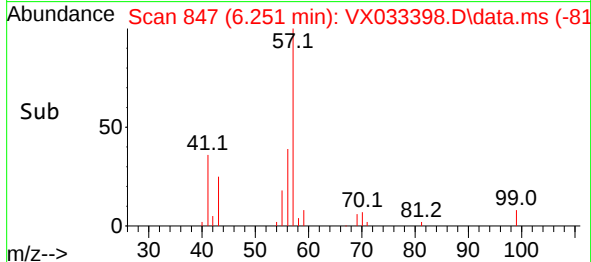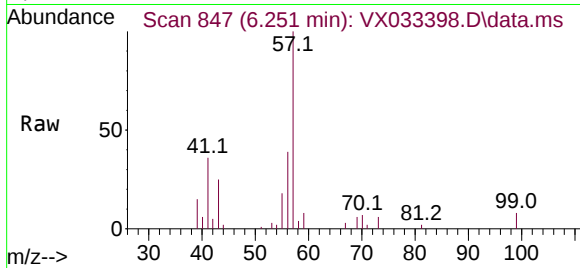

#50
Toluene-d8
Concen: 48.482 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.006 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26

Tgt Ion: 98 Resp: 89634
Ion Ratio Lower Upper
98 100
100 63.3 50.9 76.3




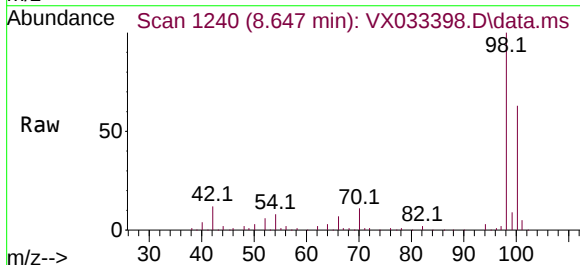




#51
4-Methyl-2-Pentanone
Concen: 0.407 ug/l
RT: 8.507 min Scan# 11
Delta R.T. -0.067 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26




Instrument :
MSVOA_X
ClientSampleId :
MW-12


Tgt Ion: 43 Resp: 675
Ion Ratio Lower Upper
43 100
58 0.0 30.9 46.3#

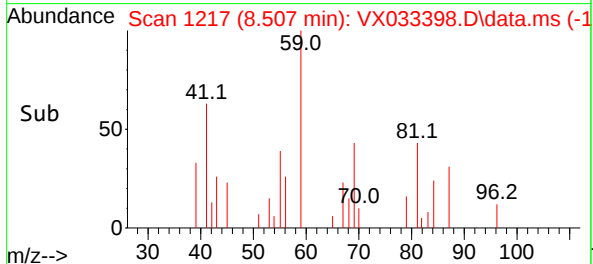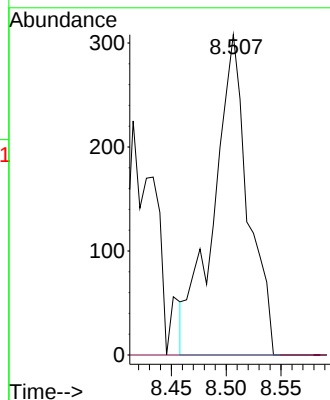

#52
Toluene
Concen: 0.814 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.000 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26

Tgt Ion: 92 Resp: 2643
Ion Ratio Lower Upper
92 100
91 173.4 138.3 207.5

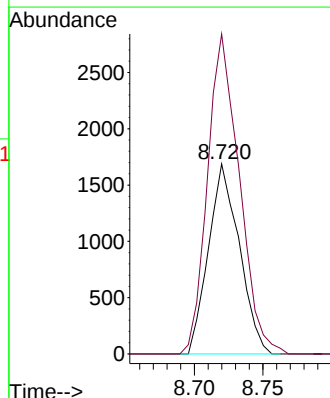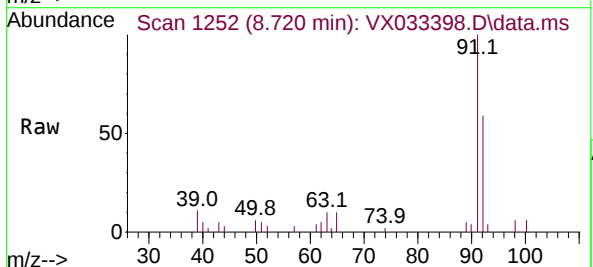




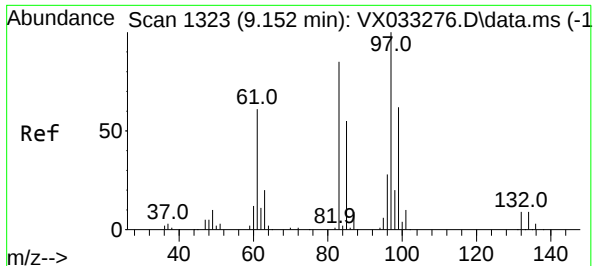


#55
 1,1,2-Trichloroethane
 Concen: 0.426 ug/l
 RT: 9.104 min Scan# 11
 Delta R.T. -0.048 min
 Lab File: VX033398.D
 Acq: 13 Dec 2022 17:26

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-12

Tgt Ion: 97 Resp: 582




Ion	Ratio	Lower	Upper
97	100		
83	0.0	68.1	102.1#
85	0.0	43.3	64.9#
99	0.0	50.4	75.6#

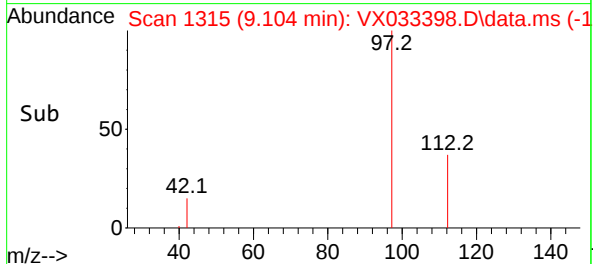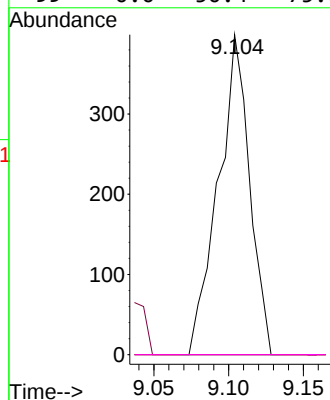


#59
 2-Hexanone
 Concen: 0.254 ug/l
 RT: 9.244 min Scan# 1338
 Delta R.T. -0.189 min
 Lab File: VX033398.D
 Acq: 13 Dec 2022 17:26

Tgt Ion: 43 Resp: 310

Ion	Ratio	Lower	Upper
43	100		
58	37.7	26.5	79.5


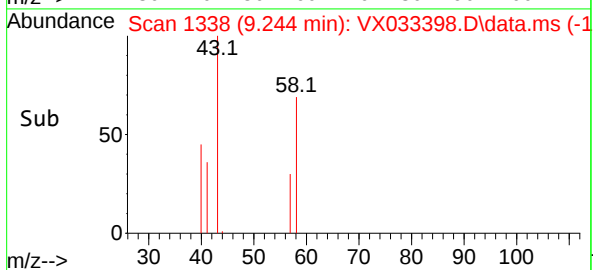
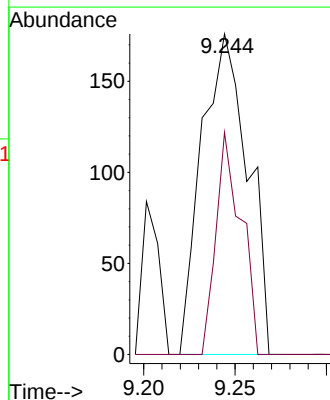
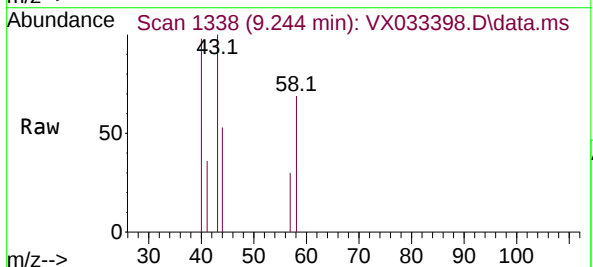


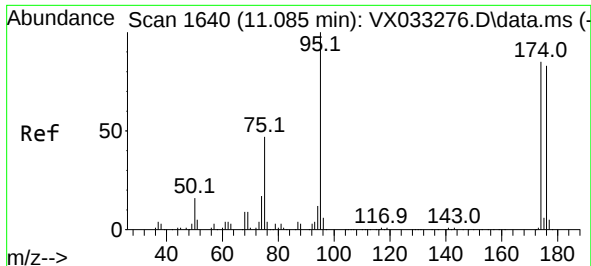

#62
4-Bromofluorobenzene
Concen: 50.117 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26




Instrument :
MSVOA_X
ClientSampleId :
MW-12


Tgt Ion: 95 Resp: 70847
Ion Ratio Lower Upper
95 100
174 82.1 0.0 164.0
176 78.9 0.0 154.4

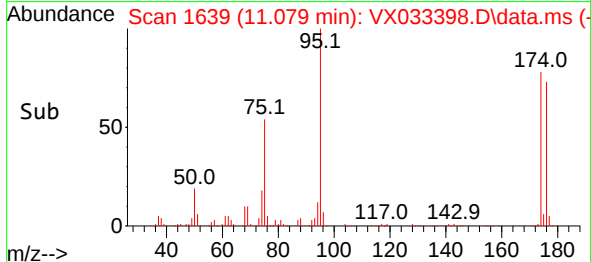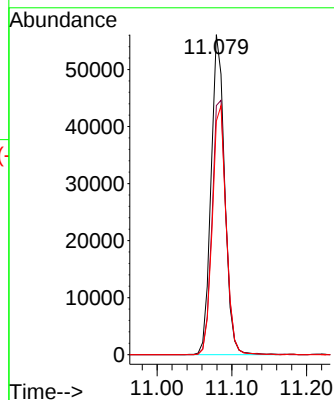

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26

Tgt Ion: 117 Resp: 180890
Ion Ratio Lower Upper
117 100
82 55.8 44.3 66.5
119 32.7 25.7 38.5


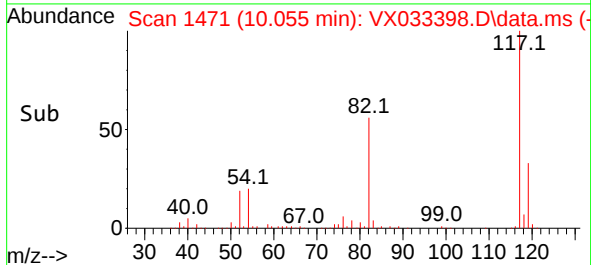
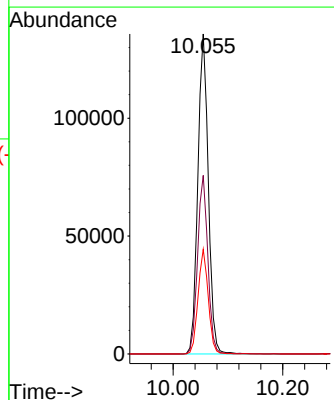





#67
Ethyl Benzene
Concen: 19.852 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26




Instrument :
MSVOA_X
ClientSampleId :
MW-12


Tgt Ion: 91 Resp: 126688
Ion Ratio Lower Upper
91 100
106 31.6 25.0 37.6

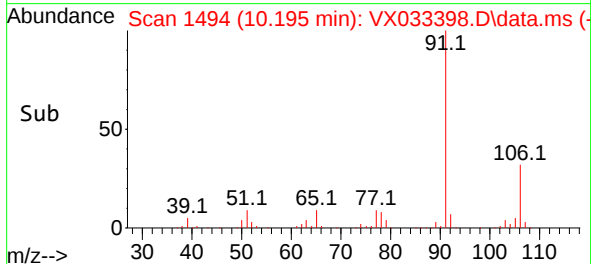

#68
m/p-Xylenes
Concen: 1.567 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26

Tgt Ion: 106 Resp: 3890
Ion Ratio Lower Upper
106 100
91 213.4 164.5 246.7


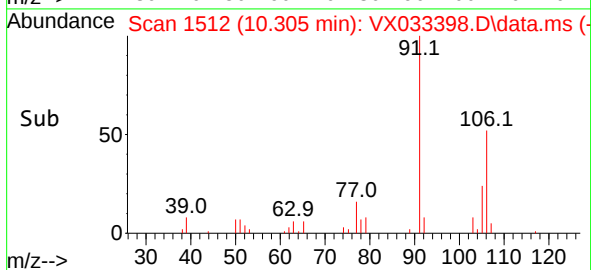






#69
o-Xylene
Concen: 0.471 ug/l
RT: 10.640 min Scan# 1156
Delta R.T. 0.000 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26




Instrument :
MSVOA_X
ClientSampleId :
MW-12


Tgt Ion:106 Resp: 1156
Ion Ratio Lower Upper
106 100
91 248.1 109.2 327.6

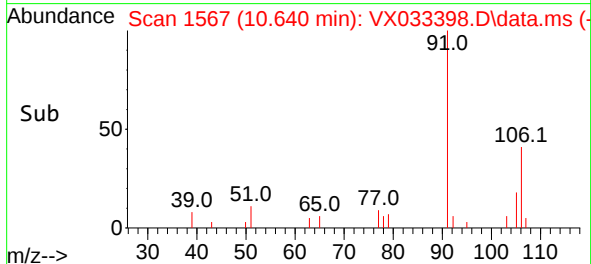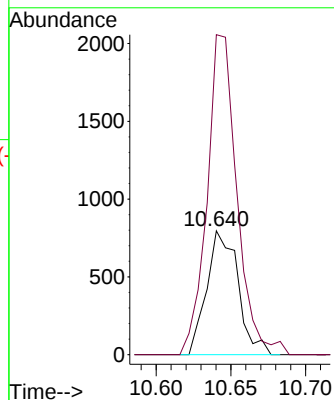

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26

Tgt Ion:152 Resp: 85330
Ion Ratio Lower Upper
152 100
115 59.7 44.0 132.0
150 158.0 0.0 351.8

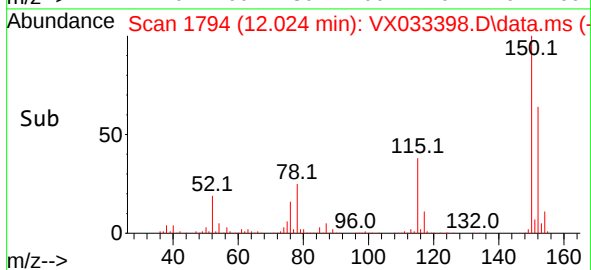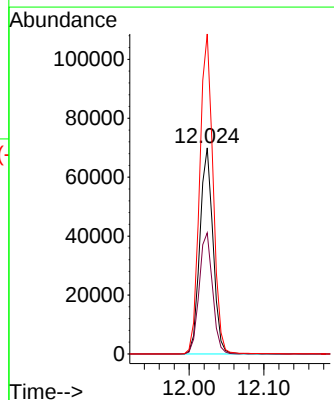



#73

Isopropylbenzene

Concen: 1.603 ug/l

RT: 10.963 min Scan# 1620

Delta R.T. 0.000 min

Lab File: VX033398.D

Acq: 13 Dec 2022 17:26

Instrument :

MSVOA_X

ClientSampleId :





MW-12

Tgt Ion:105 Resp: 9912

Ion Ratio Lower Upper

105 100

120 26.7 13.1 39.3

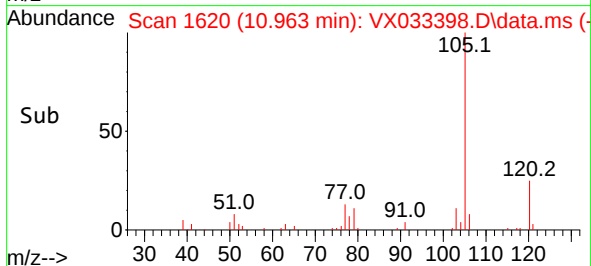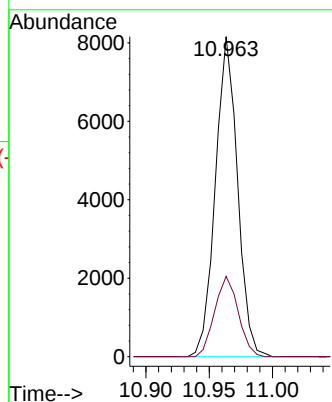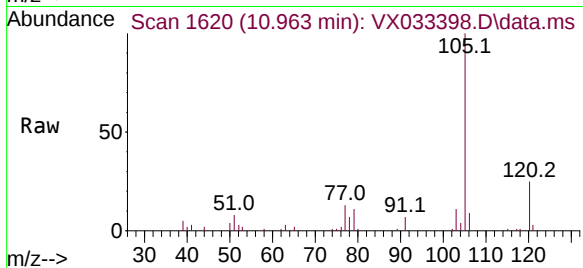

#76

1,2,3-Trichloropropane

Concen: 21.022 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.164 min

Lab File: VX033398.D




Acq: 13 Dec 2022 17:26


Tgt Ion: 75 Resp: 36495

Ion Ratio Lower Upper

75 100

77 1.0 20.0 60.0#

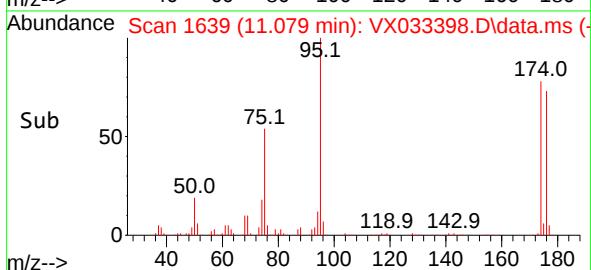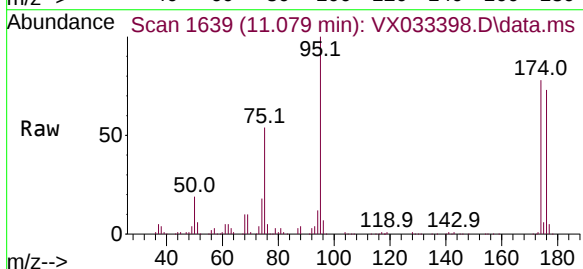



#78

n-propylbenzene

Concen: 1.961 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX033398.D

Acq: 13 Dec 2022 17:26

Instrument :

MSVOA_X

ClientSampleId :





MW-12

Tgt Ion: 91 Resp: 13544

Ion Ratio Lower Upper

91 100

120 23.5 11.6 34.8

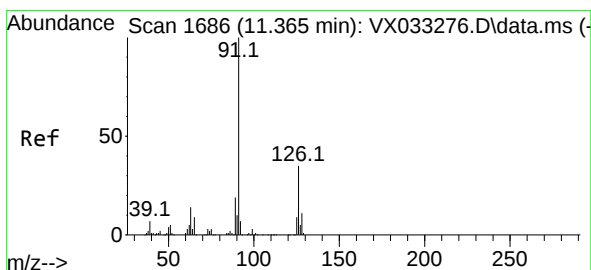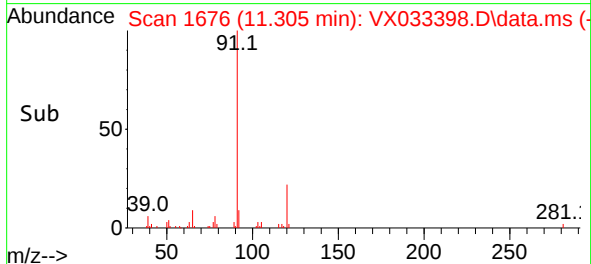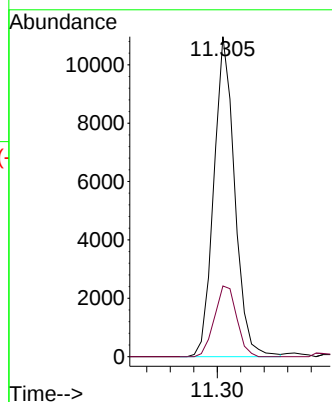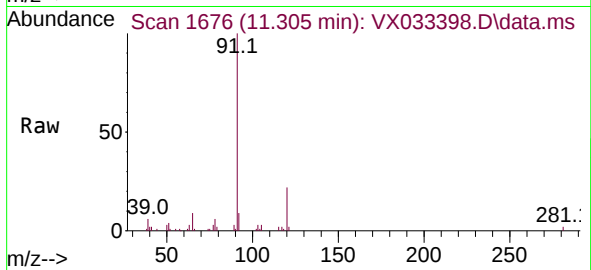

#79

2-Chlorotoluene

Concen: 3.173 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.061 min

Lab File: VX033398.D




Acq: 13 Dec 2022 17:26


Tgt Ion: 91 Resp: 13544

Ion Ratio Lower Upper

91 100

126 0.0 17.1 51.2#


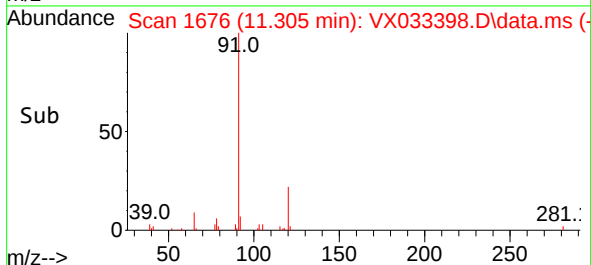




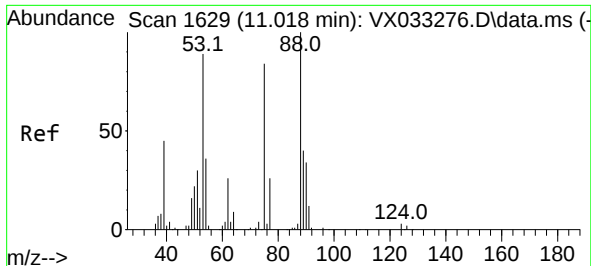

#81
trans-1,4-Dichloro-2-butene
Concen: 65.392 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26




Instrument :
MSVOA_X
ClientSampleId :
MW-12


Tgt Ion: 75 Resp: 36495
Ion Ratio Lower Upper
75 100
53 0.0 86.9 130.3#
89 0.0 38.3 57.5#

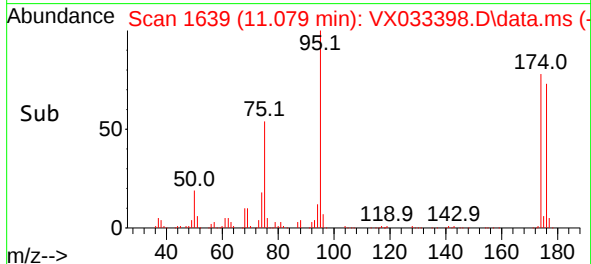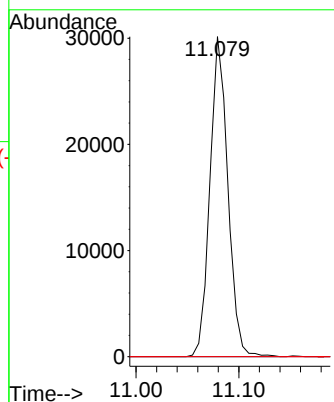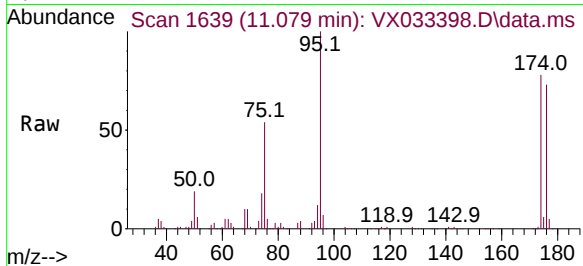

#82
4-Chlorotoluene
Concen: 2.729 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.152 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26

Tgt Ion: 91 Resp: 13544
Ion Ratio Lower Upper
91 100
126 0.0 14.8 44.4#



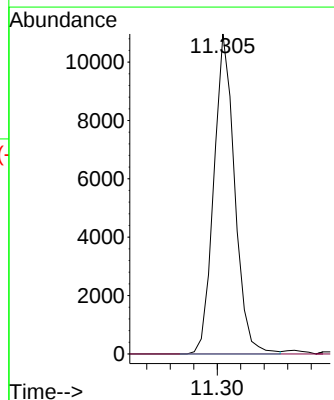
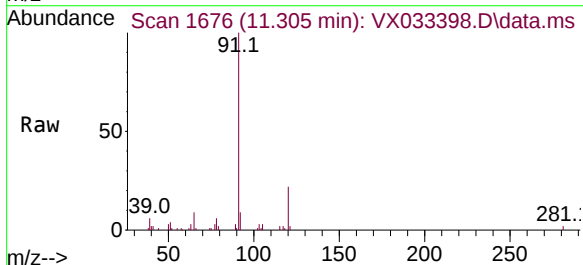


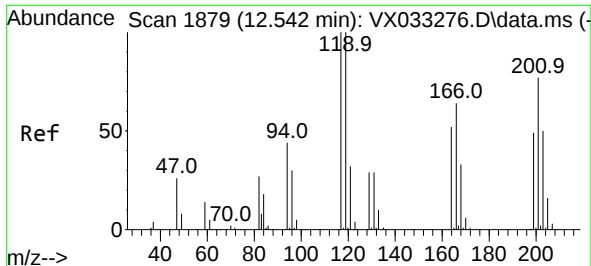

#90
Hexachloroethane
Concen: 1.032 ug/l
RT: 12.646 min Scan# 1879
Delta R.T. 0.104 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26

Instrument :
MSVOA_X
ClientSampleId :
MW-12

Tgt Ion:117 Resp: 906
Ion Ratio Lower Upper
117 100
201 0.0 37.6 112.9#

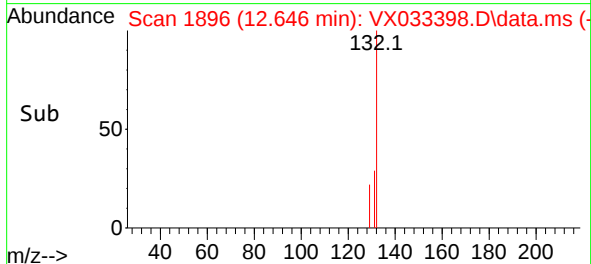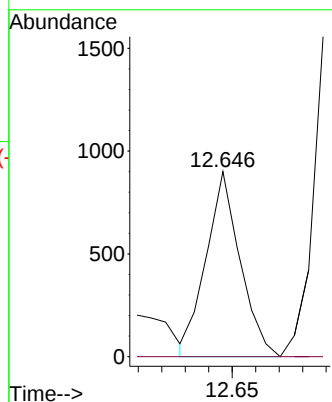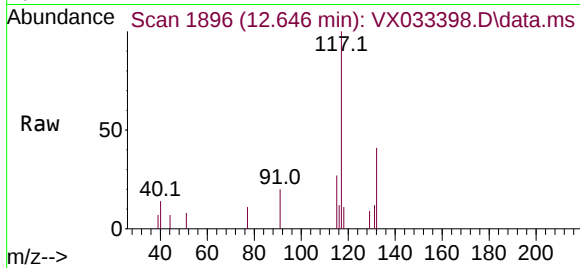

#95
Naphthalene
Concen: 1.796 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX033398.D
Acq: 13 Dec 2022 17:26

Tgt Ion:128 Resp: 10233
Ion Ratio Lower Upper
128 100
127 12.3 10.2 15.4
129 10.8 8.9 13.3

