

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121322\
 Data File : VX033394.D
 Acq On : 13 Dec 2022 15:54
 Operator : JC/MD
 Sample : N5865-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB-01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M

Title : SW846 8260

Signal : TIC: VX033394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	48	rBV	147874	232689	39.46%	7.208%
2	2.392	207	214	223	rBV2	3066	5970	1.01%	0.185%
3	2.794	273	280	290	rVB2	5903	11935	2.02%	0.370%
4	5.385	691	705	720	rBV	56130	162271	27.52%	5.027%
5	5.556	721	733	749	rVB	141086	404242	68.55%	12.522%
6	5.958	790	799	816	rBV2	41710	113647	19.27%	3.520%
7	6.763	921	931	945	rBV	215335	506310	85.85%	15.684%
8	8.647	1234	1240	1248	rBV	159134	255670	43.35%	7.920%
9	10.055	1465	1471	1487	rBV	442260	589734	100.00%	18.268%
10	10.195	1490	1494	1499	rVB	4994	6497	1.10%	0.201%
11	10.305	1507	1512	1518	rBV	11321	16793	2.85%	0.520%
12	11.079	1634	1639	1650	rBV	295688	378093	64.11%	11.712%
13	12.024	1788	1794	1802	rBV	430800	544441	92.32%	16.865%




Sum of corrected areas: 3228292

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121322\
Data File : VX033394.D
Acq On : 13 Dec 2022 15:54
Operator : JC/MD
Sample : N5865-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

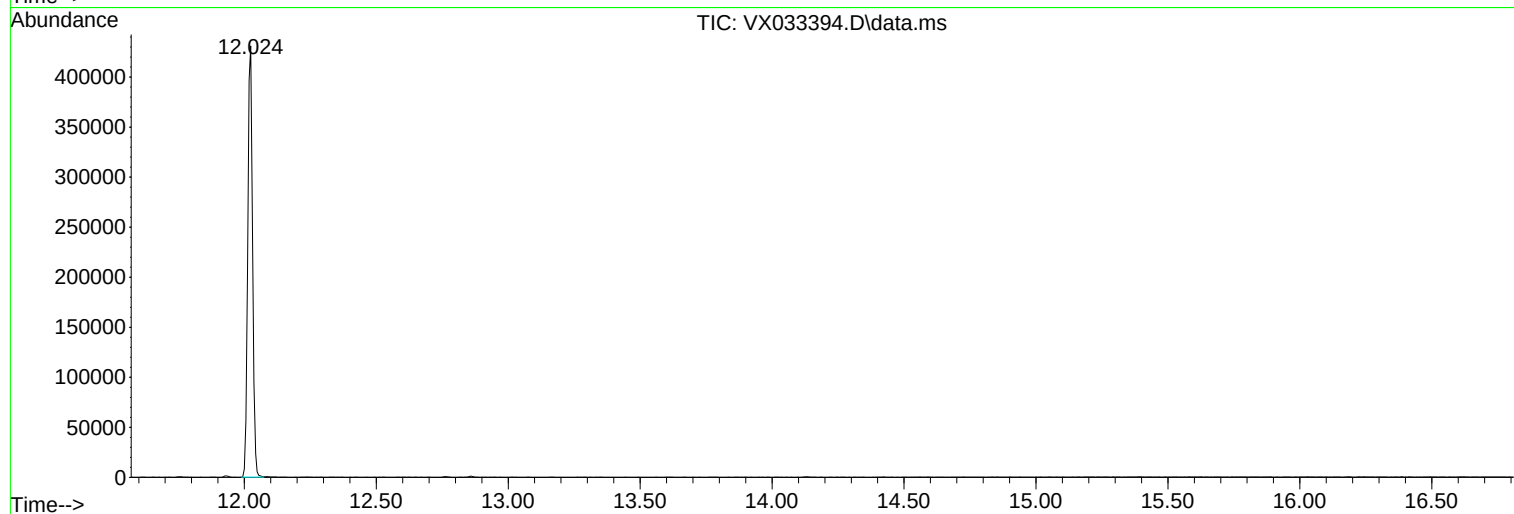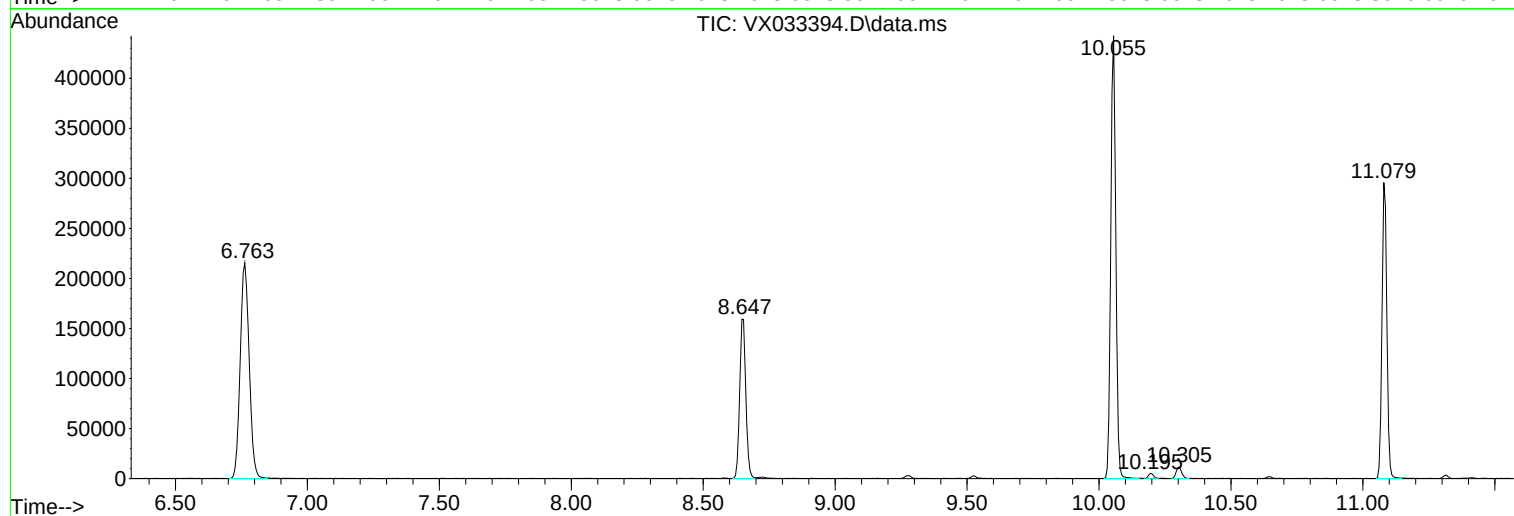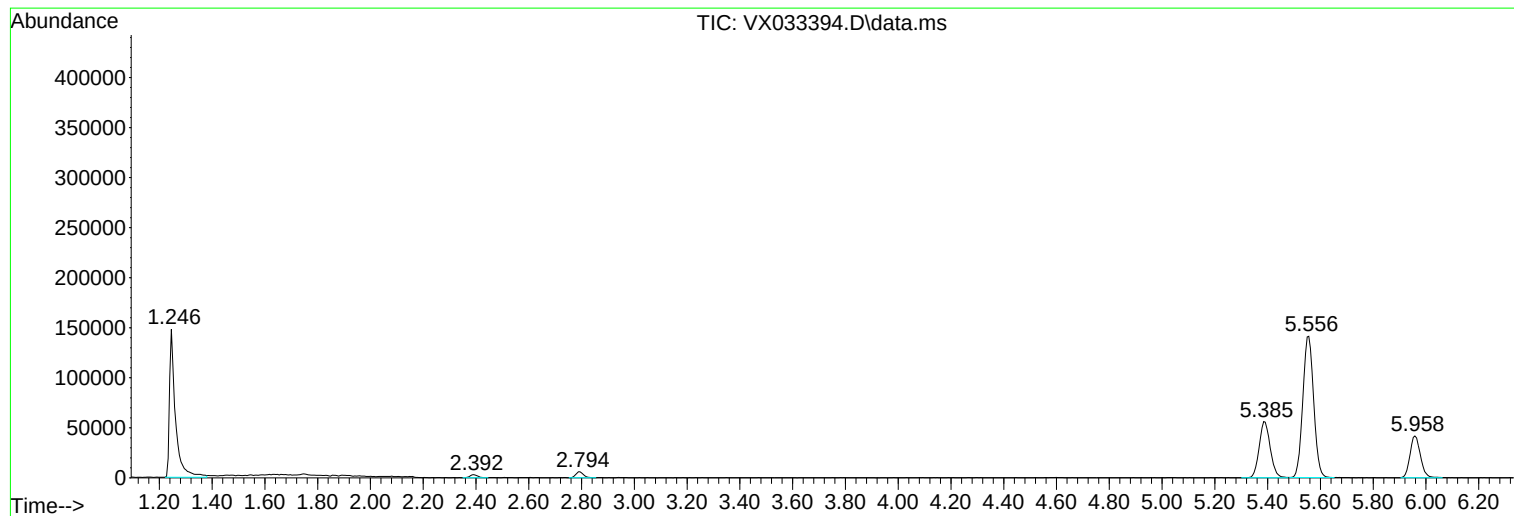

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121322\
Data File : VX033394.D
Acq On : 13 Dec 2022 15:54
Operator : JC/MD
Sample : N5865-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.246	28.78 ug/l	232689	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	83
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

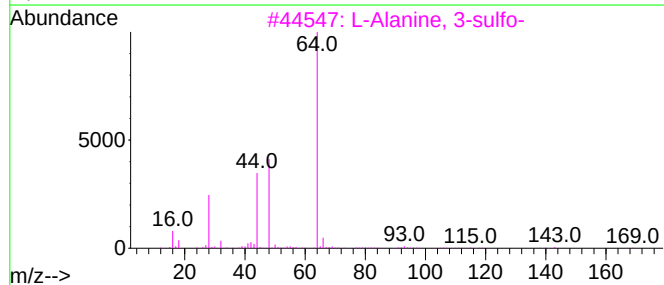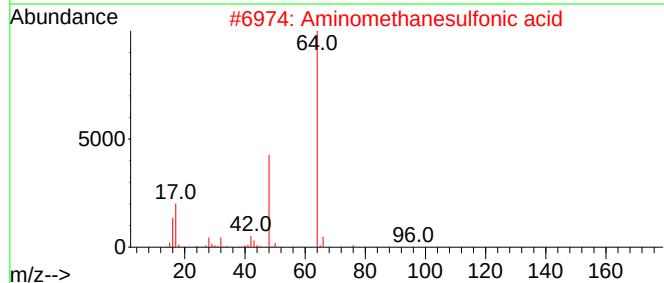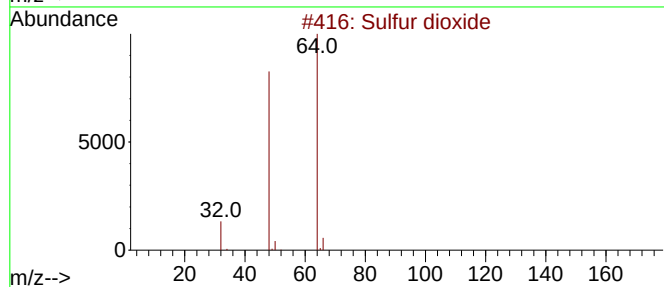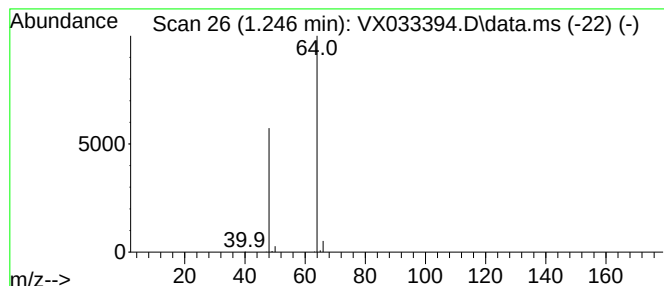

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121322\
Data File : VX033394.D
Acq On : 13 Dec 2022 15:54
Operator : JC/MD
Sample : N5865-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.246	28.8	ug/l	232689	1	5.556	404242	50.0