

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121322\
 Data File : VX033396.D
 Acq On : 13 Dec 2022 16:40
 Operator : JC/MD
 Sample : N6001-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-11B

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
 Title : SW846 8260

Signal : TIC: VX033396.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	40	rBV	46769	84740	16.26%	3.083%
2	1.374	43	47	53	rVB	4803	6011	1.15%	0.219%
3	1.752	104	109	114	rVB2	6660	8328	1.60%	0.303%
4	5.391	694	706	719	rBV	48086	140551	26.97%	5.113%
5	5.550	721	732	746	rVV	126381	356486	68.41%	12.968%
6	5.958	787	799	807	rBV	37132	98945	18.99%	3.599%
7	6.043	807	813	828	rVB2	10864	29226	5.61%	1.063%
8	6.763	920	931	948	rBV	189337	443251	85.06%	16.124%
9	8.647	1234	1240	1249	rBV	145720	230597	44.25%	8.388%
10	10.055	1465	1471	1482	rBV	393333	521120	100.00%	18.956%
11	10.195	1491	1494	1500	rVB	4949	6391	1.23%	0.232%
12	10.305	1505	1512	1517	rBV	8686	12834	2.46%	0.467%
13	11.079	1634	1639	1652	rBV	258456	333898	64.07%	12.146%
14	12.024	1788	1794	1803	rBV	378340	476685	91.47%	17.340%




Sum of corrected areas: 2749063

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121322\
Data File : VX033396.D
Acq On : 13 Dec 2022 16:40
Operator : JC/MD
Sample : N6001-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11B

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

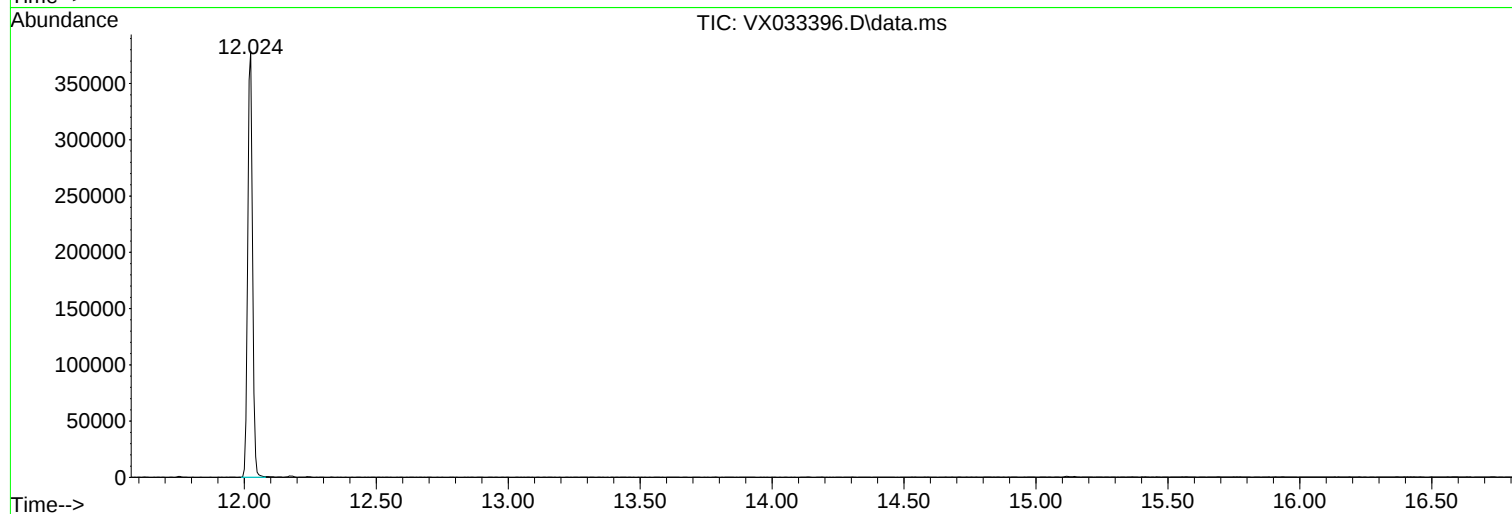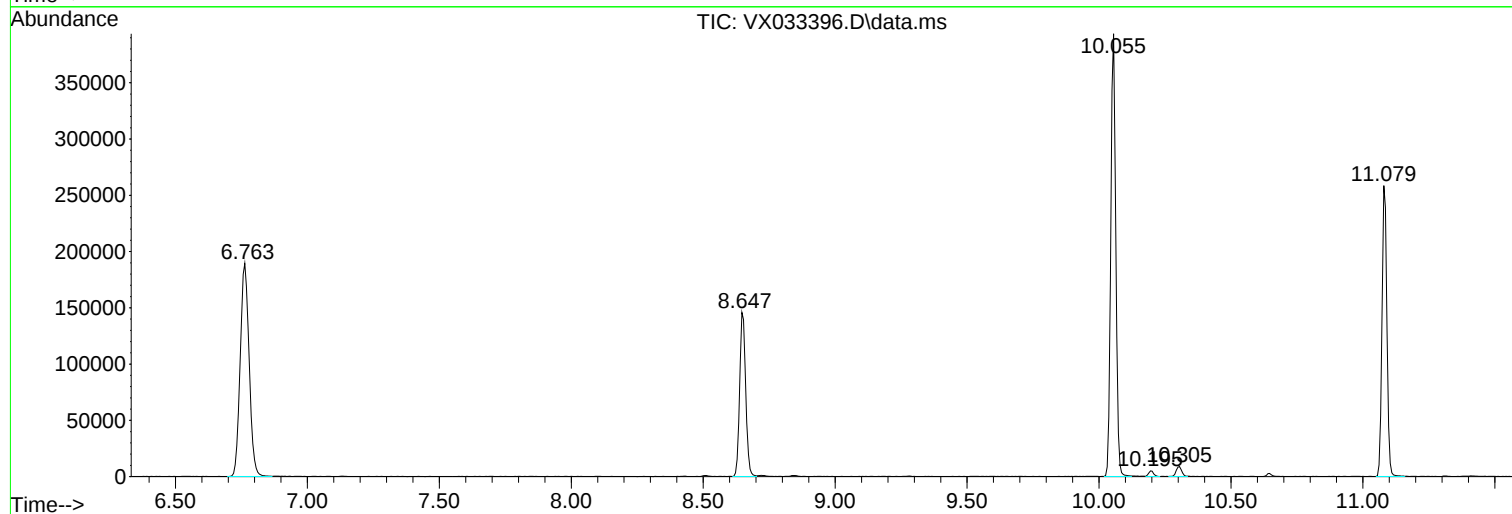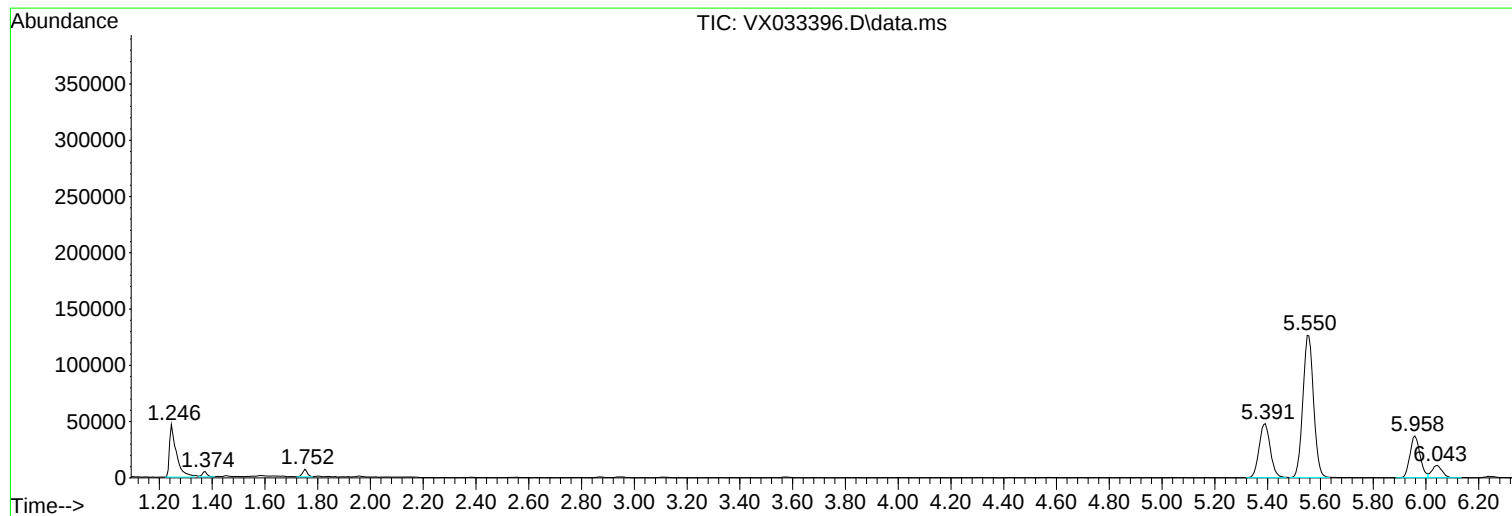

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121322\
Data File : VX033396.D
Acq On : 13 Dec 2022 16:40
Operator : JC/MD
Sample : N6001-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11B









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.246	11.89 ug/l	84740	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	90
2			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
3			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

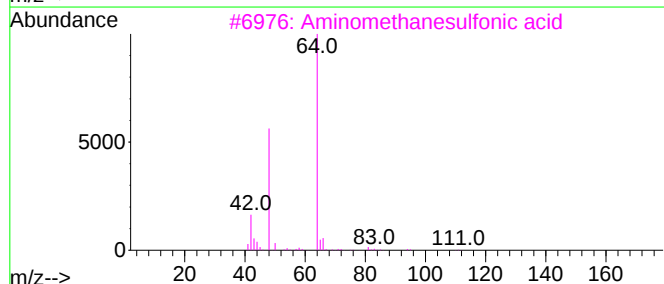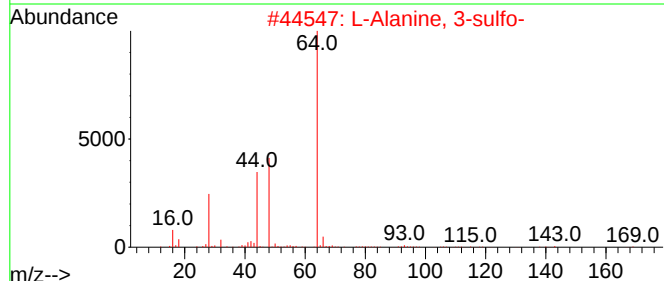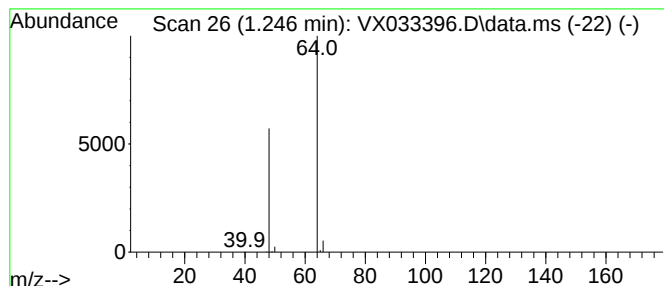

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121322\
Data File : VX033396.D
Acq On : 13 Dec 2022 16:40
Operator : JC/MD
Sample : N6001-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11B

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.246	11.9	ug/l	84740	1	5.556	356486	50.0