

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121322\
 Data File : VX033404.D
 Acq On : 13 Dec 2022 19:44
 Operator : JC/MD
 Sample : N6026-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB-2022-12-12

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M

Title : SW846 8260

Signal : TIC: VX033404.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	23	29	43	rBV2	14030	38156	7.71%	1.479%
2	2.940	297	304	317	rBV	8988	20784	4.20%	0.806%
3	4.562	560	570	583	rBV2	1914	6470	1.31%	0.251%
4	5.385	694	705	721	rBV	49634	142584	28.82%	5.527%
5	5.556	721	733	748	rVV	121379	344647	69.67%	13.359%
6	5.958	787	799	810	rBV2	37379	99054	20.02%	3.839%
7	6.763	921	931	948	rBV	182330	431964	87.32%	16.743%
8	8.647	1234	1240	1250	rBV	144160	226688	45.83%	8.787%
9	10.055	1465	1471	1481	rBV	372692	494666	100.00%	19.174%
10	11.079	1634	1639	1652	rBV	254574	325162	65.73%	12.604%
11	12.024	1788	1794	1805	rBV	354978	449751	90.92%	17.433%




Sum of corrected areas: 2579926

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121322\
Data File : VX033404.D
Acq On : 13 Dec 2022 19:44
Operator : JC/MD
Sample : N6026-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2022-12-12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

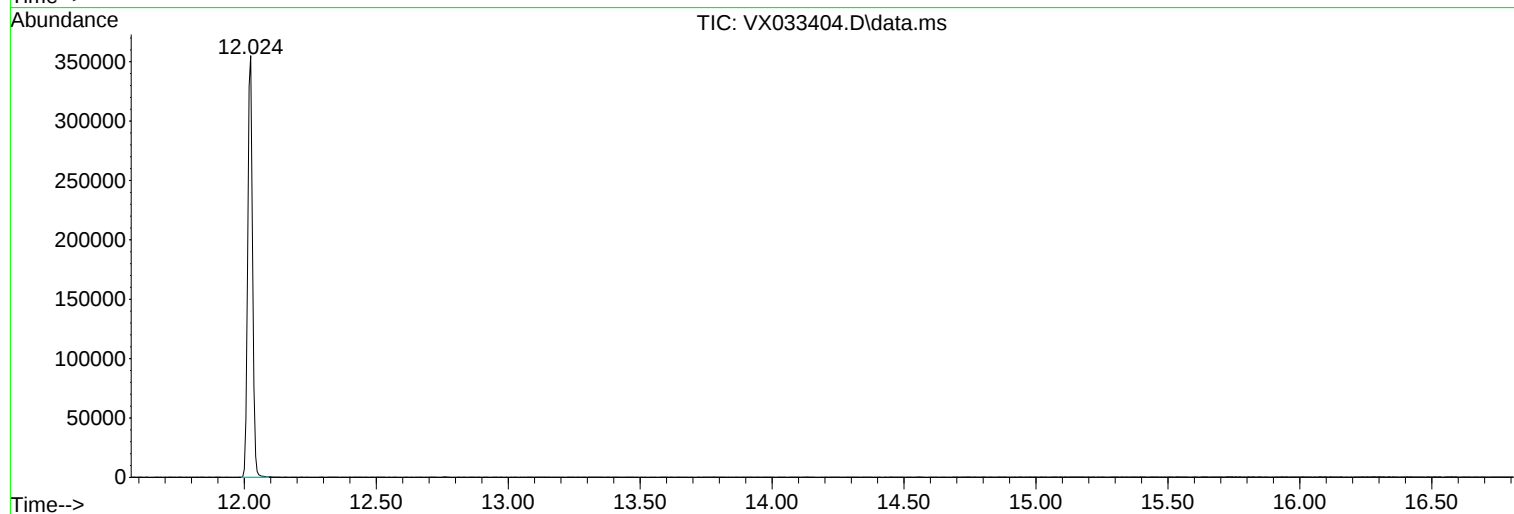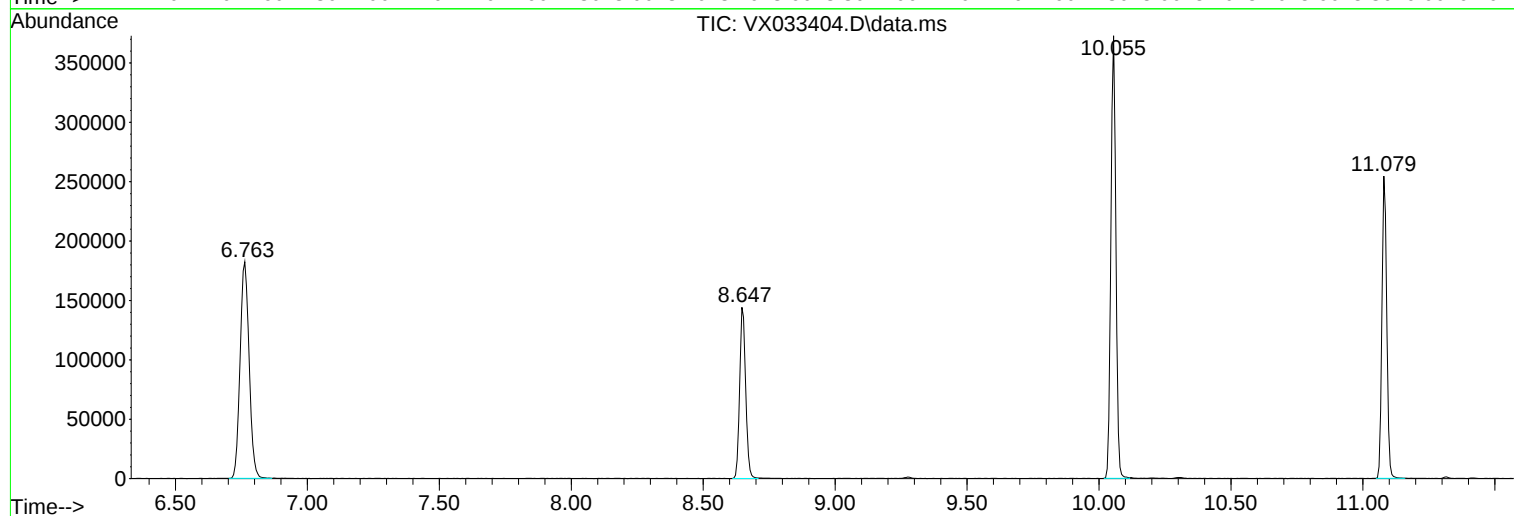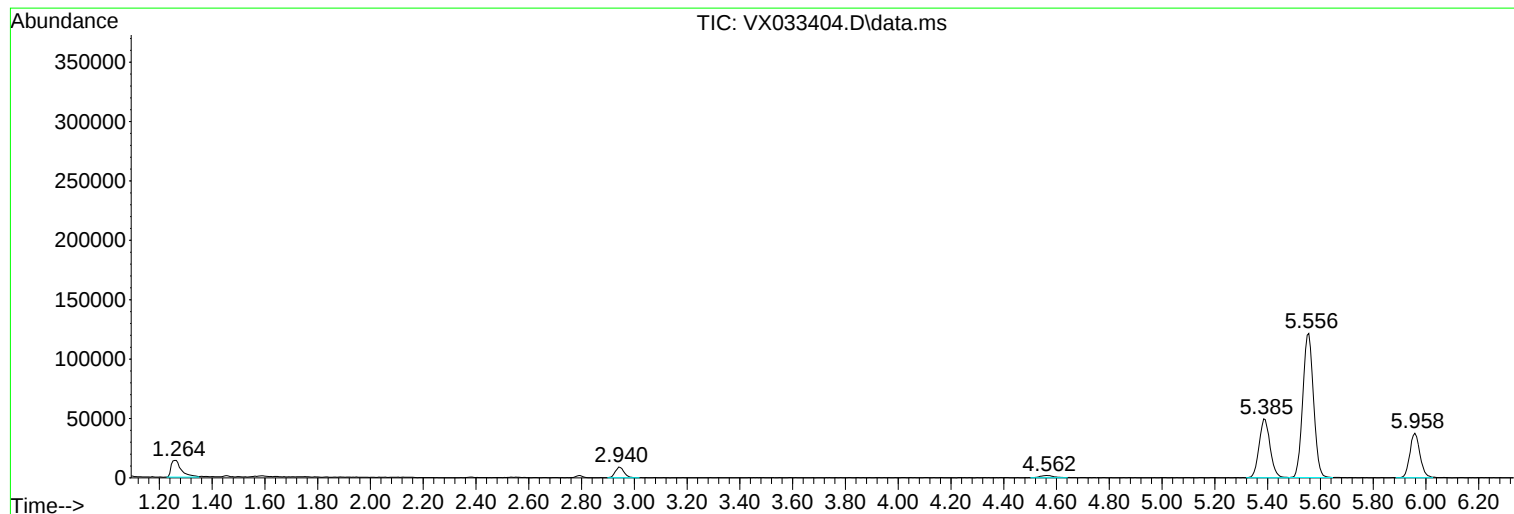

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121322\
Data File : VX033404.D
Acq On : 13 Dec 2022 19:44
Operator : JC/MD
Sample : N6026-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2022-12-12







Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.264	5.54 ug/l	38156	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	90
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	5
5			Ethene, 1,2-difluoro-	64	C2H2F2	001691-13-0	4

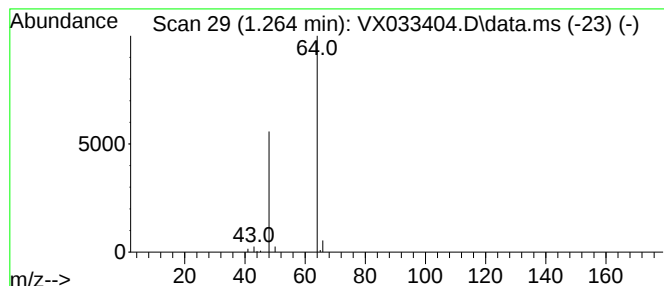

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121322\
Data File : VX033404.D
Acq On : 13 Dec 2022 19:44
Operator : JC/MD
Sample : N6026-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2022-12-12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.264	5.5	ug/l	38156	1	5.556	344647	50.0