

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121323\
 Data File : VX039189.D
 Acq On : 13 Dec 2023 15:11
 Operator : JC/MD
 Sample : VX1213WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1213WBL01

Quant Time: Dec 14 01:32:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 01:28:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	112881	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	231638	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	237362	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	117591	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	100554	48.626	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.260%
35) Dibromofluoromethane	5.385	113	76755	47.964	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.920%
50) Toluene-d8	8.647	98	291276	49.028	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.060%
62) 4-Bromofluorobenzene	11.079	95	133027	54.269	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	108.540%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121323\
Data File : VX039189.D
Acq On : 13 Dec 2023 15:11
Operator : JC/MD
Sample : VX1213WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1213WBL01

Quant Time: Dec 14 01:32:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 01:28:15 2023
Response via : Initial Calibration




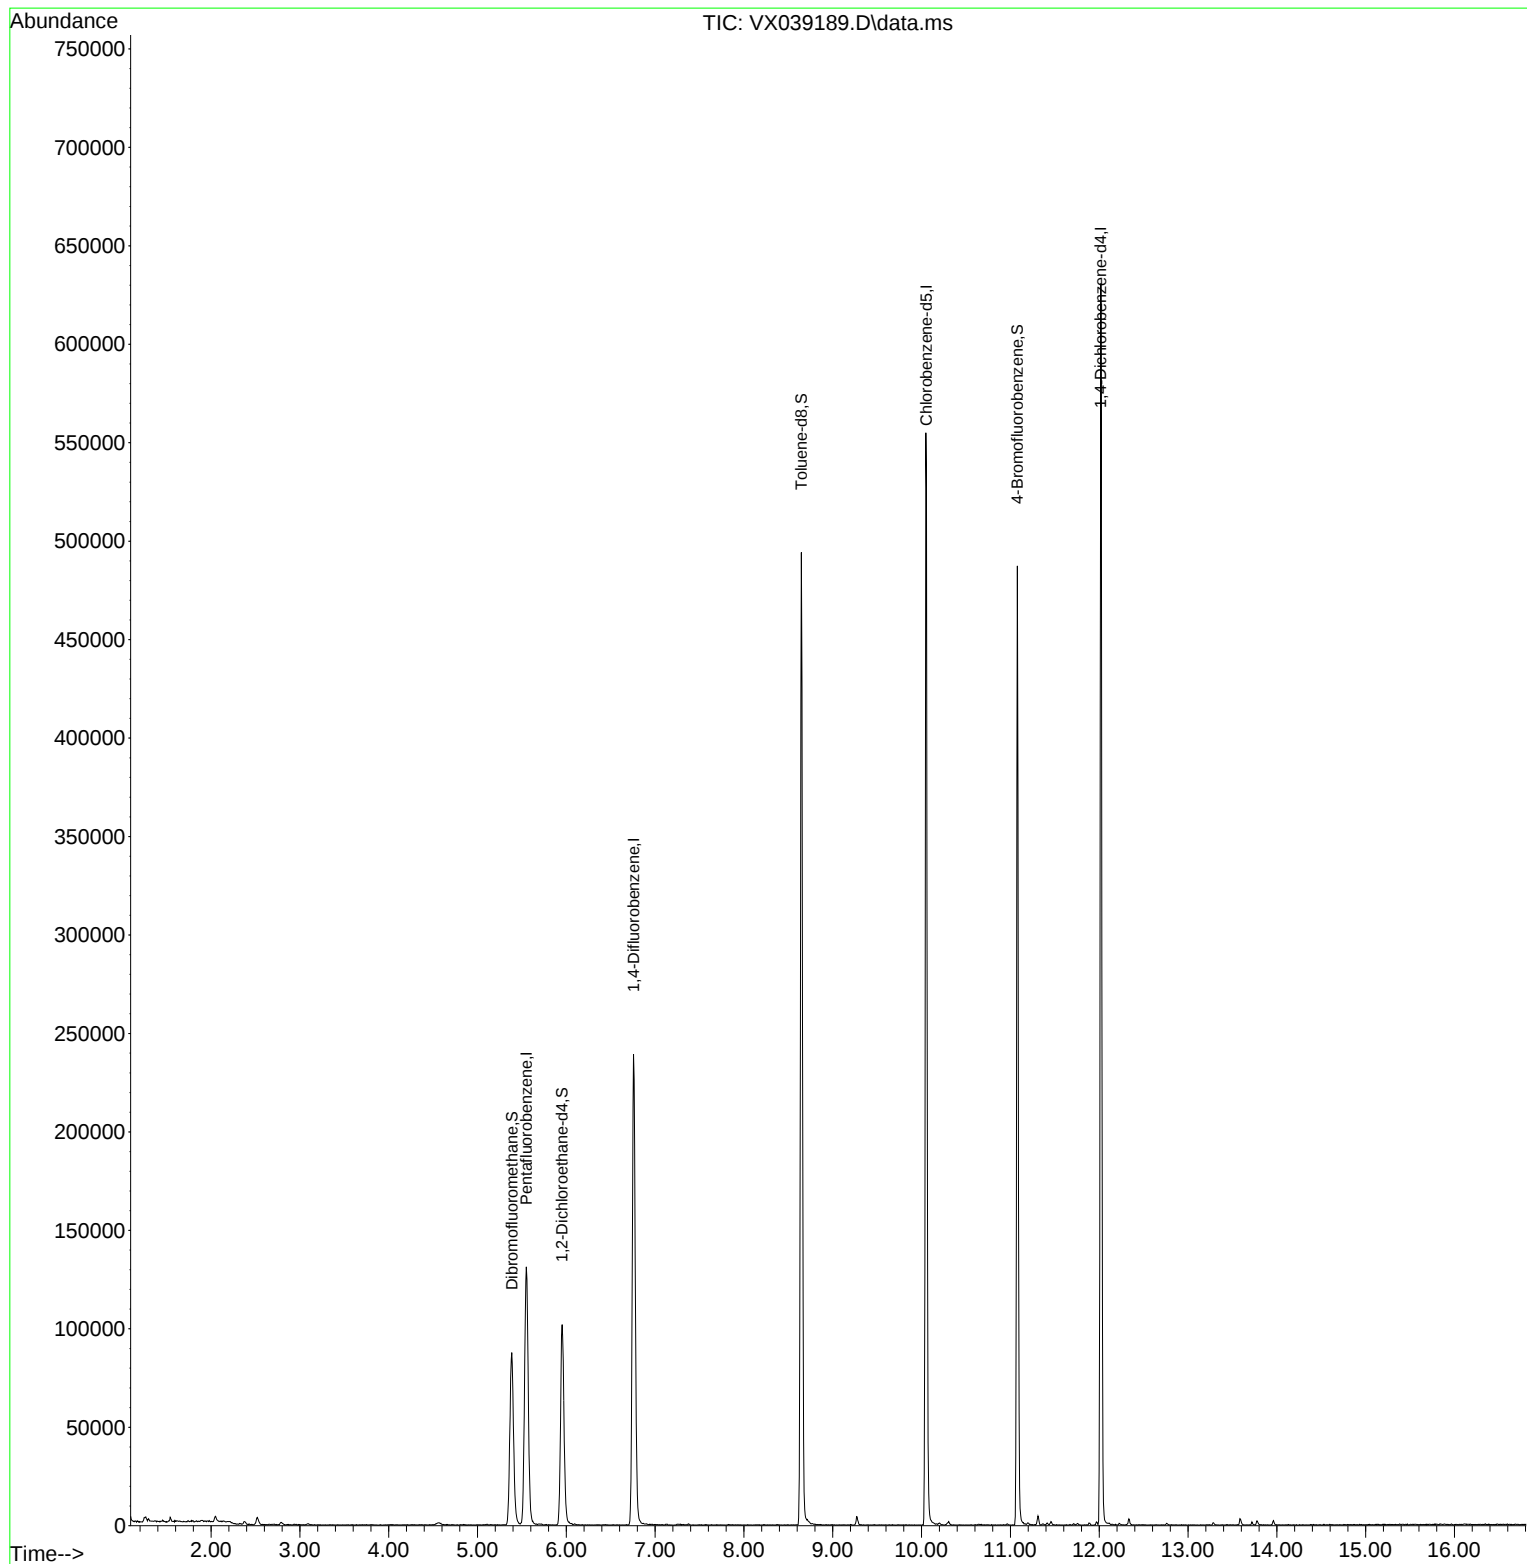


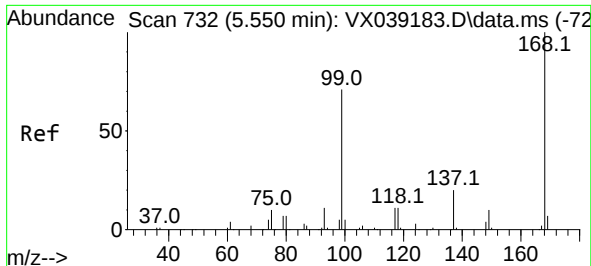

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.000 min
Lab File: VX039189.D
Acq: 13 Dec 2023 15:11




Instrument :
MSVOA_X
ClientSampleId :
VX1213WBL01

Tgt Ion:168 Resp: 112881
Ion Ratio Lower Upper
168 100
99 71.1 56.6 85.0

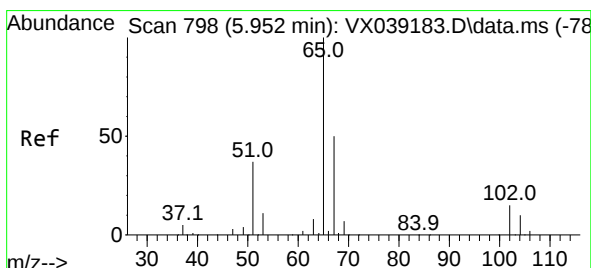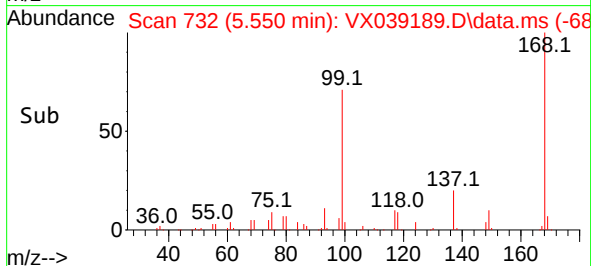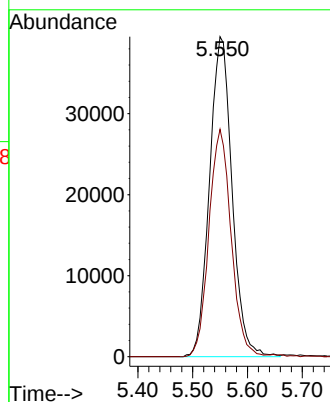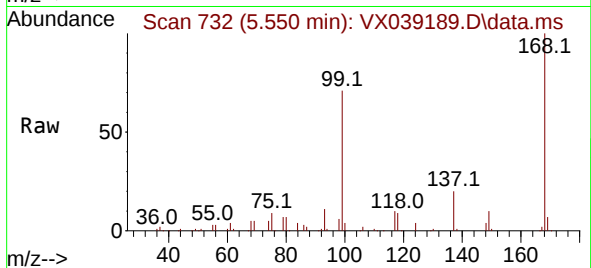

#33
1,2-Dichloroethane-d4
Concen: 48.626 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX039189.D
Acq: 13 Dec 2023 15:11

Tgt Ion: 65 Resp: 100554
Ion Ratio Lower Upper
65 100
67 51.8 0.0 100.2


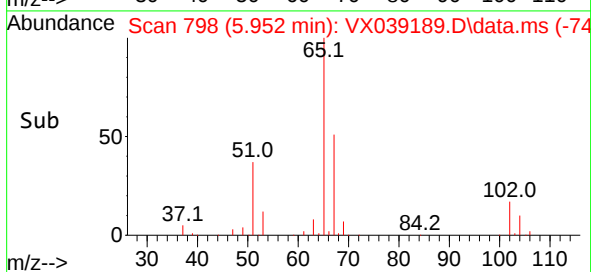
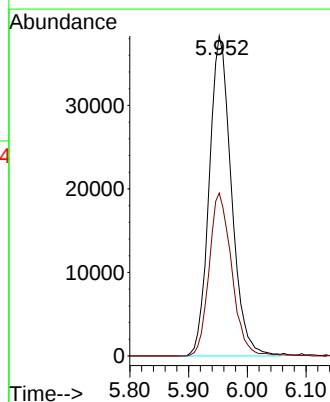
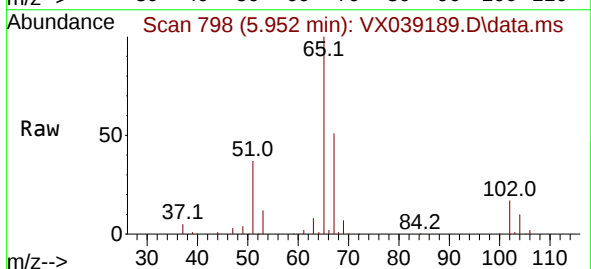




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX039189.D
Acq: 13 Dec 2023 15:11




Instrument :
MSVOA_X
ClientSampleId :
VX1213WBL01

Tgt Ion:114 Resp: 231638
Ion Ratio Lower Upper
114 100
63 23.8 0.0 45.0
88 17.9 0.0 36.6

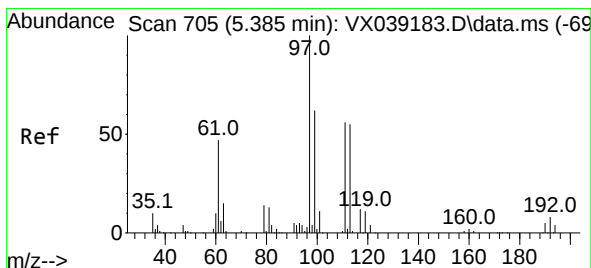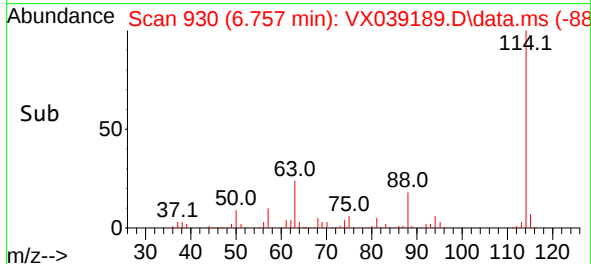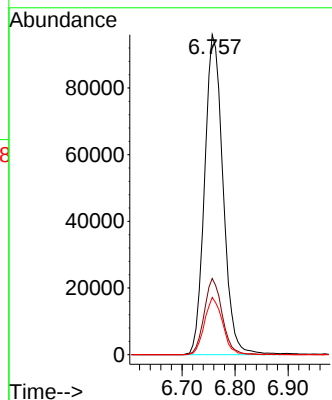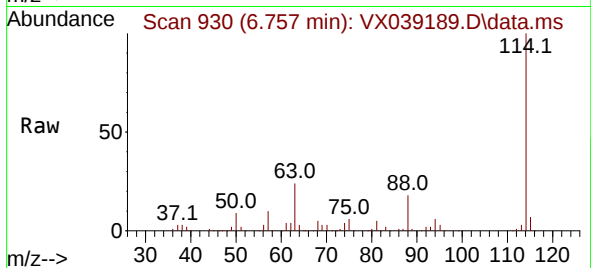

#35
Dibromofluoromethane
Concen: 47.964 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX039189.D
Acq: 13 Dec 2023 15:11

Tgt Ion:113 Resp: 76755
Ion Ratio Lower Upper
113 100
111 102.7 82.9 124.3
192 15.1 13.3 19.9


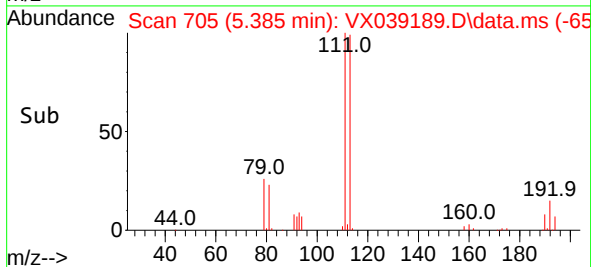
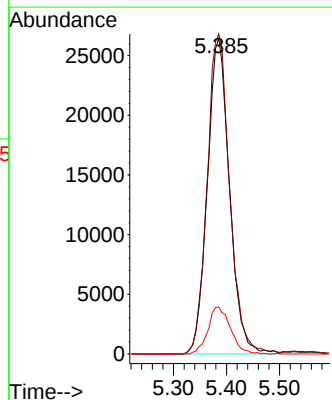
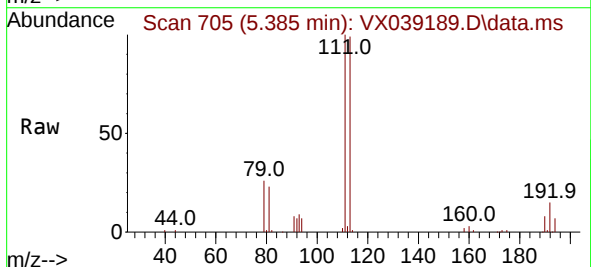




#50
Toluene-d8
Concen: 49.028 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX039189.D
Acq: 13 Dec 2023 15:11




Instrument :
MSVOA_X
ClientSampleId :
VX1213WBL01


Tgt Ion: 98 Resp: 291276
Ion Ratio Lower Upper
98 100
100 63.4 53.1 79.7

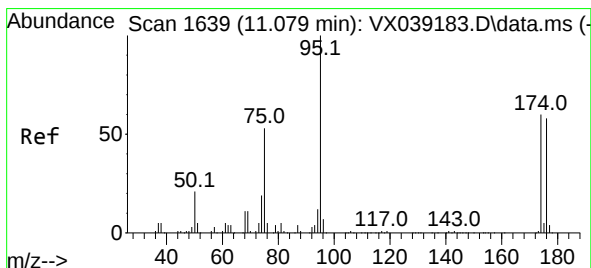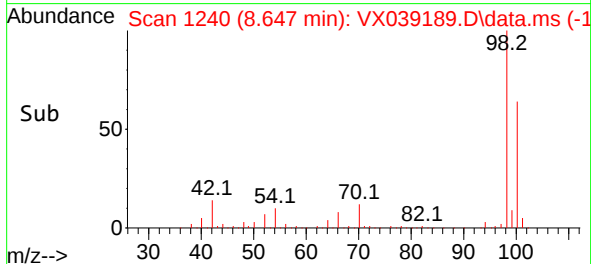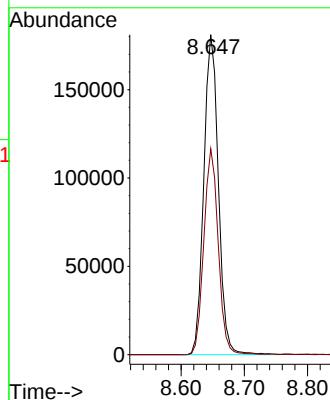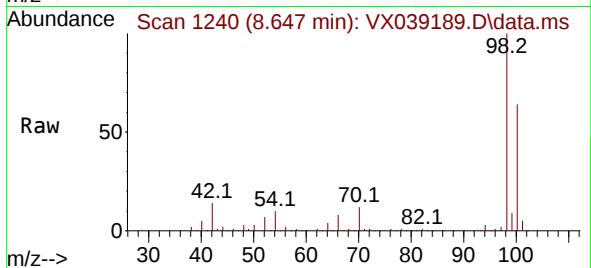

#62
4-Bromofluorobenzene
Concen: 54.269 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX039189.D
Acq: 13 Dec 2023 15:11

Tgt Ion: 95 Resp: 133027
Ion Ratio Lower Upper
95 100
174 61.6 0.0 135.6
176 60.8 0.0 131.0


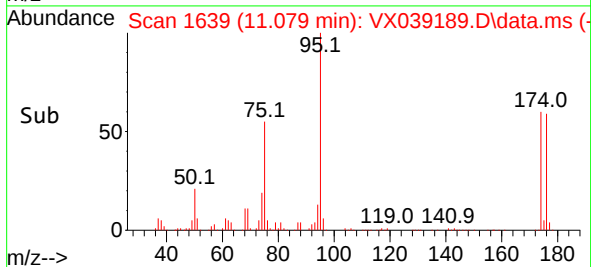
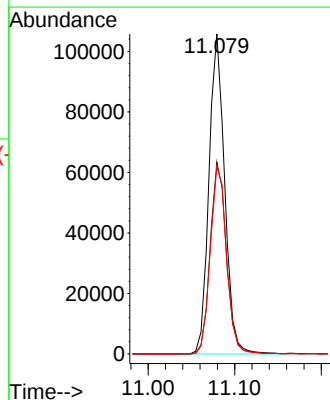
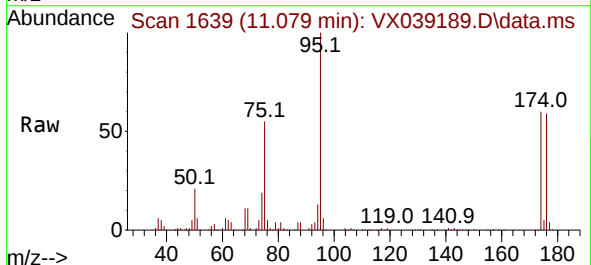


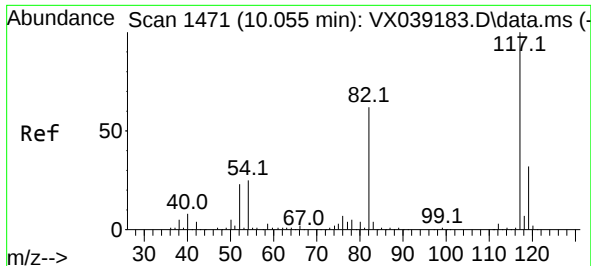

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX039189.D
Acq: 13 Dec 2023 15:11

Instrument :
MSVOA_X
ClientSampleId :
VX1213WBL01

Tgt Ion:117 Resp: 237362
Ion Ratio Lower Upper
117 100
82 59.8 46.2 69.4
119 31.8 25.5 38.3

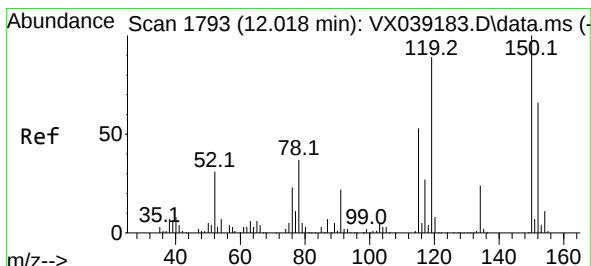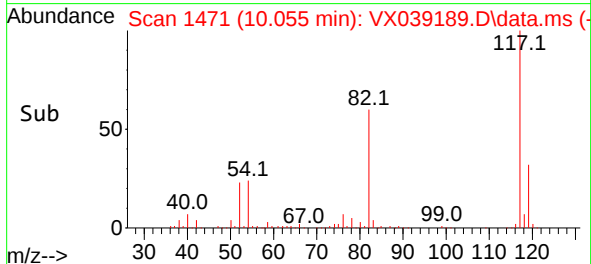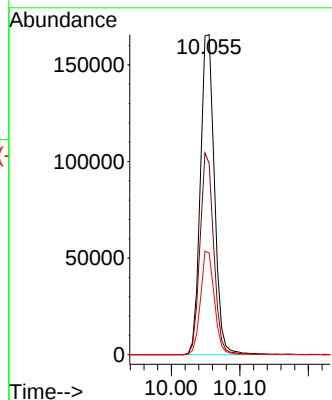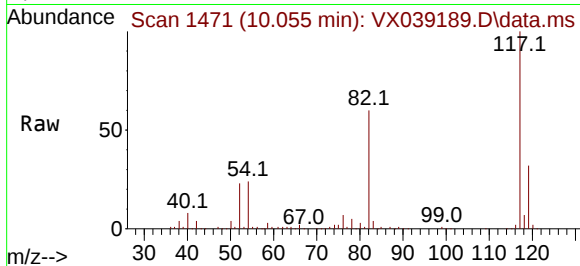

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX039189.D
Acq: 13 Dec 2023 15:11

Tgt Ion:152 Resp: 117591
Ion Ratio Lower Upper
152 100
115 67.4 43.3 129.9
150 157.1 0.0 345.0

