

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121323\
 Data File : VX039190.D
 Acq On : 13 Dec 2023 15:34
 Operator : JC/MD
 Sample : 05720-01RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TT-TB-20231207RE

Quant Time: Dec 14 01:32:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 01:28:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	118834	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	246253	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	251998	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	126849	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	106008	48.696	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.400%
35) Dibromofluoromethane	5.385	113	81708	48.029	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.060%
50) Toluene-d8	8.647	98	310772	49.205	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.400%
62) 4-Bromofluorobenzene	11.079	95	143339	55.005	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	110.020%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121323\
Data File : VX039190.D
Acq On : 13 Dec 2023 15:34
Operator : JC/MD
Sample : 05720-01RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT-TB-20231207RE

Quant Time: Dec 14 01:32:50 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 01:28:15 2023
Response via : Initial Calibration




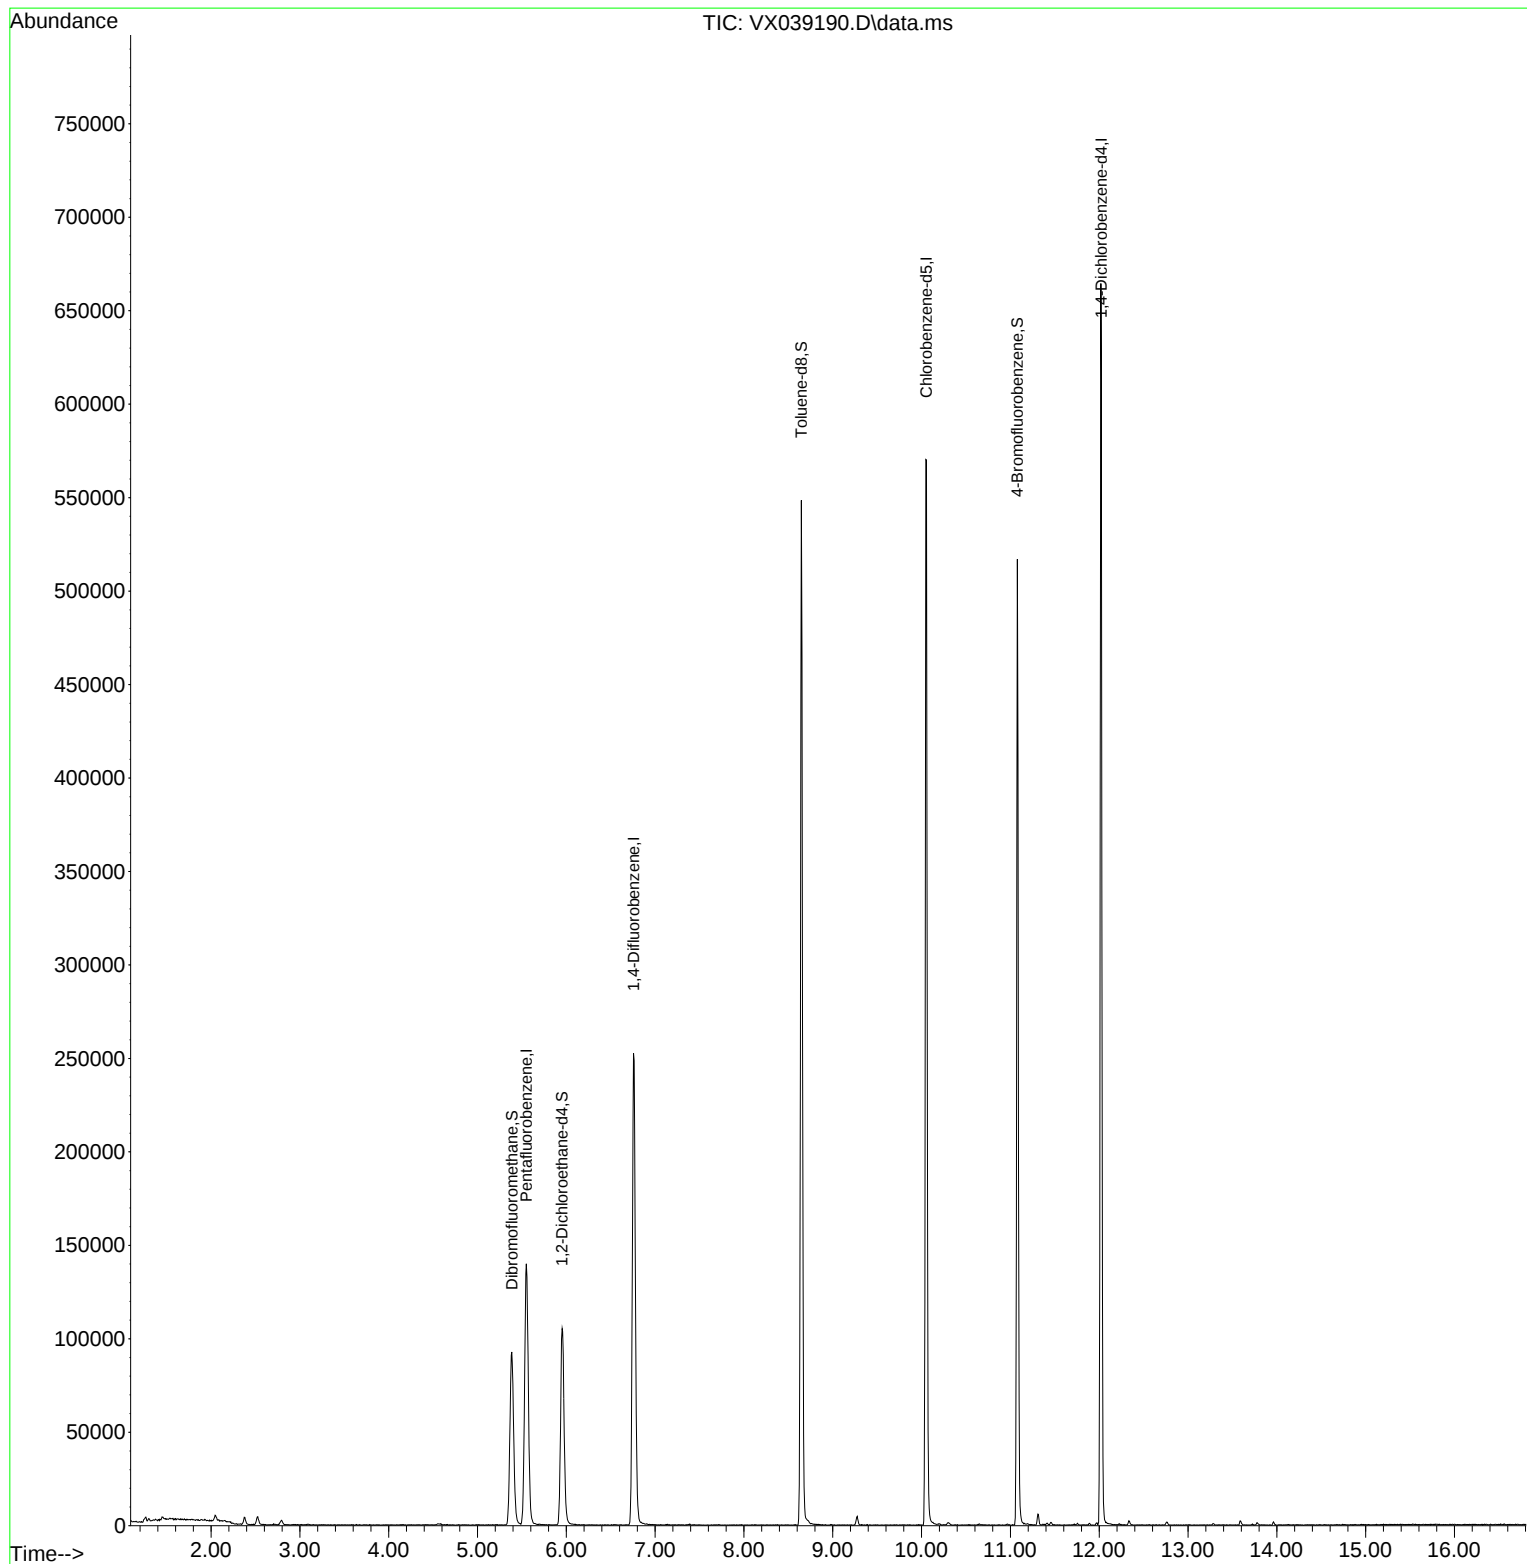


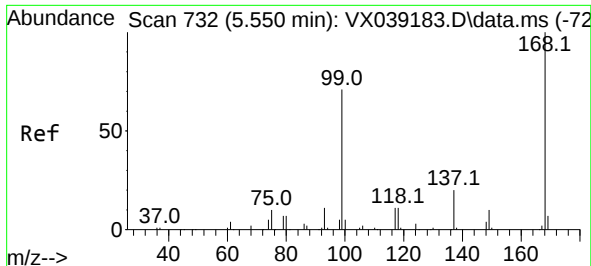

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX039190.D
Acq: 13 Dec 2023 15:34




Instrument :
MSVOA_X
ClientSampleId :
TT-TB-20231207RE

Tgt Ion:168 Resp: 118834
Ion Ratio Lower Upper
168 100
99 68.2 56.6 85.0

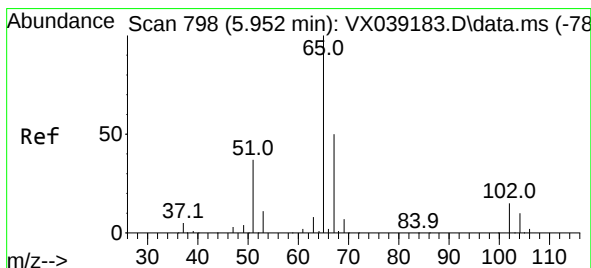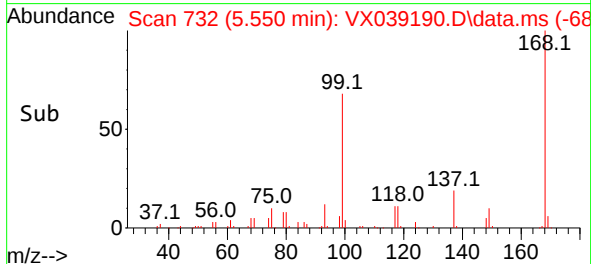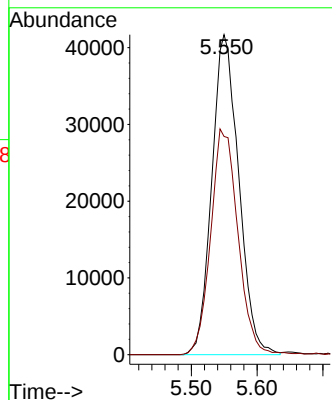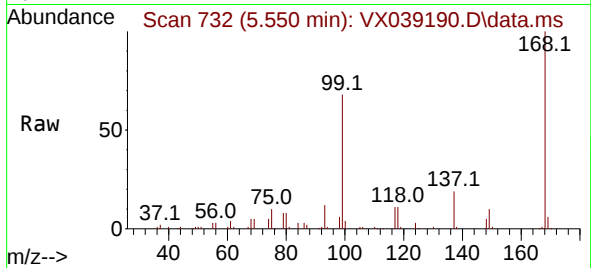

#33
1,2-Dichloroethane-d4
Concen: 48.696 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX039190.D
Acq: 13 Dec 2023 15:34

Tgt Ion: 65 Resp: 106008
Ion Ratio Lower Upper
65 100
67 51.6 0.0 100.2


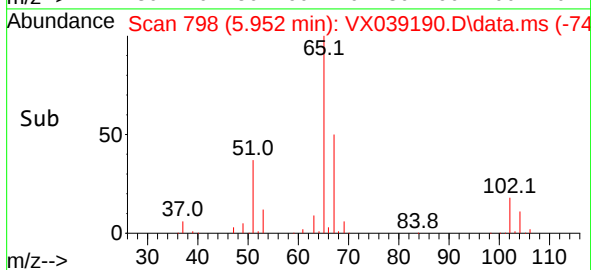
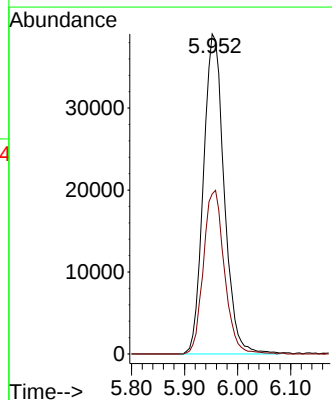
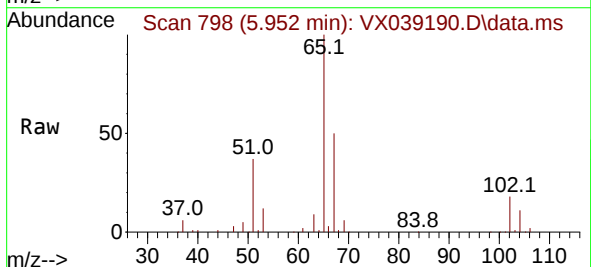




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX039190.D
Acq: 13 Dec 2023 15:34




Instrument :
MSVOA_X
ClientSampleId :
TT-TB-20231207RE

Tgt Ion:114 Resp: 246253
Ion Ratio Lower Upper
114 100
63 23.4 0.0 45.0
88 17.7 0.0 36.6

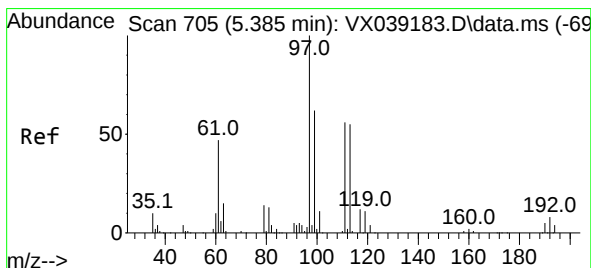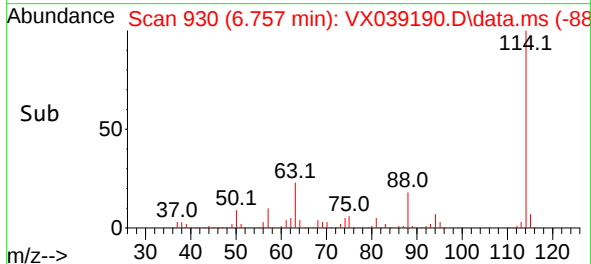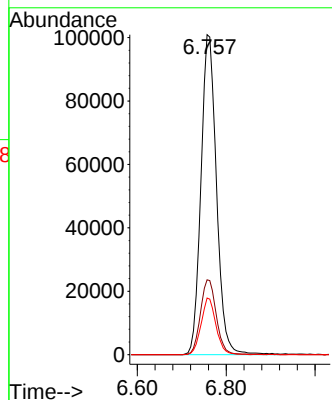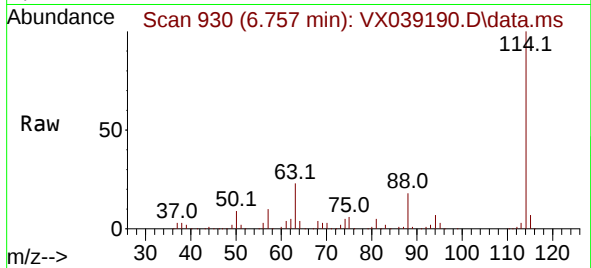

#35
Dibromofluoromethane
Concen: 48.029 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX039190.D
Acq: 13 Dec 2023 15:34

Tgt Ion:113 Resp: 81708
Ion Ratio Lower Upper
113 100
111 102.8 82.9 124.3
192 16.2 13.3 19.9

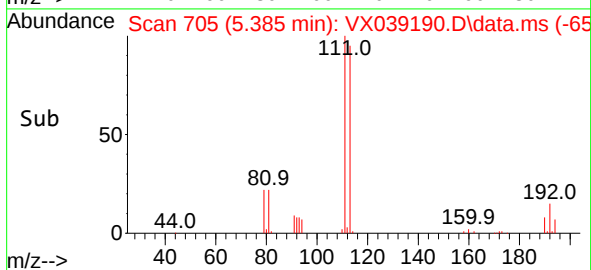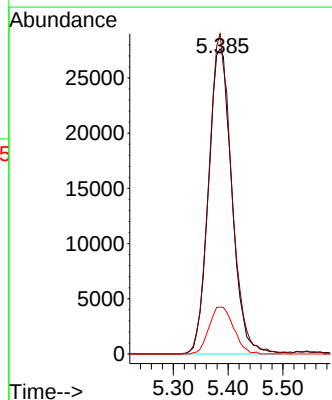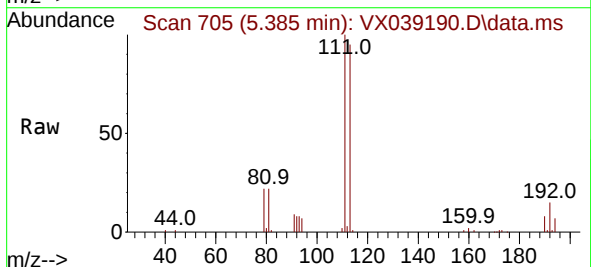



#50

Toluene-d8

Concen: 49.205 ug/l

RT: 8.647 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX039190.D

Acq: 13 Dec 2023 15:34

Instrument :

MSVOA_X

ClientSampleId :





TT-TB-20231207RE

Tgt Ion: 98 Resp: 310772

Ion Ratio Lower Upper

98 100

100 63.9 53.1 79.7

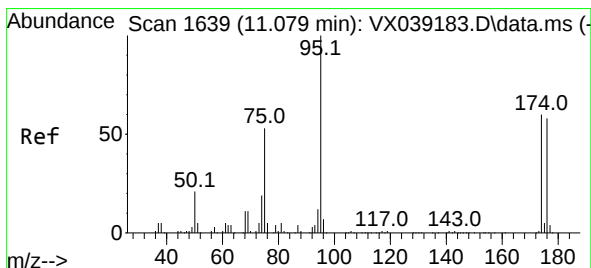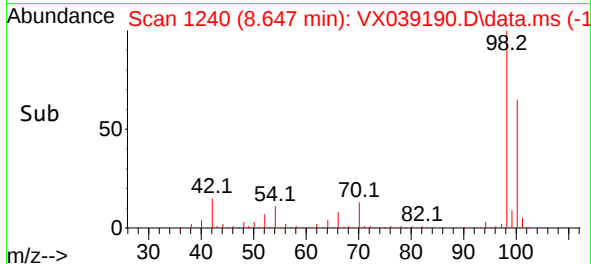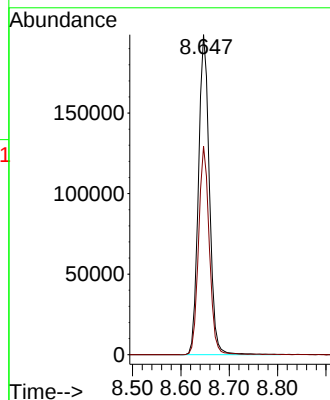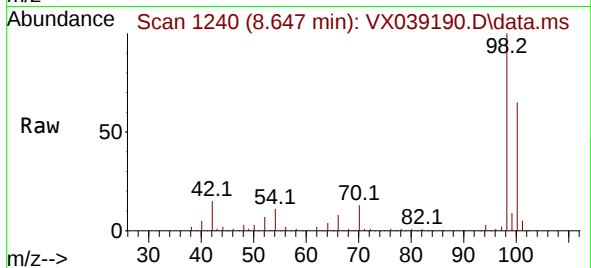

#62

4-Bromofluorobenzene

Concen: 55.005 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX039190.D

Acq: 13 Dec 2023 15:34




Tgt Ion: 95 Resp: 143339


Ion Ratio Lower Upper

95 100

174 62.1 0.0 135.6

176 60.4 0.0 131.0

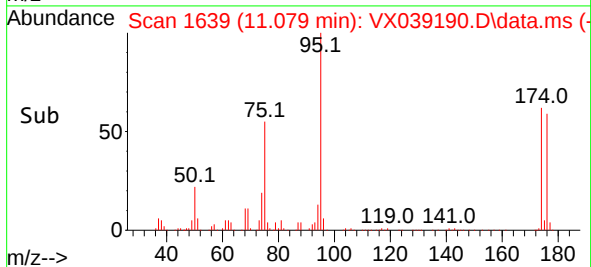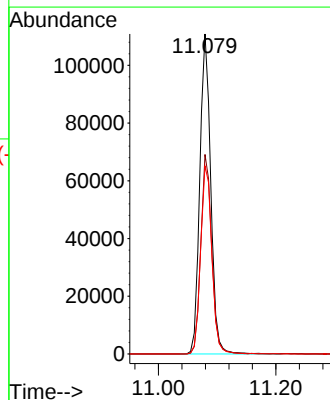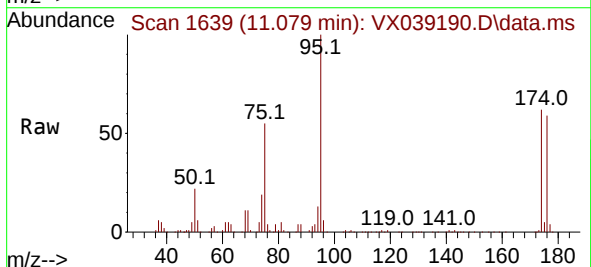

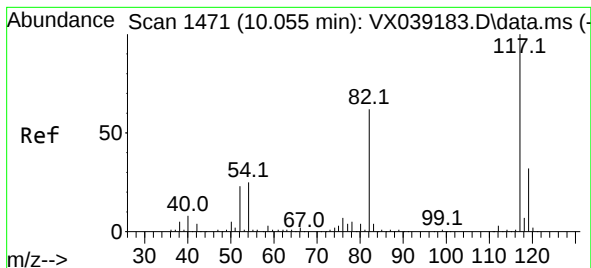

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX039190.D

Acq: 13 Dec 2023 15:34

Instrument :

MSVOA_X

ClientSampleId :

TT-TB-20231207RE





Tgt Ion:117 Resp: 251998

Ion Ratio Lower Upper

117 100

82 60.2 46.2 69.4

119 31.7 25.5 38.3

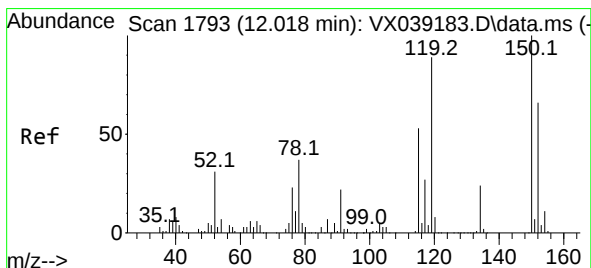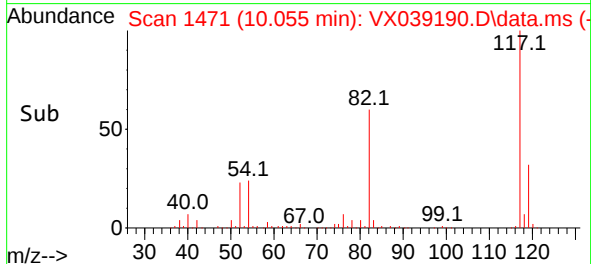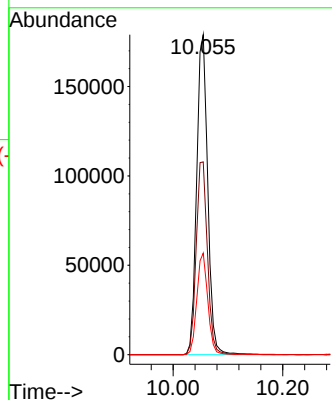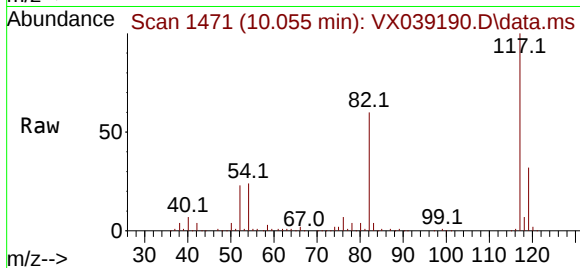

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.006 min

Lab File: VX039190.D

Acq: 13 Dec 2023 15:34

Tgt Ion:152 Resp: 126849

Ion Ratio Lower Upper

152 100

115 67.8 43.3 129.9

150 158.4 0.0 345.0

