



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121323\
Data File : VX039179.D
Acq On : 13 Dec 2023 09:01
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Title : SW846 8260
Last Update : Thu Dec 14 01:28:15 2023

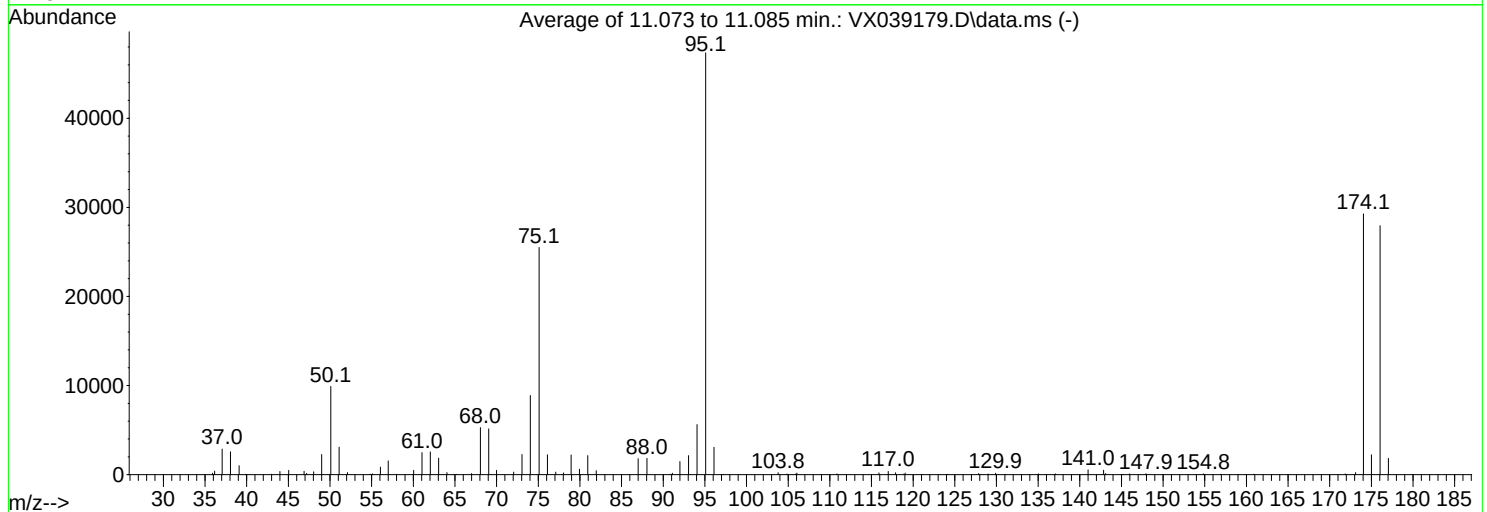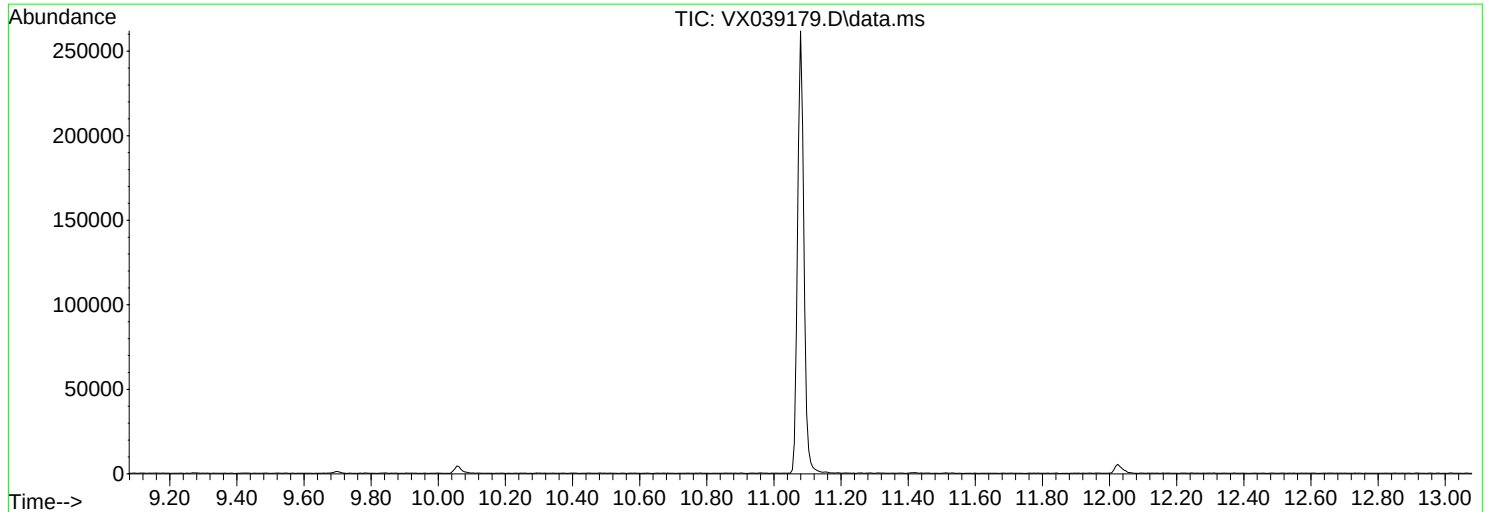

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	9889	PASS
75	95	30	60	53.9	25501	PASS
95	95	100	100	100.0	47344	PASS
96	95	5	9	6.5	3072	PASS
173	174	0.00	2	0.8	243	PASS
174	95	50	100	61.8	29277	PASS
175	174	5	9	7.6	2229	PASS
176	174	95	101	95.4	27936	PASS
177	176	5	9	6.5	1825	PASS