

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044294.D
 Acq On : 13 Dec 2024 20:09
 Operator : JC/MD
 Sample : P5232-08ME
 Misc : 6.26g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 13 23:25:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 07 03:56:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	309683	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	272032	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	122248	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	57569	20.314	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	40.620%#	
7) Chloroethane-d5	1.648	69	27368	12.467	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	24.940%#	
11) 1,1-Dichloroethene-d2	2.282	65	42552	35.109	ug/L	-0.01
Spiked Amount	50.000	Range 60 - 125	Recovery	=	70.220%	
21) 2-Butanone-d5	4.483	46	134053	77.260	ug/L	0.03
Spiked Amount	100.000	Range 40 - 130	Recovery	=	77.260%	
24) Chloroform-d	5.050	84	213772	39.729	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	79.460%	
26) 1,2-Dichloroethane-d4	5.952	65	151848	39.905	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	79.820%	
32) Benzene-d6	5.964	84	403741	42.953	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	85.900%	
36) 1,2-Dichloropropane-d6	7.305	67	126739	43.424	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	86.840%	
41) Toluene-d8	8.647	98	369115	42.471	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	84.940%	
43) trans-1,3-Dichloroprop...	8.951	79	50324	35.880	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	71.760%	
47) 2-Hexanone-d5	9.390	63	93611	82.259	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	82.260%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	163853	41.868	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	83.740%	
66) 1,2-Dichlorobenzene-d4	12.317	152	127672	44.824	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	89.640%	
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.715	43	14971	5.980	ug/L	98
48) 2-Hexanone	9.390	43	13149	4.863	ug/L #	71
61) 1,2,3-Trichloropropane	12.018	75	16691	5.895	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044294.D
Acq On : 13 Dec 2024 20:09
Operator : JC/MD
Sample : P5232-08ME
Misc : 6.26g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Dec 13 23:25:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 03:56:15 2024
Response via : Initial Calibration

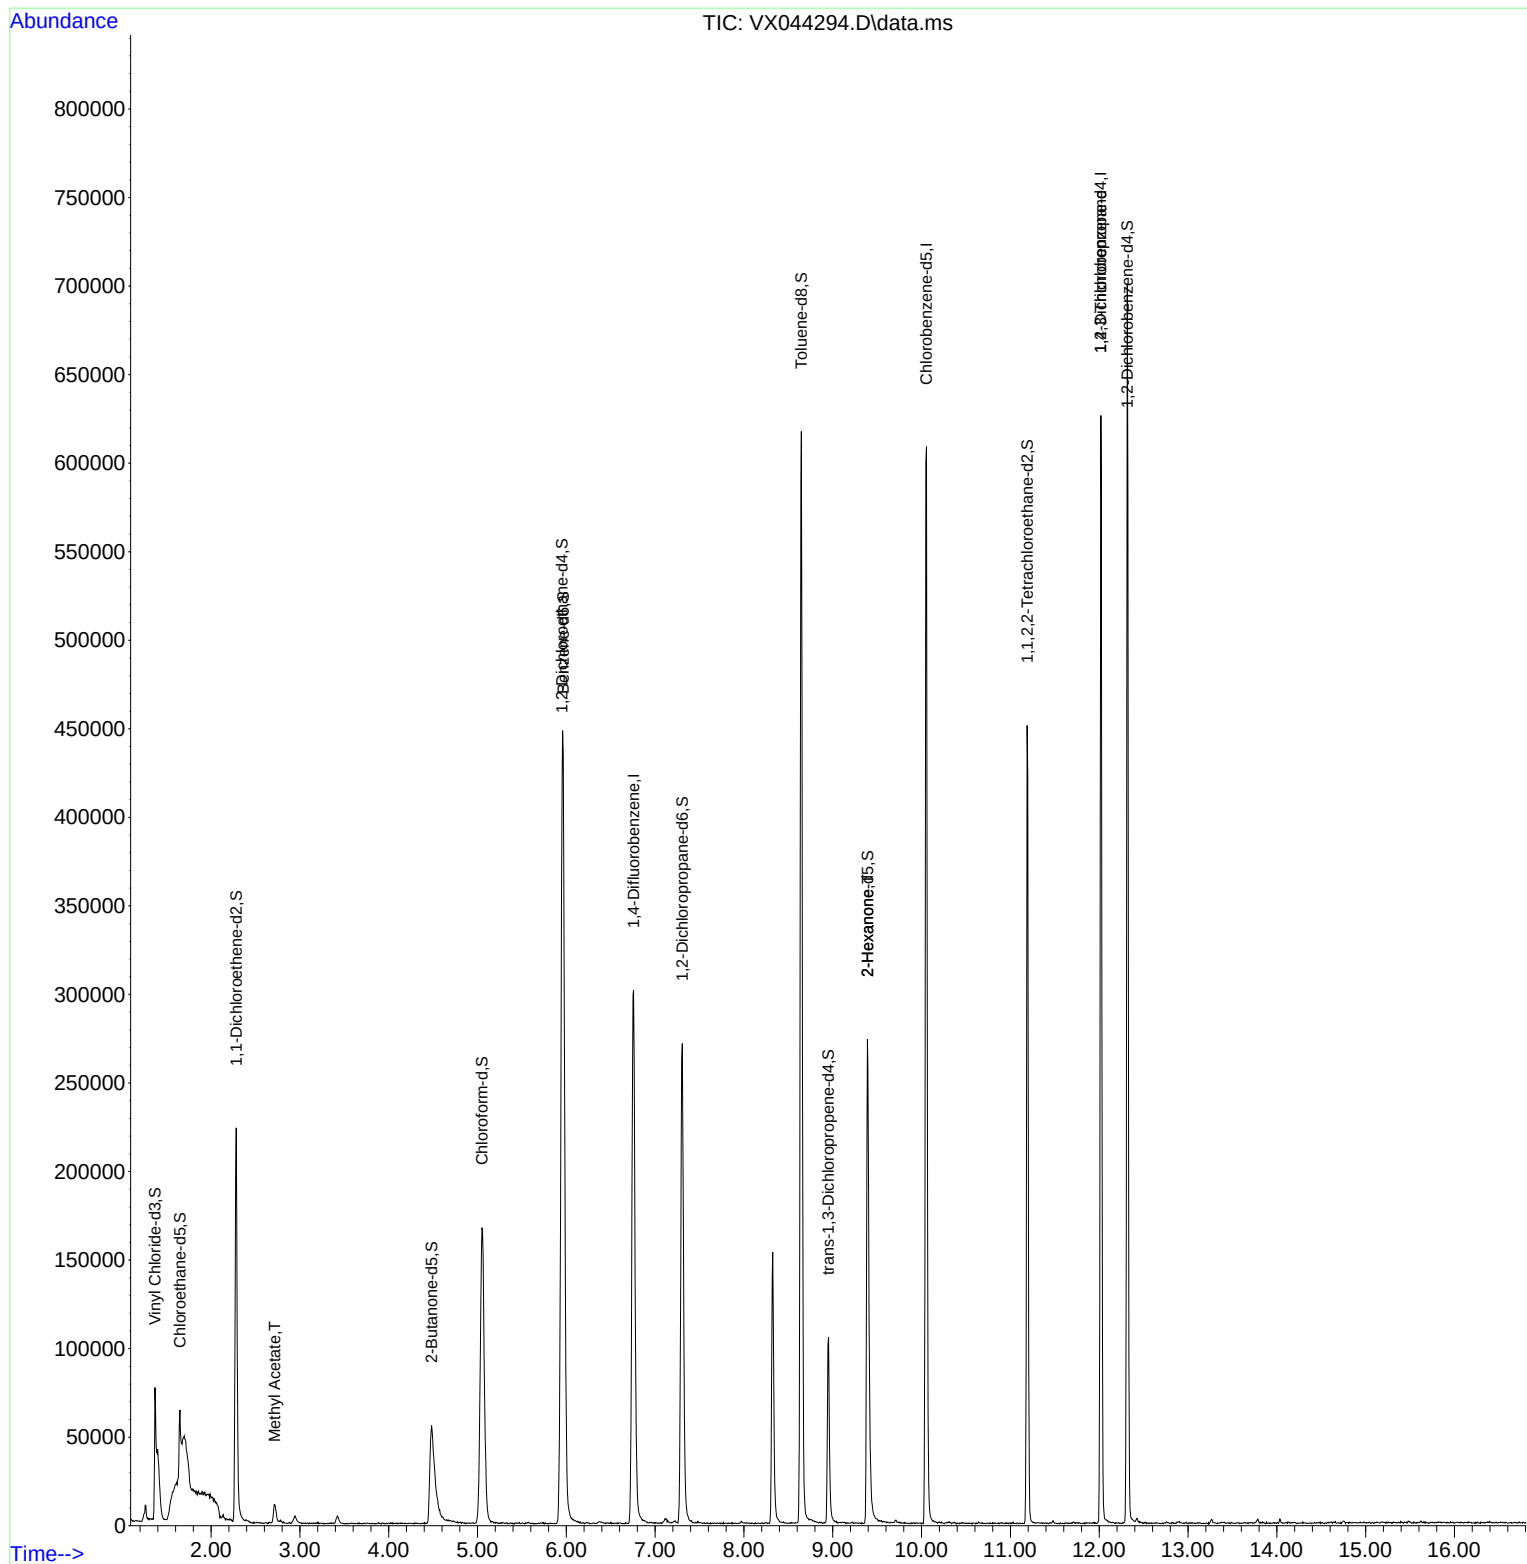



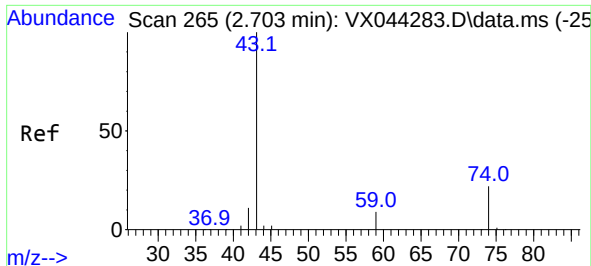


#15
Methyl Acetate
Concen: 5.980 ug/L
RT: 2.715 min Scan# 20
Delta R.T. 0.012 min
Lab File: VX044294.D
Acq: 13 Dec 2024 20:09

Instrument :
MSVOA_X
ClientSampleId :



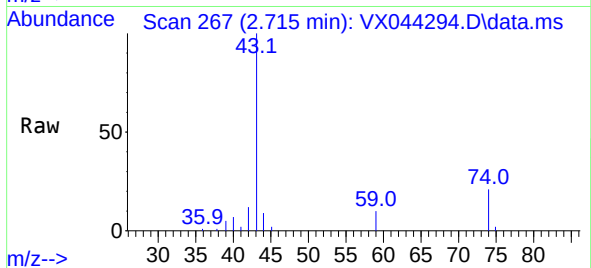



Tgt Ion: 43 Resp: 14971
Ion Ratio Lower Upper
43 100
74 23.2 19.4 29.2

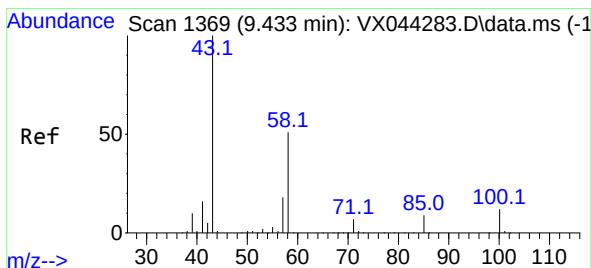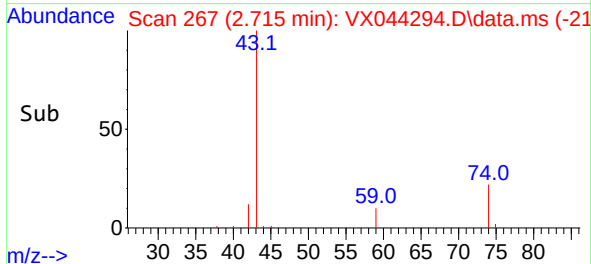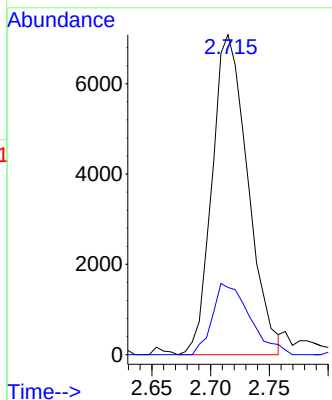

#48
2-Hexanone
Concen: 4.863 ug/L
RT: 9.390 min Scan# 1362
Delta R.T. -0.037 min
Lab File: VX044294.D
Acq: 13 Dec 2024 20:09


Tgt Ion: 43 Resp: 13149
Ion Ratio Lower Upper
43 100
58 30.6 45.4 68.2#
57 22.4 15.4 23.0
100 0.4 10.6 15.8#

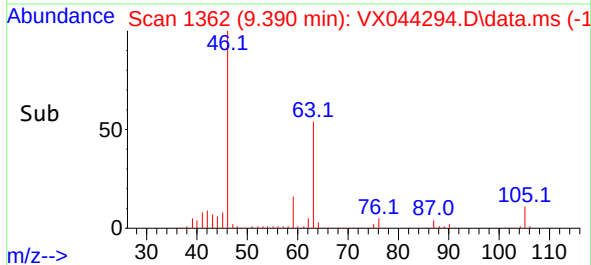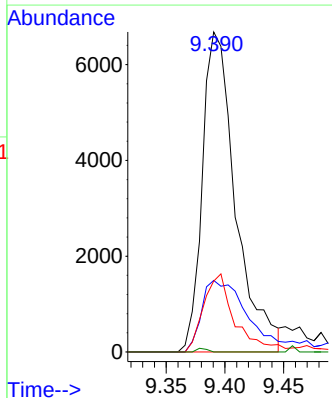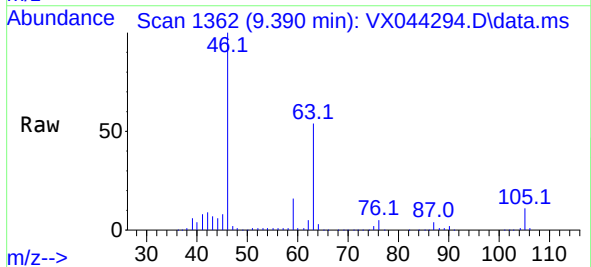

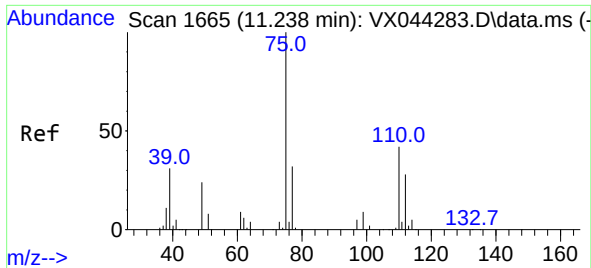

#61
1,2,3-Trichloropropane
Concen: 5.895 ug/L
RT: 12.018 min Scan# 11
Delta R.T. 0.780 min
Lab File: VX044294.D
Acq: 13 Dec 2024 20:09

Instrument :
MSVOA_X
ClientSampleId :

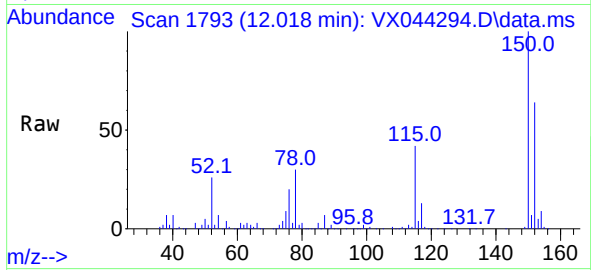

Tgt Ion: 75 Resp: 16691
Ion Ratio Lower Upper
75 100
77 34.2 25.8 38.6
110 4.1 33.3 49.9#

