




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044304.D
Acq On : 13 Dec 2024 23:58
Operator : JC/MD
Sample : P5153-05ME
Misc : 7.21g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E28P3ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/16/2024
Supervised By :Mahesh Dadoda 12/17/2024

Quant Time: Dec 14 00:30:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 03:56:15 2024
Response via : Initial Calibration

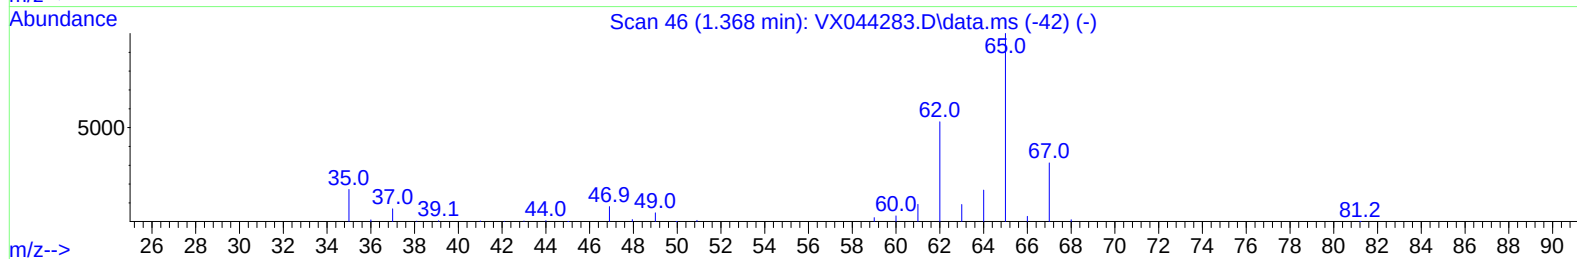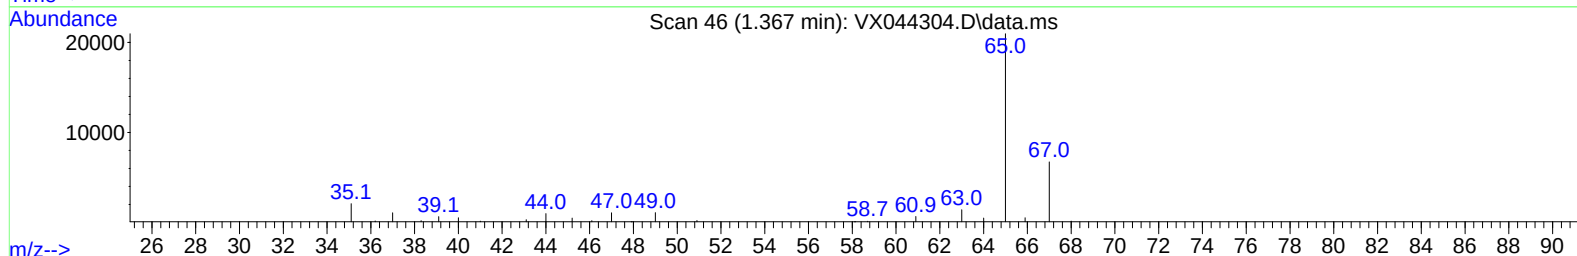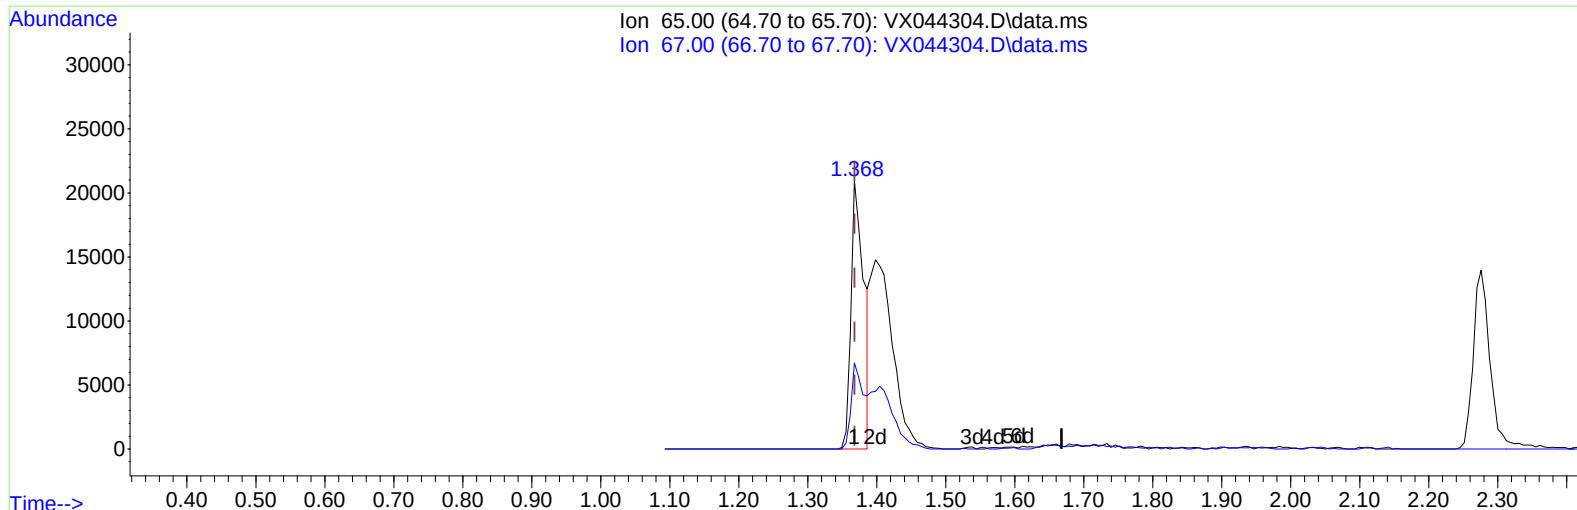

TIC: VX044304.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.367min (-0.000) 13.65 ug/L

response 27233

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	32.10	32.10
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044304.D
Acq On : 13 Dec 2024 23:58
Operator : JC/MD
Sample : P5153-05ME
Misc : 7.21g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E28P3ME

Manual IntegrationsAPPROVED

Quant Time: Dec 14 00:30:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 03:56:15 2024
Response via : Initial Calibration

Reviewed By :John Carlone 12/16/2024
Supervised By :Mahesh Dadoda 12/17/2024

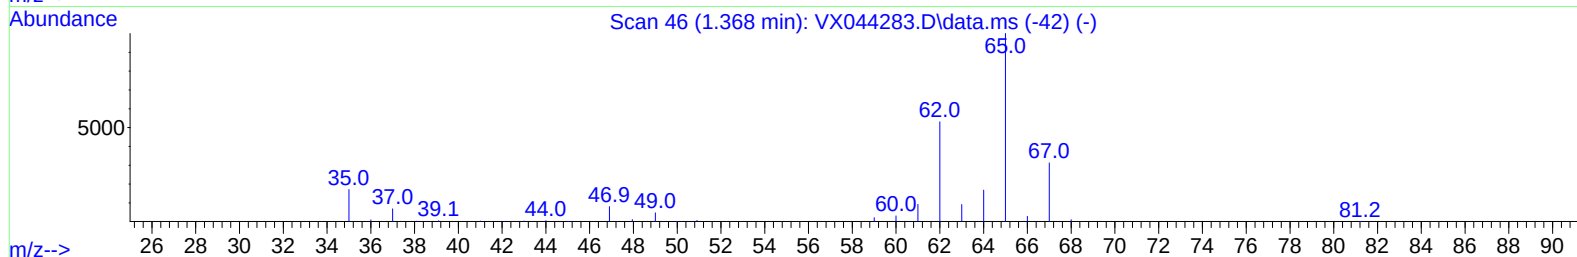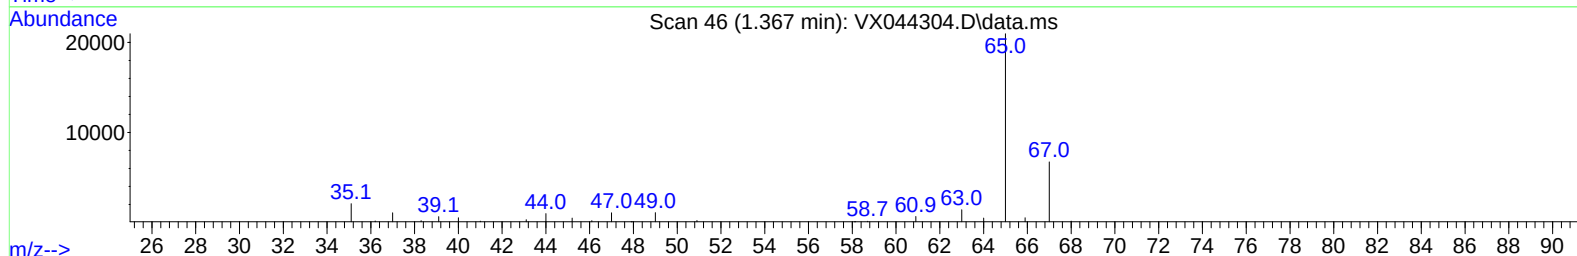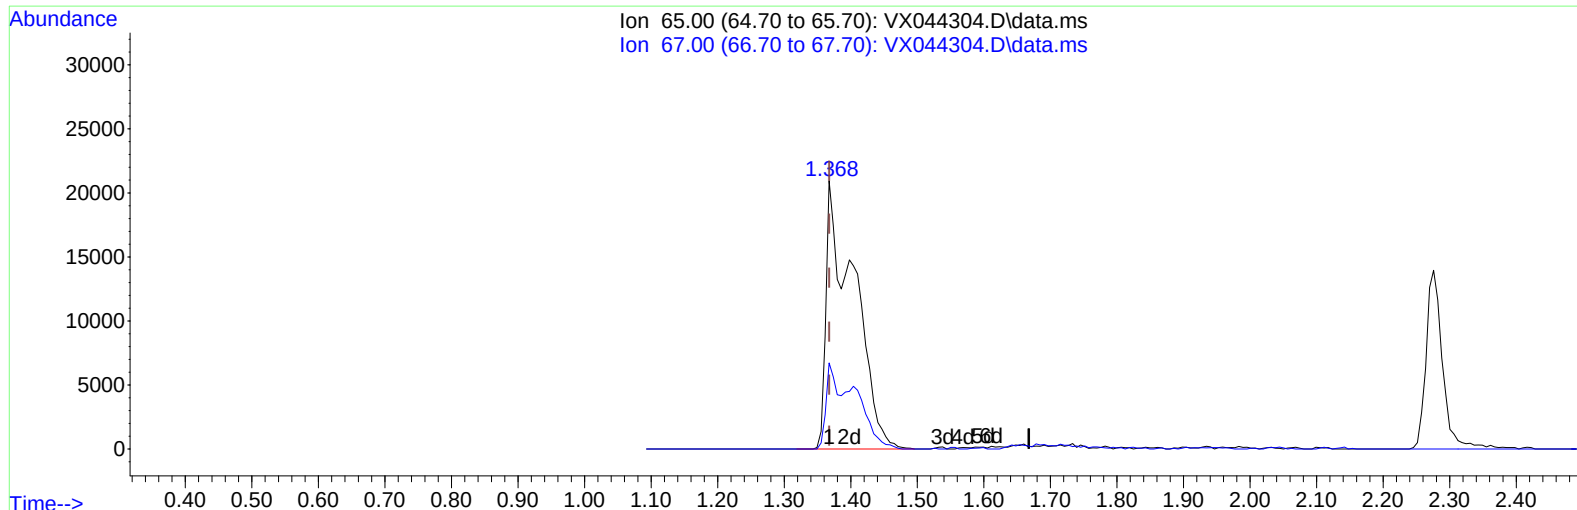

TIC: VX044304.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.367min (-0.000) 30.42 ug/L m

response 60704

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	32.10	14.40#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044304.D
Acq On : 13 Dec 2024 23:58
Operator : JC/MD
Sample : P5153-05ME
Misc : 7.21g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E28P3ME

Manual IntegrationsAPPROVED

Quant Time: Dec 14 00:30:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 03:56:15 2024
Response via : Initial Calibration

Reviewed By :John Carlone 12/16/2024
Supervised By :Mahesh Dadoda 12/17/2024

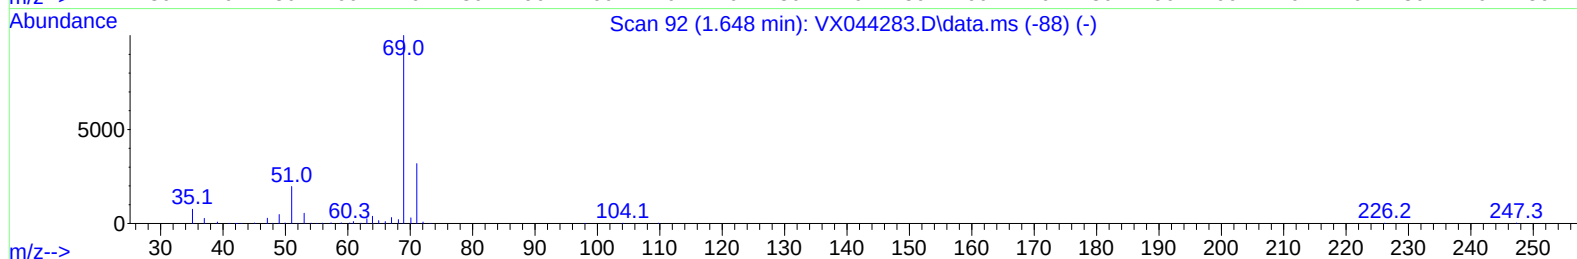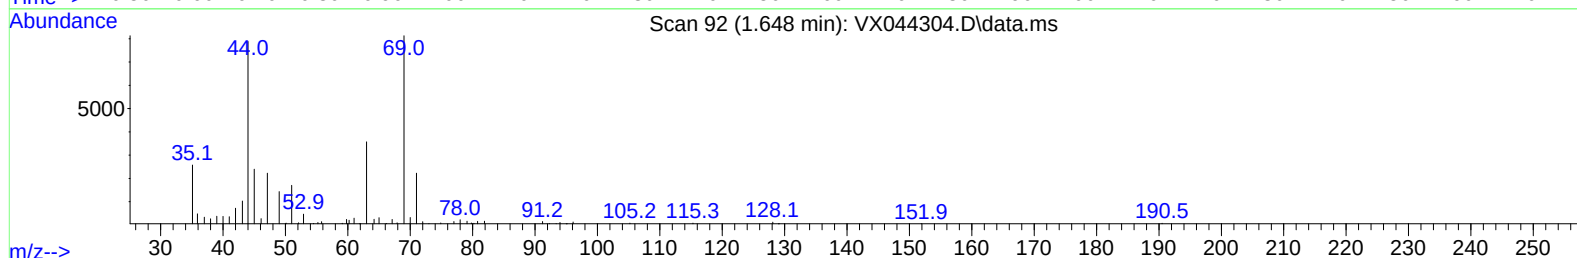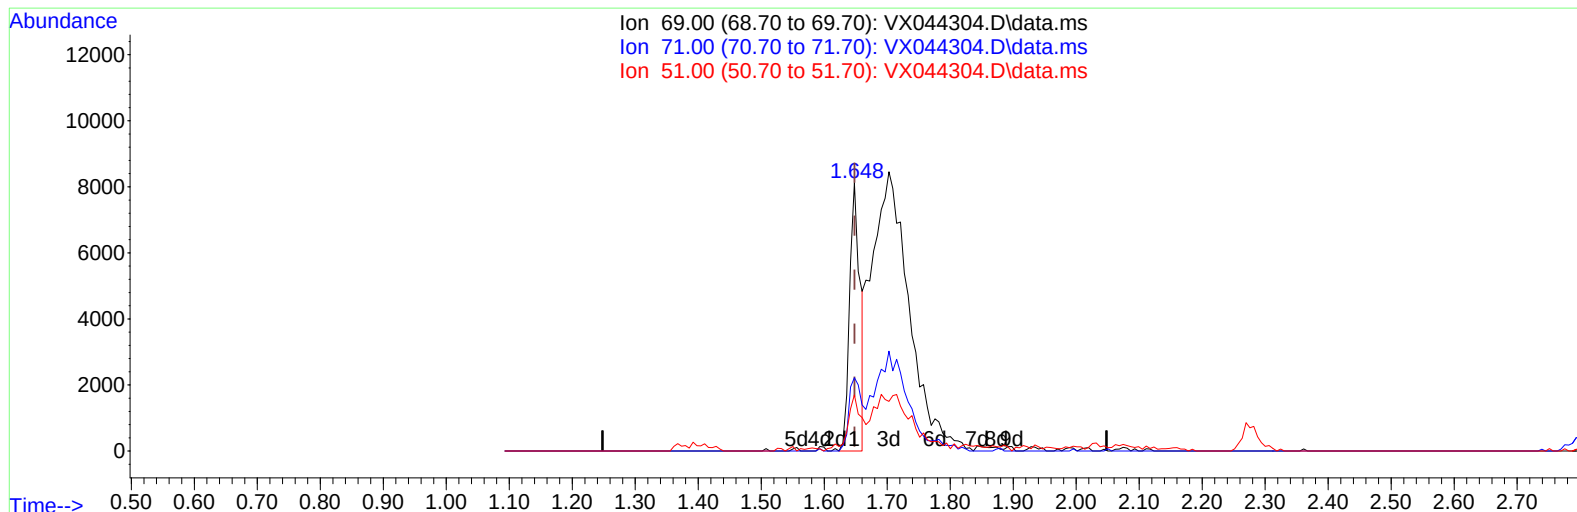

TIC: VX044304.D\data.ms

(7) Chloroethane-d5 (S)

1.648min (-0.000) 6.17 ug/L

response 9536

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	36.36
51.00	28.20	21.97
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044304.D
Acq On : 13 Dec 2024 23:58
Operator : JC/MD
Sample : P5153-05ME
Misc : 7.21g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E28P3ME

Manual IntegrationsAPPROVED

Quant Time: Dec 14 00:30:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 03:56:15 2024
Response via : Initial Calibration

Reviewed By :John Carlone 12/16/2024
Supervised By :Mahesh Dadoda 12/17/2024

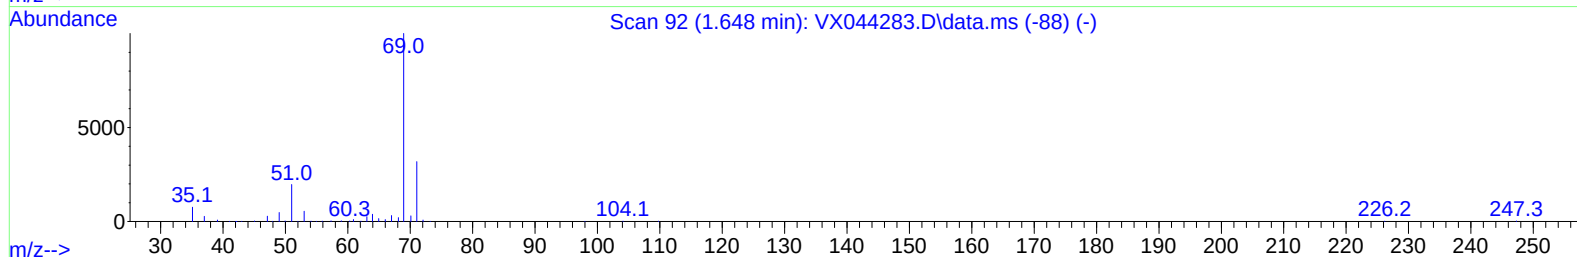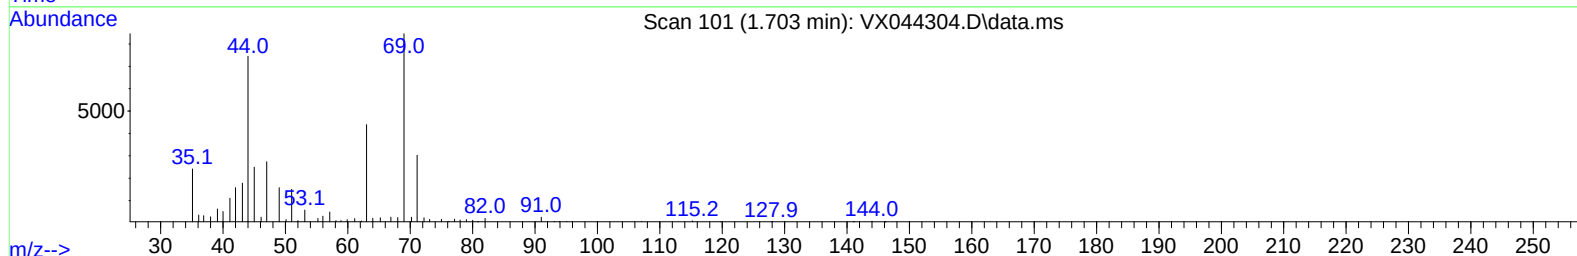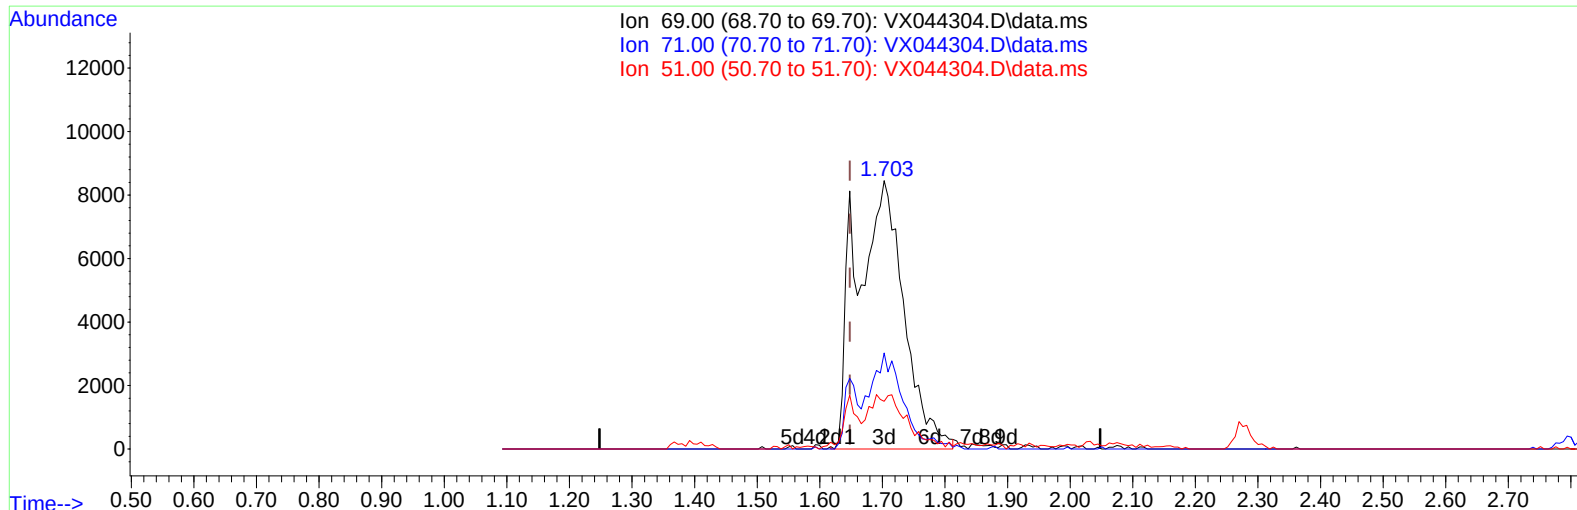

TIC: VX044304.D\data.ms

(7) Chloroethane-d5 (S)

1.703min (+ 0.055) 28.57 ug/L m

response 44156

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	7.85#
51.00	28.20	4.74#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044304.D
 Acq On : 13 Dec 2024 23:58
 Operator : JC/MD
 Sample : P5153-05ME
 Misc : 7.21g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E28P3ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/16/2024
 Supervised By :Mahesh Dadoda 12/17/2024

Quant Time: Dec 14 00:30:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 07 03:56:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.751	114	218051	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	193541	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	86067	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	60704m	30.422	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	60.840%	
7) Chloroethane-d5	1.703	69	44156m	28.566	ug/L	0.05
Spiked Amount	50.000	Range 70 - 130	Recovery	=	57.140%#	
11) 1,1-Dichloroethene-d2	2.276	65	23249	27.243	ug/L	-0.02
Spiked Amount	50.000	Range 60 - 125	Recovery	=	54.480%#	
21) 2-Butanone-d5	4.489	46	78918	64.597	ug/L	0.04
Spiked Amount	100.000	Range 40 - 130	Recovery	=	64.600%	
24) Chloroform-d	5.056	84	125890	33.228	ug/L	0.01
Spiked Amount	50.000	Range 70 - 125	Recovery	=	66.460%#	
26) 1,2-Dichloroethane-d4	5.946	65	91632	34.200	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	68.400%#	
32) Benzene-d6	5.964	84	242454	36.255	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	72.520%	
36) 1,2-Dichloropropane-d6	7.299	67	78320	37.717	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	75.440%	
41) Toluene-d8	8.647	98	215181	34.800	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	69.600%#	
43) trans-1,3-Dichloroprop...	8.951	79	28444	28.504	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	57.000%#	
47) 2-Hexanone-d5	9.390	63	55041	67.982	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	67.980%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	97008	34.840	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	69.680%	
66) 1,2-Dichlorobenzene-d4	12.317	152	79273	39.531	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	79.060%#	
Target Compounds						
					Qvalue	
35) Methylcyclohexane	7.366	83	7404	3.185	ug/L	90
42) Toluene	8.714	91	7098	1.140	ug/L	92
53) m,p-Xylene	10.299	106	4259	1.714	ug/L	88
54) o-Xylene	10.646	106	3710	1.452	ug/L	94
63) 1,2,4-Trimethylbenzene	11.756	105	6536	1.208	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044304.D
Acq On : 13 Dec 2024 23:58
Operator : JC/MD
Sample : P5153-05ME
Misc : 7.21g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E28P3ME

Manual IntegrationsAPPROVED

Quant Time: Dec 14 00:30:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 03:56:15 2024
Response via : Initial Calibration

Reviewed By :John Carlone 12/16/2024
Supervised By :Mahesh Dadoda 12/17/2024

