

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044269.D
 Acq On : 13 Dec 2024 10:12
 Operator : JC/MD
 Sample : VX1213WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK736

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044269.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	28	rBV2	3035	4648	0.50%	0.071%
2	1.368	43	46	61	rBV	107174	137804	14.93%	2.116%
3	1.599	69	84	85	rBV3	19479	69377	7.52%	1.065%
4	1.648	89	92	103	rVB	97653	144955	15.70%	2.225%
5	2.294	192	198	209	rBV	184392	287184	31.11%	4.409%
6	2.538	236	238	240	rBV2	466	494	0.05%	0.008%
7	2.562	240	242	246	rVB4	594	587	0.06%	0.009%
8	2.605	246	249	250	rBV3	465	481	0.05%	0.007%
9	2.623	250	252	257	rVB2	580	667	0.07%	0.010%
10	2.672	257	260	262	rBV2	638	806	0.09%	0.012%
11	2.782	274	278	283	rBV5	1391	1957	0.21%	0.030%
12	2.873	291	293	299	rBV3	502	794	0.09%	0.012%
13	2.940	300	304	307	rBV3	912	1496	0.16%	0.023%
14	3.038	317	320	321	rBV3	573	725	0.08%	0.011%
15	3.483	391	393	397	rBV3	646	671	0.07%	0.010%
16	3.751	436	437	440	rBV2	750	508	0.06%	0.008%
17	3.776	440	441	445	rBV2	635	569	0.06%	0.009%
18	3.867	452	456	461	rVB5	849	1463	0.16%	0.022%
19	3.922	461	465	466	rBV2	720	840	0.09%	0.013%
20	4.215	510	513	514	rBV	709	653	0.07%	0.010%
21	4.263	520	521	524	rBV3	535	554	0.06%	0.009%
22	4.294	524	526	530	rVB2	539	620	0.07%	0.010%
23	4.343	532	534	535	rBV2	721	482	0.05%	0.007%
24	4.458	544	553	569	rBV	56922	184333	19.97%	2.830%
25	4.715	593	595	597	rBV2	594	511	0.06%	0.008%
26	4.769	602	604	605	rBV	958	746	0.08%	0.011%
27	5.056	639	651	671	rVB	120247	394185	42.71%	6.052%
28	5.190	671	673	674	rBV	652	491	0.05%	0.008%
29	5.294	688	690	692	rBV2	765	831	0.09%	0.013%
30	5.958	788	799	819	rBV2	311811	922992	100.00%	14.171%
31	6.208	838	840	841	rBV2	769	438	0.05%	0.007%
32	6.354	860	864	867	rBV4	548	836	0.09%	0.013%
33	6.403	870	872	874	rVB2	600	531	0.06%	0.008%
34	6.440	876	878	880	rBV	454	426	0.05%	0.007%
35	6.647	910	912	914	rVB	507	434	0.05%	0.007%
36	6.751	921	929	942	rBV	196627	481526	52.17%	7.393%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044269.D
 Acq On : 13 Dec 2024 10:12
 Operator : JC/MD
 Sample : VX1213WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK736

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.123	983	990	994	rVV8	3302	7006	0.76%	0.108%
38	7.177	997	999	1004	rBV2	352	463	0.05%	0.007%
39	7.299	1011	1019	1033	rBV	184093	422996	45.83%	6.494%
40	7.519	1053	1055	1056	rBV2	572	427	0.05%	0.007%
41	7.629	1069	1073	1074	rBV2	631	939	0.10%	0.014%
42	7.812	1101	1103	1106	rBV2	817	693	0.08%	0.011%
43	7.897	1114	1117	1119	rVB2	833	732	0.08%	0.011%
44	7.921	1119	1121	1123	rBV2	478	518	0.06%	0.008%
45	8.007	1130	1135	1138	rBV4	299	531	0.06%	0.008%
46	8.122	1152	1154	1158	rBV3	501	668	0.07%	0.010%
47	8.275	1175	1179	1180	rVB2	581	664	0.07%	0.010%
48	8.324	1180	1187	1203	rBV	111227	196077	21.24%	3.010%
49	8.513	1216	1218	1219	rBV	672	481	0.05%	0.007%
50	8.574	1226	1228	1231	rBV2	661	776	0.08%	0.012%
51	8.641	1233	1239	1255	rBV	401210	669713	72.56%	10.282%
52	8.945	1285	1289	1300	rBV	83230	125945	13.65%	1.934%
53	9.177	1325	1327	1331	rVB3	639	609	0.07%	0.009%
54	9.384	1356	1361	1383	rBV	252735	385127	41.73%	5.913%
55	9.628	1399	1401	1403	rBV3	531	576	0.06%	0.009%
56	9.811	1426	1431	1432	rBV3	592	856	0.09%	0.013%
57	9.890	1442	1444	1446	rBV3	453	489	0.05%	0.008%
58	9.945	1452	1453	1456	rBV2	505	448	0.05%	0.007%
59	10.049	1465	1470	1485	rBV	404640	567049	61.44%	8.706%
60	10.335	1515	1517	1521	rBV3	620	803	0.09%	0.012%
61	10.720	1575	1580	1582	rBV4	556	824	0.09%	0.013%
62	10.835	1595	1599	1600	rBV	510	578	0.06%	0.009%
63	10.909	1610	1611	1614	rVB2	919	682	0.07%	0.010%
64	11.098	1639	1642	1644	rVV3	802	883	0.10%	0.014%
65	11.189	1652	1657	1669	rVB	341773	436671	47.31%	6.704%
66	11.512	1709	1710	1715	rVB3	626	828	0.09%	0.013%
67	11.555	1715	1717	1720	rBV3	656	919	0.10%	0.014%
68	11.933	1776	1779	1780	rBV3	404	485	0.05%	0.007%
69	11.975	1784	1786	1788	rBV	510	570	0.06%	0.009%
70	12.018	1788	1793	1805	rVV	382088	467655	50.67%	7.180%
71	12.262	1831	1833	1837	rBV3	374	562	0.06%	0.009%
72	12.317	1837	1842	1852	rBV	443376	550788	59.67%	8.456%
73	12.579	1882	1885	1886	rVV3	743	730	0.08%	0.011%
74	12.616	1889	1891	1893	rBV2	844	651	0.07%	0.010%
75	12.762	1913	1915	1918	rVB	1337	1037	0.11%	0.016%
76	13.280	1996	2000	2001	rBV2	501	553	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044269.D
 Acq On : 13 Dec 2024 10:12
 Operator : JC/MD
 Sample : VX1213WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK736

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.432	2022	2025	2027	rVB2	758	661	0.07%	0.010%
78	13.731	2072	2074	2076	rVB2	598	473	0.05%	0.007%
79	13.749	2076	2077	2081	rVB2	822	973	0.11%	0.015%
80	13.798	2081	2085	2086	rBV3	866	1176	0.13%	0.018%
81	13.902	2101	2102	2105	rVB2	923	744	0.08%	0.011%
82	13.957	2110	2111	2113	rBV2	633	436	0.05%	0.007%
83	14.127	2132	2139	2144	rBV3	1770	2909	0.32%	0.045%
84	14.182	2146	2148	2151	rBV3	443	501	0.05%	0.008%
85	14.396	2181	2183	2186	rBV2	836	931	0.10%	0.014%
86	14.487	2195	2198	2203	rBV4	484	883	0.10%	0.014%
87	14.585	2210	2214	2215	rBV2	495	435	0.05%	0.007%
88	14.603	2215	2217	2220	rBV4	395	523	0.06%	0.008%
89	14.658	2225	2226	2228	rBV2	624	473	0.05%	0.007%
90	14.725	2233	2237	2238	rBV3	433	545	0.06%	0.008%
91	14.822	2252	2253	2256	rBV2	436	480	0.05%	0.007%
92	14.871	2259	2261	2265	rVB3	595	524	0.06%	0.008%
93	15.072	2292	2294	2298	rVB3	541	639	0.07%	0.010%
94	15.164	2307	2309	2313	rBV2	519	749	0.08%	0.011%
95	15.652	2387	2389	2392	rVB4	894	726	0.08%	0.011%
96	15.865	2422	2424	2426	rBV3	601	456	0.05%	0.007%
97	16.048	2452	2454	2457	rVB3	850	923	0.10%	0.014%
98	16.182	2474	2476	2477	rBV2	703	511	0.06%	0.008%
99	16.493	2525	2527	2530	rBV3	756	508	0.06%	0.008%
100	16.700	2559	2561	2564	rBV2	723	663	0.07%	0.010%

Sum of corrected areas: 6513459




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044269.D
Acq On : 13 Dec 2024 10:12
Operator : JC/MD
Sample : VX1213WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK736

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

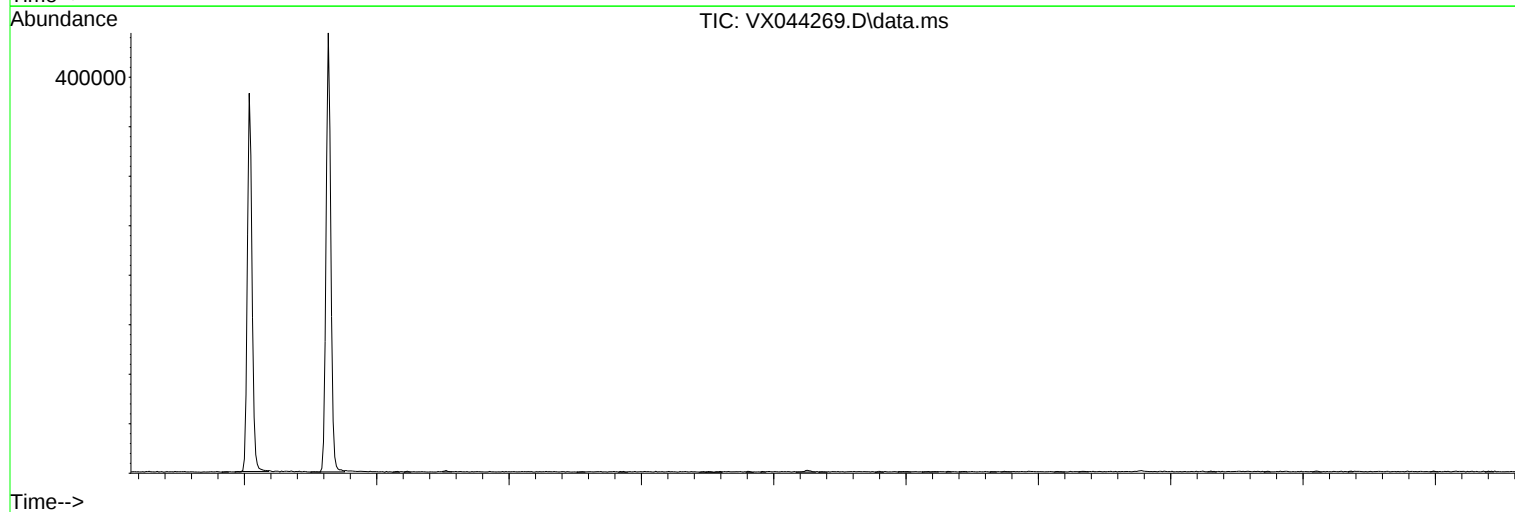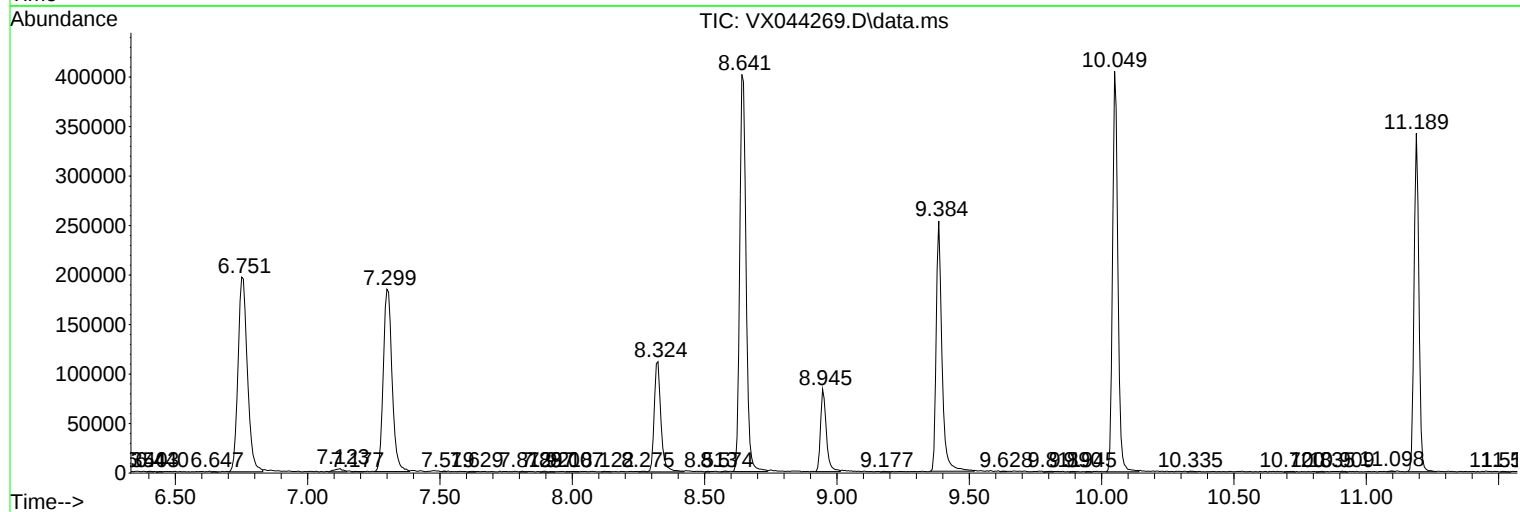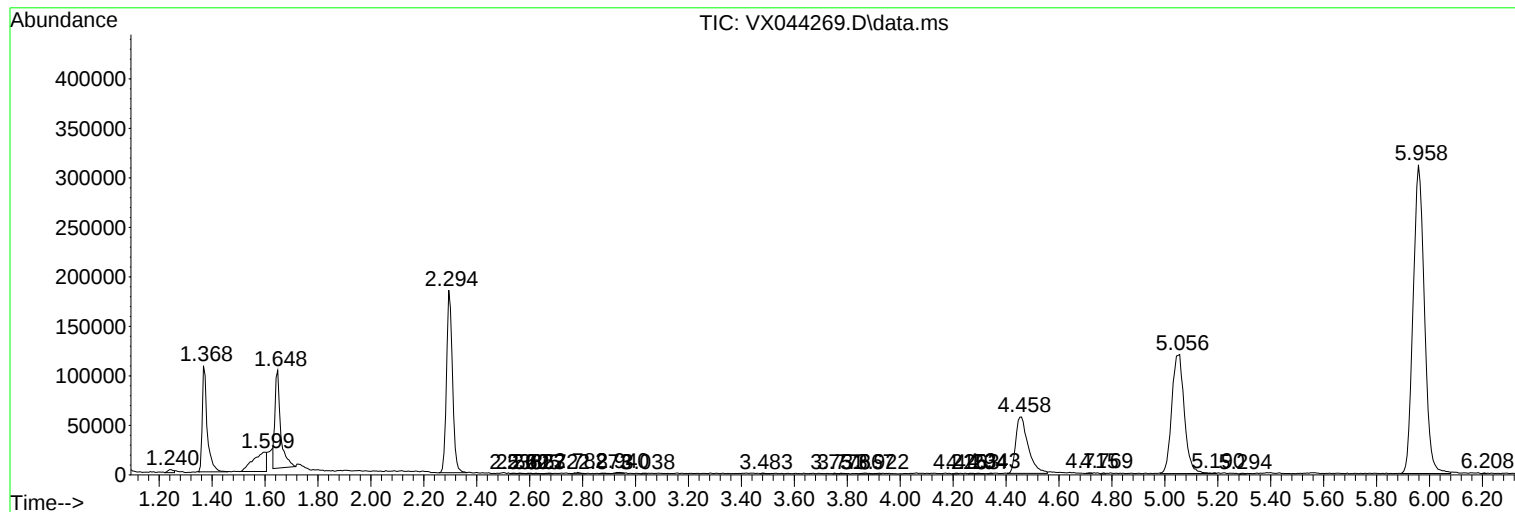

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044269.D
Acq On : 13 Dec 2024 10:12
Operator : JC/MD
Sample : VX1213WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK736

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044269.D
Acq On : 13 Dec 2024 10:12
Operator : JC/MD
Sample : VX1213WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK736

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc