

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044270.D
 Acq On : 13 Dec 2024 10:35
 Operator : JC/MD
 Sample : P5252-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044270.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rBV4	3513	6639	0.74%	0.104%
2	1.368	43	46	56	rVB	105829	128265	14.24%	2.001%
3	1.593	70	83	84	rBV5	17504	56791	6.30%	0.886%
4	1.648	89	92	102	rVB	99157	144074	15.99%	2.248%
5	2.300	192	199	208	rBV	175762	275777	30.61%	4.303%
6	2.380	209	212	217	rVB	5046	7703	0.86%	0.120%
7	2.770	274	276	278	rBV2	1196	1253	0.14%	0.020%
8	3.154	337	339	341	rBV3	615	532	0.06%	0.008%
9	3.233	349	352	354	rBV2	635	640	0.07%	0.010%
10	3.392	376	378	379	rVB	755	485	0.05%	0.008%
11	3.416	379	382	385	rBV3	642	1012	0.11%	0.016%
12	3.526	397	400	402	rBV2	477	651	0.07%	0.010%
13	3.648	417	420	421	rBV2	423	492	0.05%	0.008%
14	3.782	440	442	444	rBV2	547	485	0.05%	0.008%
15	3.916	463	464	466	rVV2	521	502	0.06%	0.008%
16	3.983	472	475	476	rBV	447	498	0.06%	0.008%
17	4.001	476	478	481	rVB2	600	564	0.06%	0.009%
18	4.117	494	497	500	rBV3	436	634	0.07%	0.010%
19	4.251	518	519	522	rVB2	556	524	0.06%	0.008%
20	4.331	530	532	534	rVB	828	497	0.06%	0.008%
21	4.361	534	537	540	rBV3	615	649	0.07%	0.010%
22	4.459	545	553	571	rBV	56872	179255	19.90%	2.797%
23	4.916	626	628	634	rBV4	541	1043	0.12%	0.016%
24	5.050	638	650	670	rVV	117754	380818	42.27%	5.941%
25	5.288	687	689	692	rVB3	732	662	0.07%	0.010%
26	5.404	704	708	709	rVB4	965	1048	0.12%	0.016%
27	5.501	722	724	727	rVB2	891	765	0.08%	0.012%
28	5.538	727	730	731	rBV2	689	768	0.09%	0.012%
29	5.721	757	760	763	rBV3	674	1101	0.12%	0.017%
30	5.958	788	799	817	rBV2	294676	900901	100.00%	14.055%
31	6.519	889	891	895	rVB3	618	521	0.06%	0.008%
32	6.647	910	912	917	rVB4	475	552	0.06%	0.009%
33	6.757	921	930	948	rVV	198437	485783	53.92%	7.579%
34	6.922	955	957	962	rVB4	615	869	0.10%	0.014%
35	6.970	964	965	967	rBV2	599	523	0.06%	0.008%
36	7.111	983	988	993	rBV6	3030	6292	0.70%	0.098%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044270.D
 Acq On : 13 Dec 2024 10:35
 Operator : JC/MD
 Sample : P5252-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.306	1011	1020	1032	rBV	185453	418437	46.45%	6.528%
38	7.434	1039	1041	1043	rBV3	656	517	0.06%	0.008%
39	7.830	1102	1106	1107	rBV3	462	604	0.07%	0.009%
40	7.897	1115	1117	1119	rBV	586	617	0.07%	0.010%
41	7.995	1131	1133	1137	rVB3	561	698	0.08%	0.011%
42	8.135	1154	1156	1159	rBV2	747	600	0.07%	0.009%
43	8.159	1159	1160	1166	rBV4	551	784	0.09%	0.012%
44	8.251	1172	1175	1179	rBV4	465	745	0.08%	0.012%
45	8.324	1181	1187	1202	rVV	112664	189694	21.06%	2.960%
46	8.531	1219	1221	1222	rBV2	838	612	0.07%	0.010%
47	8.647	1233	1240	1258	rBV	412261	670924	74.47%	10.467%
48	8.909	1280	1283	1284	rBV2	645	700	0.08%	0.011%
49	8.946	1284	1289	1298	rBV	76325	120150	13.34%	1.875%
50	9.269	1339	1342	1347	rVB5	1088	1907	0.21%	0.030%
51	9.385	1356	1361	1378	rBV	241816	379951	42.17%	5.928%
52	9.769	1420	1424	1425	rBV2	569	623	0.07%	0.010%
53	9.915	1447	1448	1451	rBV3	466	488	0.05%	0.008%
54	10.049	1465	1470	1489	rVB	398580	571077	63.39%	8.910%
55	10.336	1514	1517	1518	rBV2	494	475	0.05%	0.007%
56	10.476	1538	1540	1544	rBV3	408	637	0.07%	0.010%
57	10.518	1544	1547	1548	rVV2	553	537	0.06%	0.008%
58	10.531	1548	1549	1551	rVB2	801	570	0.06%	0.009%
59	10.787	1590	1591	1593	rBV2	738	634	0.07%	0.010%
60	10.860	1600	1603	1606	rVB3	681	1018	0.11%	0.016%
61	10.884	1606	1607	1609	rBV2	1028	836	0.09%	0.013%
62	10.976	1619	1622	1624	rVB2	576	540	0.06%	0.008%
63	11.006	1624	1627	1628	rBV2	485	490	0.05%	0.008%
64	11.189	1652	1657	1672	rBV	338591	430384	47.77%	6.715%
65	11.305	1672	1676	1679	rVB4	796	1128	0.13%	0.018%
66	11.384	1685	1689	1690	rBV4	665	566	0.06%	0.009%
67	11.537	1712	1714	1717	rVB2	544	535	0.06%	0.008%
68	11.610	1725	1726	1730	rVV2	664	891	0.10%	0.014%
69	11.768	1750	1752	1755	rBV2	518	523	0.06%	0.008%
70	12.018	1788	1793	1803	rBV	360517	458353	50.88%	7.151%
71	12.219	1821	1826	1833	rBV5	4527	8926	0.99%	0.139%
72	12.317	1837	1842	1852	rVV	430628	532157	59.07%	8.302%
73	12.561	1881	1882	1886	rVB3	730	591	0.07%	0.009%
74	12.835	1922	1927	1929	rBV3	1601	2172	0.24%	0.034%
75	12.945	1941	1945	1946	rBV	588	566	0.06%	0.009%
76	13.323	2006	2007	2010	rBV2	496	603	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044270.D
 Acq On : 13 Dec 2024 10:35
 Operator : JC/MD
 Sample : P5252-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.366	2012	2014	2017	rBV2	617	675	0.07%	0.011%
78	13.408	2019	2021	2024	rVB3	494	556	0.06%	0.009%
79	13.439	2024	2026	2029	rBV	552	609	0.07%	0.010%
80	13.481	2029	2033	2035	rBV4	911	1083	0.12%	0.017%
81	13.597	2050	2052	2059	rVV3	1195	1329	0.15%	0.021%
82	13.939	2106	2108	2110	rVV2	550	518	0.06%	0.008%
83	13.981	2114	2115	2118	rVV3	459	475	0.05%	0.007%
84	14.024	2120	2122	2123	rVV	741	481	0.05%	0.008%
85	14.085	2129	2132	2134	rBV2	744	670	0.07%	0.010%
86	14.292	2161	2166	2167	rBV2	594	740	0.08%	0.012%
87	14.335	2172	2173	2177	rBV3	512	805	0.09%	0.013%
88	14.469	2192	2195	2197	rBV3	782	841	0.09%	0.013%
89	14.579	2210	2213	2215	rBV3	416	530	0.06%	0.008%
90	14.609	2217	2218	2220	rBV	622	544	0.06%	0.008%
91	14.682	2229	2230	2233	rBV2	541	490	0.05%	0.008%
92	14.859	2255	2259	2260	rVV2	463	668	0.07%	0.010%
93	15.060	2289	2292	2294	rBV2	584	579	0.06%	0.009%
94	15.329	2333	2336	2340	rVB3	588	798	0.09%	0.012%
95	15.371	2340	2343	2344	rBV2	727	657	0.07%	0.010%
96	15.390	2344	2346	2352	rVB4	1027	1184	0.13%	0.018%
97	15.713	2397	2399	2403	rVB3	794	738	0.08%	0.012%
98	16.188	2476	2477	2482	rBV4	643	922	0.10%	0.014%
99	16.292	2491	2494	2495	rBV2	521	594	0.07%	0.009%
100	16.566	2538	2539	2542	rBV3	1215	1342	0.15%	0.021%




Sum of corrected areas: 6409656

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044270.D
Acq On : 13 Dec 2024 10:35
Operator : JC/MD
Sample : P5252-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

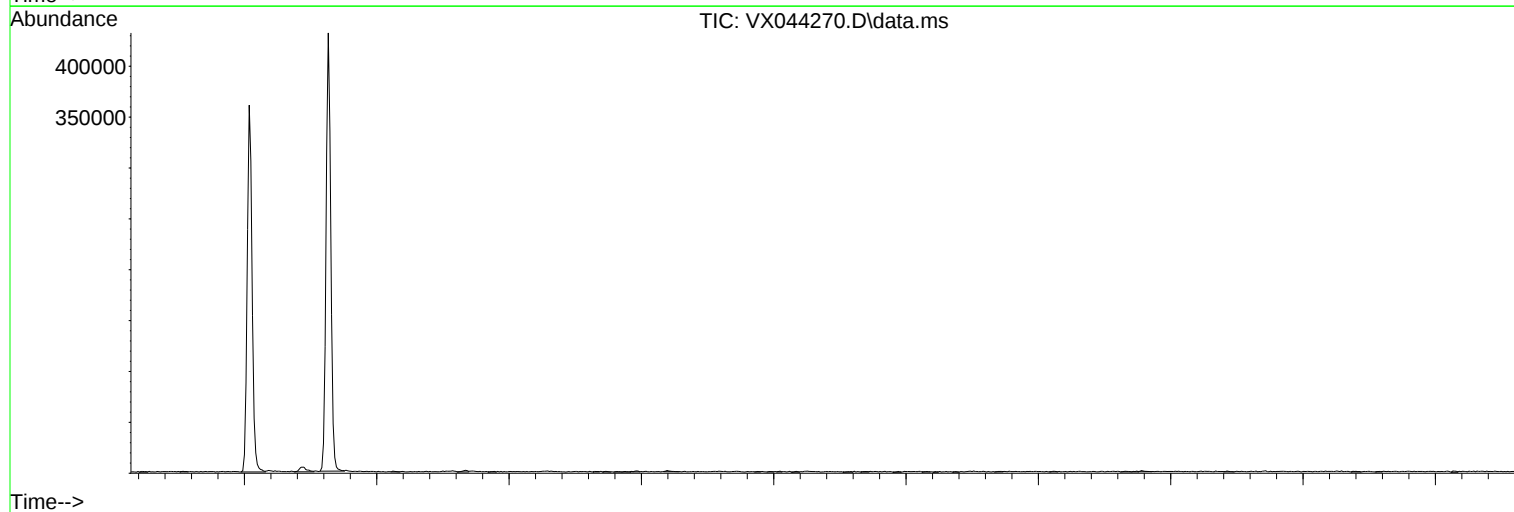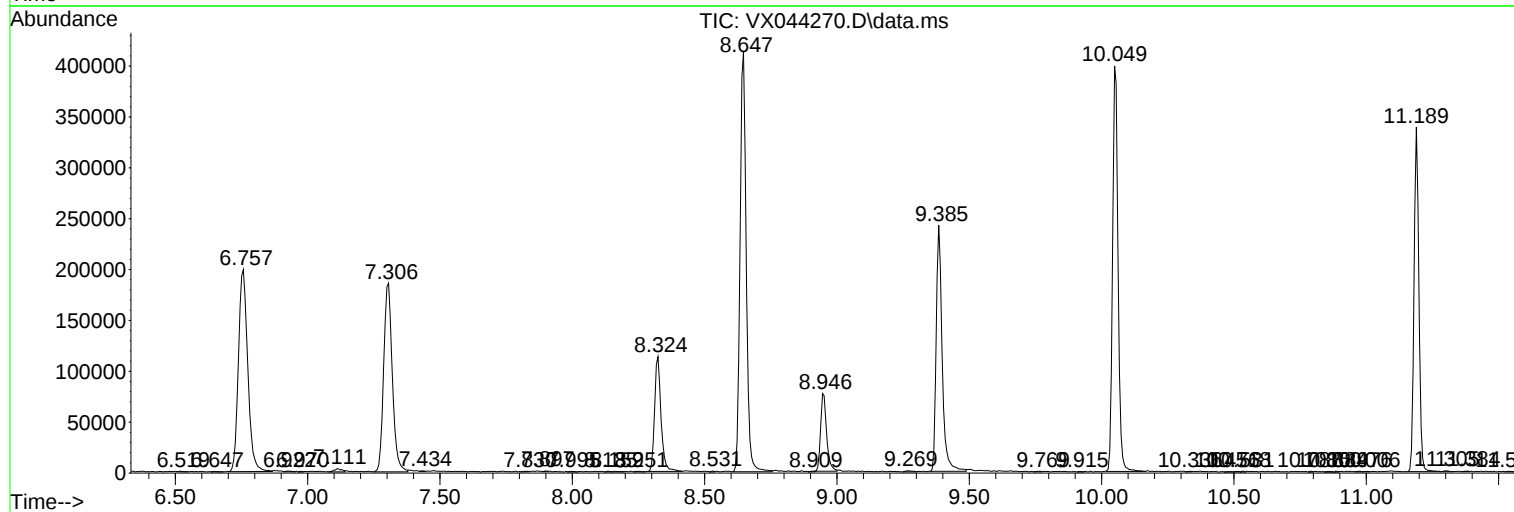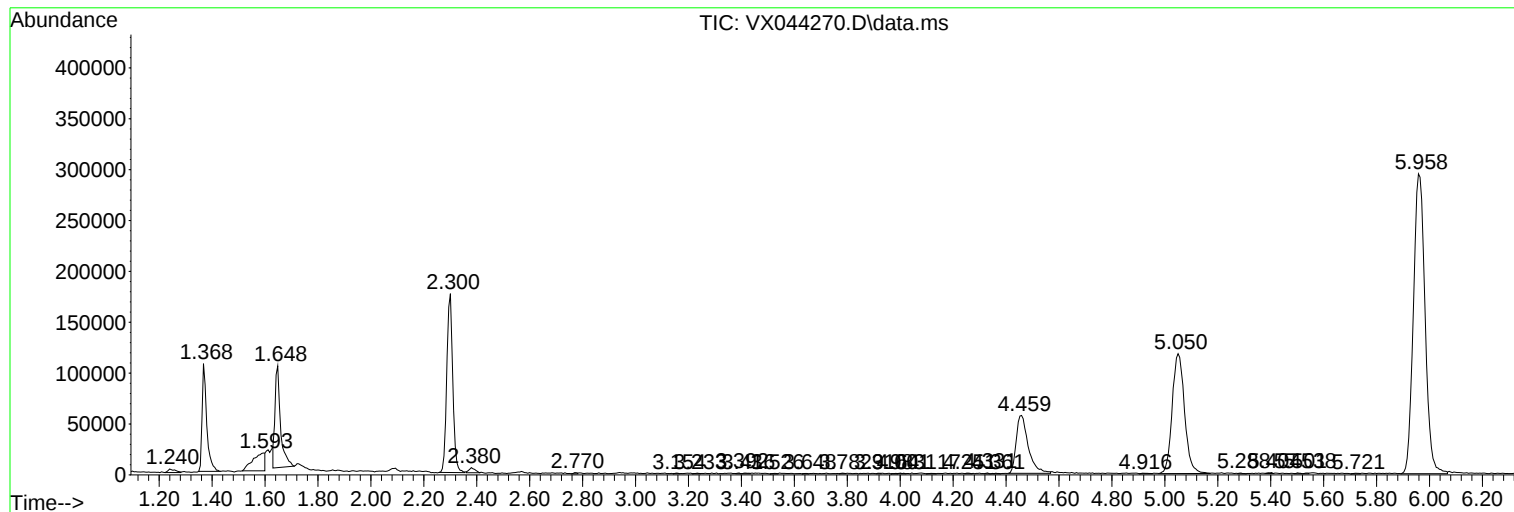

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044270.D
Acq On : 13 Dec 2024 10:35
Operator : JC/MD
Sample : P5252-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044270.D
Acq On : 13 Dec 2024 10:35
Operator : JC/MD
Sample : P5252-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc