

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044272.D
 Acq On : 13 Dec 2024 11:21
 Operator : JC/MD
 Sample : P5252-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044272.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	23	25	27	rBV	3121	2963	0.30%	0.041%
2	1.368	43	46	57	rVB	114593	139251	14.19%	1.946%
3	1.648	89	92	102	rVB	106213	146404	14.92%	2.045%
4	2.300	192	199	207	rBV	190079	297098	30.28%	4.151%
5	2.617	247	251	253	rBV4	584	806	0.08%	0.011%
6	2.715	262	267	269	rBV4	529	843	0.09%	0.012%
7	2.776	271	277	278	rBV4	975	1795	0.18%	0.025%
8	2.928	300	302	305	rVB2	641	435	0.04%	0.006%
9	3.087	326	328	333	rBV3	642	814	0.08%	0.011%
10	3.428	382	384	389	rVB4	1064	908	0.09%	0.013%
11	3.495	394	395	398	rVB2	607	484	0.05%	0.007%
12	3.599	408	412	415	rBV4	983	1577	0.16%	0.022%
13	3.684	423	426	428	rVB3	631	633	0.06%	0.009%
14	3.721	428	432	433	rBV2	308	458	0.05%	0.006%
15	3.794	443	444	447	rBV3	603	718	0.07%	0.010%
16	3.959	469	471	473	rBV3	577	699	0.07%	0.010%
17	4.020	478	481	486	rBV5	640	1332	0.14%	0.019%
18	4.117	495	497	500	rVB3	549	514	0.05%	0.007%
19	4.282	522	524	527	rVB3	621	593	0.06%	0.008%
20	4.306	527	528	532	rBV2	652	575	0.06%	0.008%
21	4.459	545	553	569	rBV	58038	185179	18.88%	2.587%
22	5.056	638	651	668	rBV	138064	428448	43.67%	5.986%
23	5.227	677	679	680	rBV2	842	527	0.05%	0.007%
24	5.525	726	728	730	rBV3	518	487	0.05%	0.007%
25	5.964	788	800	816	rBV2	326642	981044	100.00%	13.706%
26	6.348	861	863	864	rBV	920	616	0.06%	0.009%
27	6.446	878	879	882	rBV2	511	565	0.06%	0.008%
28	6.556	894	897	900	rBV3	832	1126	0.11%	0.016%
29	6.617	905	907	910	rVB2	554	447	0.05%	0.006%
30	6.751	920	929	944	rBV	209746	513120	52.30%	7.169%
31	7.123	982	990	1003	rBV	164467	358786	36.57%	5.013%
32	7.306	1012	1020	1041	rBV	204770	457765	46.66%	6.396%
33	7.489	1048	1050	1051	rBV2	749	478	0.05%	0.007%
34	7.671	1078	1080	1081	rVB	711	482	0.05%	0.007%
35	7.684	1081	1082	1084	rBV	494	487	0.05%	0.007%
36	7.720	1087	1088	1092	rVB3	830	790	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044272.D
 Acq On : 13 Dec 2024 11:21
 Operator : JC/MD
 Sample : P5252-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.775	1096	1097	1100	rBV3	488	504	0.05%	0.007%
38	7.824	1102	1105	1108	rBV4	489	715	0.07%	0.010%
39	7.982	1127	1131	1134	rVV3	650	770	0.08%	0.011%
40	8.062	1142	1144	1146	rBV2	440	479	0.05%	0.007%
41	8.080	1146	1147	1149	rBV	539	449	0.05%	0.006%
42	8.324	1179	1187	1200	rBV	119960	209465	21.35%	2.926%
43	8.647	1233	1240	1259	rBV	435657	710799	72.45%	9.931%
44	8.946	1284	1289	1301	rBV	81662	132795	13.54%	1.855%
45	9.269	1337	1342	1349	rVV3	24729	40061	4.08%	0.560%
46	9.385	1356	1361	1373	rBV	255365	389120	39.66%	5.437%
47	9.775	1423	1425	1427	rBV2	595	489	0.05%	0.007%
48	9.823	1431	1433	1435	rVB3	626	557	0.06%	0.008%
49	9.933	1447	1451	1453	rVB3	553	649	0.07%	0.009%
50	9.994	1458	1461	1463	rBV3	702	974	0.10%	0.014%
51	10.049	1465	1470	1485	rBV	406414	595277	60.68%	8.317%
52	10.189	1491	1493	1499	rBV4	1747	2880	0.29%	0.040%
53	10.275	1503	1507	1508	rVB2	687	560	0.06%	0.008%
54	10.305	1508	1512	1514	rBV3	1256	1741	0.18%	0.024%
55	10.640	1565	1567	1570	rBV3	1419	1904	0.19%	0.027%
56	10.970	1617	1621	1627	rVB4	1501	2556	0.26%	0.036%
57	11.067	1635	1637	1639	rBV2	664	557	0.06%	0.008%
58	11.189	1651	1657	1669	rBV	367205	463293	47.22%	6.473%
59	11.409	1691	1693	1694	rBV2	534	441	0.04%	0.006%
60	11.457	1699	1701	1703	rVV3	1265	1305	0.13%	0.018%
61	11.500	1706	1708	1710	rBV3	527	516	0.05%	0.007%
62	11.561	1716	1718	1721	rBV3	459	615	0.06%	0.009%
63	11.658	1731	1734	1737	rBV3	428	513	0.05%	0.007%
64	11.750	1746	1749	1755	rBV3	1487	2191	0.22%	0.031%
65	11.829	1760	1762	1765	rBV2	754	645	0.07%	0.009%
66	11.975	1782	1786	1788	rBV4	1045	1418	0.14%	0.020%
67	12.018	1788	1793	1804	rVV	375516	474799	48.40%	6.634%
68	12.152	1813	1815	1819	rVB3	705	689	0.07%	0.010%
69	12.317	1836	1842	1849	rBV	448002	565622	57.66%	7.902%
70	12.427	1858	1860	1867	rBV5	617	1031	0.11%	0.014%
71	12.792	1918	1920	1923	rVB3	636	537	0.05%	0.008%
72	12.829	1925	1926	1927	rBV	741	434	0.04%	0.006%
73	12.847	1927	1929	1932	rVB	636	524	0.05%	0.007%
74	12.994	1951	1953	1957	rBV4	601	1096	0.11%	0.015%
75	13.085	1966	1968	1970	rVV2	505	492	0.05%	0.007%
76	13.122	1970	1974	1977	rVV4	725	1237	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044272.D
 Acq On : 13 Dec 2024 11:21
 Operator : JC/MD
 Sample : P5252-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.298	2001	2003	2007	rBV3	553	766	0.08%	0.011%
78	13.451	2025	2028	2029	rBV	727	618	0.06%	0.009%
79	13.536	2040	2042	2045	rBV	599	701	0.07%	0.010%
80	13.731	2072	2074	2076	rBV2	515	488	0.05%	0.007%
81	13.926	2104	2106	2108	rVB3	627	516	0.05%	0.007%
82	14.128	2135	2139	2142	rBV2	1155	1870	0.19%	0.026%
83	14.445	2189	2191	2194	rVB2	852	820	0.08%	0.011%
84	14.536	2205	2206	2209	rBV2	570	488	0.05%	0.007%
85	14.579	2212	2213	2216	rBV2	718	609	0.06%	0.009%
86	14.701	2232	2233	2236	rBV2	448	461	0.05%	0.006%
87	14.859	2254	2259	2260	rBV3	674	931	0.09%	0.013%
88	14.884	2260	2263	2264	rBV2	675	529	0.05%	0.007%
89	15.079	2293	2295	2297	rBV2	745	677	0.07%	0.009%
90	15.121	2300	2302	2303	rBV2	750	659	0.07%	0.009%
91	15.359	2337	2341	2342	rBV3	644	944	0.10%	0.013%
92	15.487	2360	2362	2366	rVB3	772	630	0.06%	0.009%
93	15.621	2379	2384	2387	rBV4	503	973	0.10%	0.014%
94	15.652	2387	2389	2392	rVB2	637	598	0.06%	0.008%
95	15.737	2402	2403	2405	rBV2	599	493	0.05%	0.007%
96	15.804	2412	2414	2416	rBV3	601	522	0.05%	0.007%
97	16.005	2444	2447	2450	rBV4	515	609	0.06%	0.009%
98	16.066	2453	2457	2462	rBV6	670	1670	0.17%	0.023%
99	16.188	2475	2477	2479	rBV3	787	590	0.06%	0.008%
100	16.402	2510	2512	2513	rBV	903	431	0.04%	0.006%

Sum of corrected areas: 7157539




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044272.D
Acq On : 13 Dec 2024 11:21
Operator : JC/MD
Sample : P5252-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

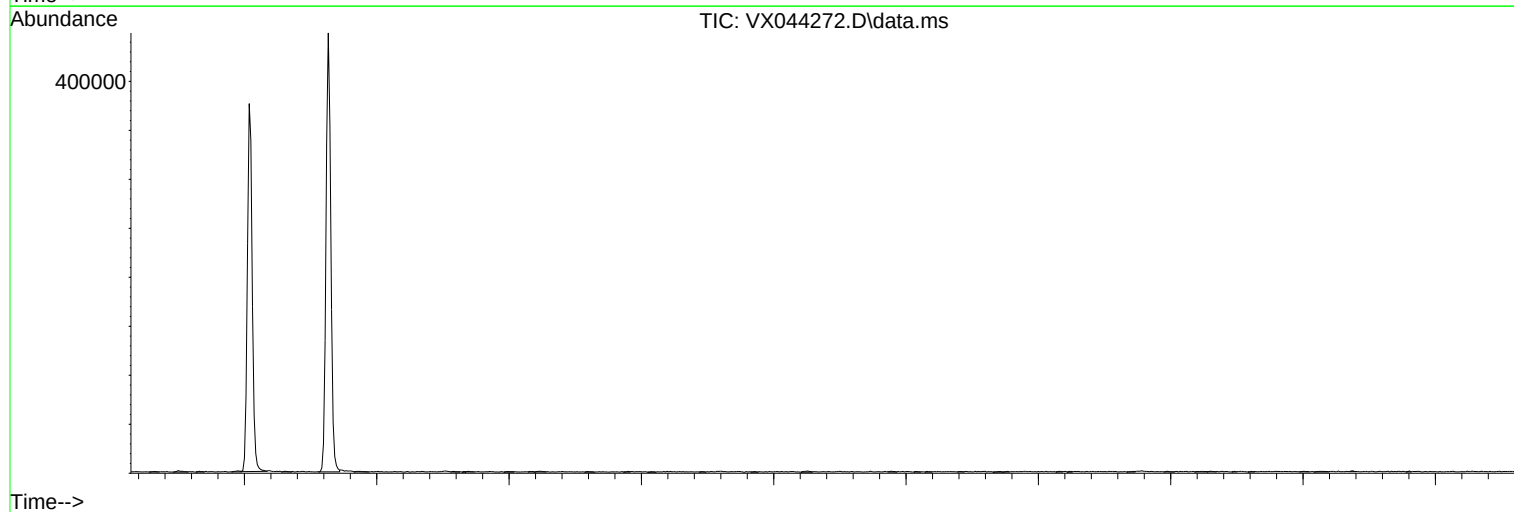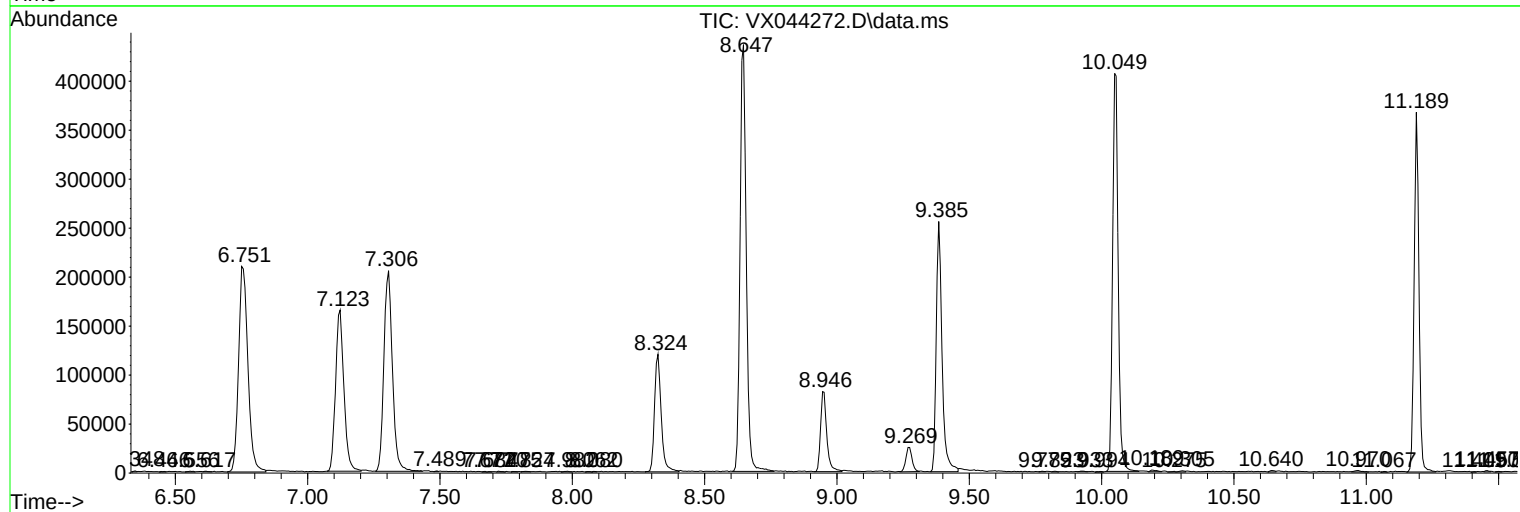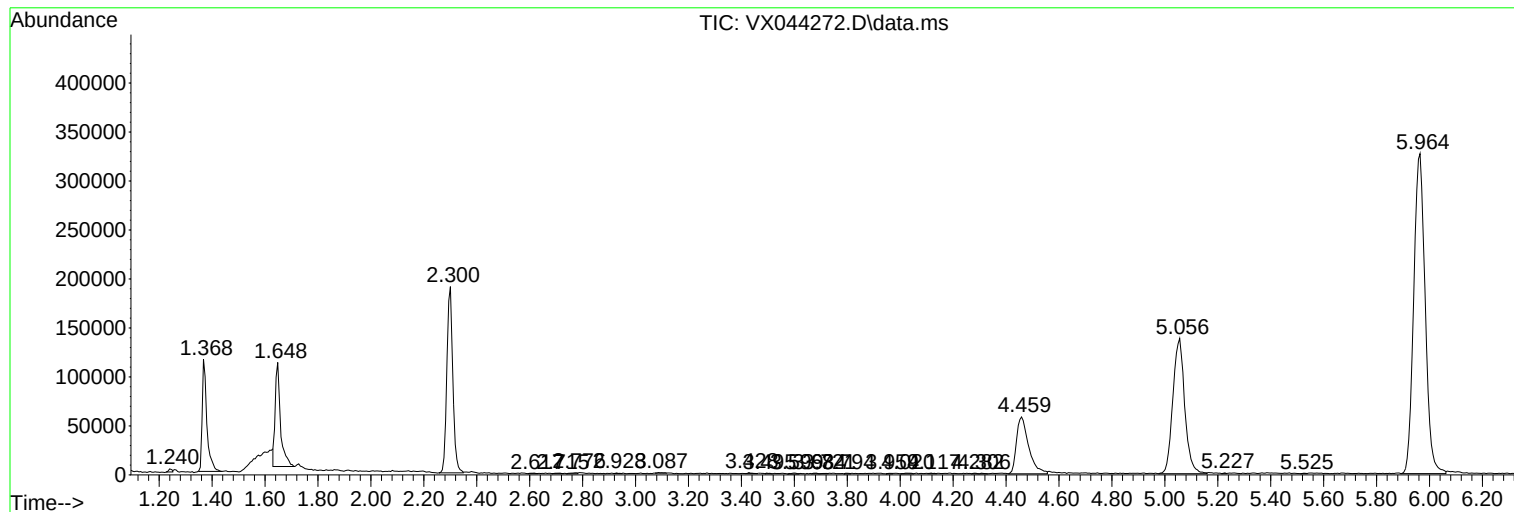

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044272.D
Acq On : 13 Dec 2024 11:21
Operator : JC/MD
Sample : P5252-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044272.D
Acq On : 13 Dec 2024 11:21
Operator : JC/MD
Sample : P5252-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
