

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044273.D
 Acq On : 13 Dec 2024 11:43
 Operator : JC/MD
 Sample : P5252-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044273.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	23	25	33	rVB3	2972	4973	0.49%	0.066%
2	1.368	42	46	57	rVB	144263	147184	14.58%	1.968%
3	1.593	70	83	84	rBV2	18411	57985	5.74%	0.775%
4	1.654	89	93	100	rBV	108367	136256	13.50%	1.822%
5	2.300	193	199	209	rBV2	204190	360955	35.76%	4.826%
6	2.550	234	240	245	rBV4	3440	7263	0.72%	0.097%
7	2.733	268	270	271	rBV2	615	500	0.05%	0.007%
8	2.843	286	288	291	rVB3	656	528	0.05%	0.007%
9	2.873	291	293	295	rBV2	495	530	0.05%	0.007%
10	3.111	331	332	335	rVB3	702	464	0.05%	0.006%
11	3.142	335	337	342	rVB3	587	532	0.05%	0.007%
12	3.184	342	344	345	rBV2	593	458	0.05%	0.006%
13	3.276	358	359	361	rBV	718	466	0.05%	0.006%
14	3.440	381	386	387	rBV3	570	837	0.08%	0.011%
15	3.538	397	402	404	rBV3	726	769	0.08%	0.010%
16	3.806	443	446	448	rBV2	560	725	0.07%	0.010%
17	3.867	453	456	457	rBV	501	478	0.05%	0.006%
18	4.099	492	494	496	rVB2	838	622	0.06%	0.008%
19	4.123	496	498	500	rBV2	640	780	0.08%	0.010%
20	4.172	505	506	510	rVV2	670	614	0.06%	0.008%
21	4.361	534	537	541	rVB3	684	804	0.08%	0.011%
22	4.452	541	552	569	rBV	67389	201153	19.93%	2.689%
23	4.757	600	602	606	rBV2	479	512	0.05%	0.007%
24	4.806	608	610	612	rBV2	536	612	0.06%	0.008%
25	5.050	640	650	668	rBV	133063	429853	42.58%	5.747%
26	5.208	674	676	679	rVB2	860	729	0.07%	0.010%
27	5.276	685	687	689	rBV3	533	453	0.04%	0.006%
28	5.367	700	702	703	rBV	766	720	0.07%	0.010%
29	5.416	708	710	713	rVV3	864	915	0.09%	0.012%
30	5.538	728	730	731	rBV	607	478	0.05%	0.006%
31	5.696	754	756	759	rVB4	736	944	0.09%	0.013%
32	5.830	774	778	781	rVB2	657	1010	0.10%	0.014%
33	5.861	781	783	784	rBV2	457	475	0.05%	0.006%
34	5.964	788	800	815	rBV2	333123	1009455	100.00%	13.496%
35	6.556	895	897	899	rVB2	797	655	0.06%	0.009%
36	6.659	910	914	915	rBV2	532	522	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044273.D
Acq On : 13 Dec 2024 11:43
Operator : JC/MD
Sample : P5252-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Title : VOC Analysis

37	6.757	921	930	945	rBV	237605	573645	56.83%	7.669%
38	7.123	983	990	1003	rBV	77452	174363	17.27%	2.331%
39	7.300	1011	1019	1038	rBV	210325	471331	46.69%	6.301%
40	7.476	1046	1048	1050	rBV3	987	1174	0.12%	0.016%
41	7.580	1064	1065	1067	rBV	535	534	0.05%	0.007%
42	8.098	1148	1150	1153	rVB2	756	714	0.07%	0.010%
43	8.324	1181	1187	1201	rVV	134779	219095	21.70%	2.929%
44	8.574	1227	1228	1232	rBV3	494	489	0.05%	0.007%
45	8.647	1234	1240	1256	rVV	472230	753049	74.60%	10.068%
46	8.909	1280	1283	1284	rBV3	533	599	0.06%	0.008%
47	8.946	1284	1289	1299	rVV2	88393	138004	13.67%	1.845%
48	9.177	1326	1327	1332	rVB2	868	646	0.06%	0.009%
49	9.275	1339	1343	1348	rVB4	1851	2958	0.29%	0.040%
50	9.385	1356	1361	1378	rBV	284978	423746	41.98%	5.665%
51	9.671	1406	1408	1410	rBV2	641	548	0.05%	0.007%
52	9.805	1429	1430	1432	rBV2	783	585	0.06%	0.008%
53	9.970	1456	1457	1461	rVB3	501	551	0.05%	0.007%
54	10.049	1465	1470	1484	rVV	495628	691121	68.46%	9.240%
55	10.549	1550	1552	1553	rBV	700	486	0.05%	0.006%
56	10.683	1572	1574	1577	rVV3	663	802	0.08%	0.011%
57	10.781	1588	1590	1595	rVB2	737	744	0.07%	0.010%
58	10.835	1595	1599	1600	rBV3	729	782	0.08%	0.010%
59	10.964	1619	1620	1623	rVB2	875	612	0.06%	0.008%
60	11.012	1623	1628	1629	rBV3	569	810	0.08%	0.011%
61	11.189	1651	1657	1670	rVV	364771	469236	46.48%	6.273%
62	11.604	1723	1725	1728	rBV2	639	506	0.05%	0.007%
63	11.701	1740	1741	1746	rVB2	841	1010	0.10%	0.014%
64	11.896	1769	1773	1774	rVB3	685	645	0.06%	0.009%
65	11.915	1774	1776	1777	rBV2	655	475	0.05%	0.006%
66	12.018	1788	1793	1802	rBV	438285	550157	54.50%	7.355%
67	12.219	1822	1826	1831	rBV3	3029	4130	0.41%	0.055%
68	12.317	1837	1842	1850	rBV	477975	602447	59.68%	8.054%
69	12.524	1874	1876	1879	rBV2	625	663	0.07%	0.009%
70	12.610	1887	1890	1893	rBV2	751	687	0.07%	0.009%
71	12.713	1905	1907	1910	rBV2	590	556	0.06%	0.007%
72	12.902	1936	1938	1939	rVB2	836	470	0.05%	0.006%
73	13.036	1958	1960	1963	rBV3	530	477	0.05%	0.006%
74	13.402	2018	2020	2024	rVB3	531	692	0.07%	0.009%
75	13.433	2024	2025	2029	rBV2	451	495	0.05%	0.007%
76	13.494	2033	2035	2038	rVB3	487	494	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044273.D
 Acq On : 13 Dec 2024 11:43
 Operator : JC/MD
 Sample : P5252-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.555	2043	2045	2047	rBV3	408	449	0.04%	0.006%
78	13.683	2062	2066	2068	rBV3	555	473	0.05%	0.006%
79	13.707	2068	2070	2074	rVB3	676	646	0.06%	0.009%
80	13.841	2088	2092	2094	rBV3	550	640	0.06%	0.009%
81	14.030	2119	2123	2124	rVB2	538	479	0.05%	0.006%
82	14.121	2136	2138	2146	rVB4	804	1357	0.13%	0.018%
83	14.189	2146	2149	2151	rBV3	562	507	0.05%	0.007%
84	14.262	2160	2161	2164	rBV	640	673	0.07%	0.009%
85	14.329	2170	2172	2175	rBV3	519	489	0.05%	0.007%
86	14.451	2191	2192	2196	rVB3	619	764	0.08%	0.010%
87	14.506	2199	2201	2207	rVB3	683	638	0.06%	0.009%
88	14.554	2207	2209	2212	rBV2	623	853	0.08%	0.011%
89	14.713	2233	2235	2238	rBV2	369	469	0.05%	0.006%
90	14.951	2273	2274	2277	rVB2	764	508	0.05%	0.007%
91	15.243	2320	2322	2324	rVB3	534	513	0.05%	0.007%
92	15.286	2327	2329	2334	rVB3	960	1315	0.13%	0.018%
93	15.329	2334	2336	2337	rBV2	1076	888	0.09%	0.012%
94	15.591	2376	2379	2380	rVB3	690	571	0.06%	0.008%
95	15.627	2383	2385	2387	rVB2	704	479	0.05%	0.006%
96	15.688	2392	2395	2398	rVV4	744	893	0.09%	0.012%
97	16.091	2457	2461	2462	rBV2	742	1067	0.11%	0.014%
98	16.395	2508	2511	2513	rBV3	689	1014	0.10%	0.014%
99	16.505	2528	2529	2531	rVB	805	447	0.04%	0.006%
100	16.536	2531	2534	2535	rBV2	821	802	0.08%	0.011%

Sum of corrected areas: 7479671




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044273.D
Acq On : 13 Dec 2024 11:43
Operator : JC/MD
Sample : P5252-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

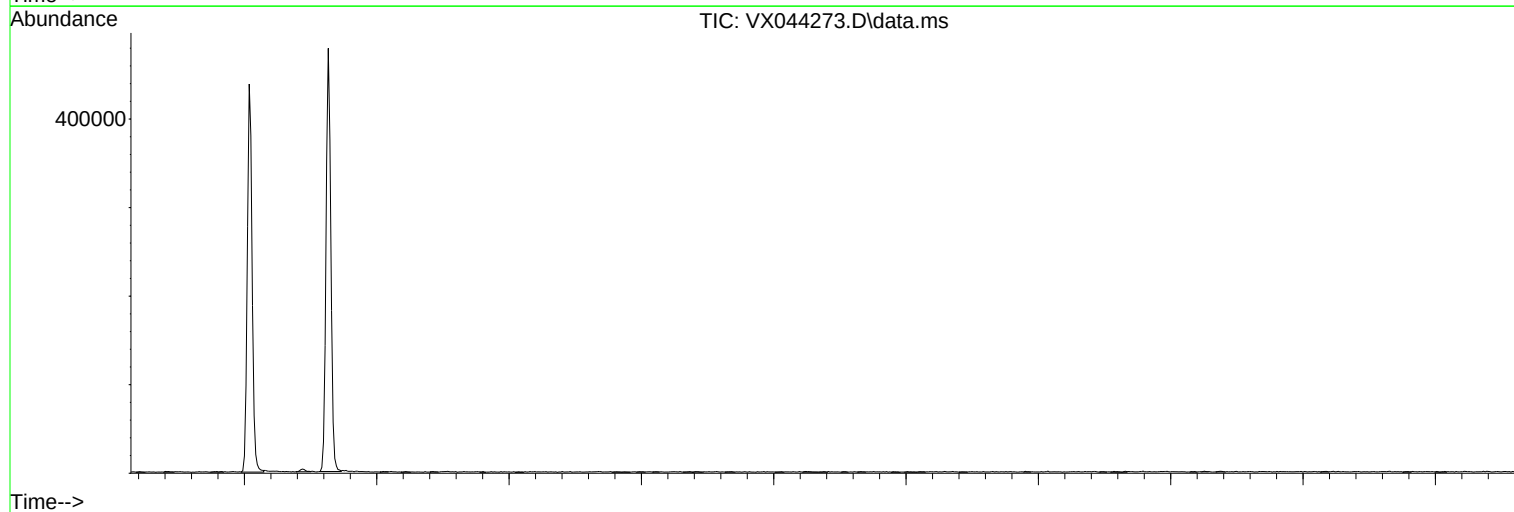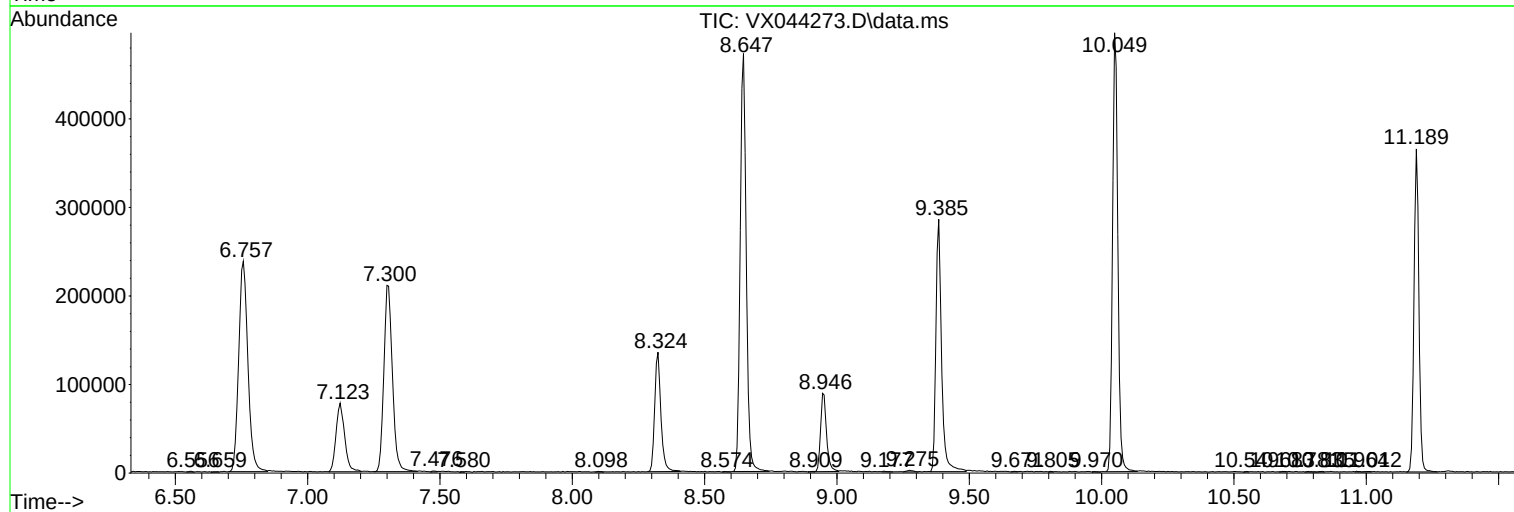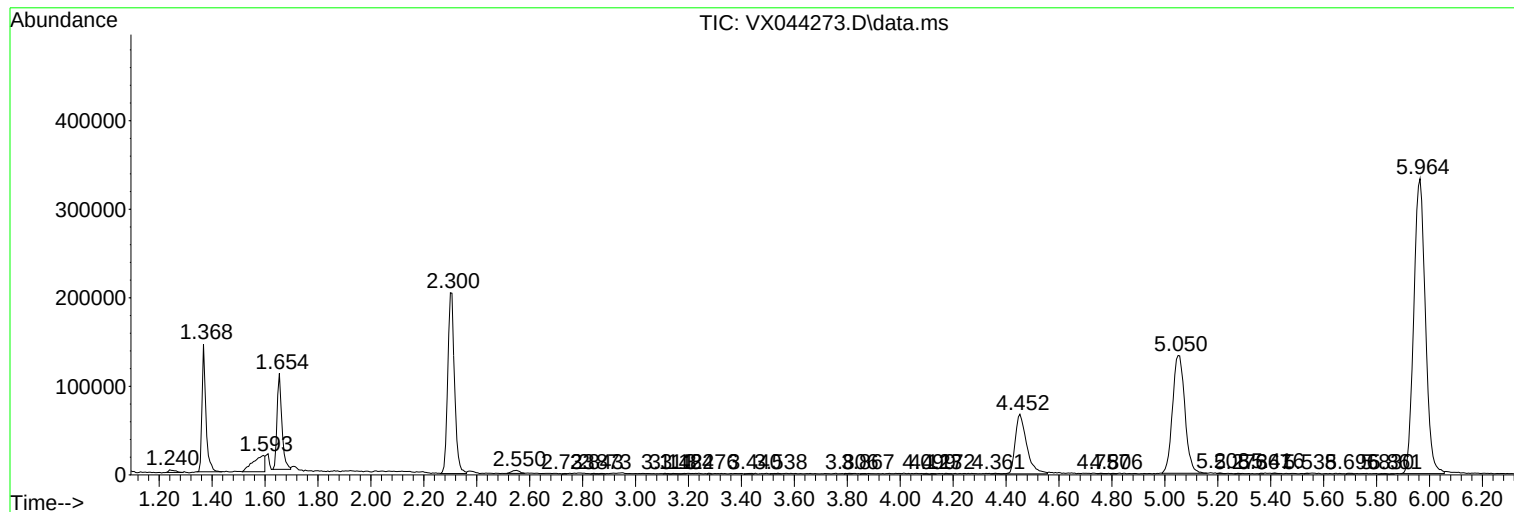

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044273.D
Acq On : 13 Dec 2024 11:43
Operator : JC/MD
Sample : P5252-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044273.D
Acq On : 13 Dec 2024 11:43
Operator : JC/MD
Sample : P5252-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
