

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044274.D
 Acq On : 13 Dec 2024 12:06
 Operator : JC/MD
 Sample : P5252-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044274.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	31	rBV2	5130	7937	0.65%	0.098%
2	1.368	42	46	55	rBV	130744	136498	11.16%	1.689%
3	1.660	90	94	98	rBV	97572	119284	9.75%	1.476%
4	2.300	193	199	210	rBV	189563	303264	24.78%	3.753%
5	2.501	230	232	235	rVB3	641	584	0.05%	0.007%
6	2.532	235	237	238	rBV	715	567	0.05%	0.007%
7	2.660	257	258	262	rVB3	857	894	0.07%	0.011%
8	2.690	262	263	266	rBV2	586	676	0.06%	0.008%
9	2.721	266	268	270	rVB2	870	512	0.04%	0.006%
10	2.751	270	273	275	rBV3	614	584	0.05%	0.007%
11	2.788	275	279	282	rVV3	942	1377	0.11%	0.017%
12	2.892	294	296	300	rVB2	505	585	0.05%	0.007%
13	2.940	300	304	311	rBV6	990	2050	0.17%	0.025%
14	3.068	323	325	329	rVB3	443	562	0.05%	0.007%
15	3.581	407	409	412	rBV3	542	634	0.05%	0.008%
16	3.812	444	447	450	rVB2	792	1146	0.09%	0.014%
17	4.117	495	497	500	rBV4	636	843	0.07%	0.010%
18	4.452	543	552	571	rBV	57945	174733	14.28%	2.162%
19	4.574	571	572	573	rBV	1159	550	0.04%	0.007%
20	4.757	598	602	605	rVB3	623	644	0.05%	0.008%
21	4.824	610	613	614	rBV4	581	608	0.05%	0.008%
22	4.842	614	616	618	rVB3	620	555	0.05%	0.007%
23	4.867	618	620	621	rBV2	603	515	0.04%	0.006%
24	5.050	638	650	671	rBV2	123425	402208	32.87%	4.977%
25	5.233	678	680	682	rBV3	646	542	0.04%	0.007%
26	5.477	718	720	725	rBV	439	594	0.05%	0.007%
27	5.550	729	732	734	rVV3	783	802	0.07%	0.010%
28	5.781	768	770	772	rVB	786	669	0.05%	0.008%
29	5.806	772	774	775	rBV	531	562	0.05%	0.007%
30	5.964	788	800	816	rBV2	303619	914811	74.76%	11.321%
31	6.482	882	885	887	rBV4	617	756	0.06%	0.009%
32	6.507	887	889	891	rBV2	552	536	0.04%	0.007%
33	6.531	891	893	896	rVB3	671	660	0.05%	0.008%
34	6.653	909	913	917	rBV3	495	646	0.05%	0.008%
35	6.757	919	930	941	rBV	228704	561418	45.88%	6.947%
36	7.037	975	976	980	rBV4	611	717	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044274.D
 Acq On : 13 Dec 2024 12:06
 Operator : JC/MD
 Sample : P5252-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.123	980	990	1007	rBV	545839	1223606	100.00%	15.142%
38	7.305	1012	1020	1036	rVB2	191690	419167	34.26%	5.187%
39	7.665	1077	1079	1082	rBV3	549	666	0.05%	0.008%
40	7.696	1082	1084	1087	rVV3	629	898	0.07%	0.011%
41	7.751	1091	1093	1096	rVV3	845	755	0.06%	0.009%
42	7.866	1108	1112	1114	rVV3	789	813	0.07%	0.010%
43	8.007	1133	1135	1140	rBV3	698	1366	0.11%	0.017%
44	8.263	1175	1177	1179	rVB2	658	646	0.05%	0.008%
45	8.281	1179	1180	1181	rBV	920	577	0.05%	0.007%
46	8.324	1181	1187	1198	rBV	113013	194588	15.90%	2.408%
47	8.506	1215	1217	1221	rBV4	594	653	0.05%	0.008%
48	8.598	1229	1232	1233	rBV2	612	609	0.05%	0.008%
49	8.647	1233	1240	1257	rVV	440717	697372	56.99%	8.630%
50	8.866	1274	1276	1280	rBV4	674	712	0.06%	0.009%
51	8.945	1284	1289	1303	rBV	82468	131842	10.77%	1.632%
52	9.165	1323	1325	1328	rVB2	897	695	0.06%	0.009%
53	9.269	1336	1342	1353	rBV	100730	158213	12.93%	1.958%
54	9.384	1356	1361	1379	rBV	240590	368741	30.14%	4.563%
55	9.592	1393	1395	1396	rVB2	938	606	0.05%	0.007%
56	9.707	1412	1414	1416	rBV3	601	661	0.05%	0.008%
57	9.835	1431	1435	1439	rBV3	528	822	0.07%	0.010%
58	9.951	1453	1454	1457	rBV2	645	642	0.05%	0.008%
59	9.988	1457	1460	1465	rBV3	556	771	0.06%	0.010%
60	10.049	1465	1470	1482	rBV	475697	681599	55.70%	8.435%
61	10.378	1522	1524	1527	rVB3	896	941	0.08%	0.012%
62	10.500	1541	1544	1549	rBV2	554	1065	0.09%	0.013%
63	10.640	1565	1567	1569	rBV2	470	572	0.05%	0.007%
64	11.018	1627	1629	1631	rVB	680	553	0.05%	0.007%
65	11.055	1631	1635	1637	rBV2	511	997	0.08%	0.012%
66	11.189	1652	1657	1665	rBV	321853	412666	33.73%	5.107%
67	11.317	1674	1678	1681	rVB3	1324	1511	0.12%	0.019%
68	11.414	1692	1694	1696	rBV2	762	576	0.05%	0.007%
69	11.530	1709	1713	1714	rBV3	512	524	0.04%	0.006%
70	11.762	1747	1751	1752	rBV2	524	555	0.05%	0.007%
71	11.823	1758	1761	1763	rBV4	654	701	0.06%	0.009%
72	12.018	1788	1793	1805	rVV	432200	552830	45.18%	6.841%
73	12.140	1811	1813	1815	rVB	1044	586	0.05%	0.007%
74	12.158	1815	1816	1819	rBV3	815	745	0.06%	0.009%
75	12.219	1823	1826	1834	rVB5	3476	4772	0.39%	0.059%
76	12.317	1837	1842	1852	rBV	434556	554772	45.34%	6.865%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044274.D
 Acq On : 13 Dec 2024 12:06
 Operator : JC/MD
 Sample : P5252-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	12.737	1908	1911	1913	rBV2	566	607	0.05%	0.008%
78	12.920	1939	1941	1945	rBV3	489	630	0.05%	0.008%
79	13.012	1953	1956	1959	rBV3	486	667	0.05%	0.008%
80	13.408	2020	2021	2023	rBV2	516	538	0.04%	0.007%
81	13.469	2030	2031	2034	rBV2	472	632	0.05%	0.008%
82	13.945	2106	2109	2113	rBV3	529	839	0.07%	0.010%
83	14.237	2155	2157	2160	rBV3	472	587	0.05%	0.007%
84	14.341	2172	2174	2179	rVB3	561	755	0.06%	0.009%
85	14.390	2181	2182	2184	rBV	513	505	0.04%	0.006%
86	14.585	2210	2214	2216	rVV3	517	830	0.07%	0.010%
87	14.658	2225	2226	2229	rBV2	583	730	0.06%	0.009%
88	14.725	2236	2237	2241	rVB3	727	632	0.05%	0.008%
89	15.133	2300	2304	2310	rBV4	639	1438	0.12%	0.018%
90	15.249	2321	2323	2326	rBV2	811	1202	0.10%	0.015%
91	15.298	2329	2331	2334	rVB3	575	577	0.05%	0.007%
92	15.993	2444	2445	2449	rBV2	750	832	0.07%	0.010%
93	16.036	2449	2452	2455	rVB3	816	994	0.08%	0.012%
94	16.133	2467	2468	2471	rBV2	827	803	0.07%	0.010%
95	16.194	2477	2478	2481	rBV2	692	696	0.06%	0.009%
96	16.286	2491	2493	2496	rBV2	863	869	0.07%	0.011%
97	16.487	2523	2526	2529	rBV3	750	1061	0.09%	0.013%
98	16.542	2533	2535	2537	rVB2	670	501	0.04%	0.006%
99	16.688	2556	2559	2562	rBV2	917	1241	0.10%	0.015%
100	16.718	2562	2564	2569	rVB3	627	929	0.08%	0.011%

Sum of corrected areas: 8081004




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044274.D
Acq On : 13 Dec 2024 12:06
Operator : JC/MD
Sample : P5252-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

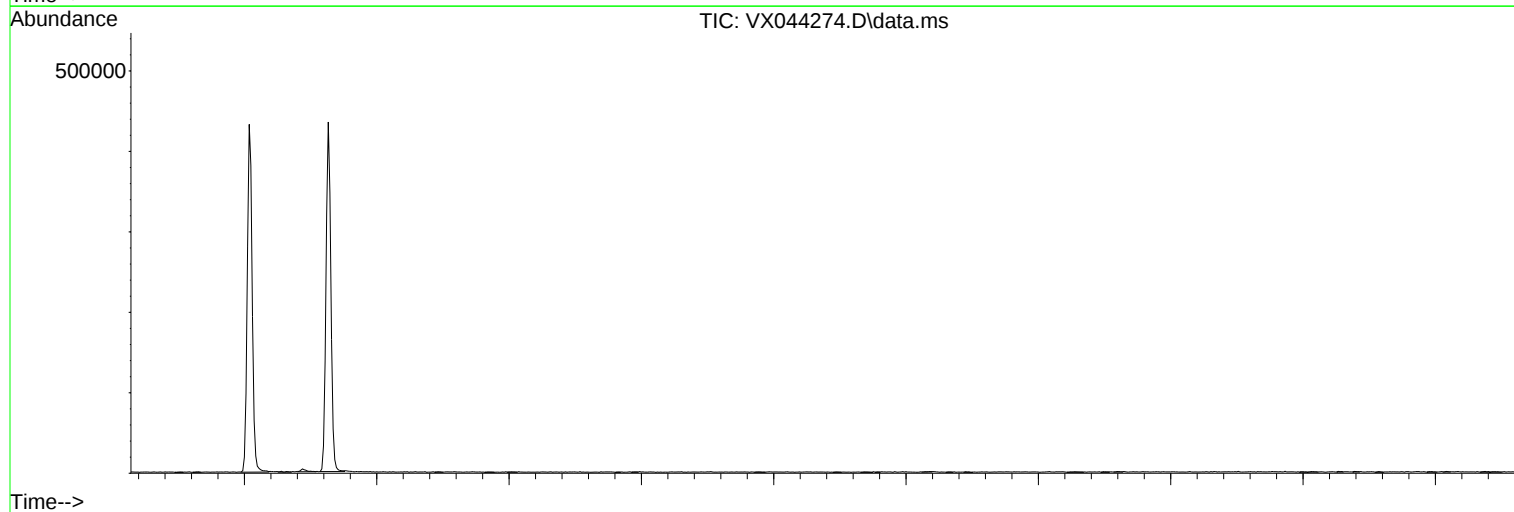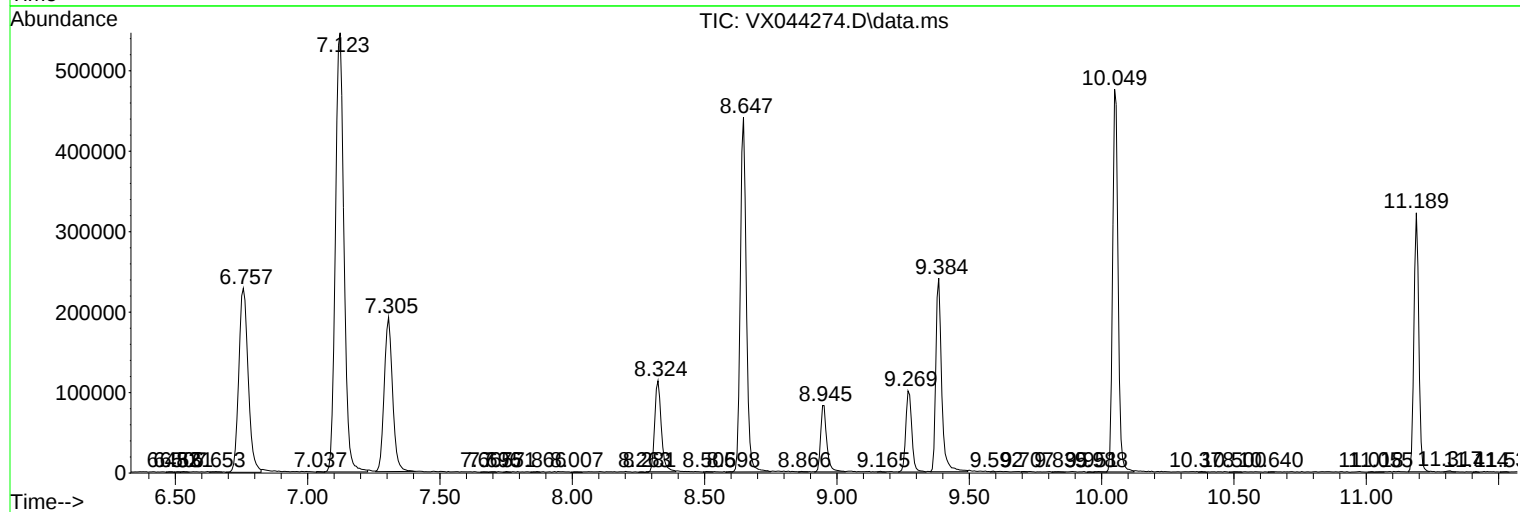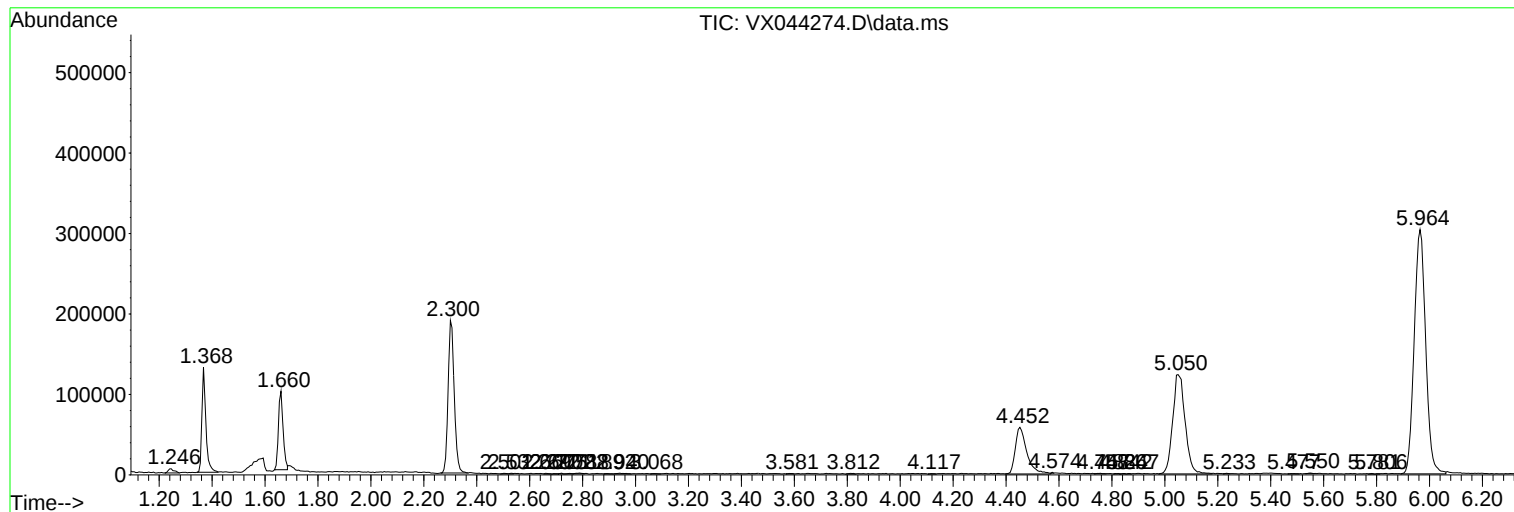

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044274.D
Acq On : 13 Dec 2024 12:06
Operator : JC/MD
Sample : P5252-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044274.D
Acq On : 13 Dec 2024 12:06
Operator : JC/MD
Sample : P5252-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc